

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
 Data File : P0048558.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2018 22:43
 Operator : SM/SJ
 Sample : J4659-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 082218-DBRI-E-U-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:09:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	4.382	3.624	4522920	4740480	23.876	17.510 #
2)	SA Decachlor...	10.062	8.600	3511284	3368966	20.391	20.116

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
Data File : P0048558.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2018 22:43
Operator : SM/SJ
Sample : J4659-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082218-DBRI-E-U-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:09:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

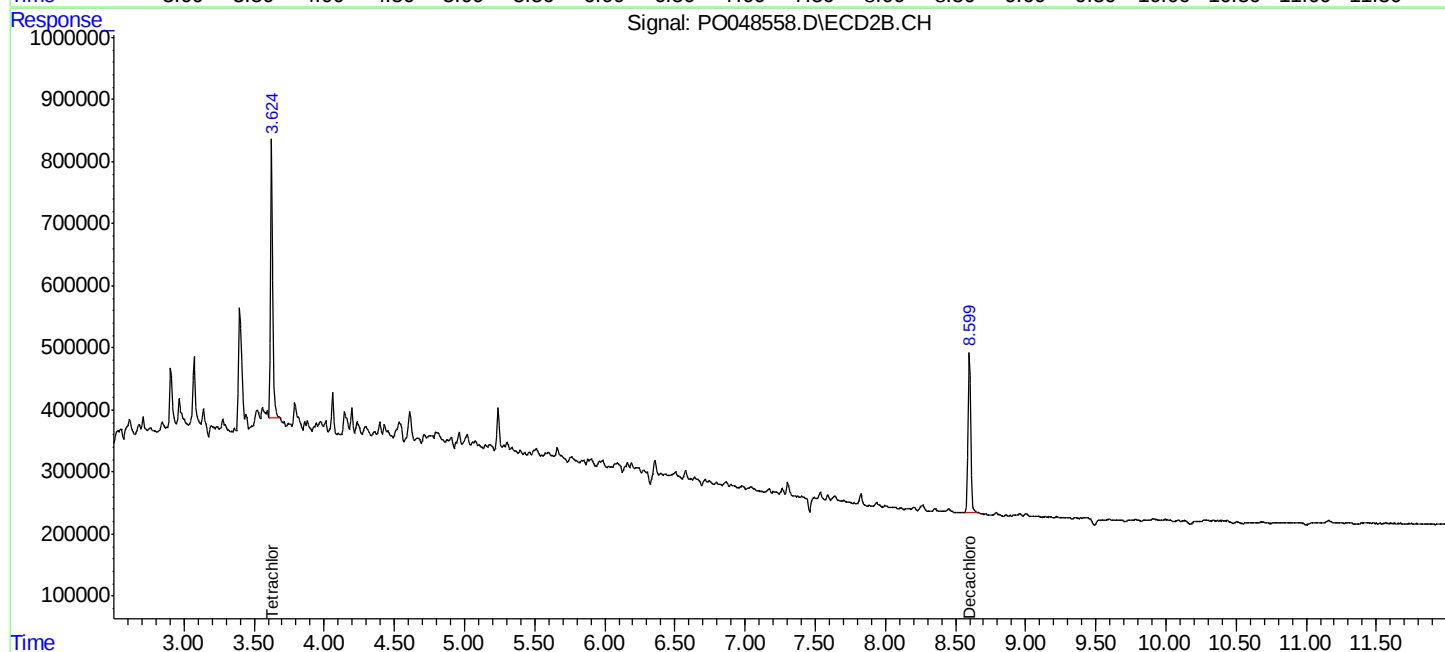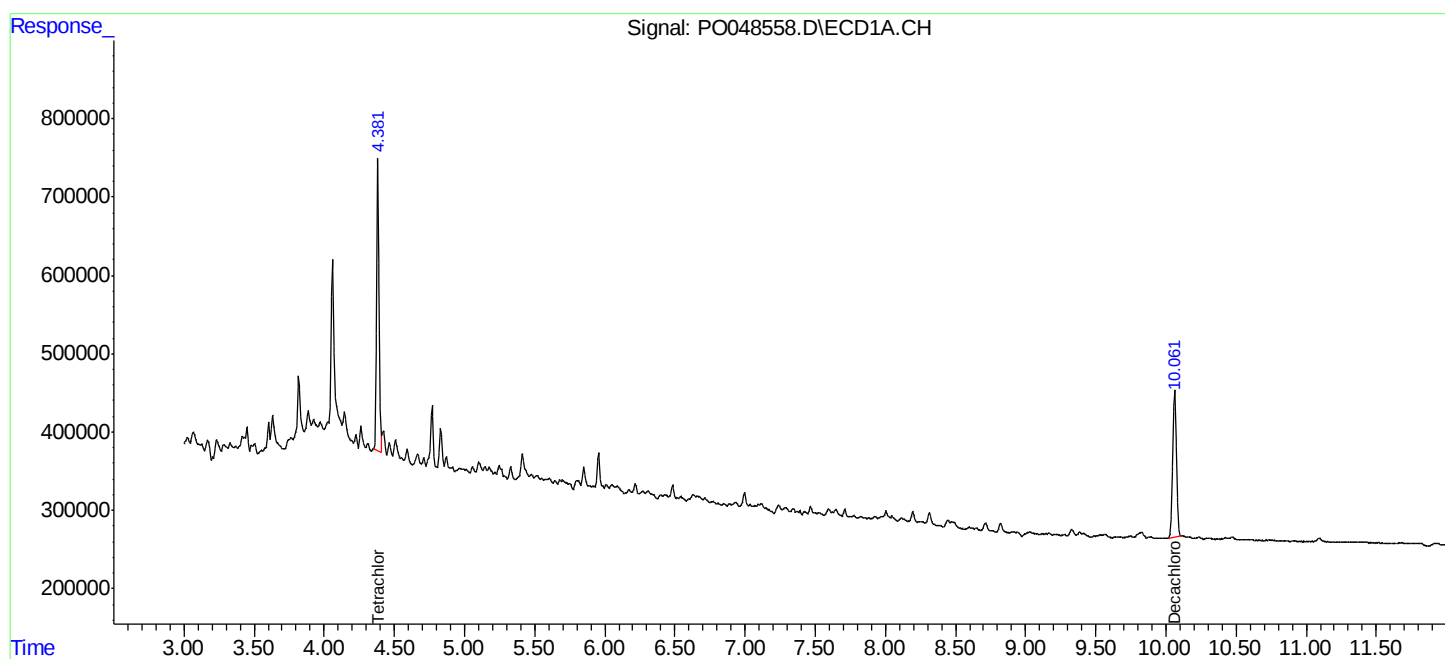


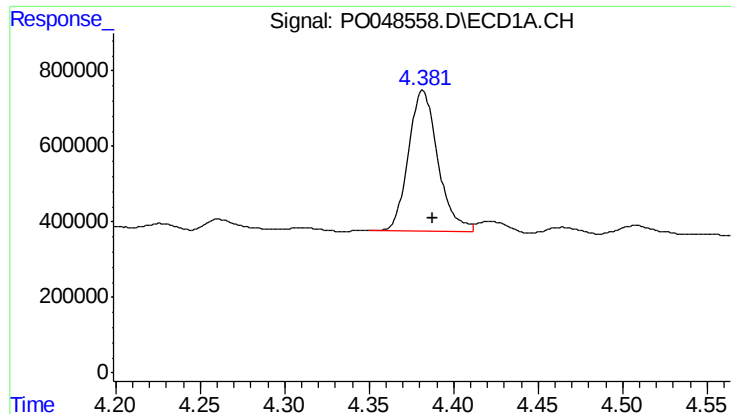

#1 Tetrachloro-m-xylene


R.T.: 4.382 min
Delta R.T.: -0.006 min
Response: 4522920
Conc: 23.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
082218-DBRI-E-U-S

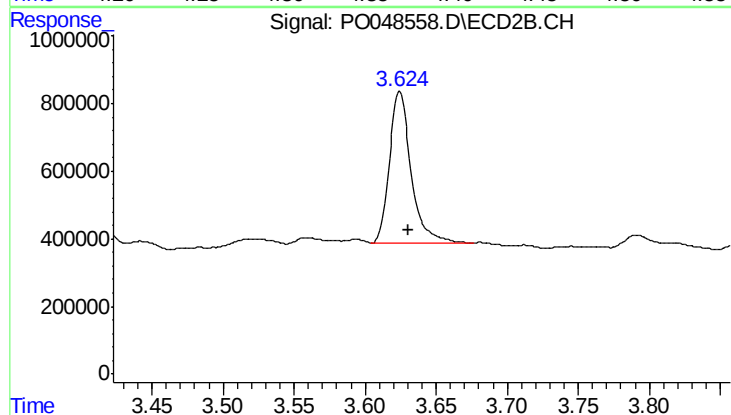


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.006 min
Response: 4740480
Conc: 17.51 ng/ml

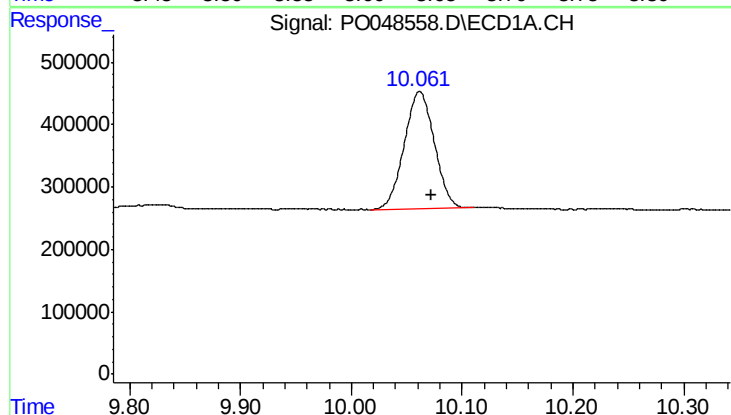

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.010 min
Response: 3511284
Conc: 20.39 ng/ml

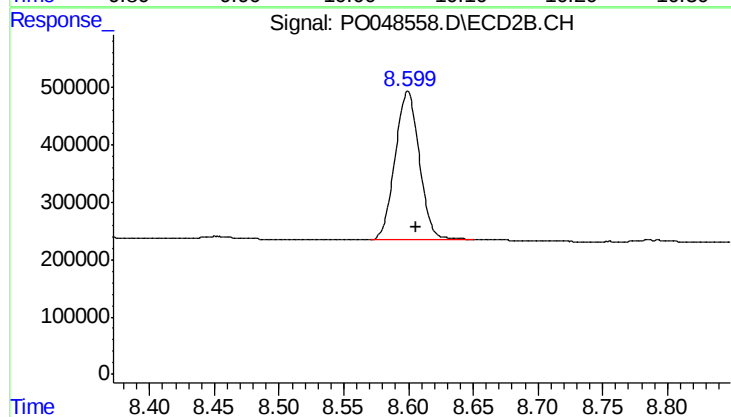

#2 Decachlorobiphenyl

R.T.: 8.600 min
Delta R.T.: -0.007 min
Response: 3368966
Conc: 20.12 ng/ml