

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
Data File : P0048562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2018 23:46
Operator : SM/SJ
Sample : J4660-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082318-SIDI-F-D-B

Manual Integrations
APPROVED

Sohil
8/28/2018 2:31:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:10:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.624	4611935	4741850	24.346m	17.515m#
2) SA Decachlor...	10.062	8.599	3820981	3648512	22.189	21.785

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
Data File : P0048562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2018 23:46
Operator : SM/SJ
Sample : J4660-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
082318-SIDI-F-D-B


Manual Integrations
APPROVED

Sohil
8/28/2018 2:31:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:10:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

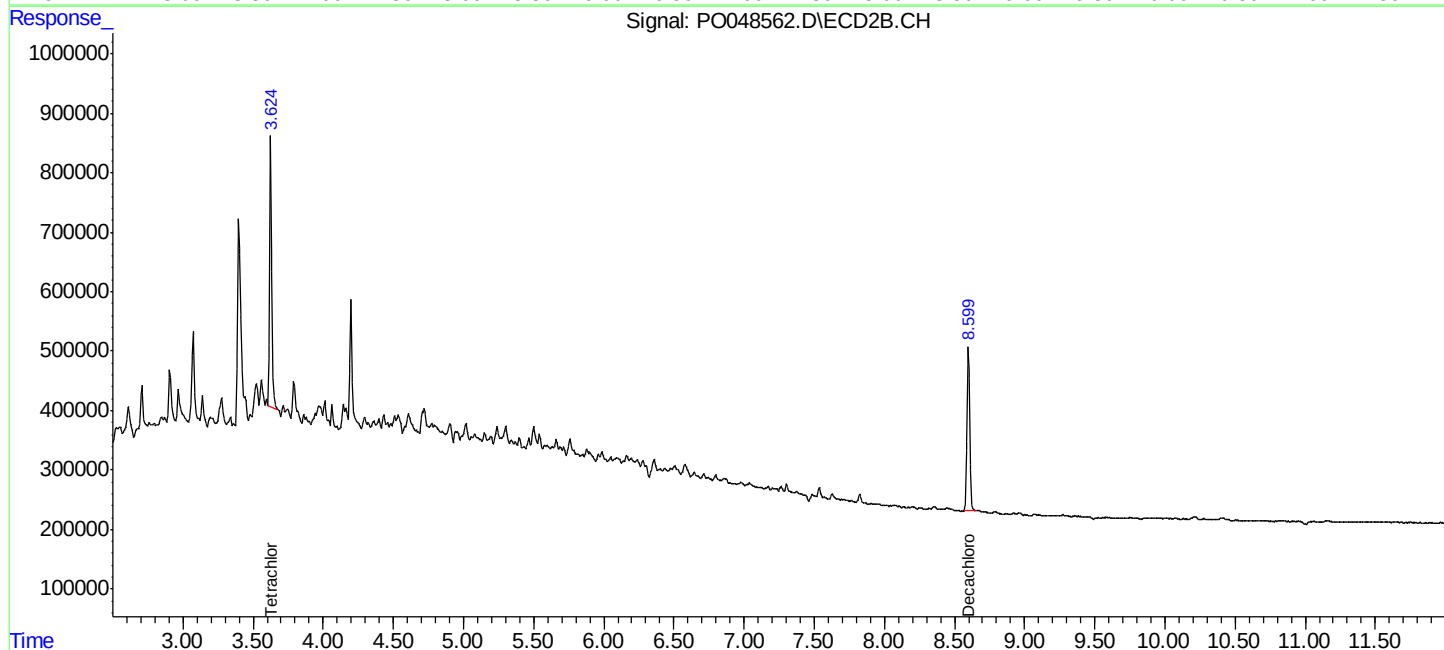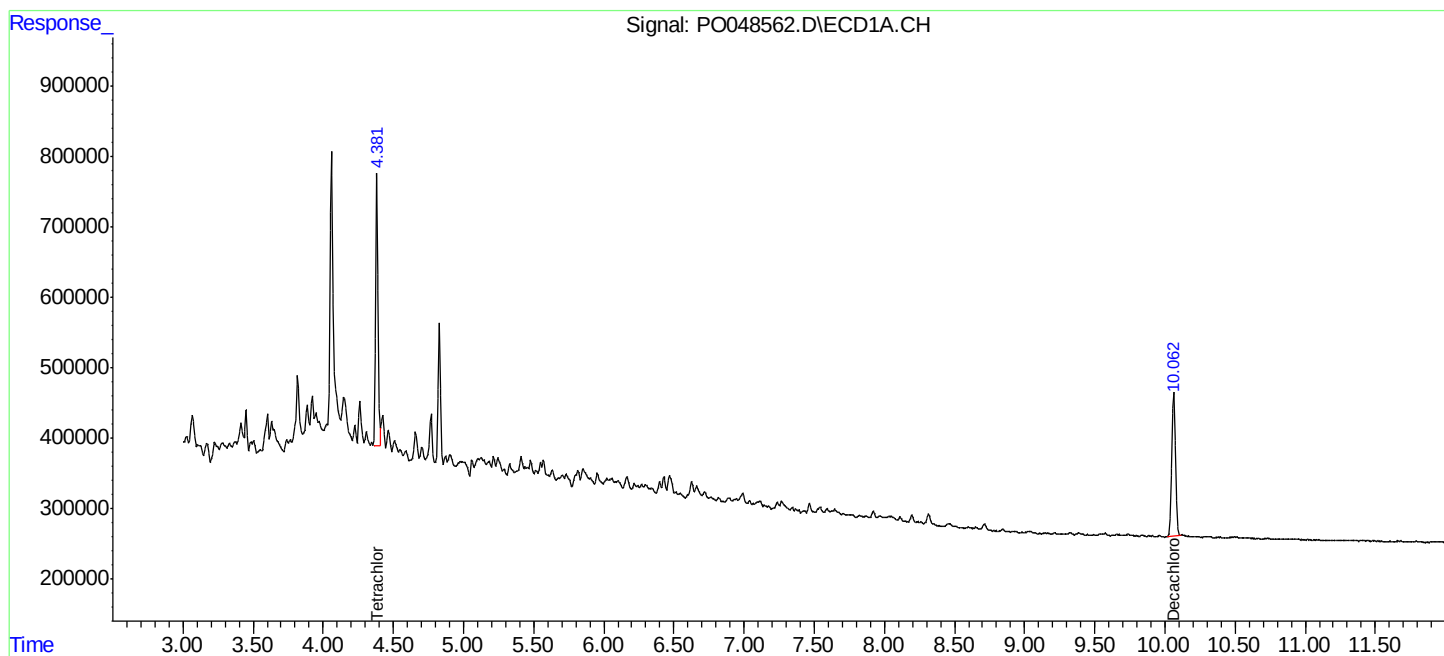

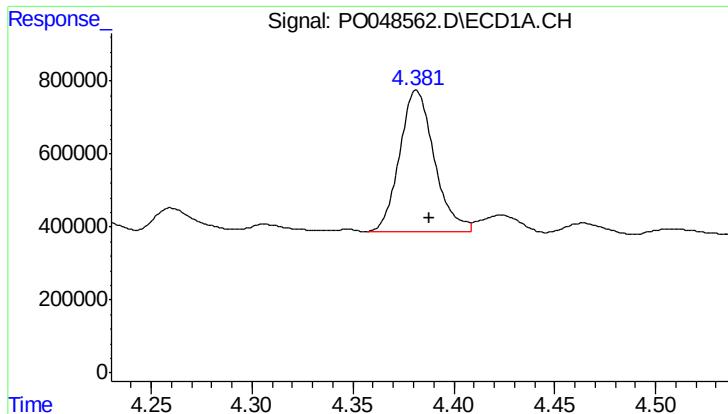


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: -0.007 min
Response: 4611935
Conc: 24.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
082318-SIDI-F-D-B


Manual Integrations
APPROVED

Sohil
8/28/2018 2:31:58 PM

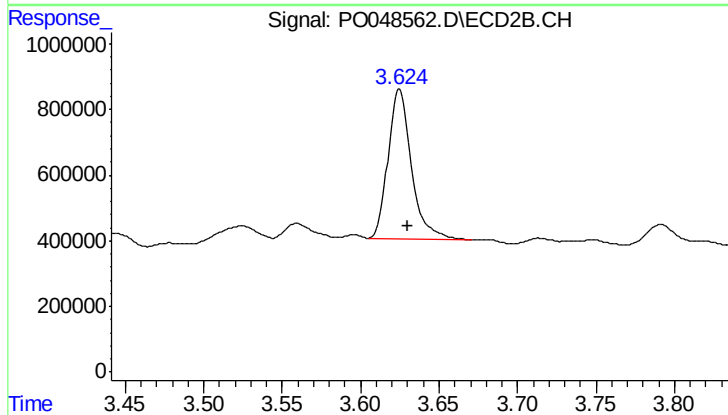


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.006 min
Response: 4741850
Conc: 17.52 ng/ml m

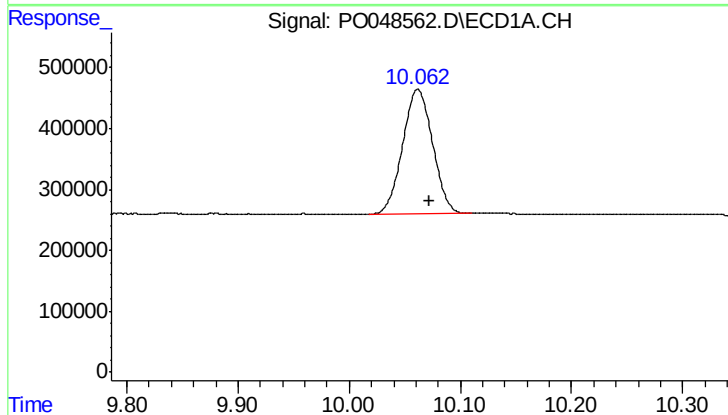

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.010 min
Response: 3820981
Conc: 22.19 ng/ml

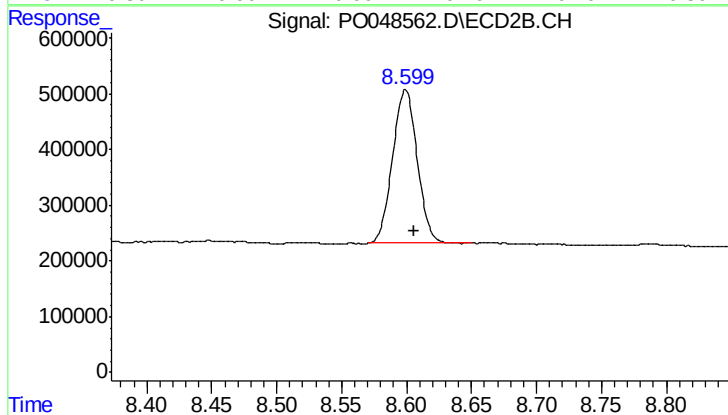

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: -0.007 min
Response: 3648512
Conc: 21.79 ng/ml