

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
 Data File : P0048576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2018 3:30
 Operator : SM/SJ
 Sample : J4660-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 082318-TIPC-F-D-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:28:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.382	3.624	4067519	4165120	21.472	15.385 #
2) SA Decachlor...	10.062	8.599	3116501	2863592	18.098	17.099

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
Data File : P0048576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2018 3:30
Operator : SM/SJ
Sample : J4660-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082318-TIPC-F-D-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:28:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

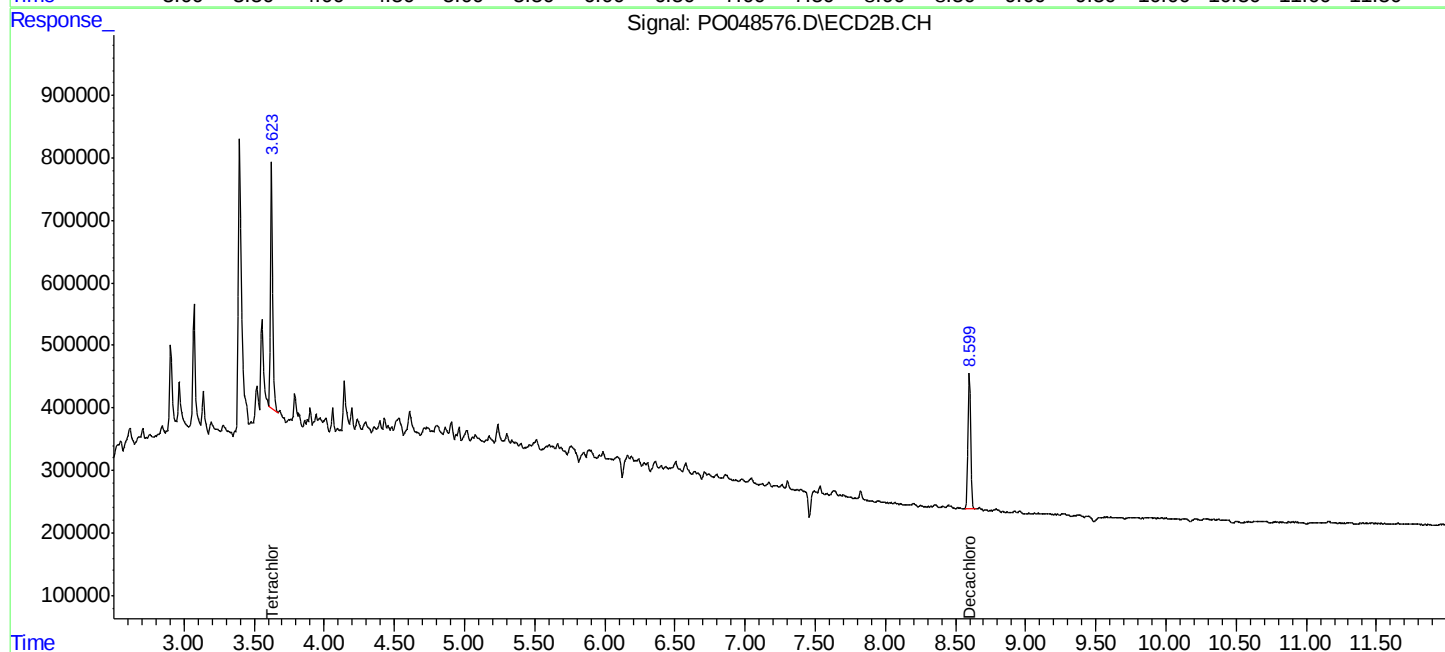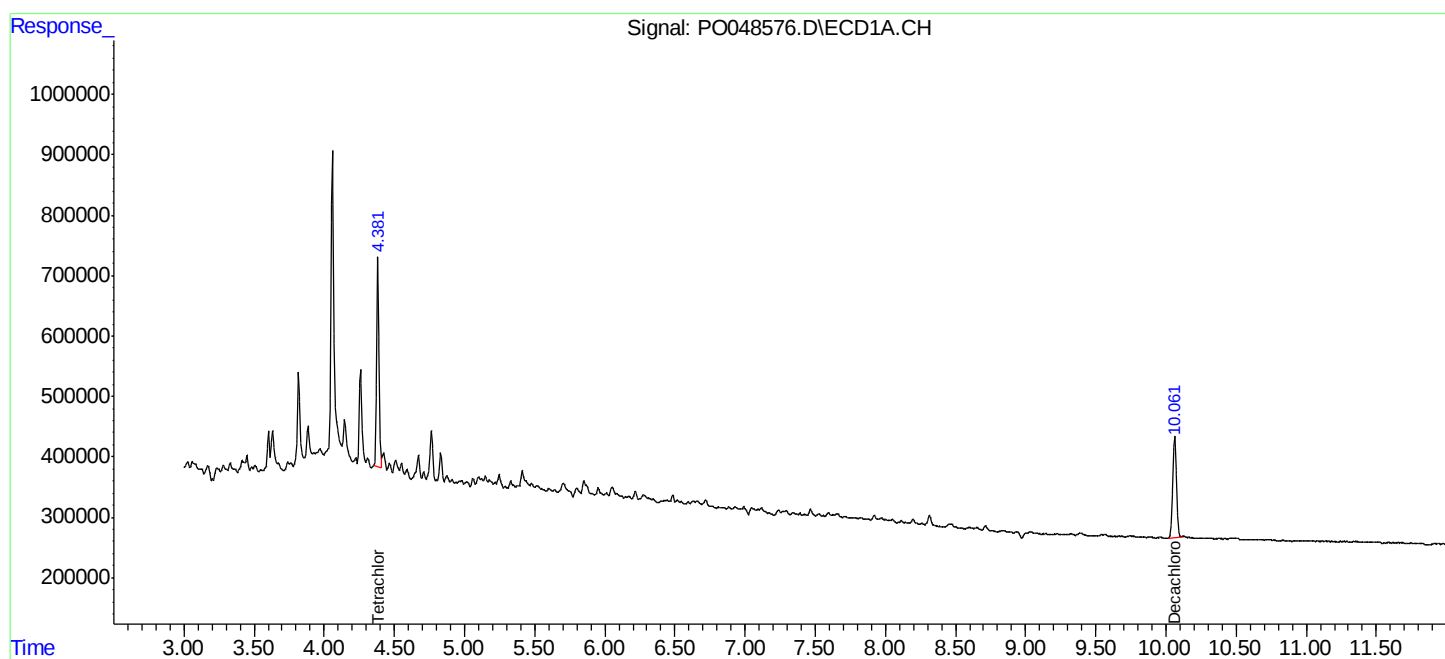


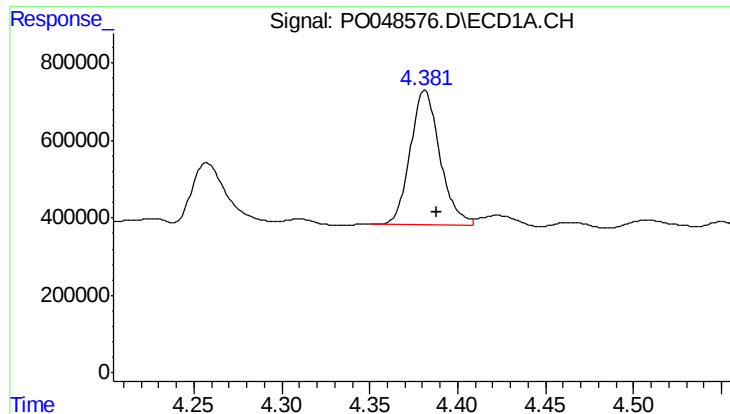

#1 Tetrachloro-m-xylene


R.T.: 4.382 min
Delta R.T.: -0.006 min
Response: 4067519
Conc: 21.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
082318-TIPC-F-D-B

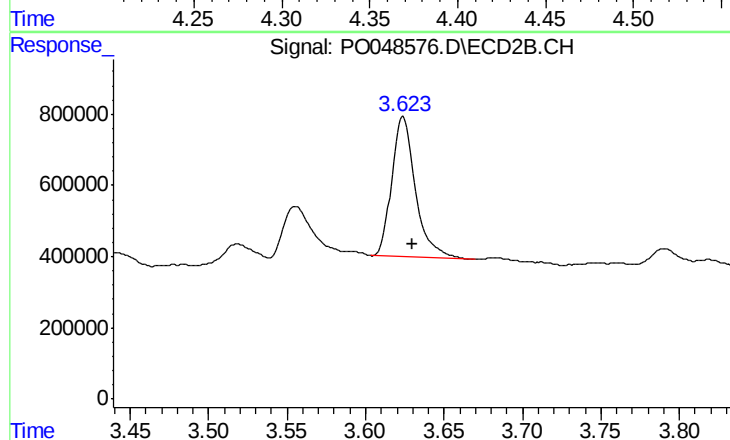


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.007 min
Response: 4165120
Conc: 15.38 ng/ml

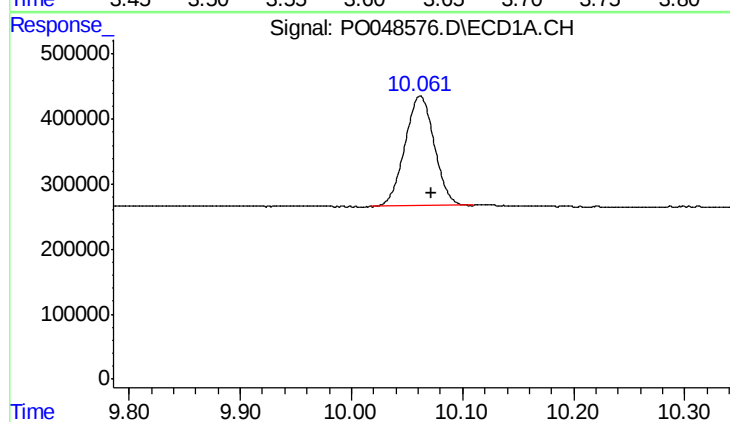

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.010 min
Response: 3116501
Conc: 18.10 ng/ml

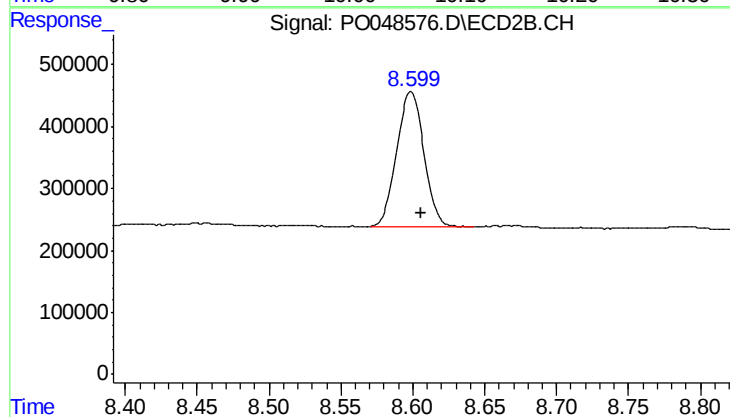

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: -0.007 min
Response: 2863592
Conc: 17.10 ng/ml