

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
 Data File : P0048577.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2018 3:46
 Operator : SM/SJ
 Sample : J4660-14
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 082318-TIPC-F-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:29:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.623	4472264	4697203	23.609	17.350 #
2) SA Decachlor...	10.059	8.597	3374638	3058352	19.597	18.261

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
Data File : P0048577.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2018 3:46
Operator : SM/SJ
Sample : J4660-14
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082318-TIPC-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:29:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

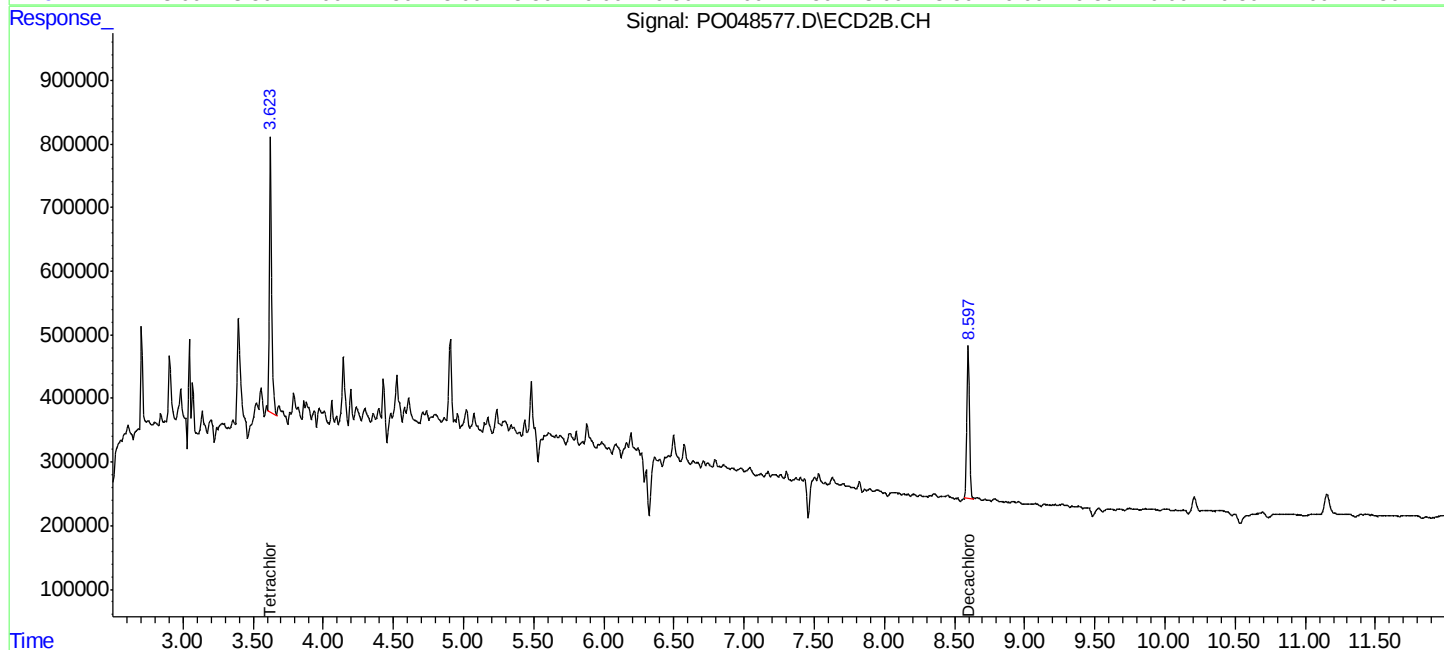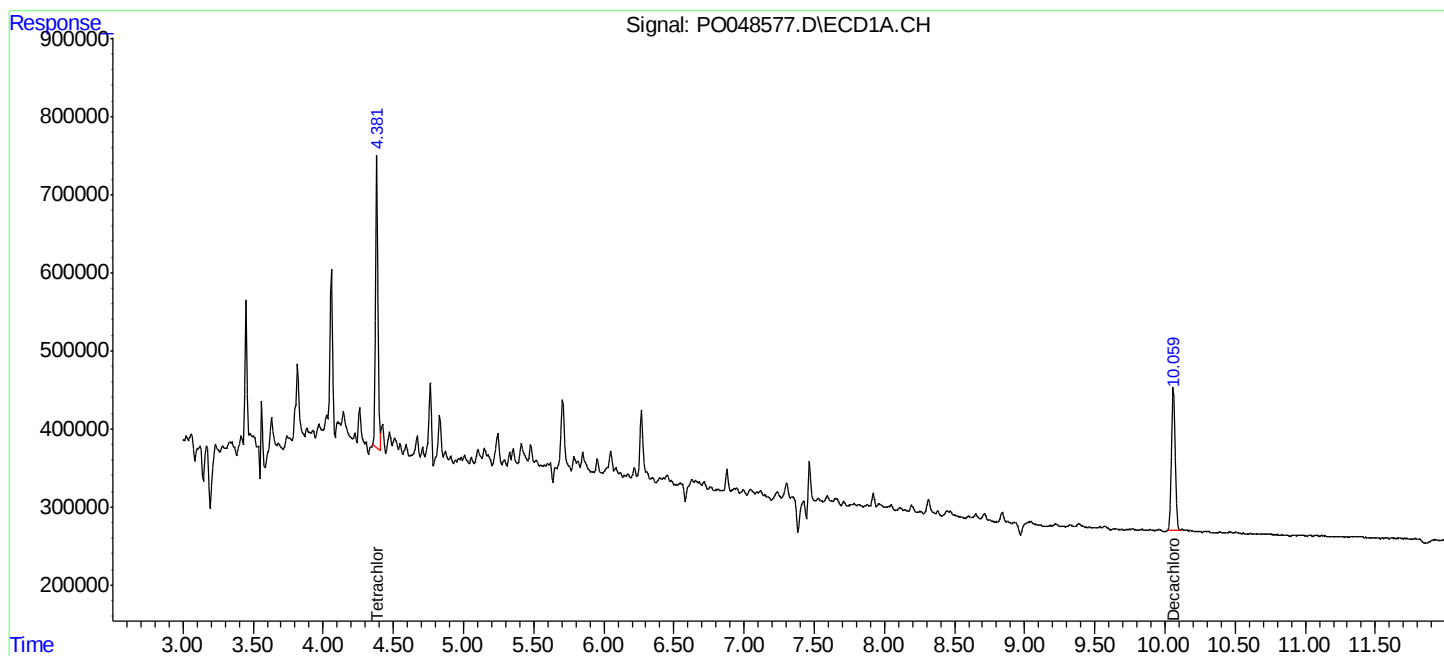


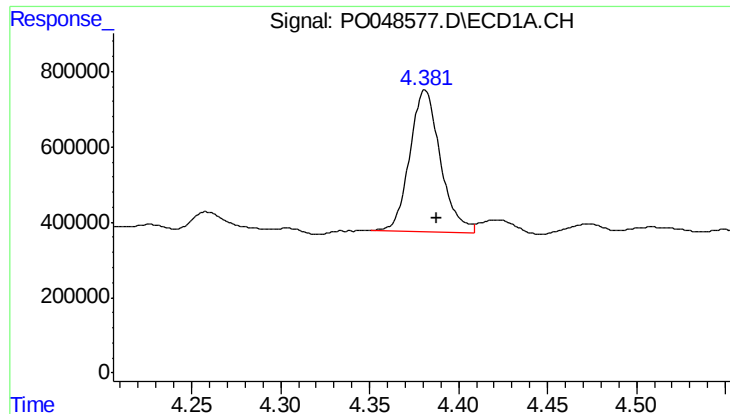

#1 Tetrachloro-m-xylene


R.T.: 4.381 min
Delta R.T.: -0.007 min
Response: 4472264
Conc: 23.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
082318-TIPC-F-D-S

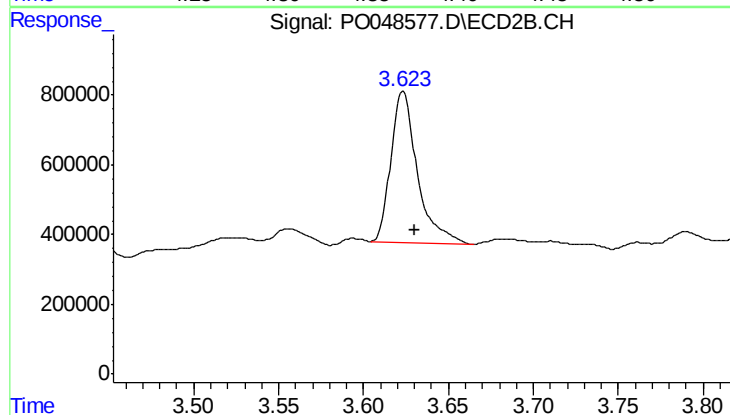


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.007 min
Response: 4697203
Conc: 17.35 ng/ml

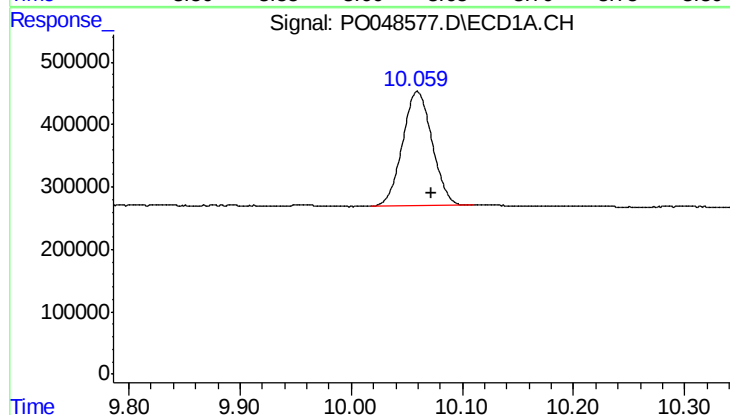

#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: -0.013 min
Response: 3374638
Conc: 19.60 ng/ml

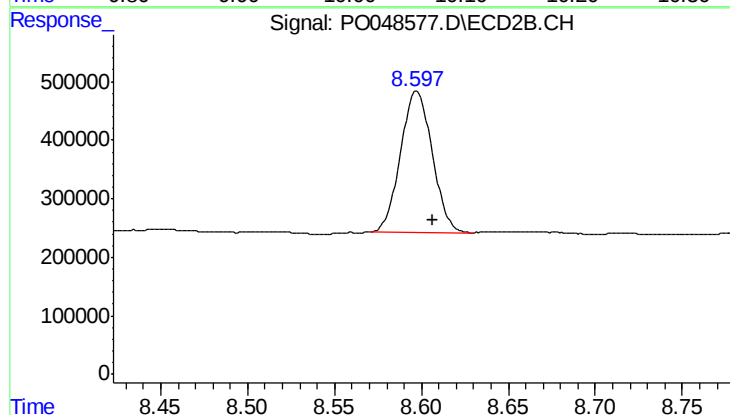

#2 Decachlorobiphenyl

R.T.: 8.597 min
Delta R.T.: -0.009 min
Response: 3058352
Conc: 18.26 ng/ml