

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
 Data File : P0059937.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2019 5:48
 Operator : SM/AJ
 Sample : K4543-11
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 08:44:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.125	3.500	1070818	925653	30.584	25.716
2)	SA Decachlor...	9.595	8.358	1023026	750690	19.230	18.618
Target Compounds							
3)	L1 AR-1016-1	5.292	0.000	13497	0	8.415	N.D. #
4)	L1 AR-1016-2	5.292	0.000	13497	0	5.641	N.D. #
5)	L1 AR-1016-3	5.354	0.000	7036	0	4.724	N.D. #
6)	L1 AR-1016-4	5.494	0.000	6530	0	5.398	N.D. #
7)	L1 AR-1016-5	5.735	0.000	789	0	0.614	N.D. #
8)	L2 AR-1221-1	4.357	0.000	10809	0	25.524	N.D. #
9)	L2 AR-1221-2	4.445	3.801	9440	195034	29.064	640.243 #
10)	L2 AR-1221-3	4.508	3.826	29746	10345	28.280	10.573 #
11)	L3 AR-1232-1	4.508	3.826	29746	10345	23.865	9.074 #
12)	L3 AR-1232-2	5.021	0.000	33986	0	48.112	N.D. #
13)	L3 AR-1232-3	5.337	0.000	6894	0	4.502	N.D. #
14)	L3 AR-1232-4	5.494	0.000	6530	0	8.352	N.D. #
15)	L3 AR-1232-5	5.551	0.000	12472	0	20.748	N.D. #
16)	L4 AR-1242-1	5.292	0.000	13497	0	10.632	N.D. #
17)	L4 AR-1242-2	5.337	0.000	6894	0	3.715	N.D. #
18)	L4 AR-1242-3	5.382	0.000	22702	0	19.422	N.D. #
19)	L4 AR-1242-4	5.494	0.000	6530	0	6.747	N.D. #
20)	L4 AR-1242-5	6.210	0.000	11344	0	9.028	N.D. #
21)	L5 AR-1248-1	5.292	0.000	13497	0	13.463	N.D. #
22)	L5 AR-1248-2	5.551	0.000	12472	0	8.596	N.D. #
23)	L5 AR-1248-3	5.735	0.000	789	0	0.475	N.D. #
24)	L5 AR-1248-4	6.145	0.000	14383	0	7.036	N.D. #
25)	L5 AR-1248-5	6.172	0.000	9604	0	4.843	N.D. #
26)	L6 AR-1254-1	6.109	0.000	16825	0	8.064	N.D. #
27)	L6 AR-1254-2	6.309	0.000	40210	0	12.052	N.D. #
28)	L6 AR-1254-3	6.712	0.000	138046	0	38.903	N.D. #
29)	L6 AR-1254-4	6.967	0.000	40380	0	13.709	N.D. #
30)	L6 AR-1254-5	7.390	0.000	18165	0	5.874	N.D. #
31)	L7 AR-1260-1	6.850	0.000	88125	0	32.690	N.D. #
32)	L7 AR-1260-2	7.108	0.000	46445	0	12.517	N.D. #
33)	L7 AR-1260-3	7.457	0.000	14883	0	4.543	N.D. #
34)	L7 AR-1260-4	7.684	0.000	7575	0	2.466	N.D. #
35)	L7 AR-1260-5	7.995	0.000	14756	0	2.084	N.D. #
36)	L8 AR-1262-1	7.516	0.000	8058	0	1.660	N.D. #
37)	L8 AR-1262-2	8.049	0.000	8167	0	1.058	N.D. #
38)	L8 AR-1262-3	8.300	0.000	3099	0	0.607	N.D. #
39)	L8 AR-1262-4	8.409	0.000	17480	0	4.535	N.D. #
40)	L8 AR-1262-5	8.948	0.000	79905	0	31.133	N.D. #
41)	L9 AR-1268-1	8.300	0.000	3099	0	0.329	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
Data File : P0059937.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 5:48
Operator : SM/AJ
Sample : K4543-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:44:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
42)	L9 AR-1268-2	8.409	0.000	17480	0	2.218	N.D.	#
43)	L9 AR-1268-3	8.557	0.000	25081	0	3.558	N.D.	#
44)	L9 AR-1268-4	8.948	0.000	79905	0	28.742	N.D.	#
45)	L9 AR-1268-5	9.312	0.000	47123	0	2.555	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082719\
Data File : PO059937.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 5:48
Operator : SM/AJ
Sample : K4543-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:44:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

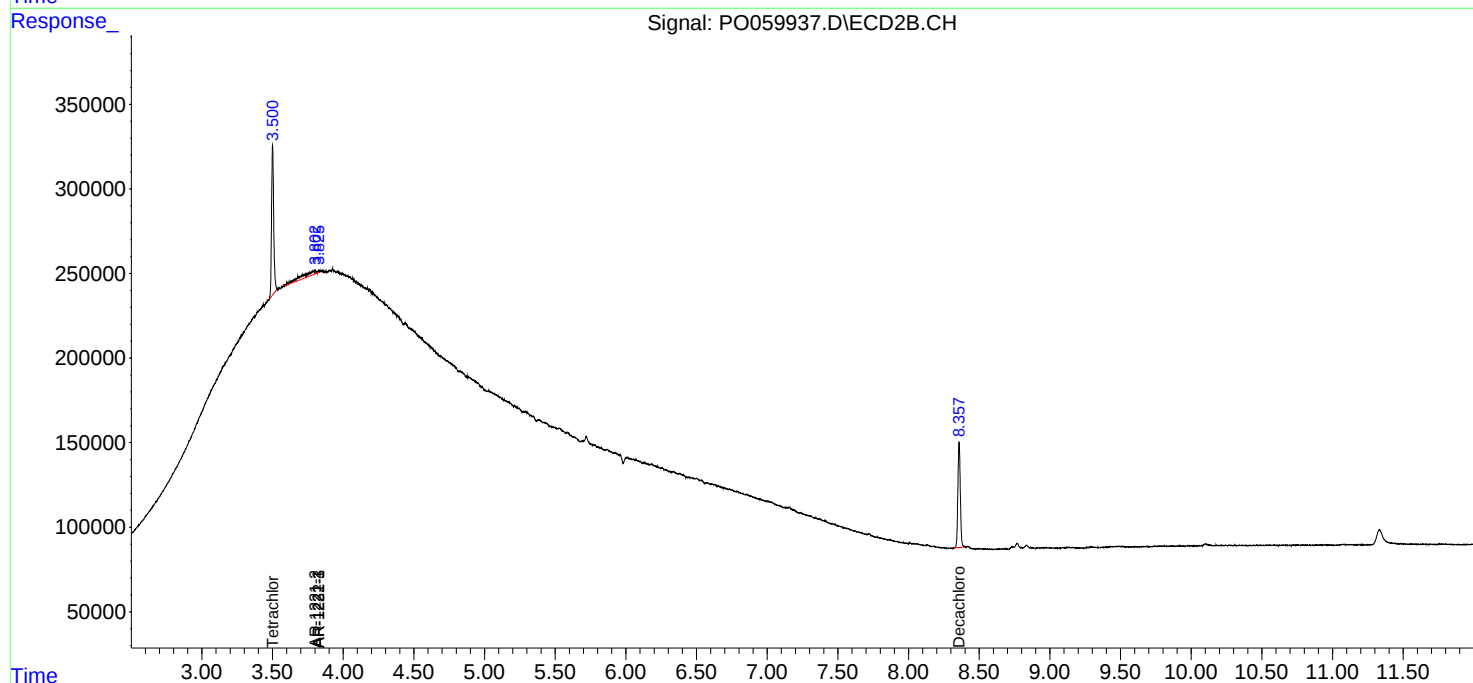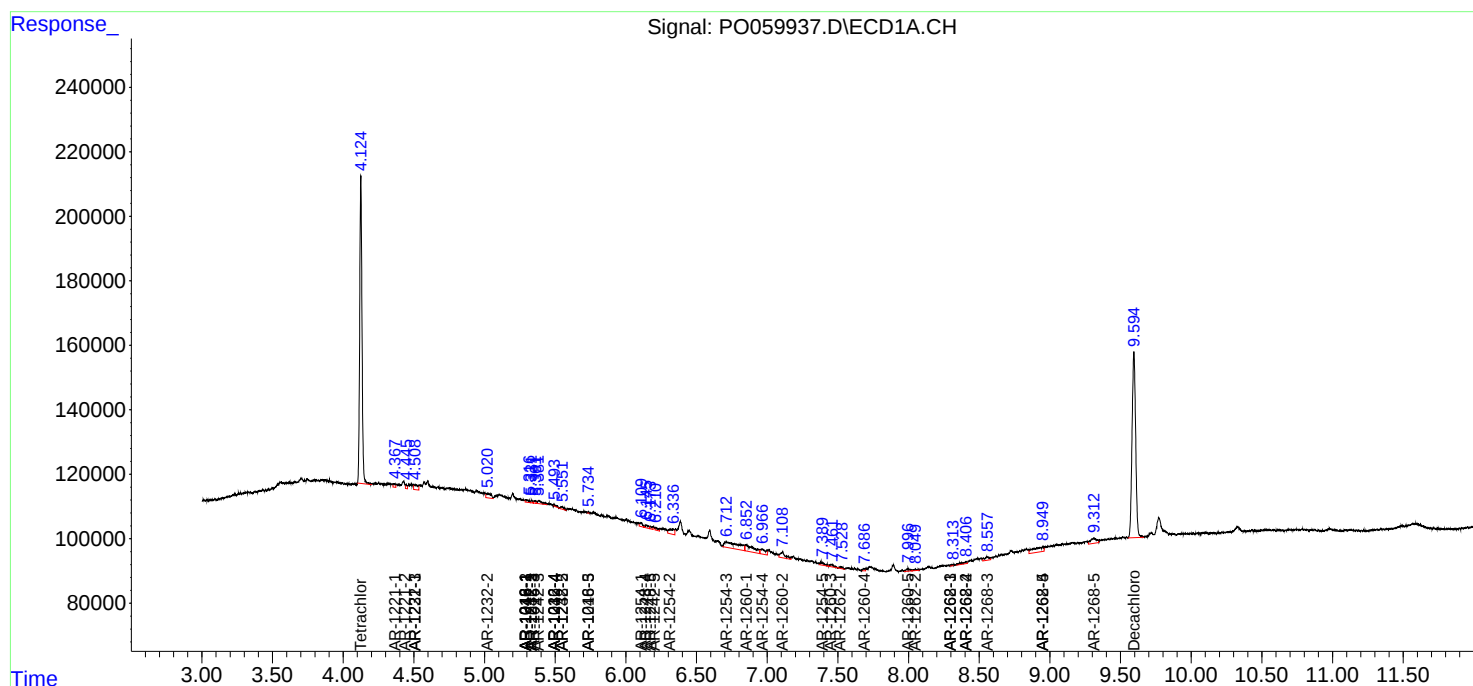


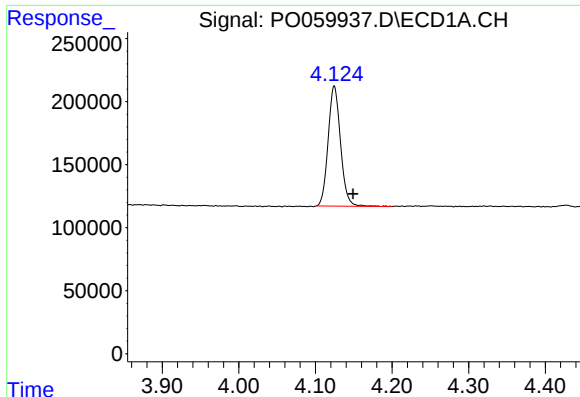

#1 Tetrachloro-m-xylene


R.T.: 4.125 min
Delta R.T.: -0.024 min
Response: 1070818
Conc: 30.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

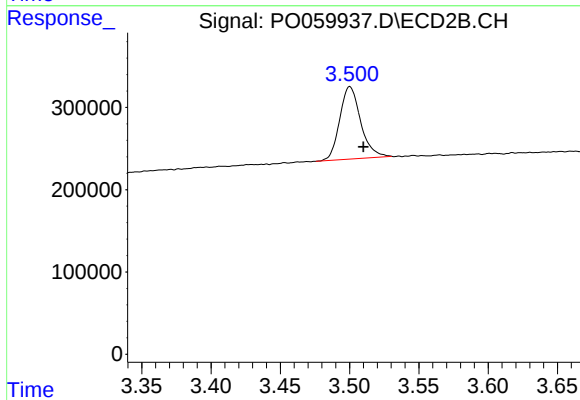


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 925653
Conc: 25.72 ng/ml

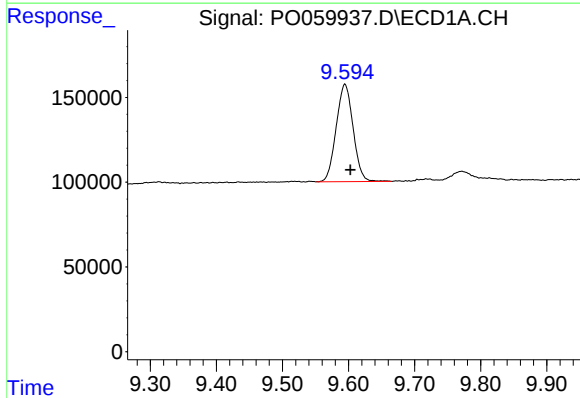


#2 Decachlorobiphenyl

R.T.: 9.595 min
Delta R.T.: -0.008 min
Response: 1023026
Conc: 19.23 ng/ml

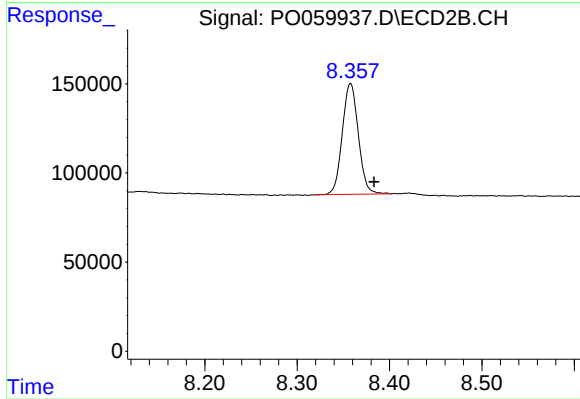

#2 Decachlorobiphenyl


R.T.: 8.358 min
Delta R.T.: -0.026 min
Response: 750690
Conc: 18.62 ng/ml

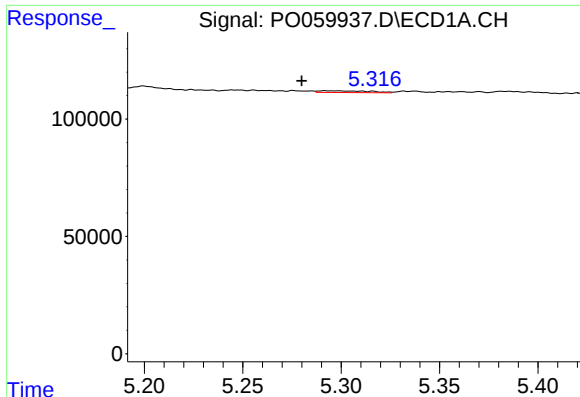

#3 AR-1016-1


R.T.: 5.292 min
Delta R.T.: 0.012 min
Response: 13497
Conc: 8.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

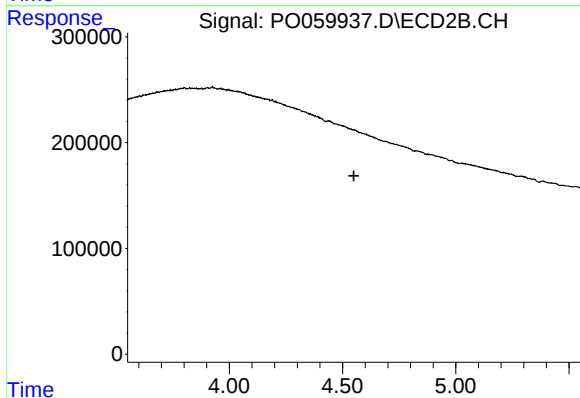


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

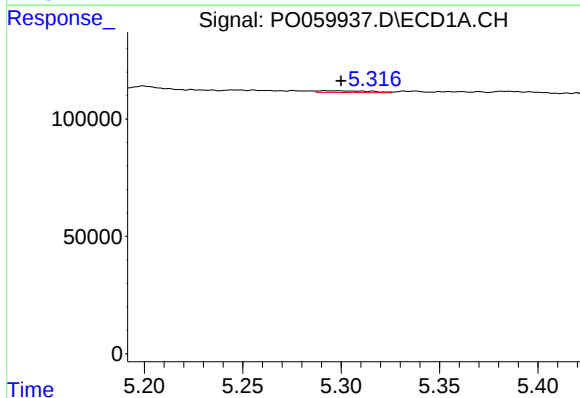


#4 AR-1016-2

R.T.: 5.292 min
Delta R.T.: -0.008 min
Response: 13497
Conc: 5.64 ng/ml

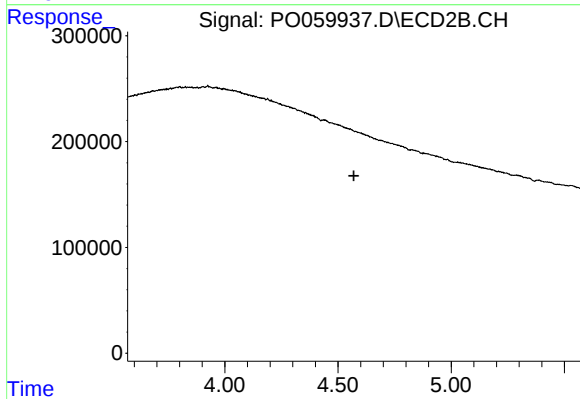

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.570 min
Response: 0
Conc: N.D.

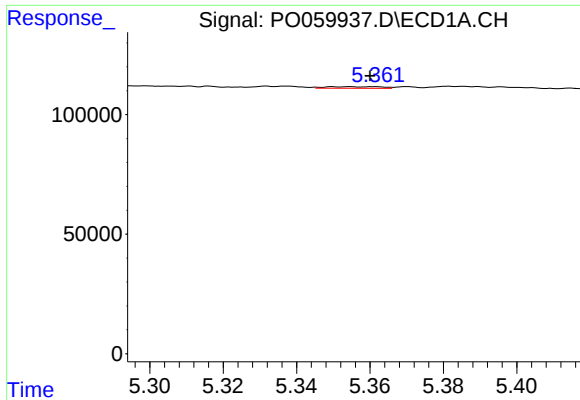

#5 AR-1016-3


R.T.: 5.354 min
Delta R.T.: -0.006 min
Response: 7036
Conc: 4.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

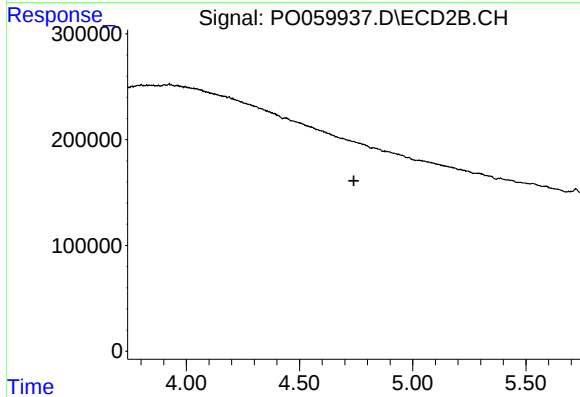


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

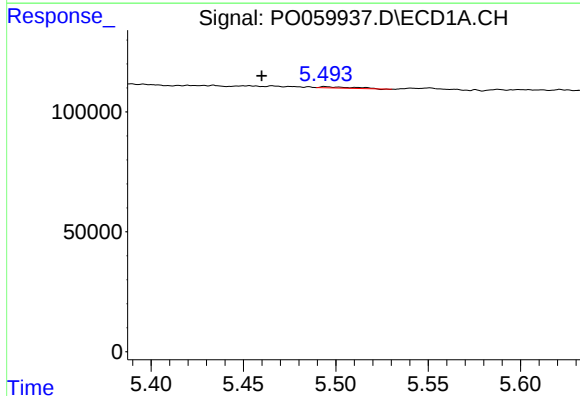


#6 AR-1016-4

R.T.: 5.494 min
Delta R.T.: 0.034 min
Response: 6530
Conc: 5.40 ng/ml

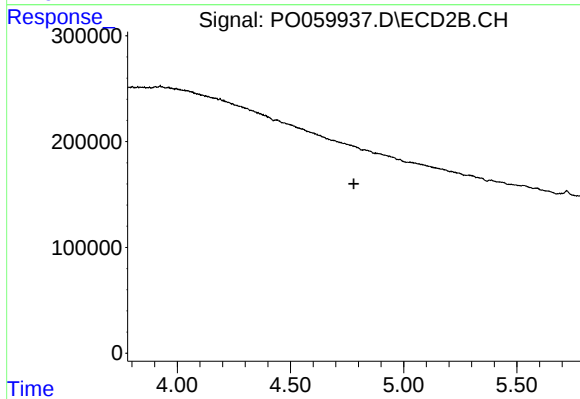

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.780 min
Response: 0
Conc: N.D.

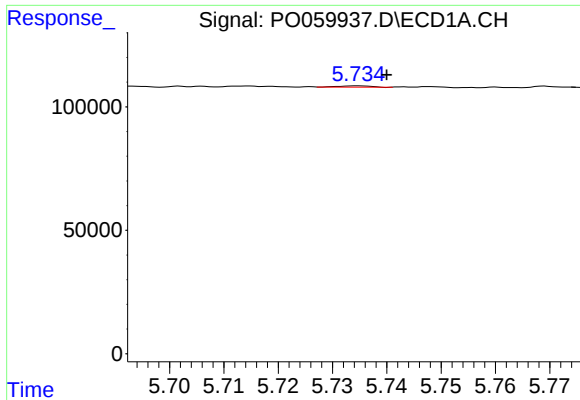

#7 AR-1016-5


R.T.: 5.735 min
Delta R.T.: -0.005 min
Response: 789
Conc: 0.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

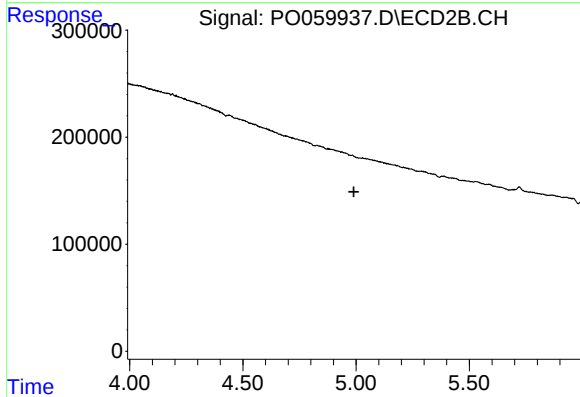


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.990 min
Response: 0
Conc: N.D.

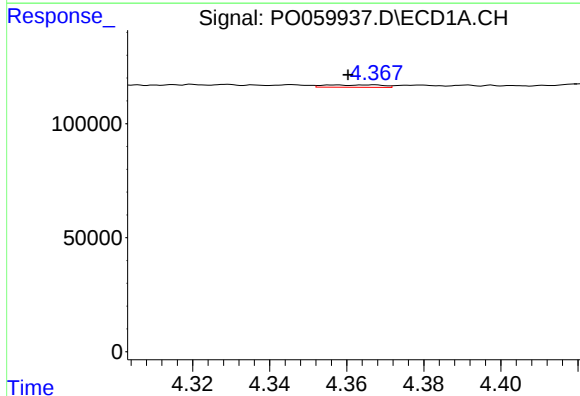


#8 AR-1221-1

R.T.: 4.357 min
Delta R.T.: -0.003 min
Response: 10809
Conc: 25.52 ng/ml

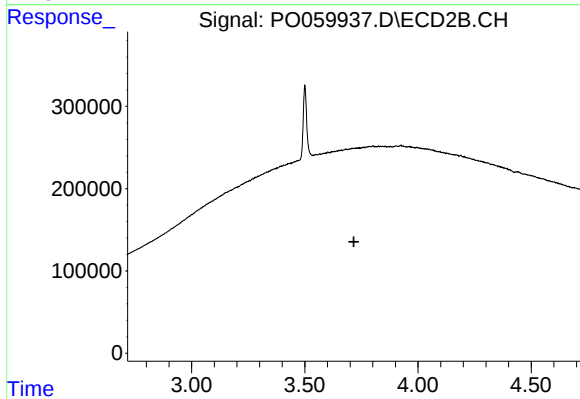

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.717 min
Response: 0
Conc: N.D.

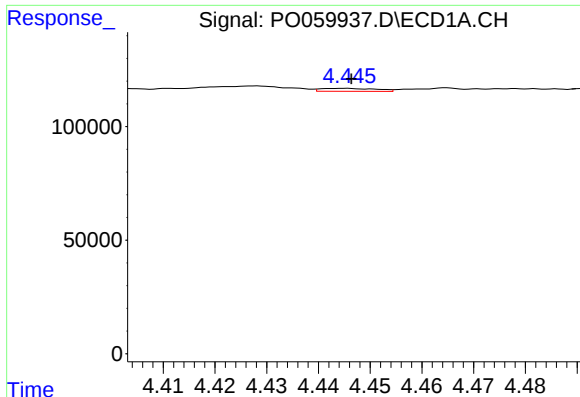

#9 AR-1221-2


R.T.: 4.445 min
Delta R.T.: -0.002 min
Response: 9440
Conc: 29.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

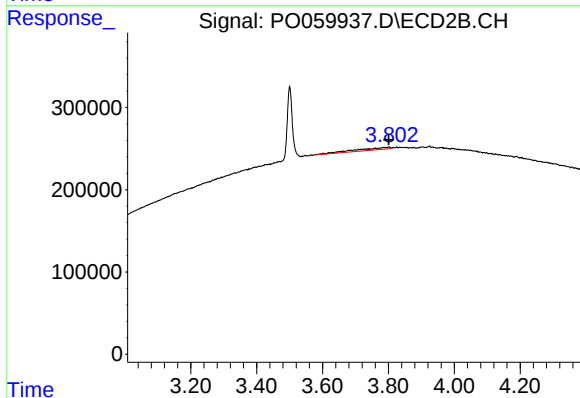


#9 AR-1221-2

R.T.: 3.801 min
Delta R.T.: 0.000 min
Response: 195034
Conc: 640.24 ng/ml

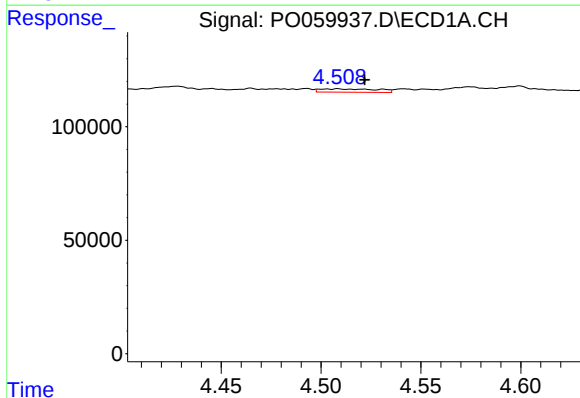


#10 AR-1221-3

R.T.: 4.508 min
Delta R.T.: -0.013 min
Response: 29746
Conc: 28.28 ng/ml

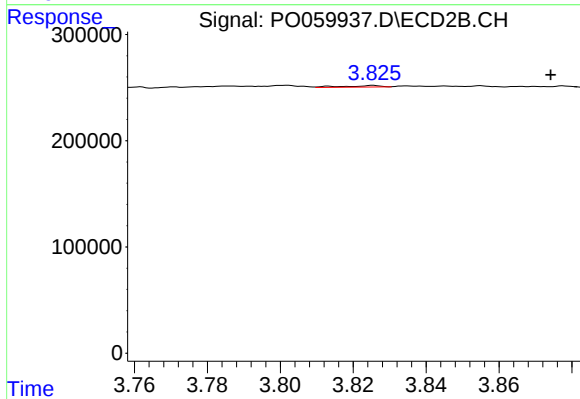

#10 AR-1221-3


R.T.: 3.826 min
Delta R.T.: -0.049 min
Response: 10345
Conc: 10.57 ng/ml

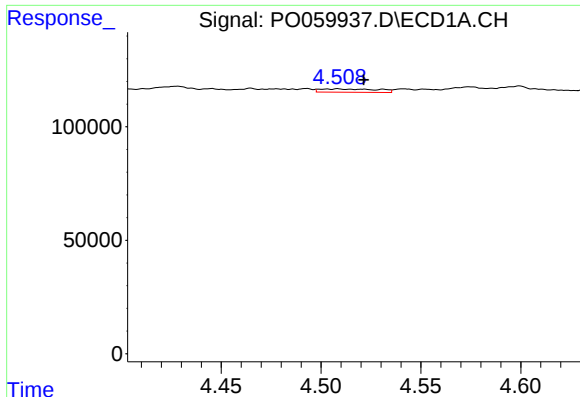

#11 AR-1232-1


R.T.: 4.508 min
Delta R.T.: -0.013 min
Response: 29746
Conc: 23.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

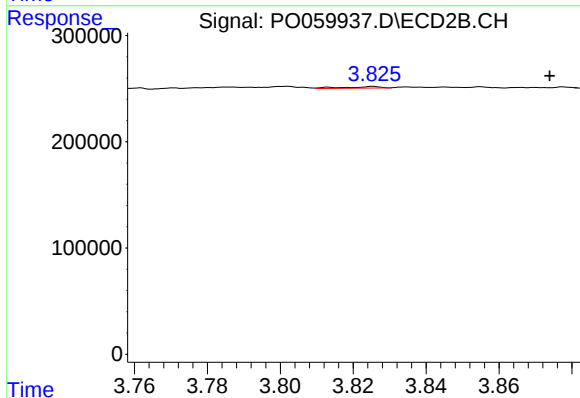


#11 AR-1232-1

R.T.: 3.826 min
Delta R.T.: -0.048 min
Response: 10345
Conc: 9.07 ng/ml

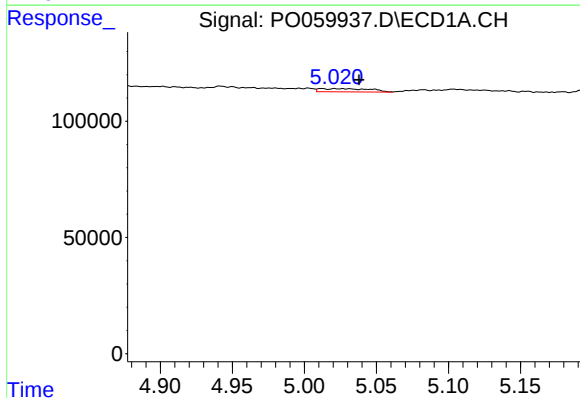


#12 AR-1232-2

R.T.: 5.021 min
Delta R.T.: -0.017 min
Response: 33986
Conc: 48.11 ng/ml

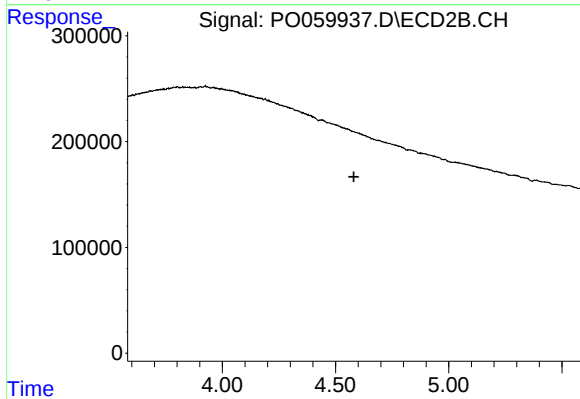

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

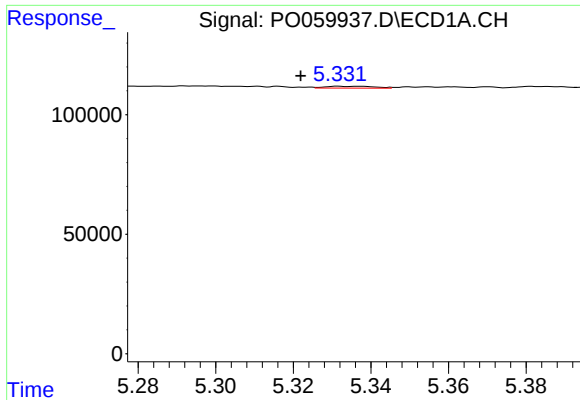

#13 AR-1232-3


R.T.: 5.337 min
Delta R.T.: 0.015 min
Response: 6894
Conc: 4.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

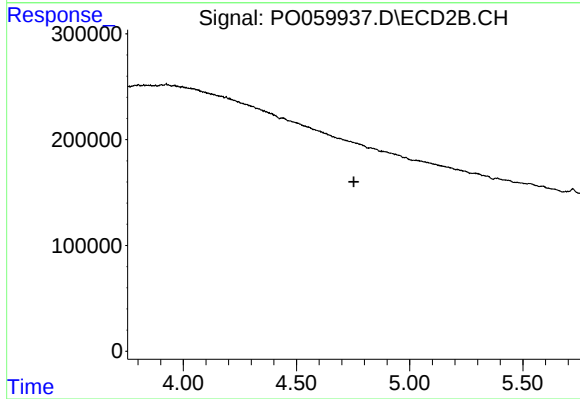


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.753 min
Response: 0
Conc: N.D.

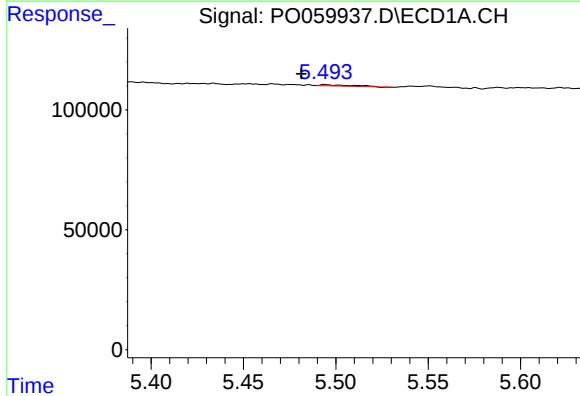


#14 AR-1232-4

R.T.: 5.494 min
Delta R.T.: 0.013 min
Response: 6530
Conc: 8.35 ng/ml

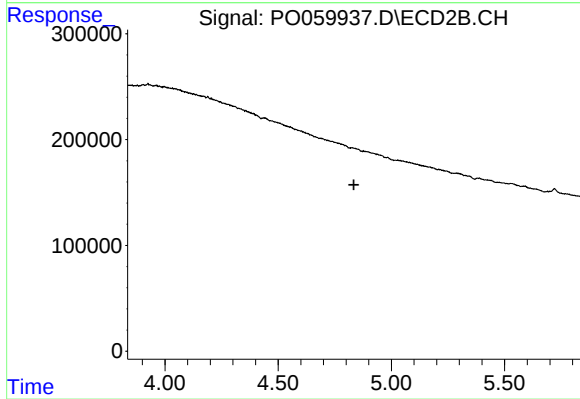

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.834 min
Response: 0
Conc: N.D.

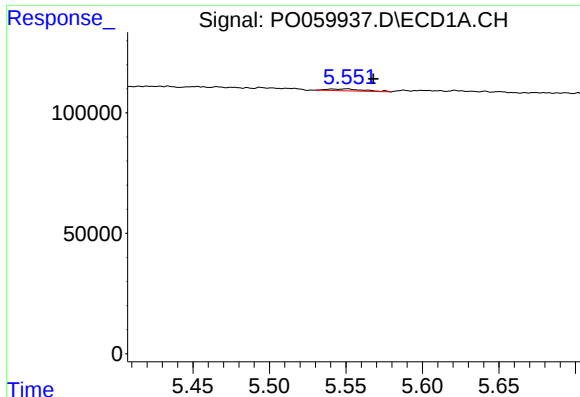

#15 AR-1232-5


R.T.: 5.551 min
Delta R.T.: -0.017 min
Response: 12472
Conc: 20.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

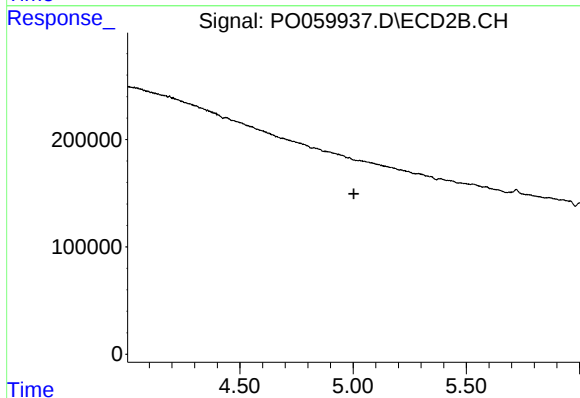


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

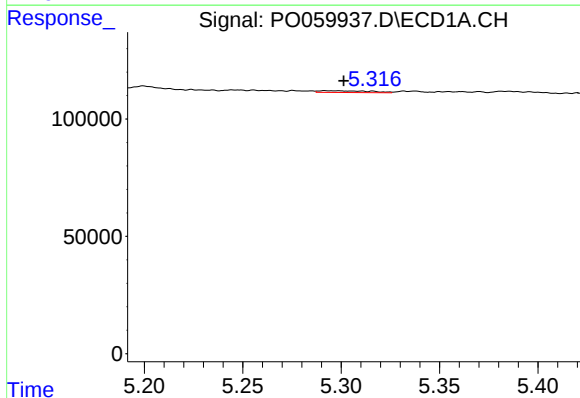


#16 AR-1242-1

R.T.: 5.292 min
Delta R.T.: -0.009 min
Response: 13497
Conc: 10.63 ng/ml

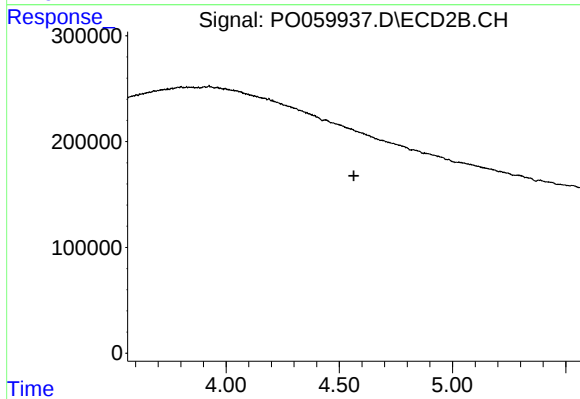

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

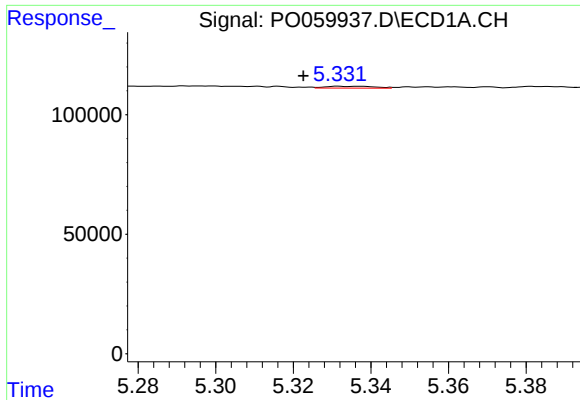

#17 AR-1242-2


R.T.: 5.337 min
Delta R.T.: 0.015 min
Response: 6894
Conc: 3.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

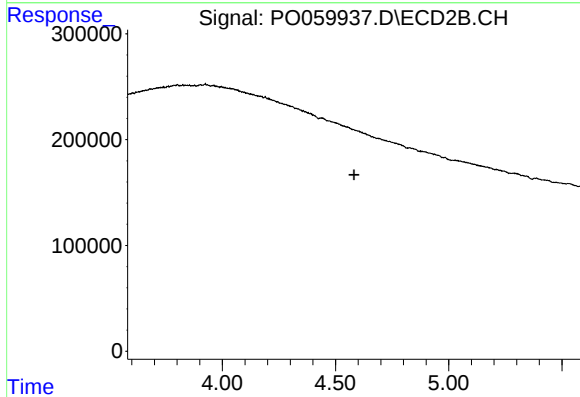


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

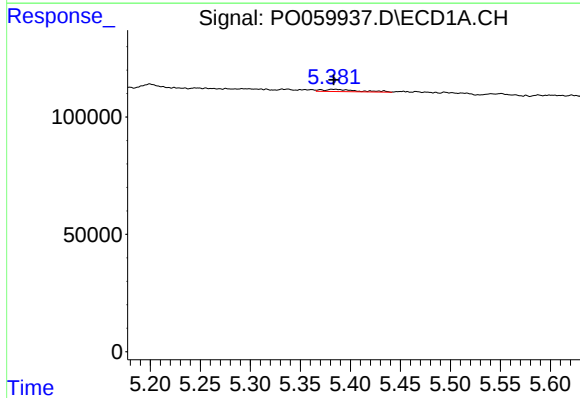


#18 AR-1242-3

R.T.: 5.382 min
Delta R.T.: -0.001 min
Response: 22702
Conc: 19.42 ng/ml

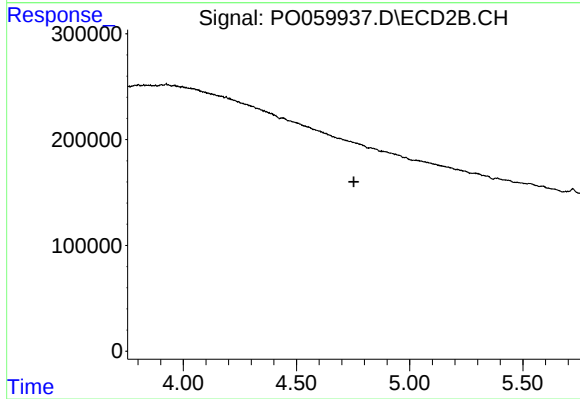

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.754 min
Response: 0
Conc: N.D.

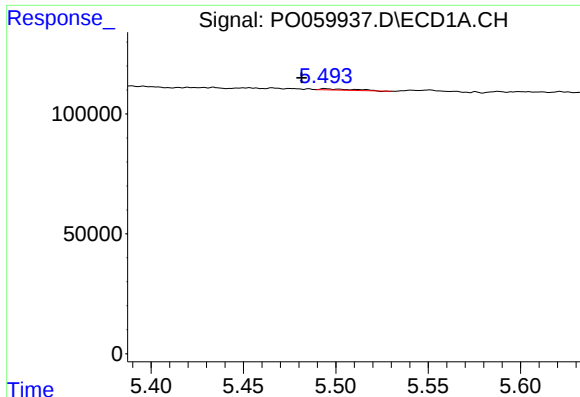

#19 AR-1242-4


R.T.: 5.494 min
Delta R.T.: 0.013 min
Response: 6530
Conc: 6.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

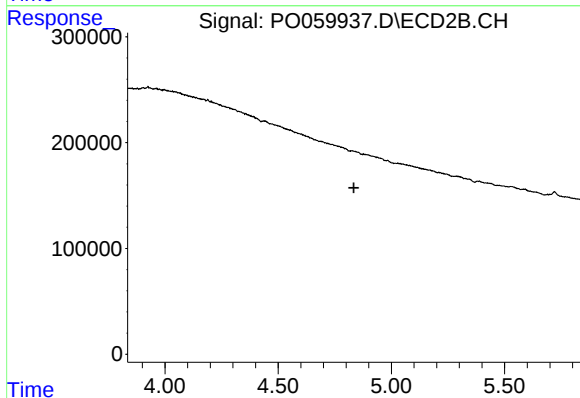


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.834 min
Response: 0
Conc: N.D.

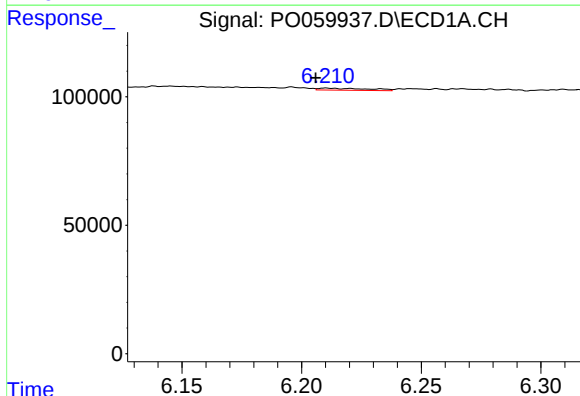


#20 AR-1242-5

R.T.: 6.210 min
Delta R.T.: 0.005 min
Response: 11344
Conc: 9.03 ng/ml

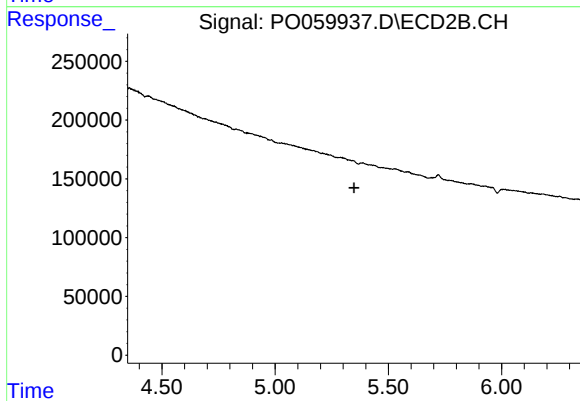

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.348 min
Response: 0
Conc: N.D.

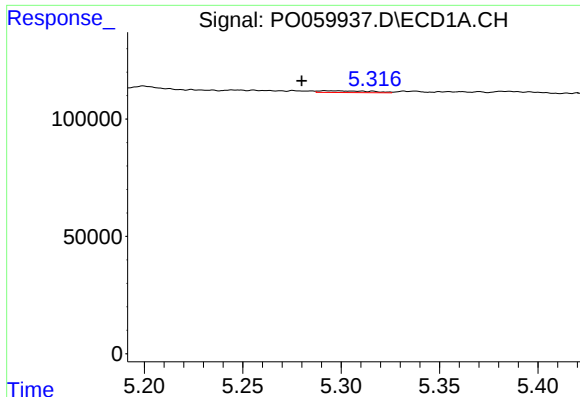

#21 AR-1248-1


R.T.: 5.292 min
Delta R.T.: 0.012 min
Response: 13497
Conc: 13.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

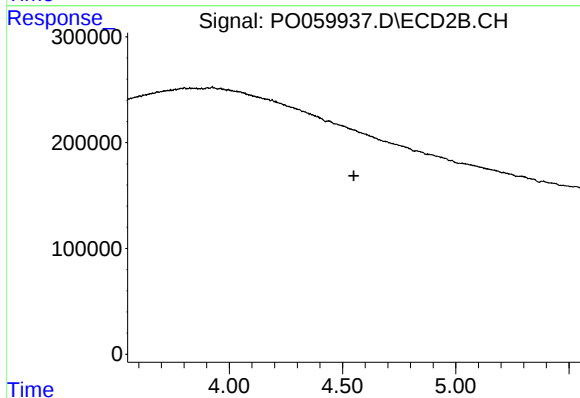


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

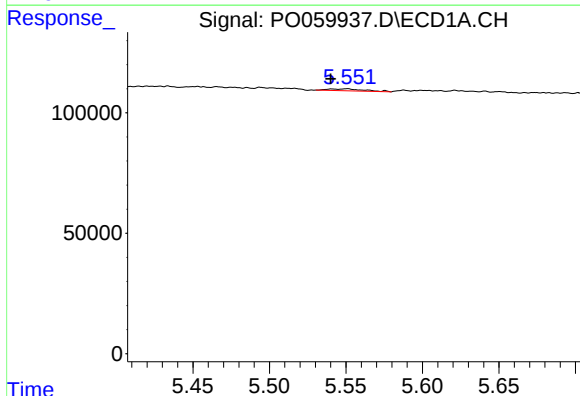


#22 AR-1248-2

R.T.: 5.551 min
Delta R.T.: 0.011 min
Response: 12472
Conc: 8.60 ng/ml

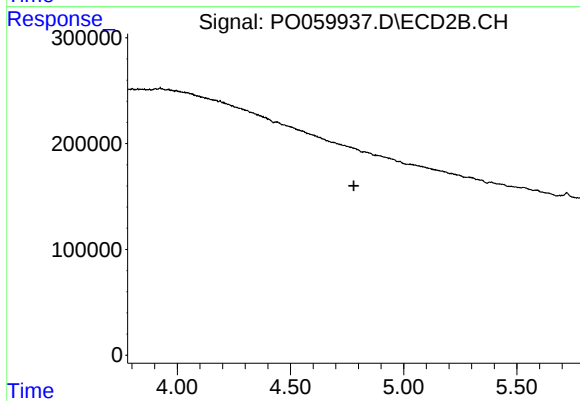

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.780 min
Response: 0
Conc: N.D.

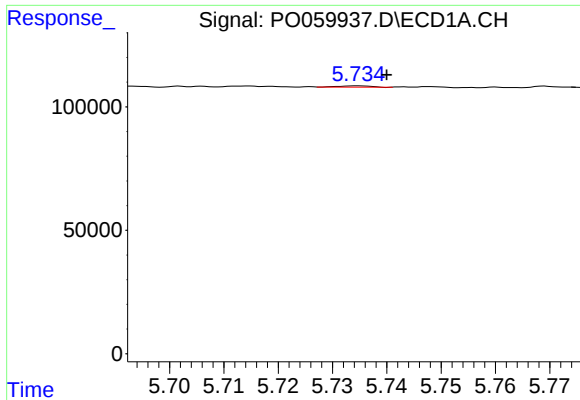

#23 AR-1248-3


R.T.: 5.735 min
Delta R.T.: -0.005 min
Response: 789
Conc: 0.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

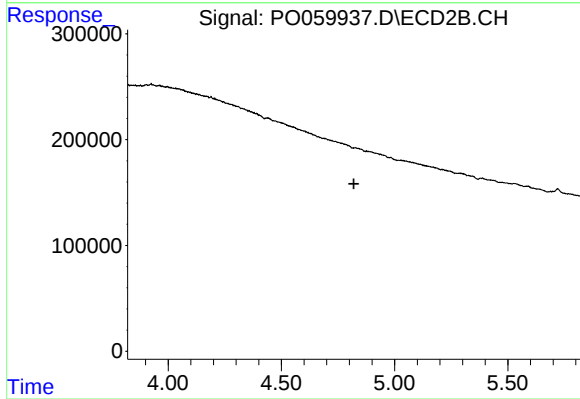


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.820 min
Response: 0
Conc: N.D.

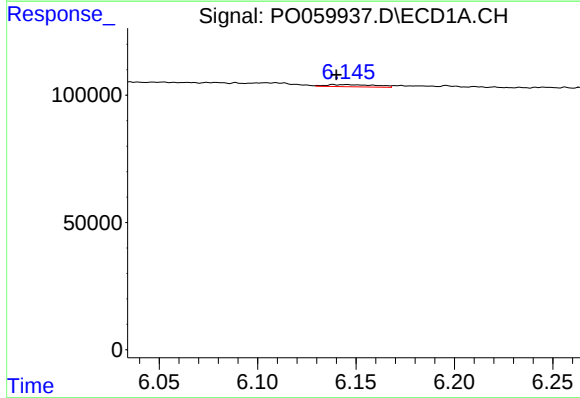


#24 AR-1248-4

R.T.: 6.145 min
Delta R.T.: 0.005 min
Response: 14383
Conc: 7.04 ng/ml

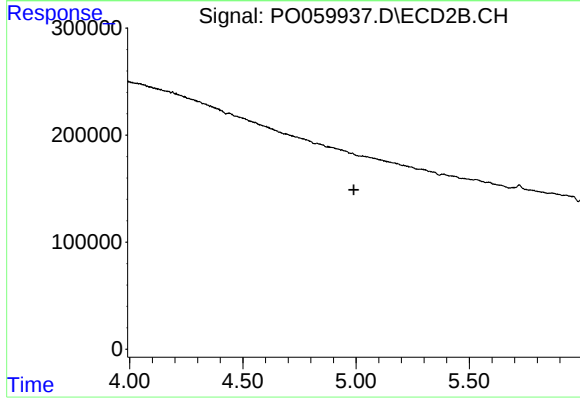

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.990 min
Response: 0
Conc: N.D.

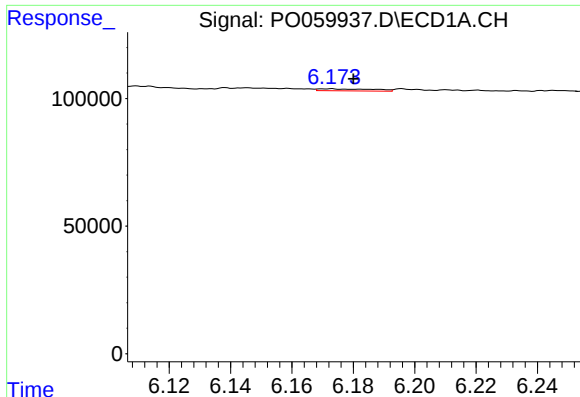

#25 AR-1248-5


R.T.: 6.172 min
Delta R.T.: -0.008 min
Response: 9604
Conc: 4.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

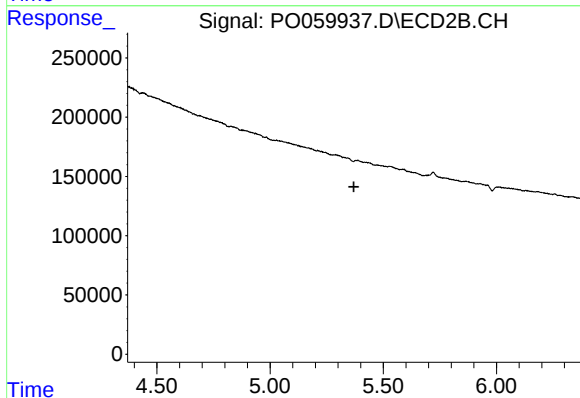


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

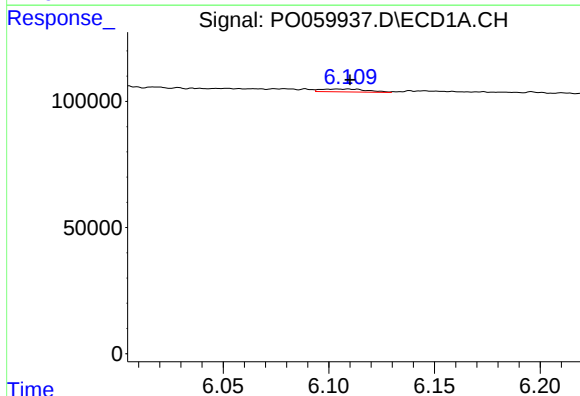


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 16825
Conc: 8.06 ng/ml

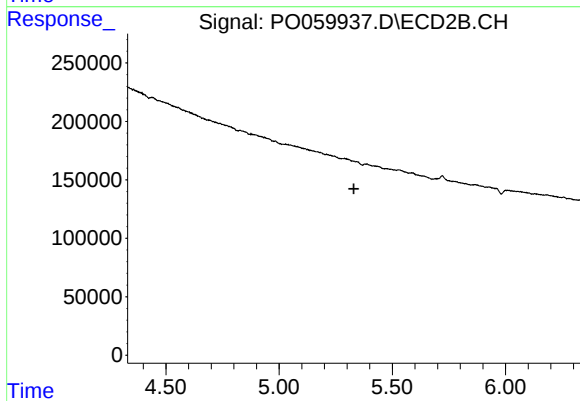

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

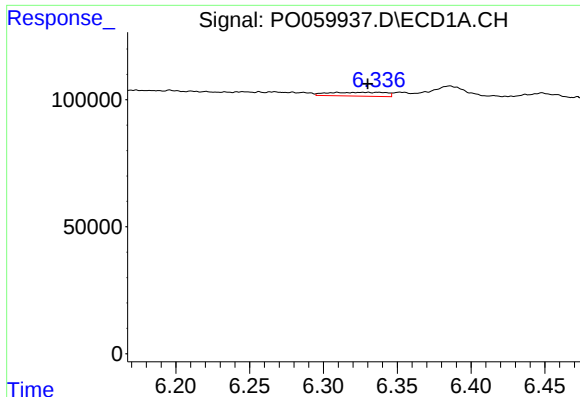

#27 AR-1254-2


R.T.: 6.309 min
Delta R.T.: -0.021 min
Response: 40210
Conc: 12.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

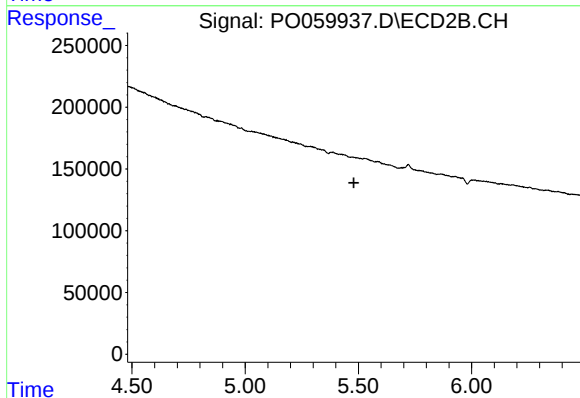


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

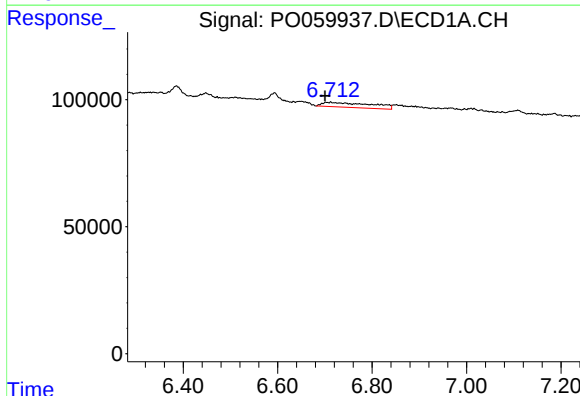


#28 AR-1254-3

R.T.: 6.712 min
Delta R.T.: 0.012 min
Response: 138046
Conc: 38.90 ng/ml

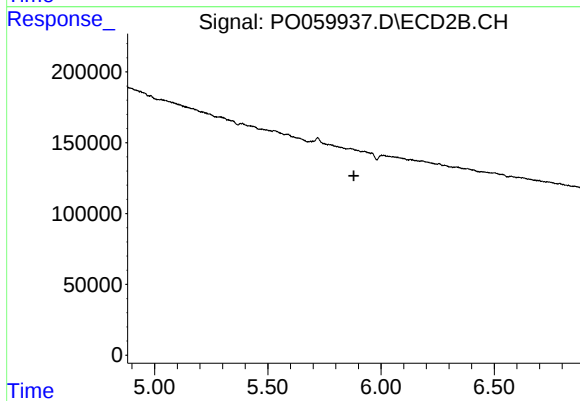

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.880 min
Response: 0
Conc: N.D.

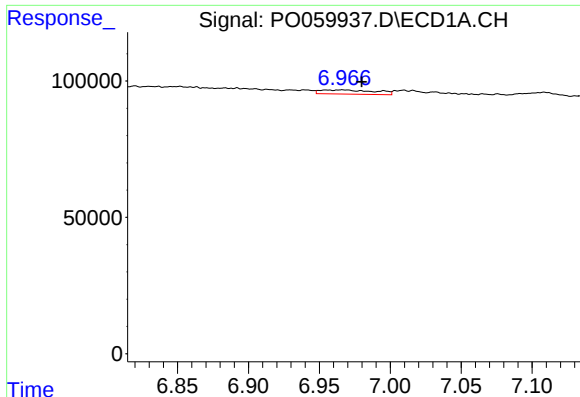

#29 AR-1254-4


R.T.: 6.967 min
Delta R.T.: -0.013 min
Response: 40380
Conc: 13.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

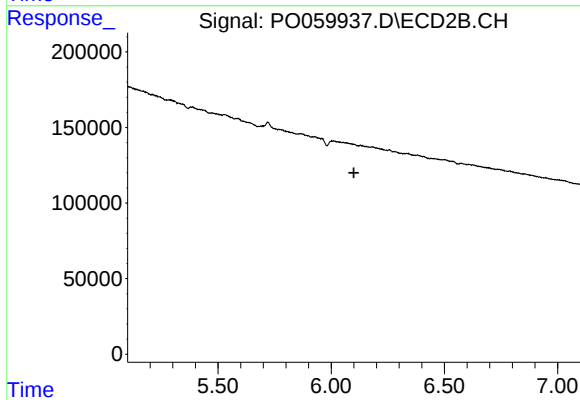


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

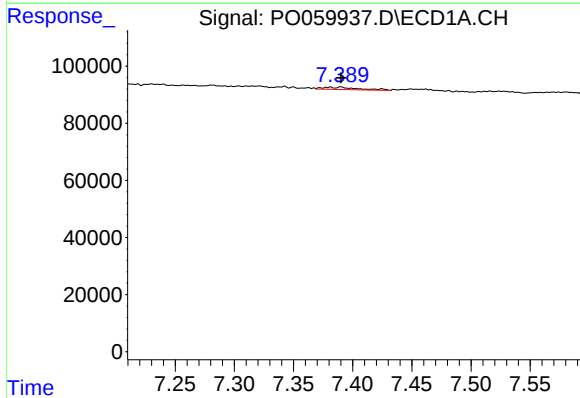


#30 AR-1254-5

R.T.: 7.390 min
Delta R.T.: 0.000 min
Response: 18165
Conc: 5.87 ng/ml

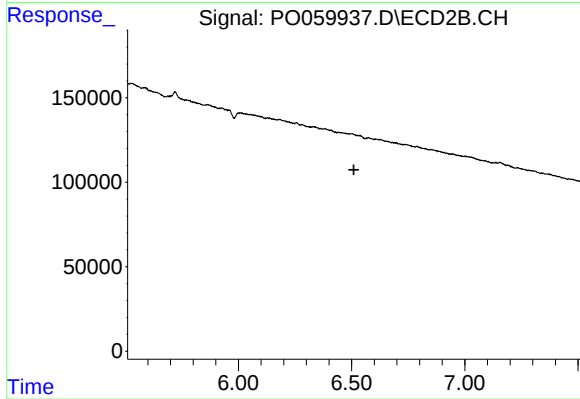

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.510 min
Response: 0
Conc: N.D.

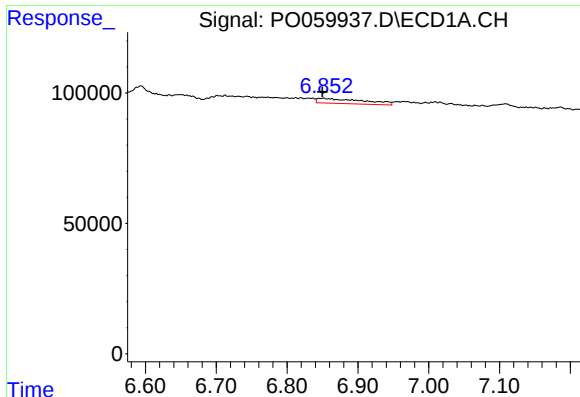

#31 AR-1260-1


R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 88125
Conc: 32.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

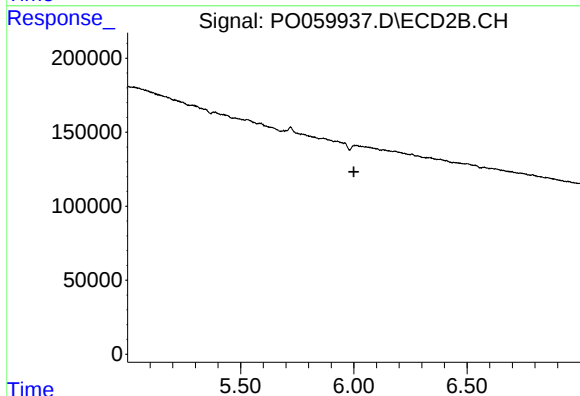


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.000 min
Response: 0
Conc: N.D.

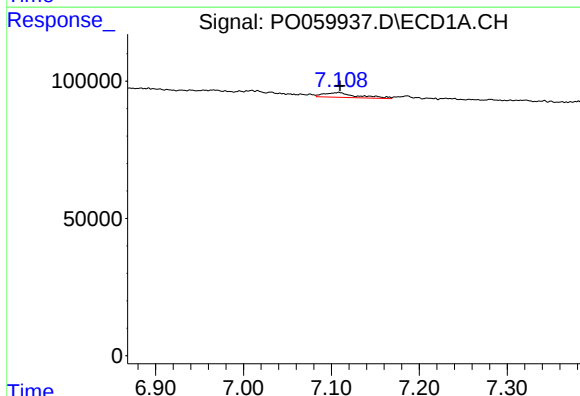


#32 AR-1260-2

R.T.: 7.108 min
Delta R.T.: -0.002 min
Response: 46445
Conc: 12.52 ng/ml

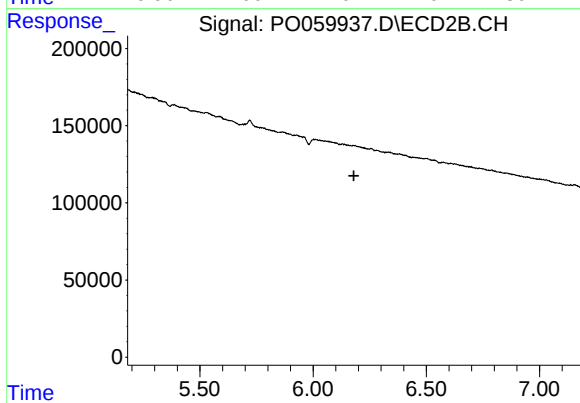

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.180 min
Response: 0
Conc: N.D.

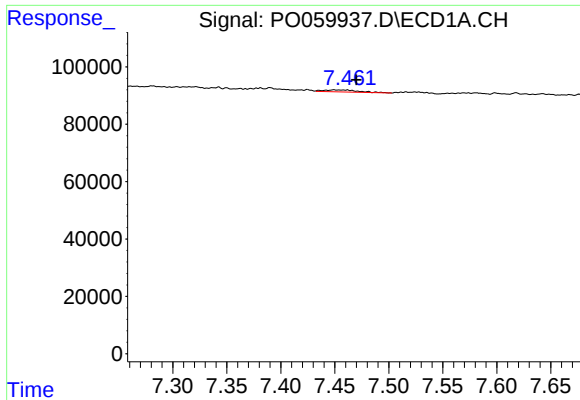

#33 AR-1260-3


R.T.: 7.457 min
Delta R.T.: -0.013 min
Response: 14883
Conc: 4.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

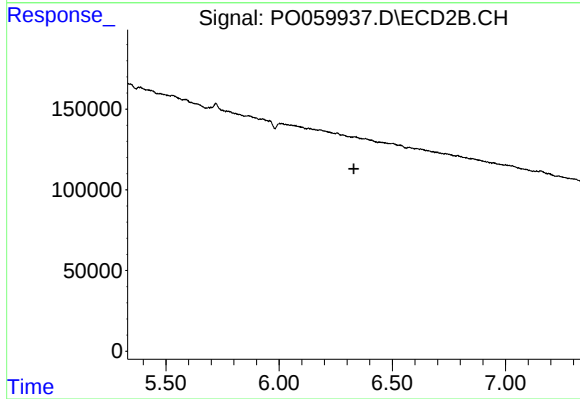


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.330 min
Response: 0
Conc: N.D.

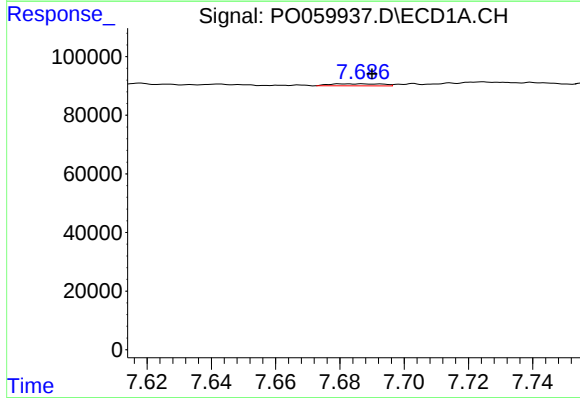


#34 AR-1260-4

R.T.: 7.684 min
Delta R.T.: -0.006 min
Response: 7575
Conc: 2.47 ng/ml

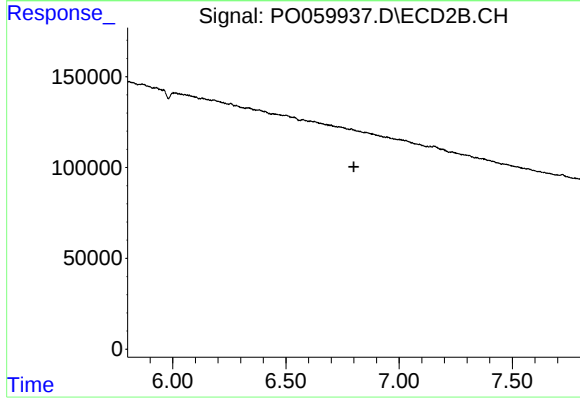

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

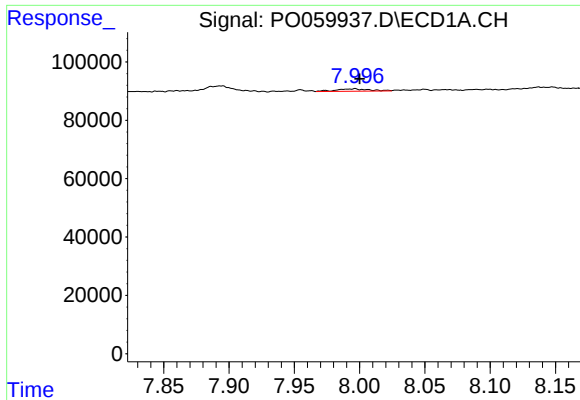

#35 AR-1260-5


R.T.: 7.995 min
Delta R.T.: -0.005 min
Response: 14756
Conc: 2.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

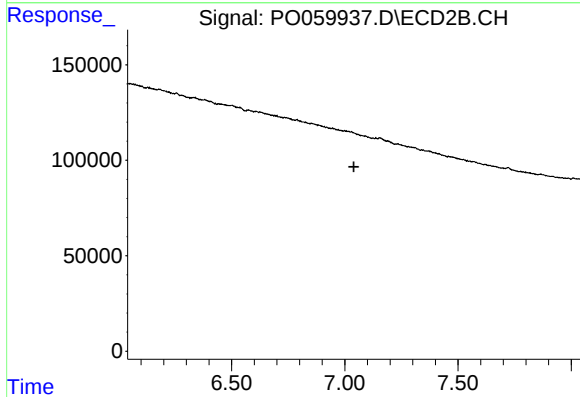


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.040 min
Response: 0
Conc: N.D.

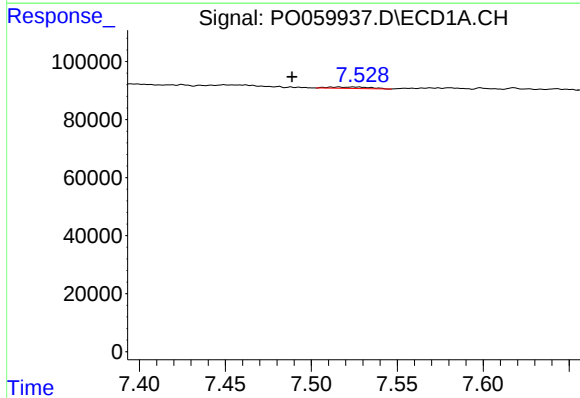


#36 AR-1262-1

R.T.: 7.516 min
Delta R.T.: 0.027 min
Response: 8058
Conc: 1.66 ng/ml

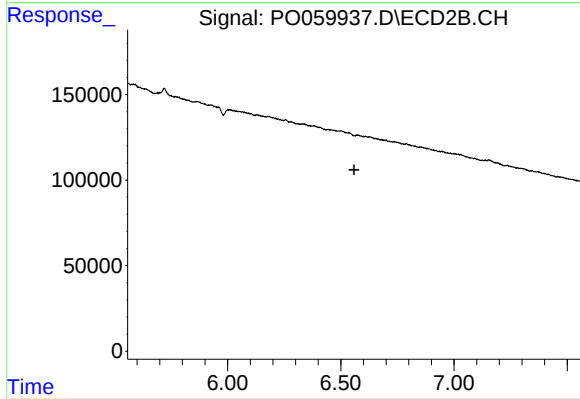

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.558 min
Response: 0
Conc: N.D.

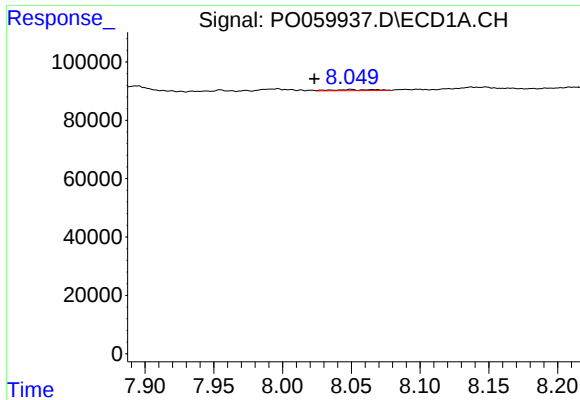

#37 AR-1262-2


R.T.: 8.049 min
Delta R.T.: 0.026 min
Response: 8167
Conc: 1.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

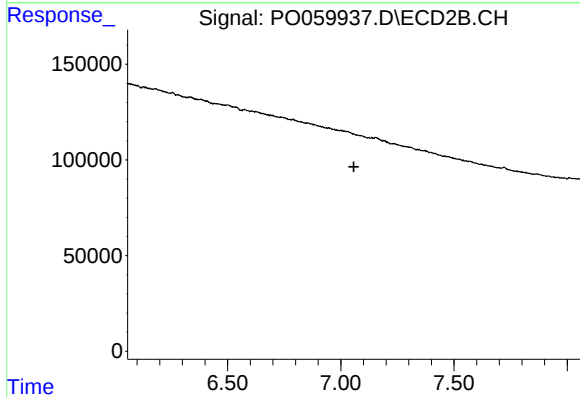


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

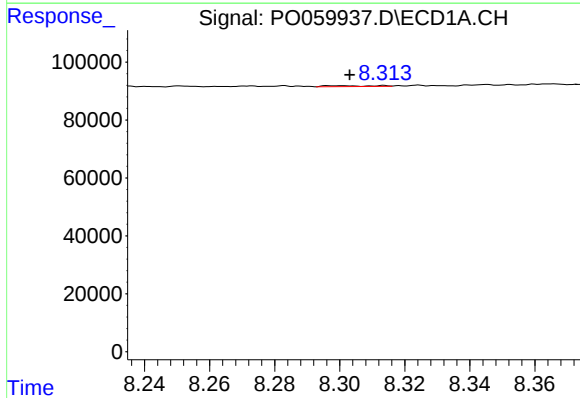


#38 AR-1262-3

R.T.: 8.300 min
Delta R.T.: -0.003 min
Response: 3099
Conc: 0.61 ng/ml

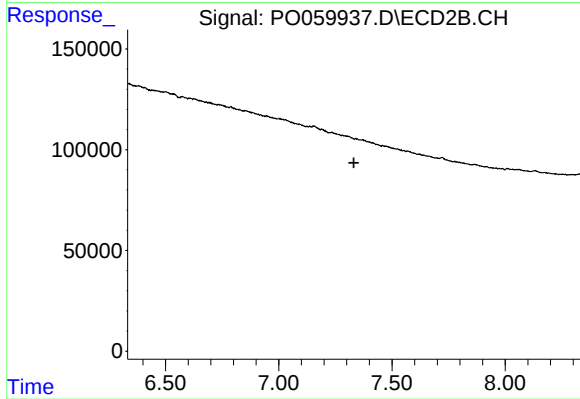

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

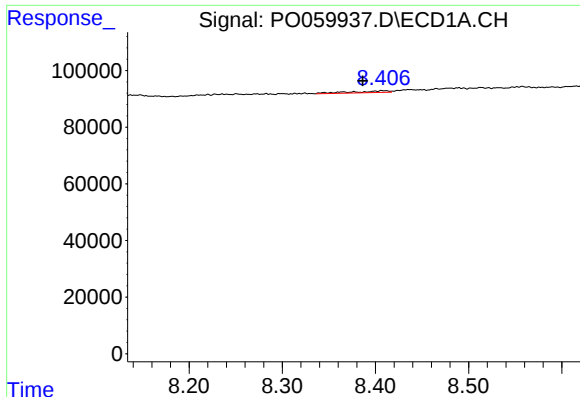

#39 AR-1262-4


R.T.: 8.409 min
Delta R.T.: 0.023 min
Response: 17480
Conc: 4.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

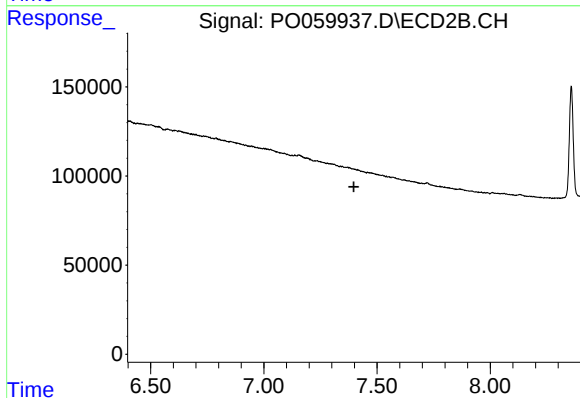


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.398 min
Response: 0
Conc: N.D.

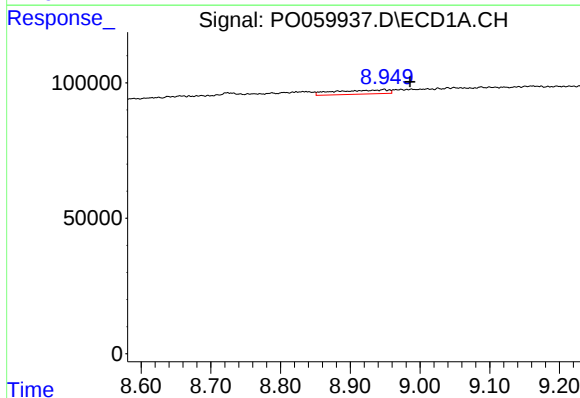


#40 AR-1262-5

R.T.: 8.948 min
Delta R.T.: -0.038 min
Response: 79905
Conc: 31.13 ng/ml

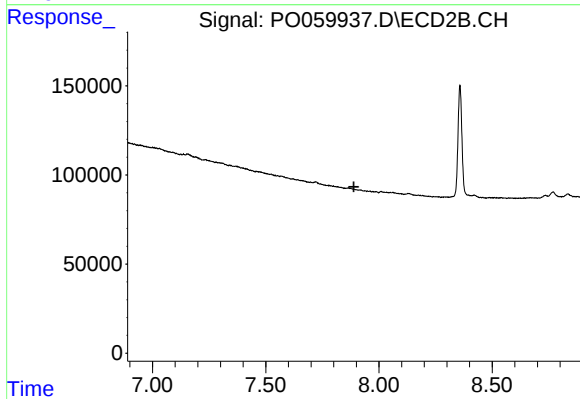

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 7.889 min
Response: 0
Conc: N.D.

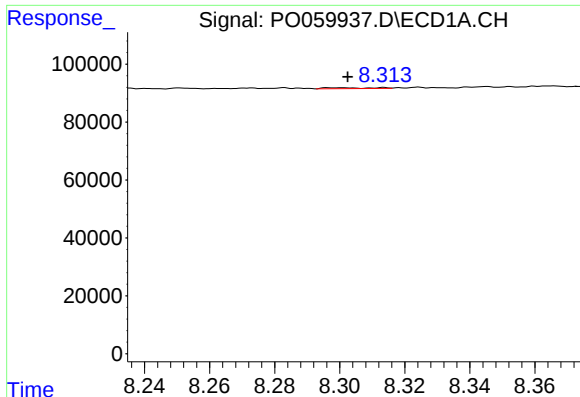

#41 AR-1268-1


R.T.: 8.300 min
Delta R.T.: -0.003 min
Response: 3099
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

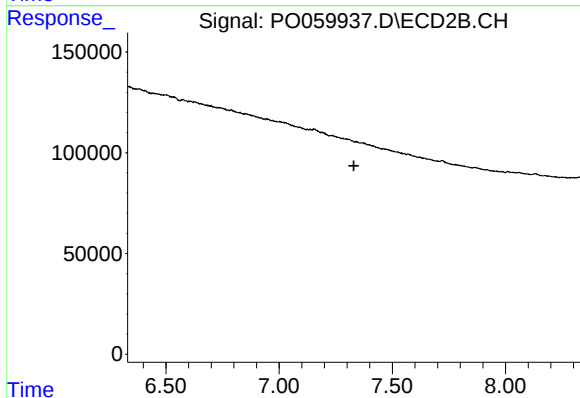


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

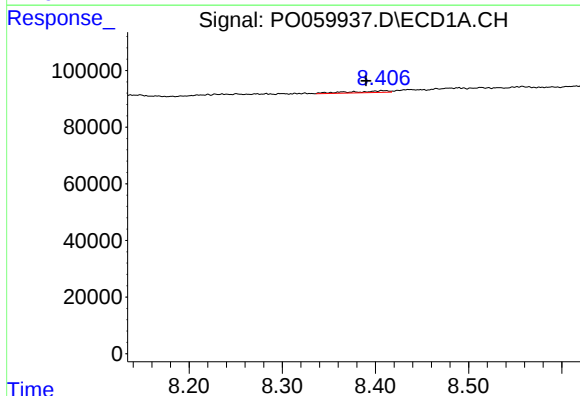


#42 AR-1268-2

R.T.: 8.409 min
Delta R.T.: 0.019 min
Response: 17480
Conc: 2.22 ng/ml

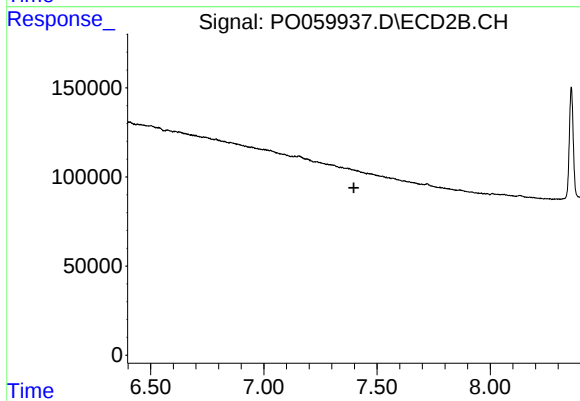

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.397 min
Response: 0
Conc: N.D.

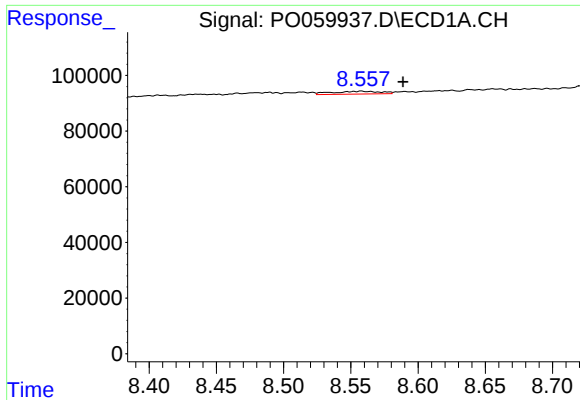

#43 AR-1268-3


R.T.: 8.557 min
Delta R.T.: -0.031 min
Response: 25081
Conc: 3.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

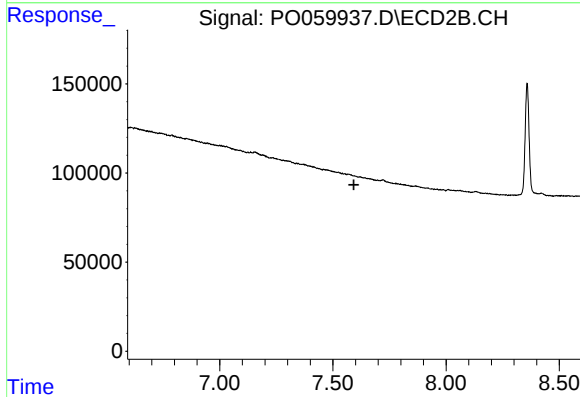


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

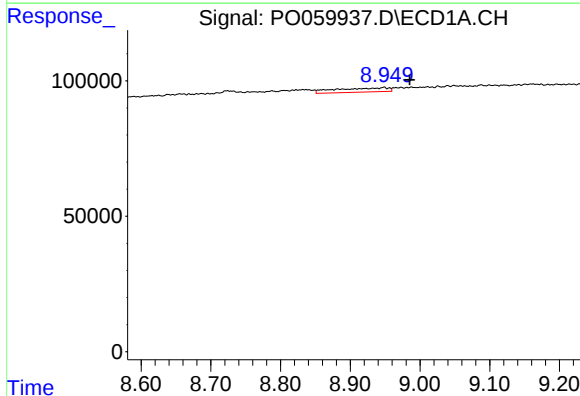


#44 AR-1268-4

R.T.: 8.948 min
Delta R.T.: -0.038 min
Response: 79905
Conc: 28.74 ng/ml

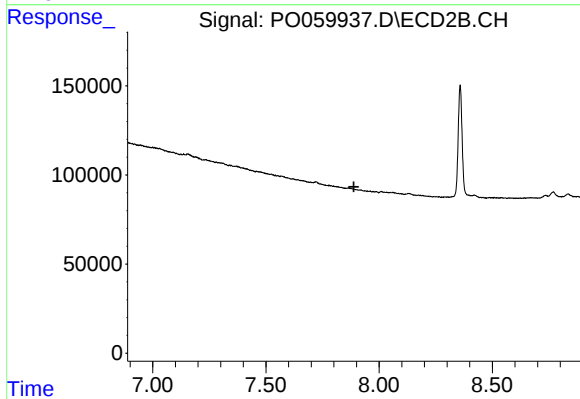

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.888 min
Response: 0
Conc: N.D.

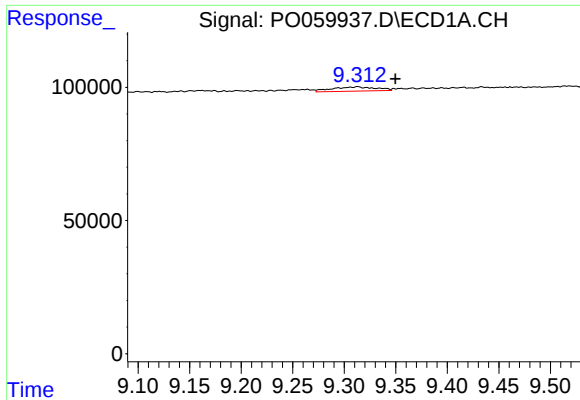

#45 AR-1268-5

R.T.: 9.312 min
Delta R.T.: -0.037 min
Response: 47123
Conc: 2.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

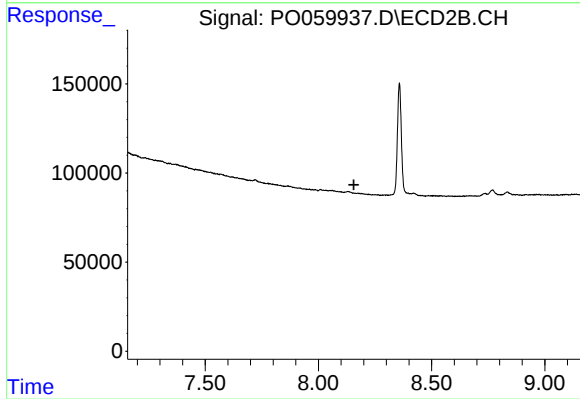

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.157 min
Response: 0
Conc: N.D.