

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
 Data File : P0059885.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2019 12:12
 Operator : SM/AJ
 Sample : K4506-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-COMP

Manual Integrations
 APPROVED

Ankita
 8/28/2019 4:14:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 13:07:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.134	3.496	897674	713138	25.639	19.812
2)	SA Decachlor...	9.604	8.357	694098	513395	13.047	12.733
Target Compounds							
31)	L7 AR-1260-1	6.858	5.993	1473502	1250527	546.588	548.740
32)	L7 AR-1260-2	7.113	6.182	2326753	1679099	627.076	573.096
33)	L7 AR-1260-3	7.468	6.329	1476066	1028799	450.524	388.353
34)	L7 AR-1260-4	7.694	6.792	1352206	884679	440.268	391.005
35)	L7 AR-1260-5	8.001	7.036	3273382	2716663	462.283m	493.641

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082719\
Data File : PO059885.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2019 12:12
Operator : SM/AJ
Sample : K4506-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
RO-COMP


Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 13:07:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

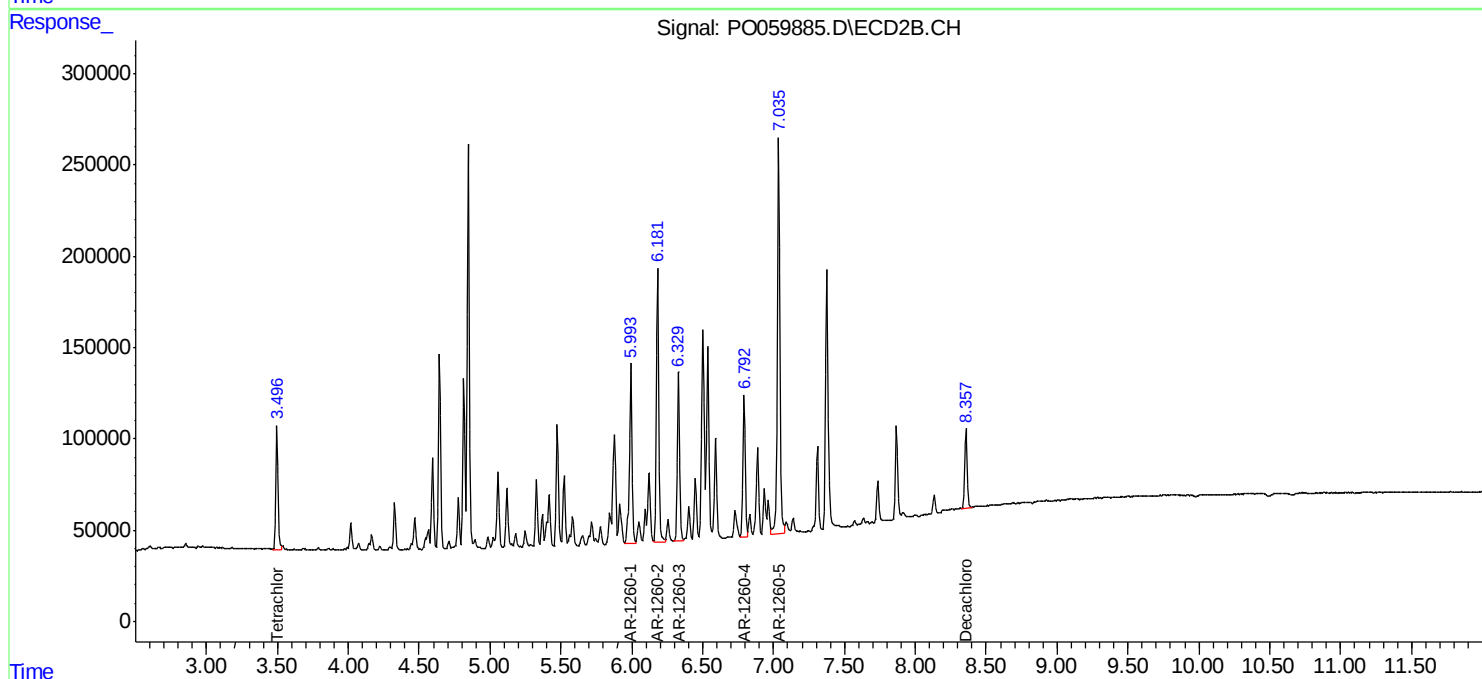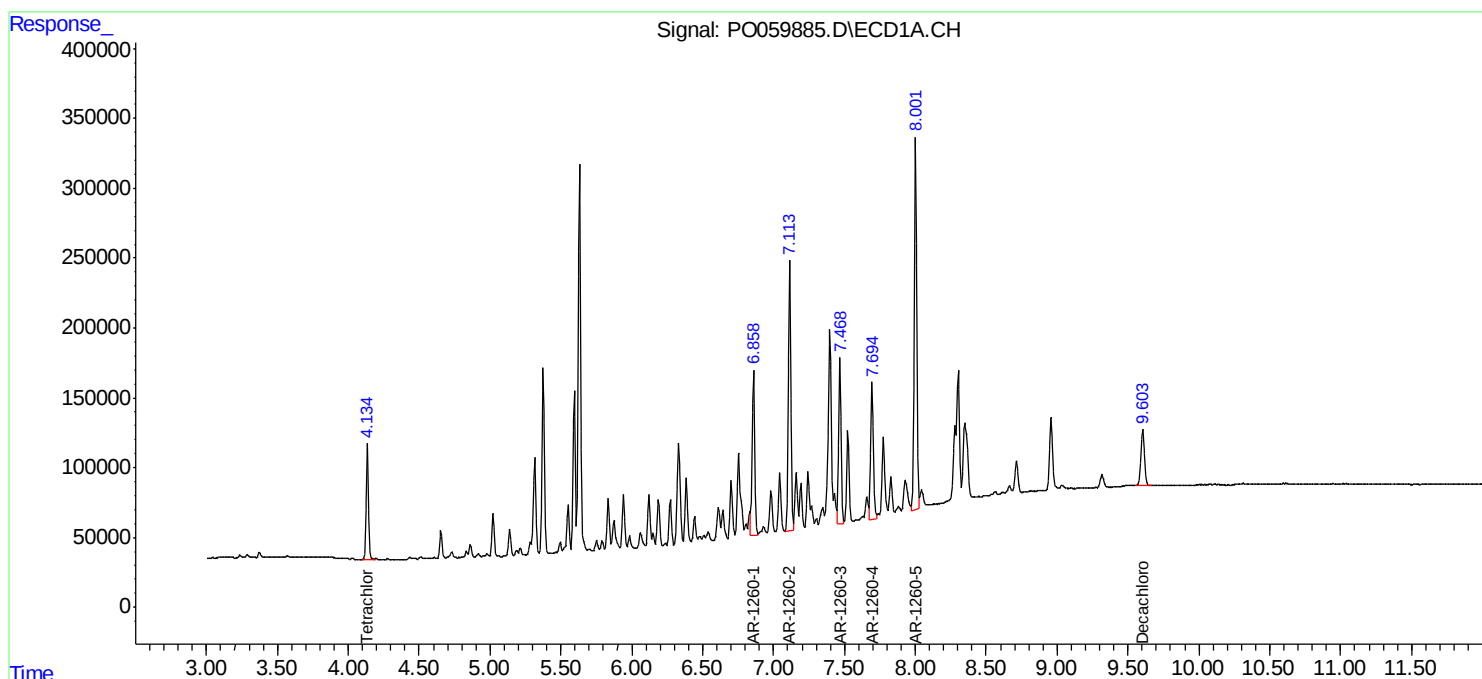

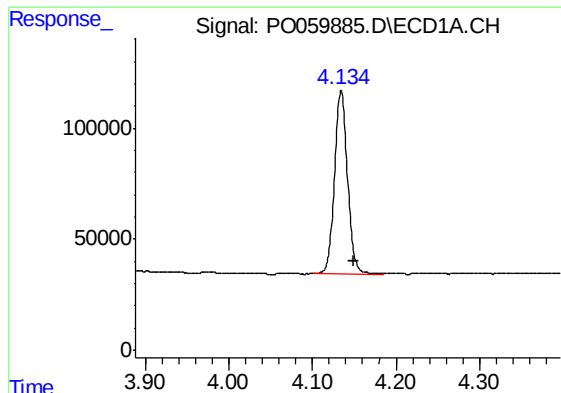


#1 Tetrachloro-m-xylene

R.T.: 4.134 min
Delta R.T.: -0.015 min
Response: 897674
Conc: 25.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:36 PM

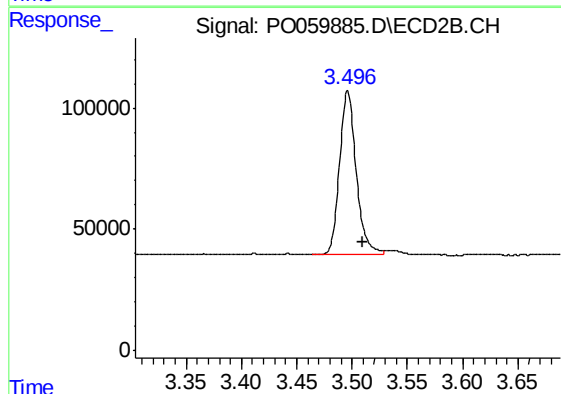


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.014 min
Response: 713138
Conc: 19.81 ng/ml

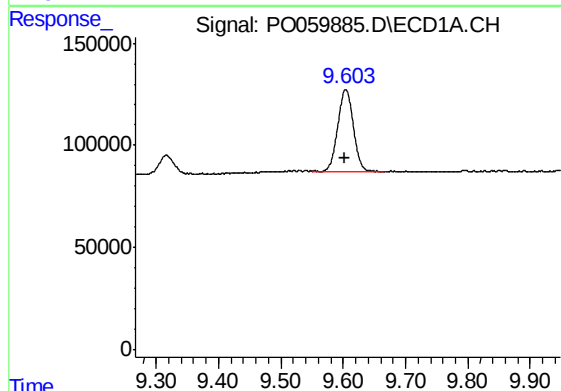


#2 Decachlorobiphenyl

R.T.: 9.604 min
Delta R.T.: 0.001 min
Response: 694098
Conc: 13.05 ng/ml

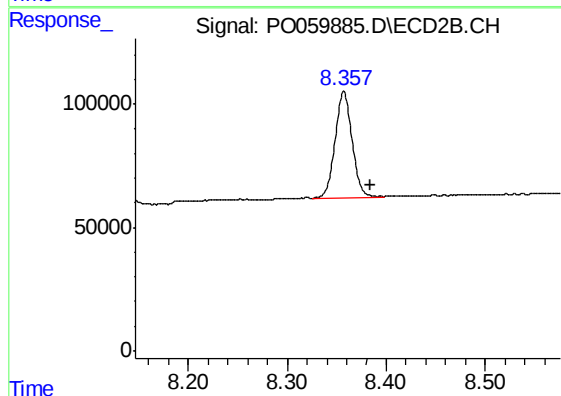

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.026 min
Response: 513395
Conc: 12.73 ng/ml

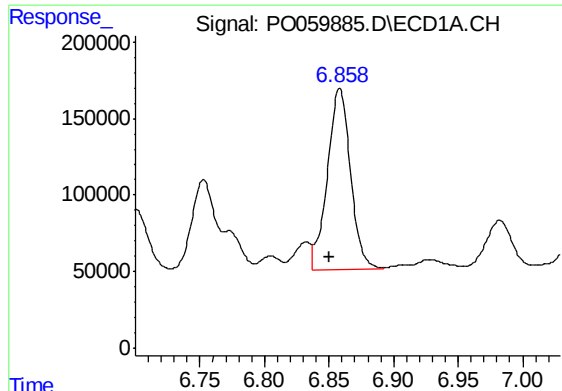


#31 AR-1260-1

R.T.: 6.858 min
Delta R.T.: 0.008 min
Response: 1473502
Conc: 546.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:36 PM

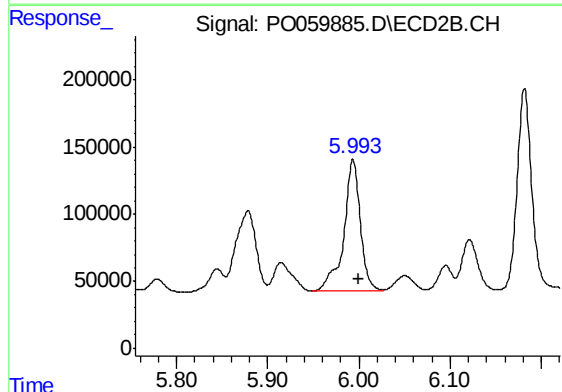


#31 AR-1260-1

R.T.: 5.993 min
Delta R.T.: -0.007 min
Response: 1250527
Conc: 548.74 ng/ml

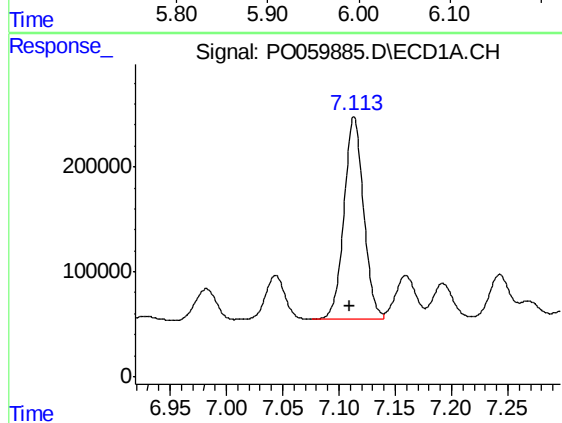


#32 AR-1260-2

R.T.: 7.113 min
Delta R.T.: 0.003 min
Response: 2326753
Conc: 627.08 ng/ml

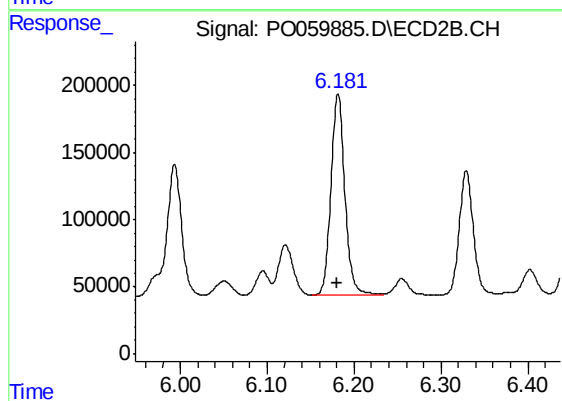

#32 AR-1260-2

R.T.: 6.182 min
Delta R.T.: 0.002 min
Response: 1679099
Conc: 573.10 ng/ml

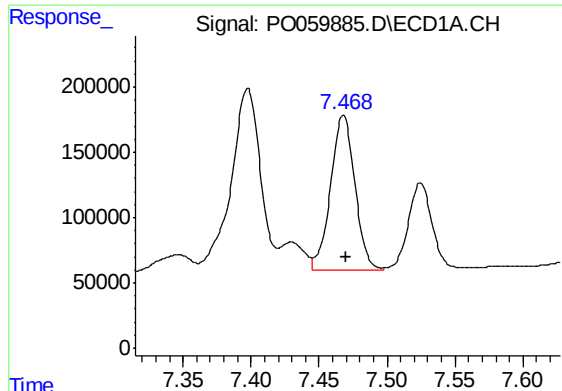


#33 AR-1260-3

R.T.: 7.468 min
Delta R.T.: -0.002 min
Response: 1476066
Conc: 450.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:36 PM

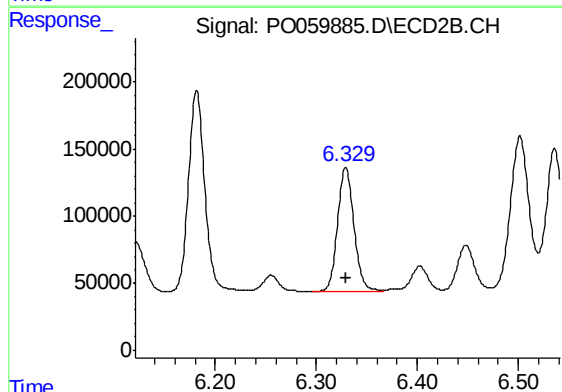


#33 AR-1260-3

R.T.: 6.329 min
Delta R.T.: 0.000 min
Response: 1028799
Conc: 388.35 ng/ml

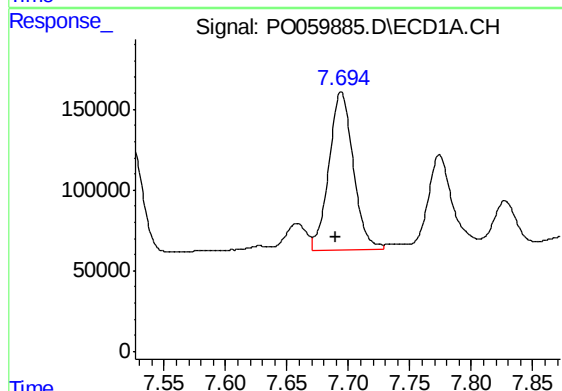


#34 AR-1260-4

R.T.: 7.694 min
Delta R.T.: 0.004 min
Response: 1352206
Conc: 440.27 ng/ml

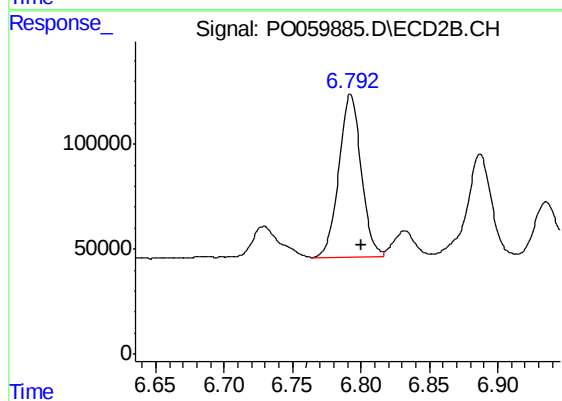

#34 AR-1260-4

R.T.: 6.792 min
Delta R.T.: -0.008 min
Response: 884679
Conc: 391.00 ng/ml

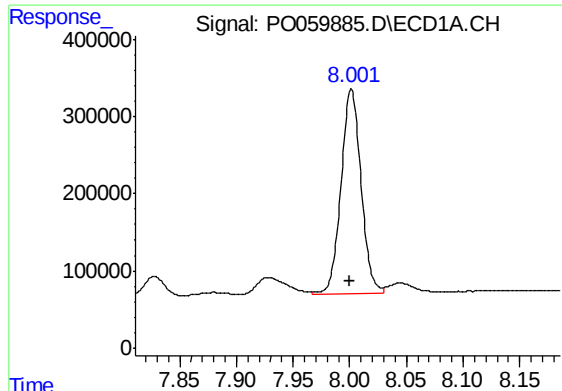


#35 AR-1260-5

R.T.: 8.001 min
Delta R.T.: 0.000 min
Response: 3273382
Conc: 462.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RO-COMP

Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:36 PM

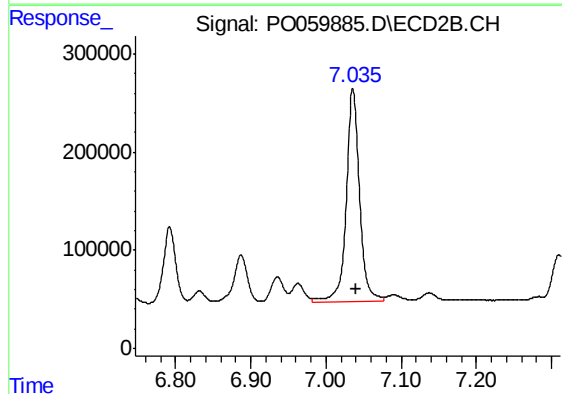

#35 AR-1260-5

R.T.: 7.036 min
Delta R.T.: -0.004 min
Response: 2716663
Conc: 493.64 ng/ml