

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
 Data File : P0059889.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2019 15:50
 Operator : SM/AJ
 Sample : K4523-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-005-IDWGW-20190823RE

Manual Integrations
 APPROVED

Ankita
 8/28/2019 4:14:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 16:05:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.131	3.500	406500	359273	11.610	9.981m
2) SA Decachlor...	9.602	8.361	119229	76390	2.241	1.895m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082719\
Data File : PO059889.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2019 15:50
Operator : SM/AJ
Sample : K4523-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-005-IDWGW-20190823RE


Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 16:05:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

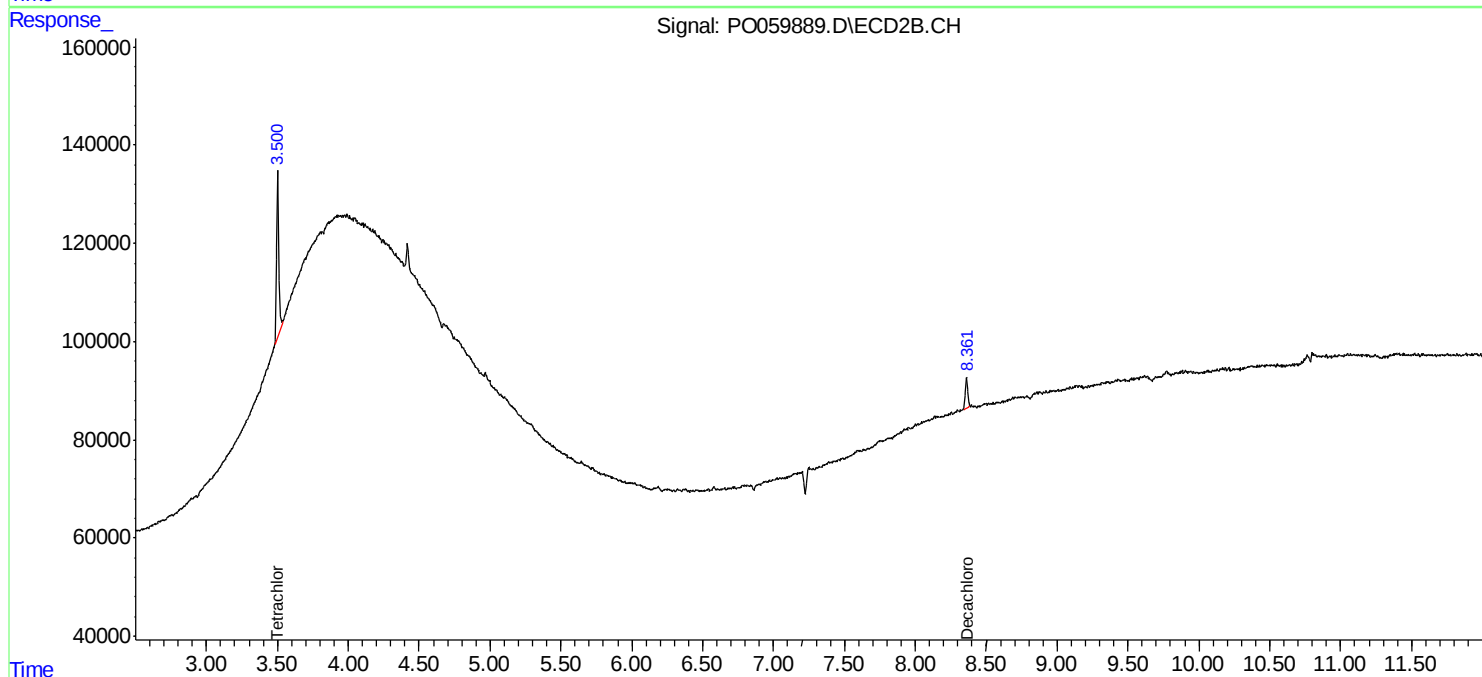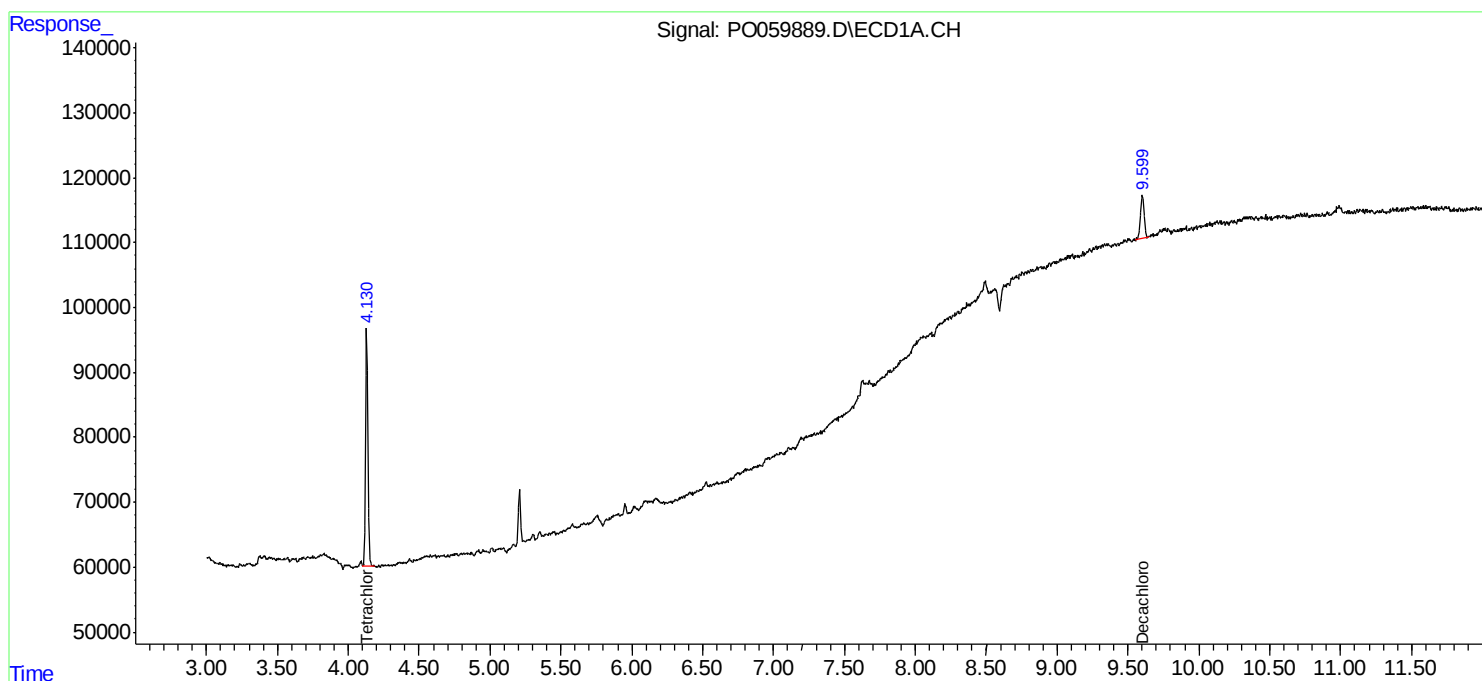

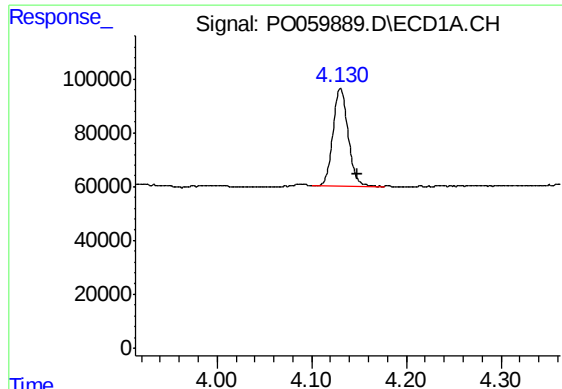


#1 Tetrachloro-m-xylene

R.T.: 4.131 min
Delta R.T.: -0.018 min
Response: 406500
Conc: 11.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-005-IDWGW-20190823RE


Manual Integrations
APPROVED

Ankita
8/28/2019 4:14:42 PM

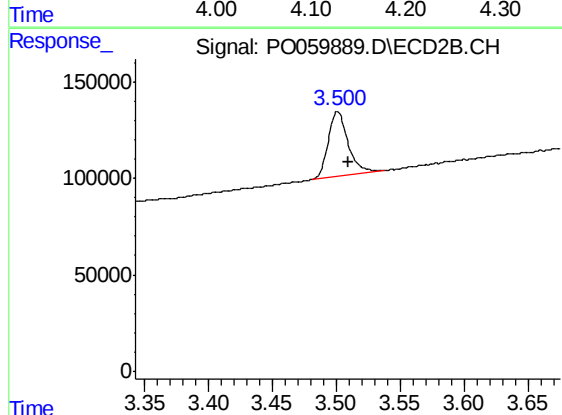


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 359273
Conc: 9.98 ng/ml m

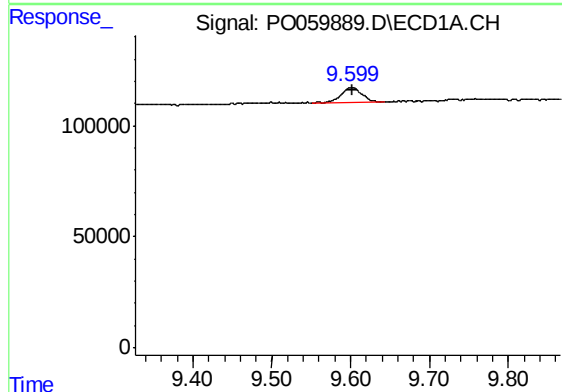

#2 Decachlorobiphenyl

R.T.: 9.602 min
Delta R.T.: -0.001 min
Response: 119229
Conc: 2.24 ng/ml

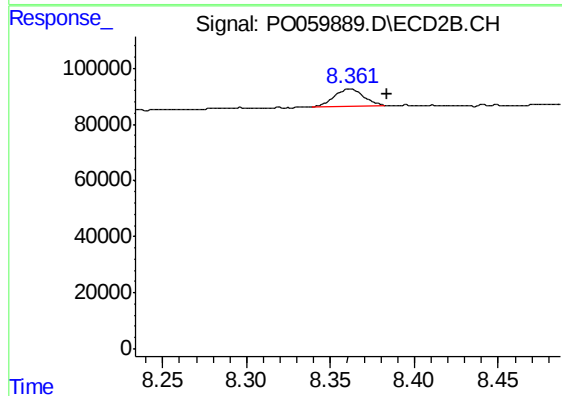

#2 Decachlorobiphenyl

R.T.: 8.361 min
Delta R.T.: -0.022 min
Response: 76390
Conc: 1.89 ng/ml m