

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
 Data File : P0059904.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2019 20:08
 Operator : SM/AJ
 Sample : K4086-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-07-082619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:29:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.125	3.501	1203612	1076733	34.377	29.913
2)	SA Decachlor...	9.595	8.359	1116783	764370	20.992	18.957

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
Data File : P0059904.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2019 20:08
Operator : SM/AJ
Sample : K4086-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NB-07-082619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:29:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

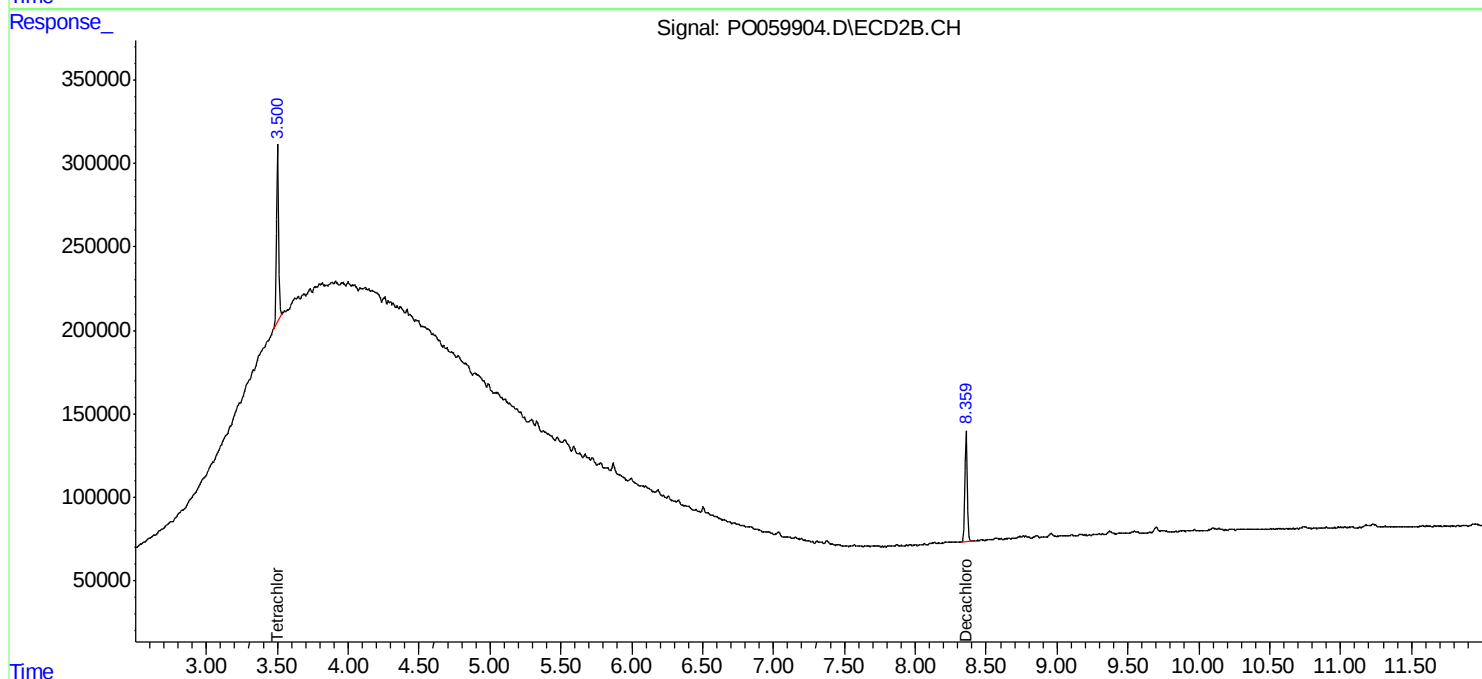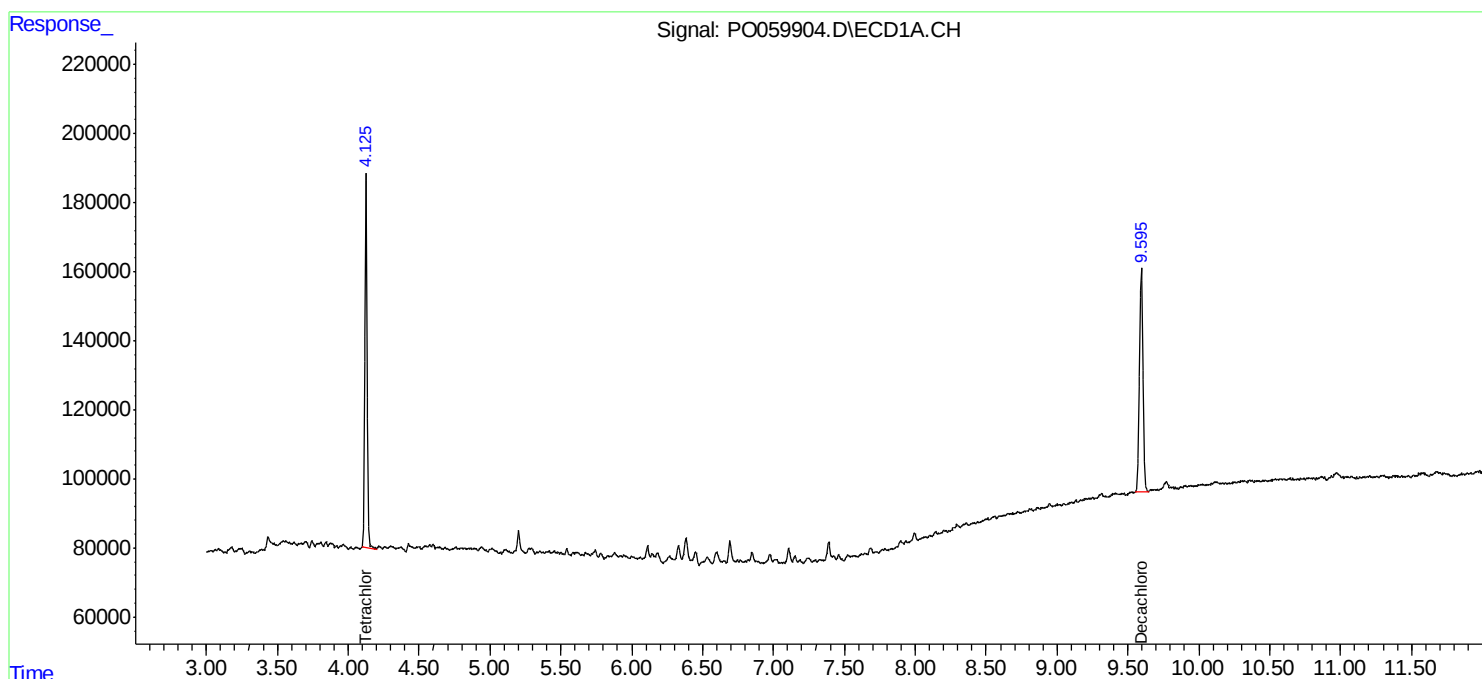


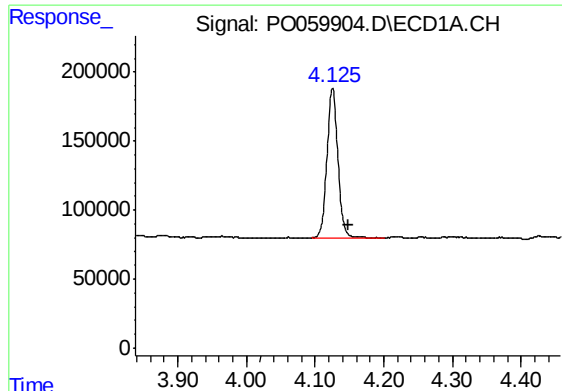

#1 Tetrachloro-m-xylene


R.T.: 4.125 min
Delta R.T.: -0.024 min
Response: 1203612
Conc: 34.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-07-082619

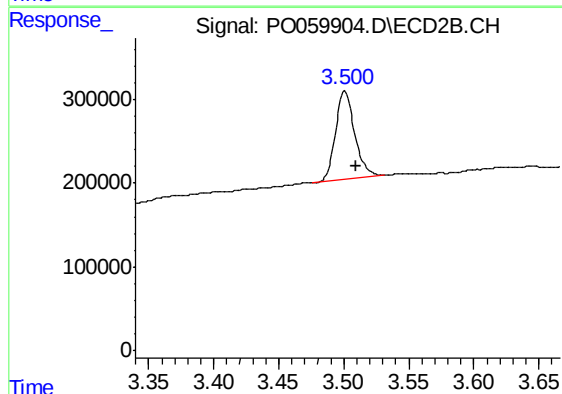


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.009 min
Response: 1076733
Conc: 29.91 ng/ml

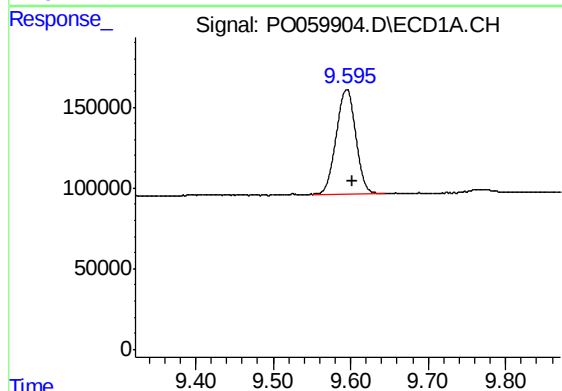

#2 Decachlorobiphenyl

R.T.: 9.595 min
Delta R.T.: -0.008 min
Response: 1116783
Conc: 20.99 ng/ml

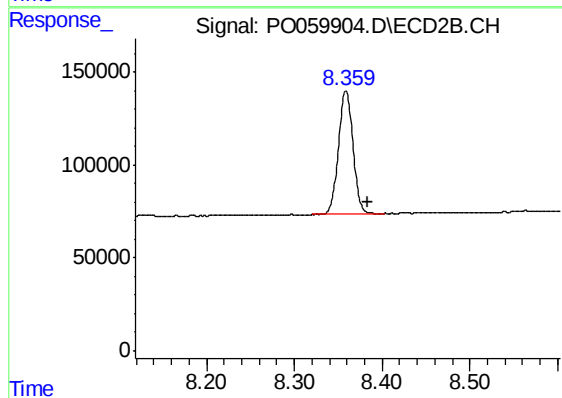

#2 Decachlorobiphenyl

R.T.: 8.359 min
Delta R.T.: -0.024 min
Response: 764370
Conc: 18.96 ng/ml