

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
Data File : P0059937.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 5:48
Operator : SM/AJ
Sample : K4543-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:44:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.125	3.500	1070818	925653	30.584	25.716
2) SA Decachlor...	9.595	8.358	1023026	750690	19.230	18.618

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
Data File : P0059937.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 5:48
Operator : SM/AJ
Sample : K4543-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:44:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

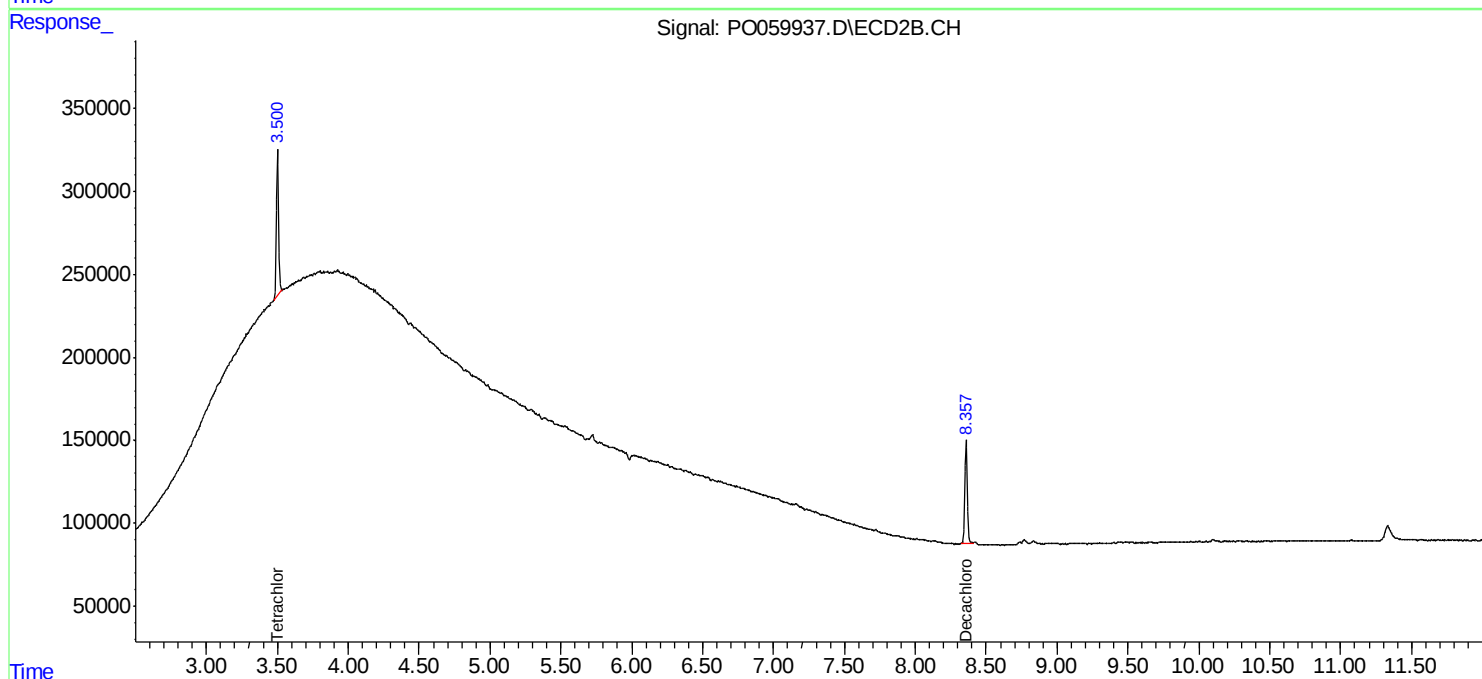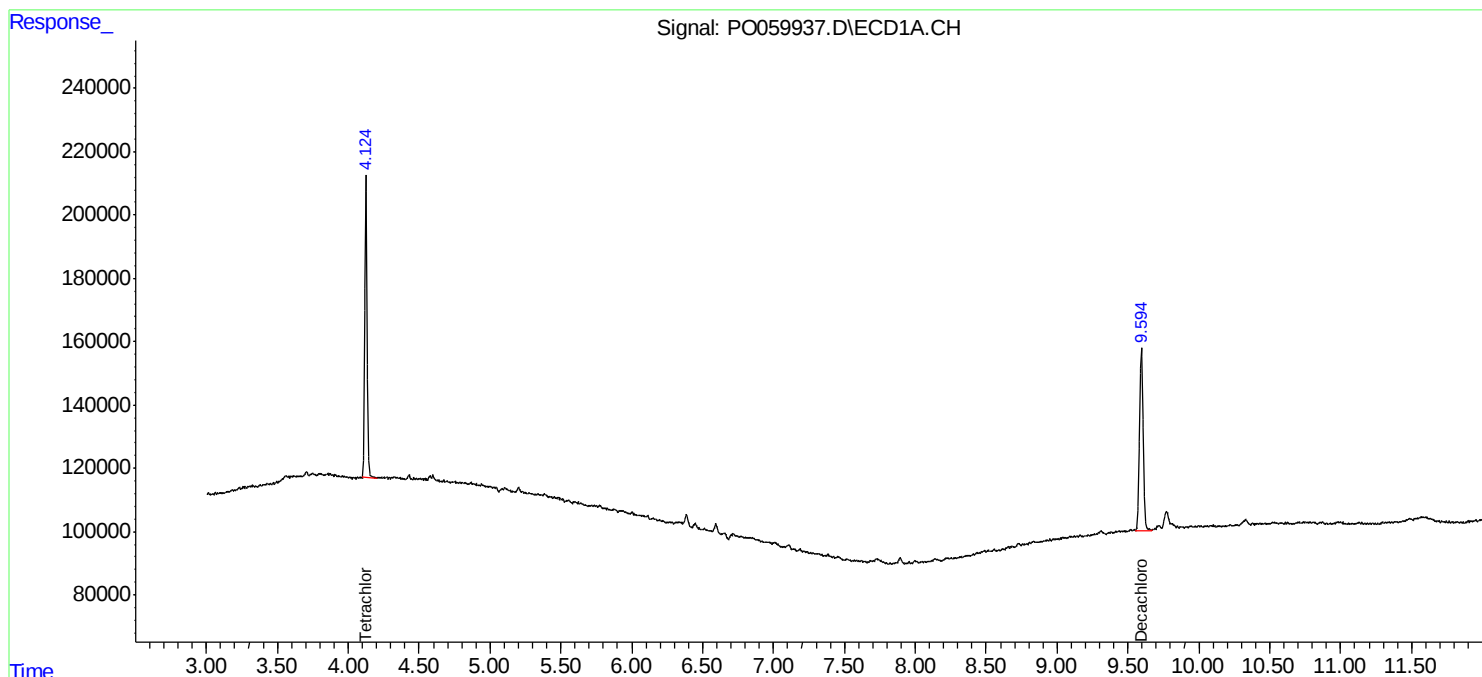


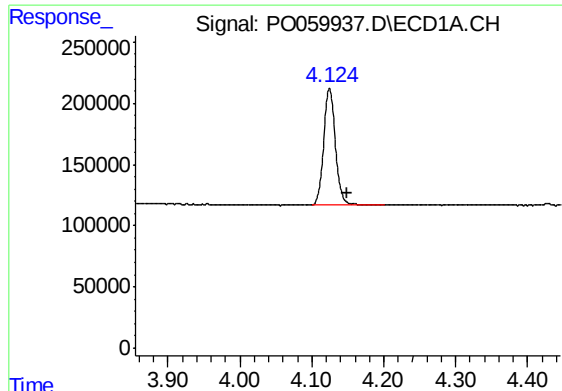

#1 Tetrachloro-m-xylene


R.T.: 4.125 min
Delta R.T.: -0.024 min
Response: 1070818
Conc: 30.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-S

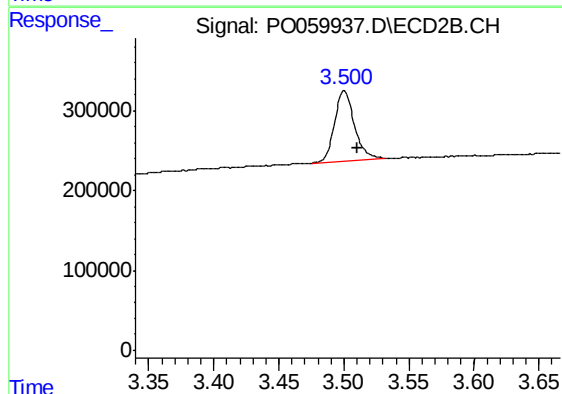


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 925653
Conc: 25.72 ng/ml

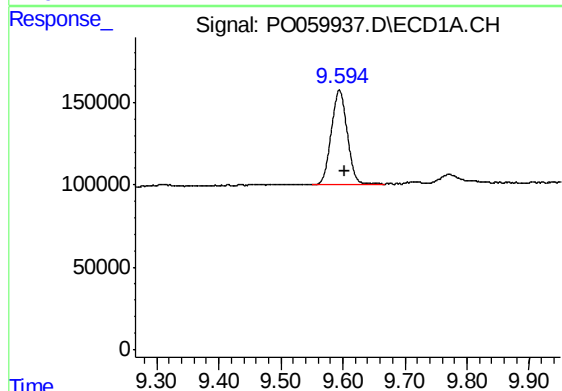

#2 Decachlorobiphenyl

R.T.: 9.595 min
Delta R.T.: -0.008 min
Response: 1023026
Conc: 19.23 ng/ml

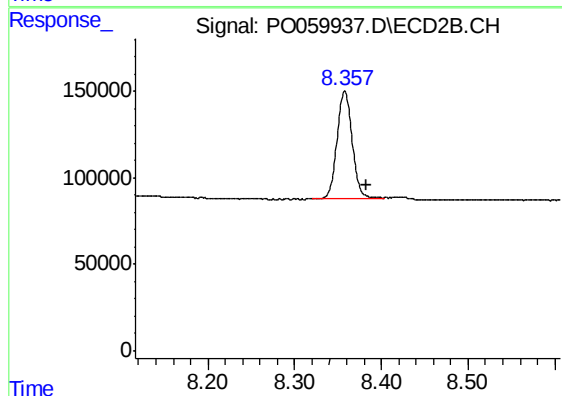

#2 Decachlorobiphenyl

R.T.: 8.358 min
Delta R.T.: -0.026 min
Response: 750690
Conc: 18.62 ng/ml