

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
 Data File : P0059940.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2019 6:36
 Operator : SM/AJ
 Sample : K4546-12
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 T3-S-A

Manual Integrations
 APPROVED

Ankita
 8/28/2019 4:16:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 08:45:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.124	3.500	998663	847764	28.523m	23.552
2)	SA Decachlor...	9.594	8.357	845224	615634	15.888	15.268
Target Compounds							
31)	L7 AR-1260-1	6.849	5.994	169638	114149	62.926	50.089m
32)	L7 AR-1260-2	7.106	6.182	198969	100248	53.623	34.216 #
33)	L7 AR-1260-3	7.458	6.330	116866	114348	35.670	43.164
34)	L7 AR-1260-4	7.684	6.791	146256	76466	47.620	33.796m#
35)	L7 AR-1260-5	7.993	7.037	242825	170277	34.293	30.941

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082719\
Data File : P0059940.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 6:36
Operator : SM/AJ
Sample : K4546-12
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/28/2019 4:16:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 08:45:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

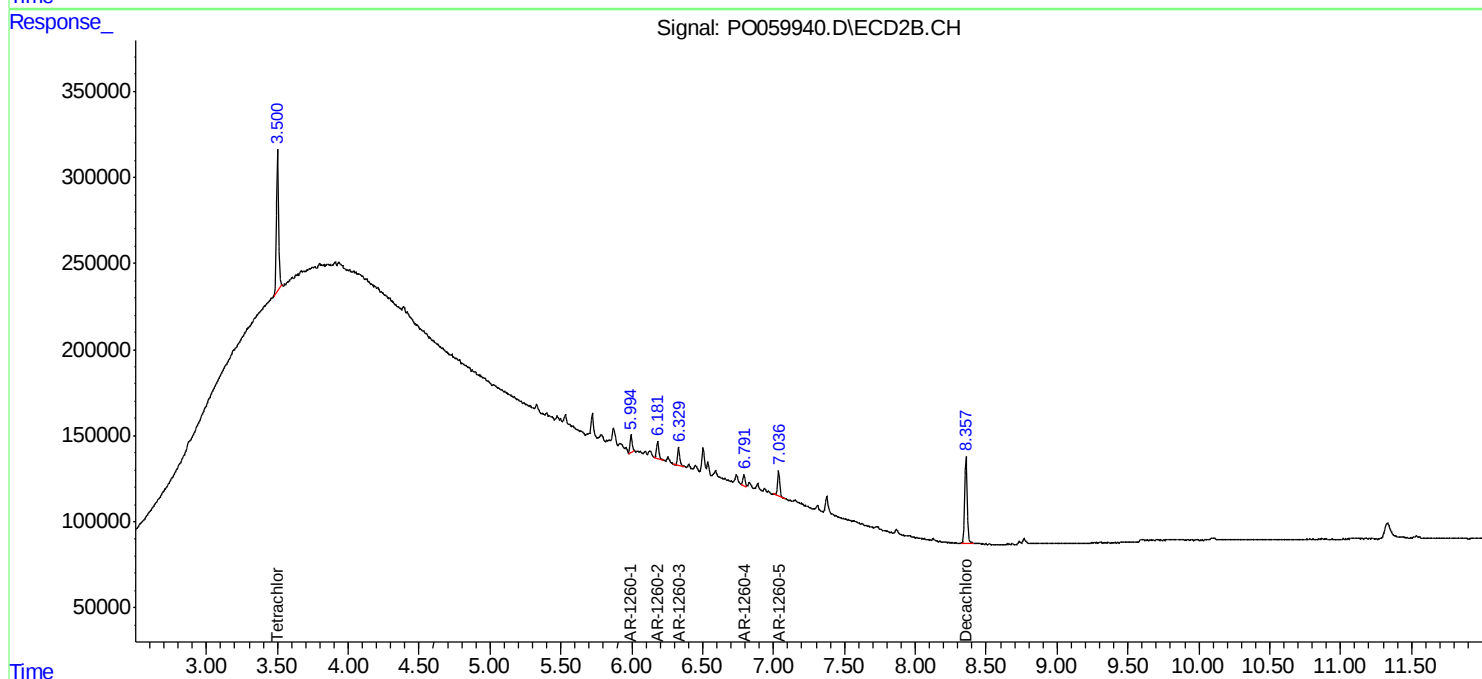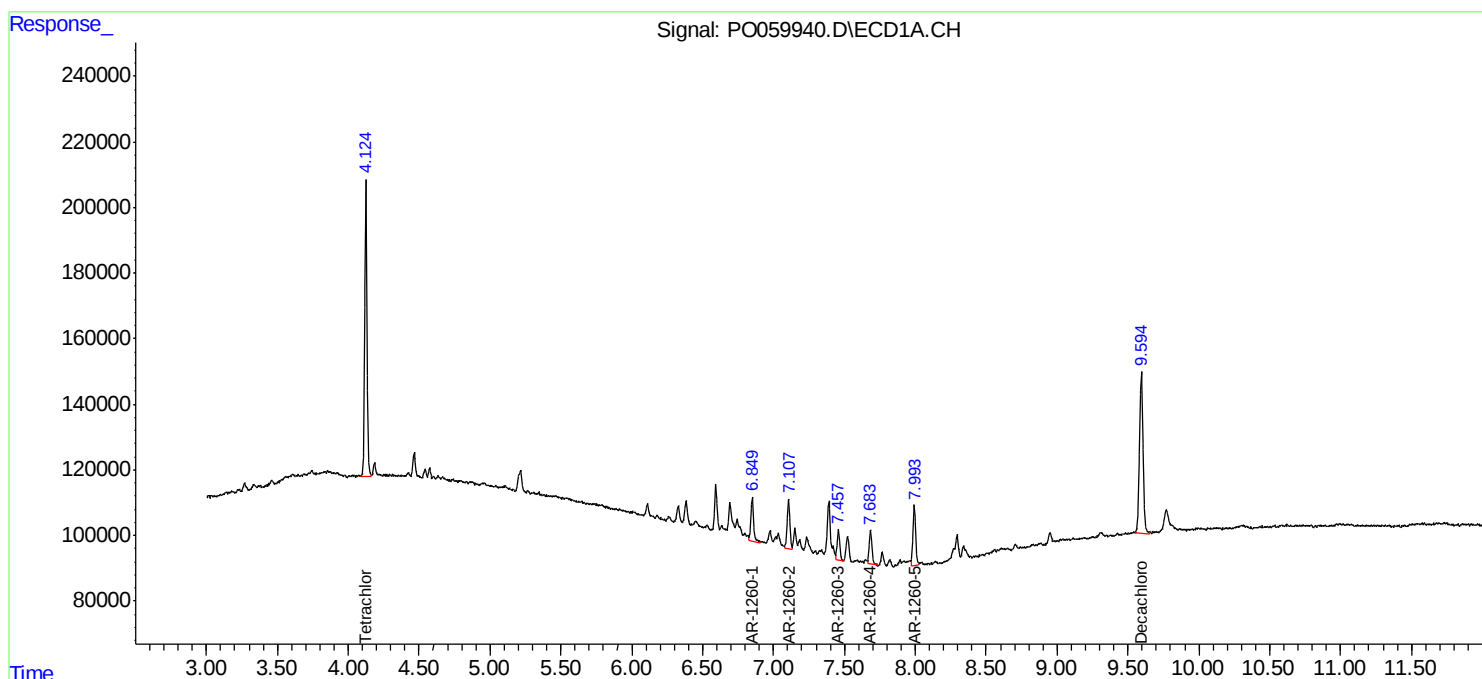

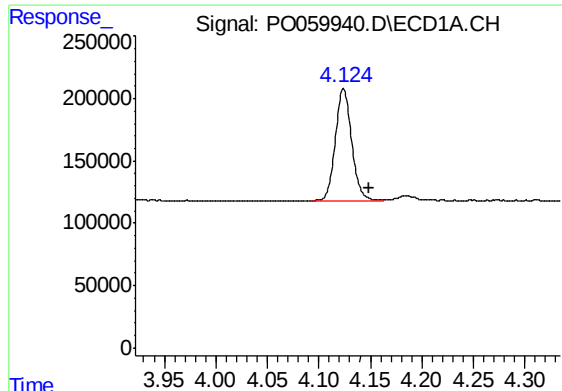


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.025 min
Response: 998663
Conc: 28.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/28/2019 4:16:24 PM

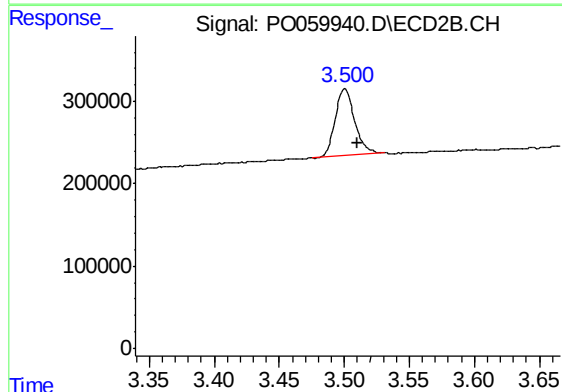


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 847764
Conc: 23.55 ng/ml

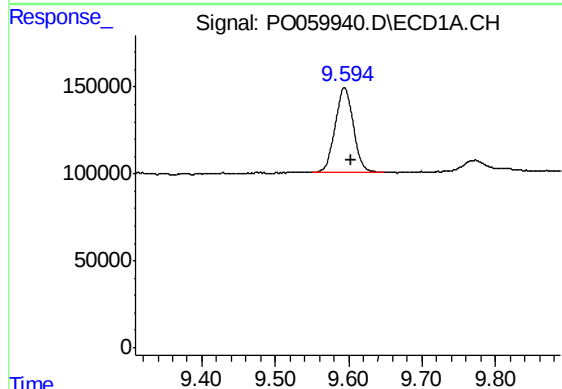


#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: -0.009 min
Response: 845224
Conc: 15.89 ng/ml

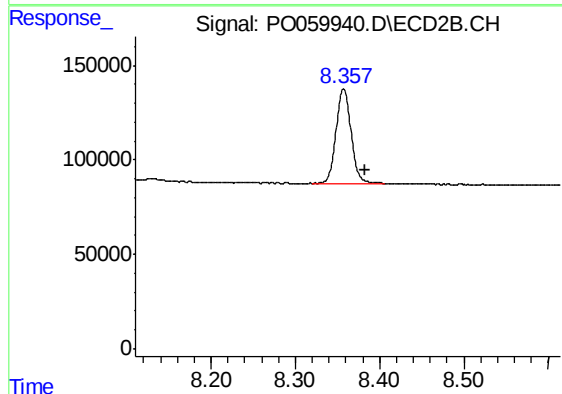

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.026 min
Response: 615634
Conc: 15.27 ng/ml

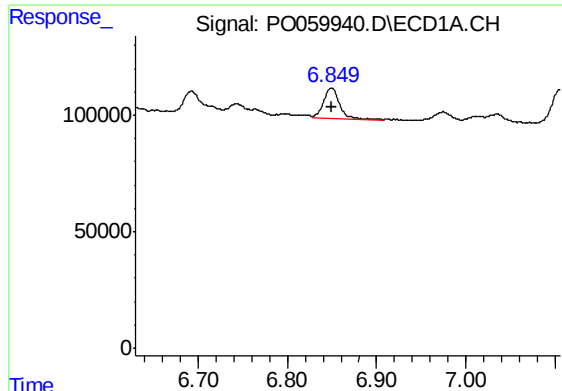


#31 AR-1260-1

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 169638
Conc: 62.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/28/2019 4:16:24 PM

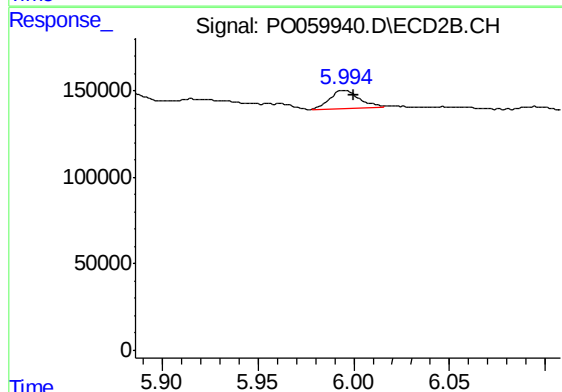


#31 AR-1260-1

R.T.: 5.994 min
Delta R.T.: -0.006 min
Response: 114149
Conc: 50.09 ng/ml m

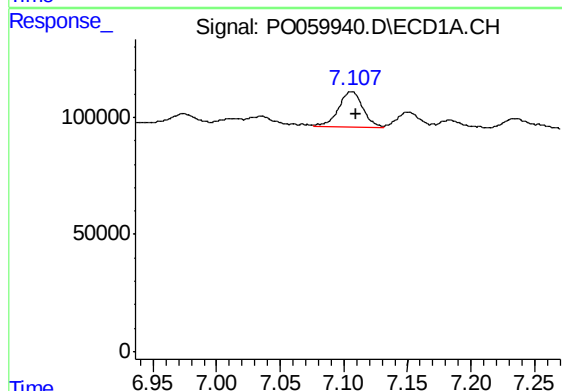


#32 AR-1260-2

R.T.: 7.106 min
Delta R.T.: -0.004 min
Response: 198969
Conc: 53.62 ng/ml

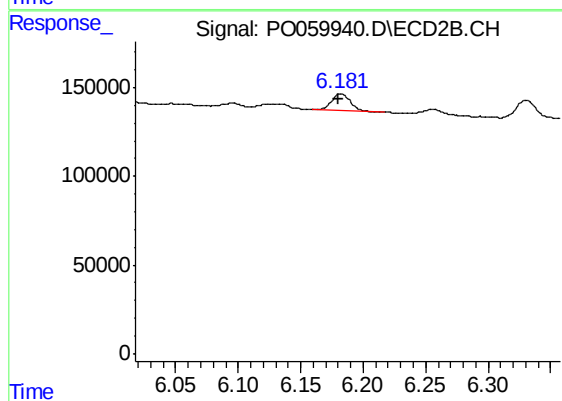

#32 AR-1260-2

R.T.: 6.182 min
Delta R.T.: 0.002 min
Response: 100248
Conc: 34.22 ng/ml

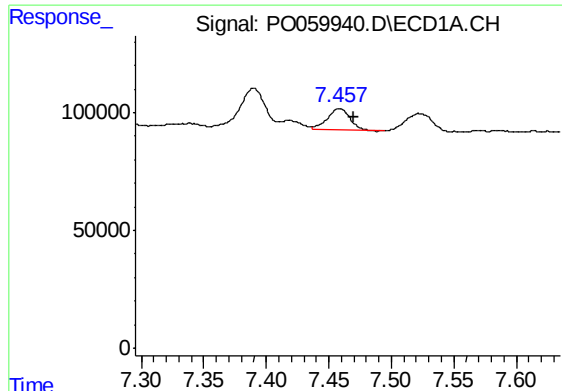


#33 AR-1260-3

R.T.: 7.458 min
Delta R.T.: -0.012 min
Response: 116866
Conc: 35.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/28/2019 4:16:24 PM

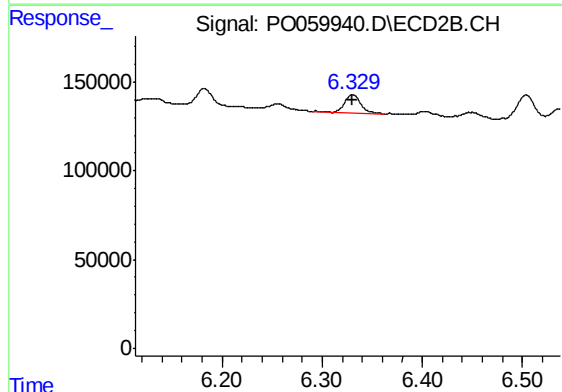


#33 AR-1260-3

R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 114348
Conc: 43.16 ng/ml

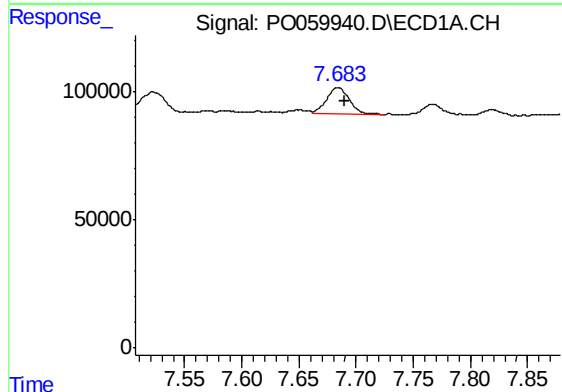


#34 AR-1260-4

R.T.: 7.684 min
Delta R.T.: -0.006 min
Response: 146256
Conc: 47.62 ng/ml

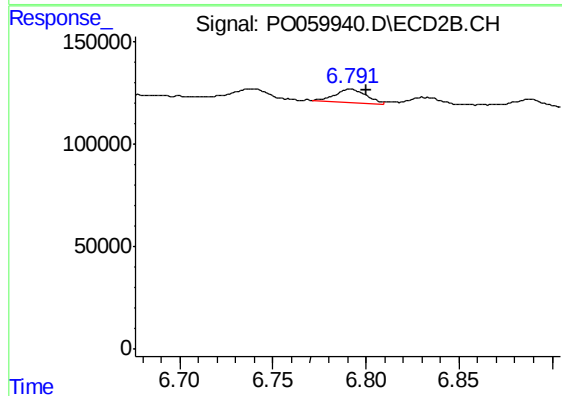

#34 AR-1260-4

R.T.: 6.791 min
Delta R.T.: -0.009 min
Response: 76466
Conc: 33.80 ng/ml m

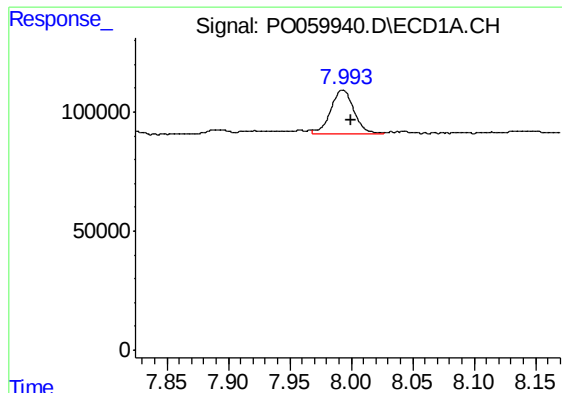


#35 AR-1260-5

R.T.: 7.993 min
Delta R.T.: -0.007 min
Response: 242825
Conc: 34.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
T3-S-A

Manual Integrations
APPROVED

Ankita
8/28/2019 4:16:24 PM

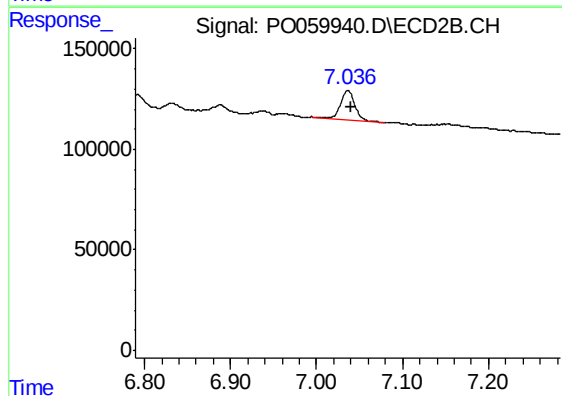

#35 AR-1260-5

R.T.: 7.037 min
Delta R.T.: -0.003 min
Response: 170277
Conc: 30.94 ng/ml