

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082720\
 Data File : P0070911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2020 12:56
 Operator : DD\AJ
 Sample : L3803-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260025COK-END-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 15:33:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.559	1507079	967234	21.634	24.027
2) SA Decachlor...	10.000	8.743	1869766	1040083	19.972	18.470

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082720\
Data File : P0070911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2020 12:56
Operator : DD\AJ
Sample : L3803-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC260025COK-END-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 15:33:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

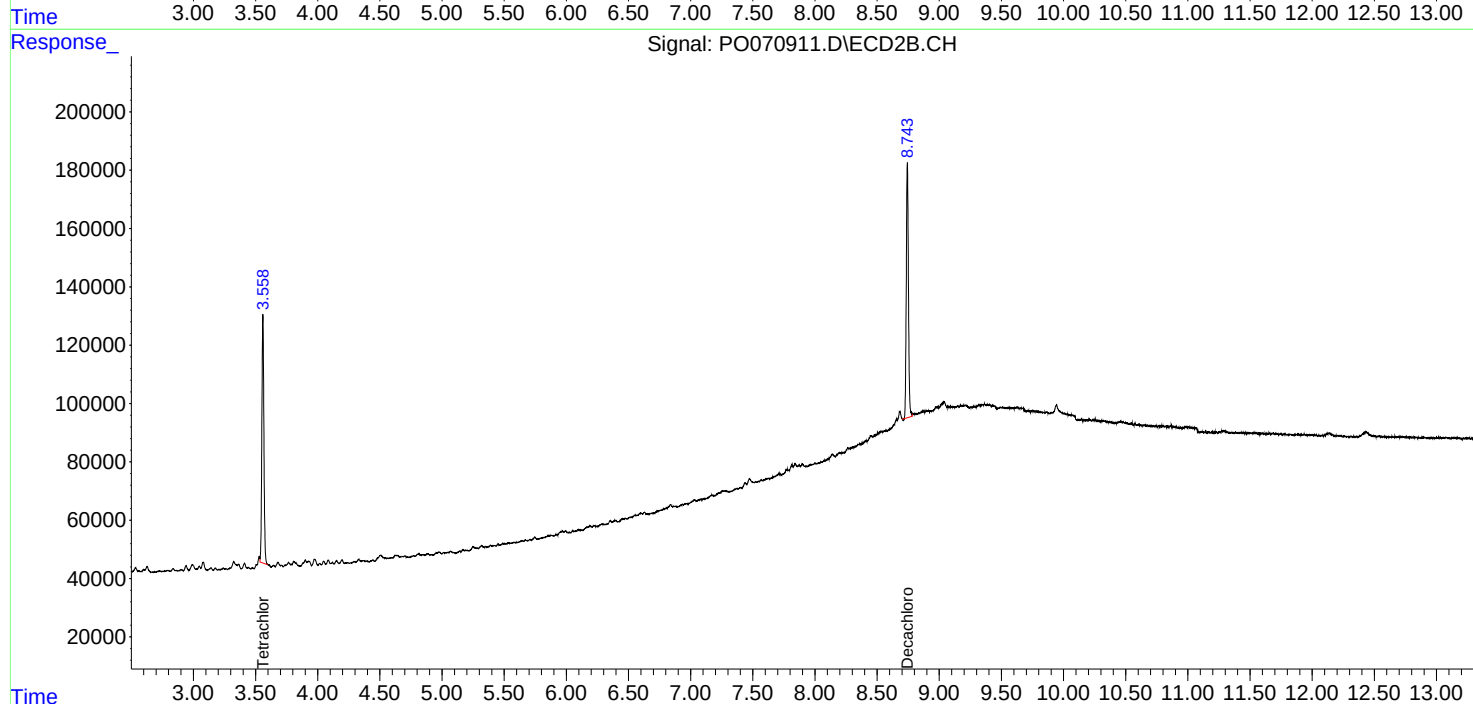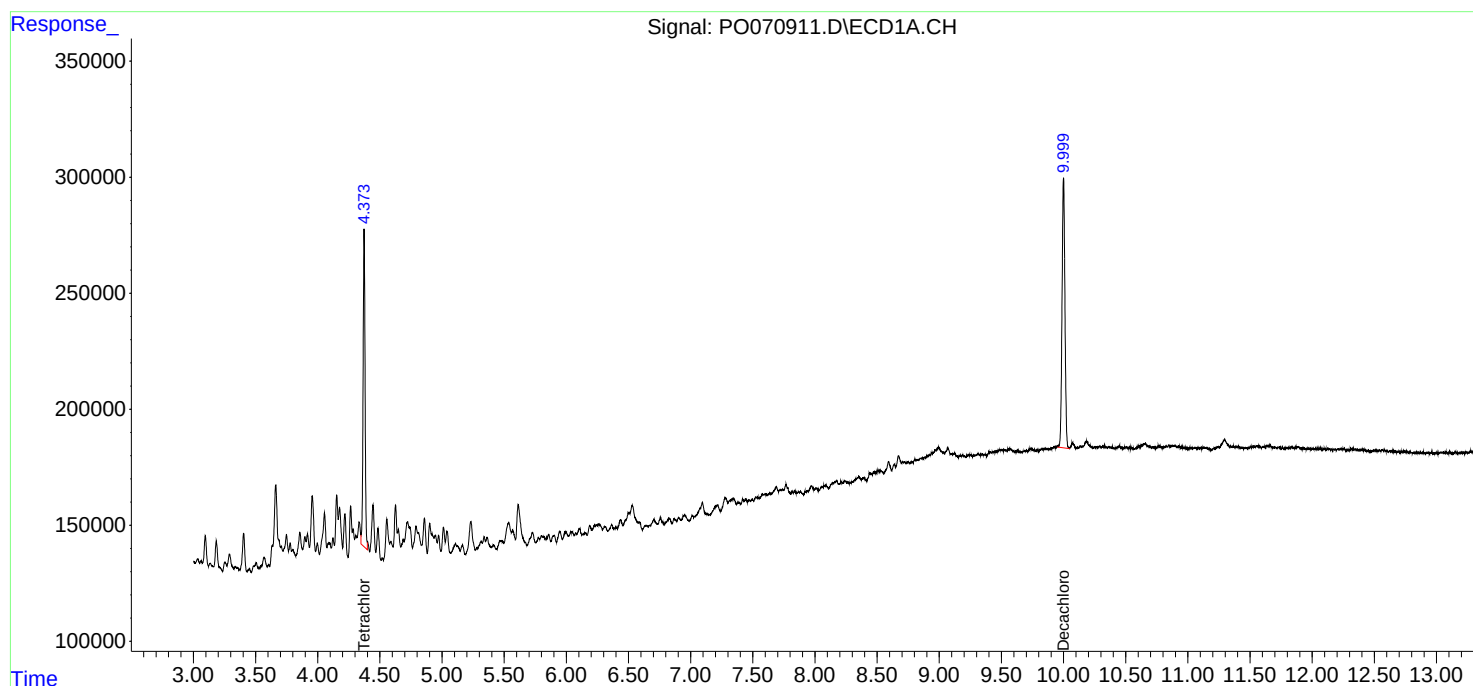


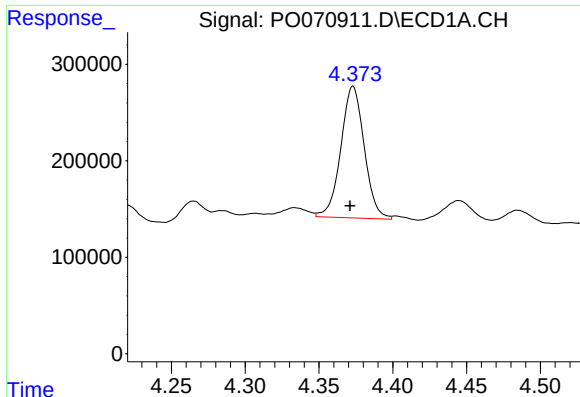

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: 0.002 min
Response: 1507079
Conc: 21.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260025COK-END-2

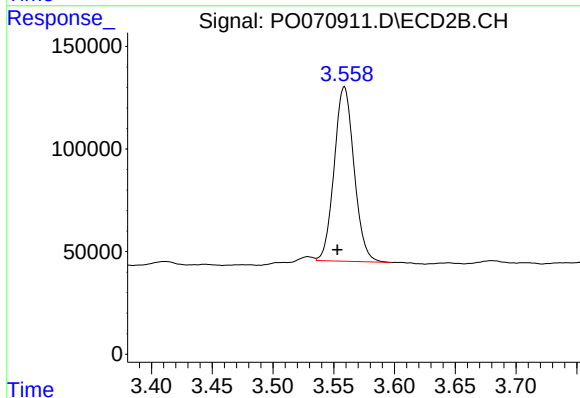


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: 0.006 min
Response: 967234
Conc: 24.03 ng/ml

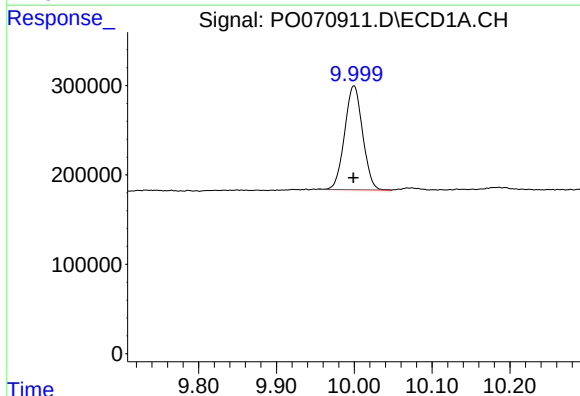

#2 Decachlorobiphenyl

R.T.: 10.000 min
Delta R.T.: 0.000 min
Response: 1869766
Conc: 19.97 ng/ml

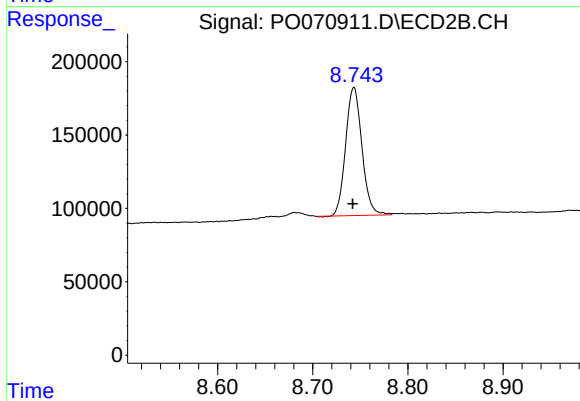

#2 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.001 min
Response: 1040083
Conc: 18.47 ng/ml