

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082724\
 Data File : P0105919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 19:29
 Operator : YP/AJ
 Sample : P3737-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/28/2024
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 02:57:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.720	203.1E6	60643056	22.264m	22.446
2) SA Decachlor...	10.195	8.754	90881264	37374075	16.746	17.120

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082724\
Data File : PO105919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 19:29
Operator : YP/AJ
Sample : P3737-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:57:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

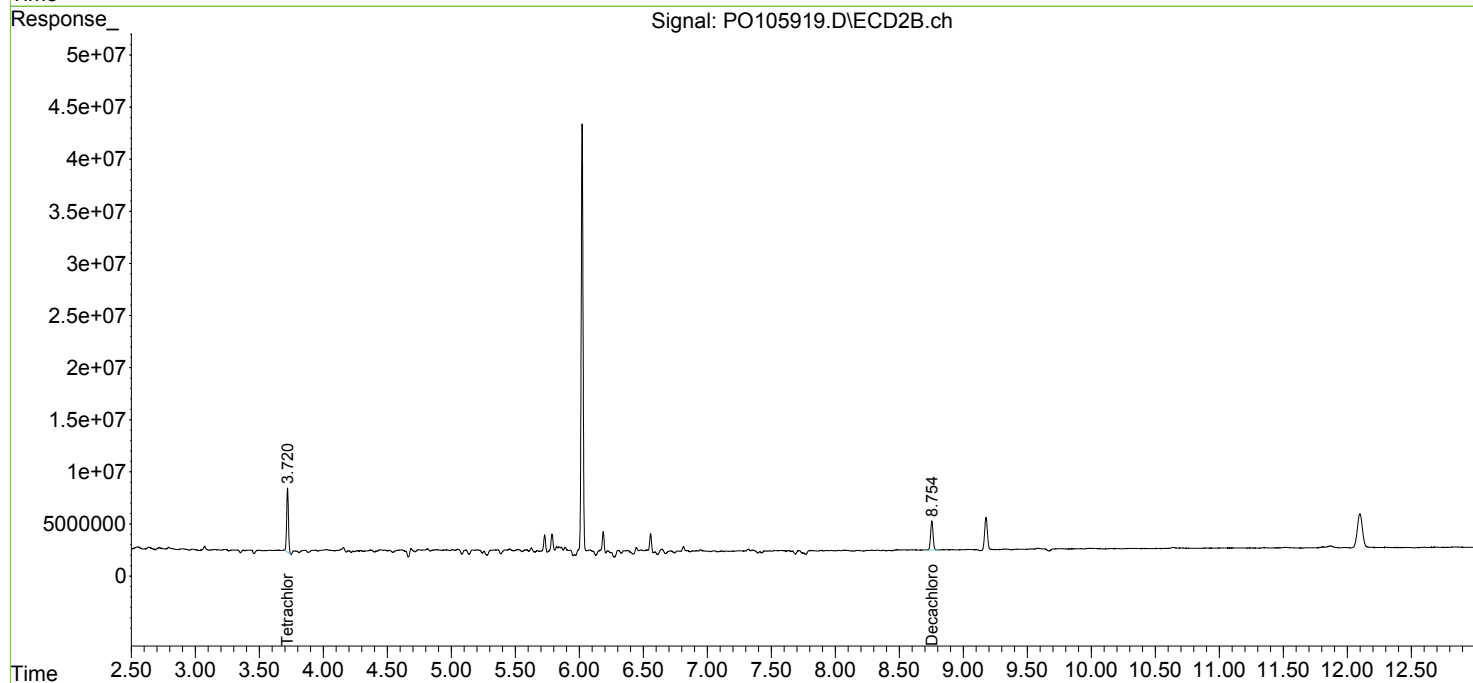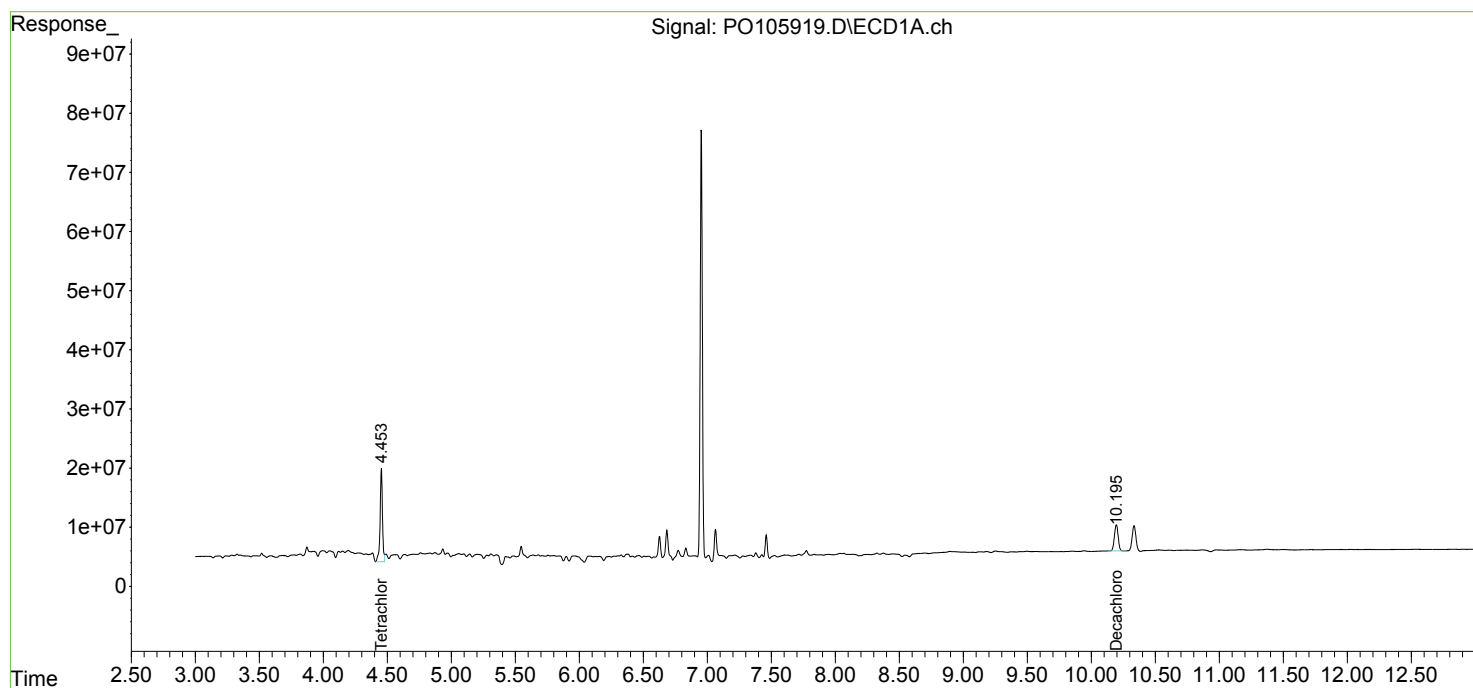

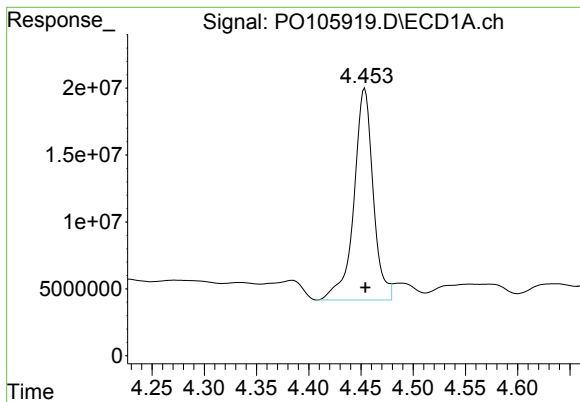


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: -0.001 min
Response: 203116878
Conc: 22.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

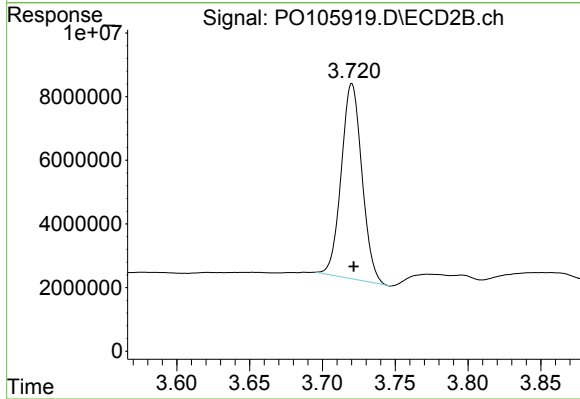


#1 Tetrachloro-m-xylene

R.T.: 3.720 min
Delta R.T.: -0.001 min
Response: 60643056
Conc: 22.45 ng/ml

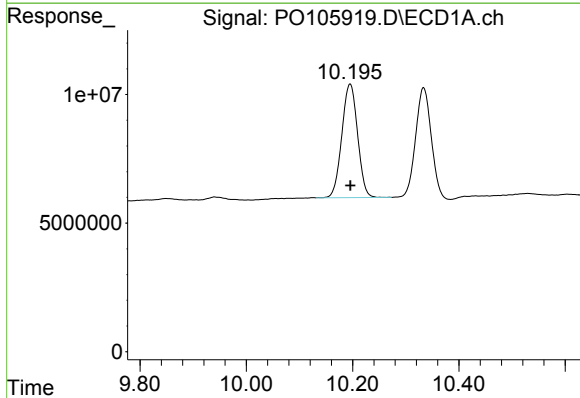

#2 Decachlorobiphenyl

R.T.: 10.195 min
Delta R.T.: 0.000 min
Response: 90881264
Conc: 16.75 ng/ml

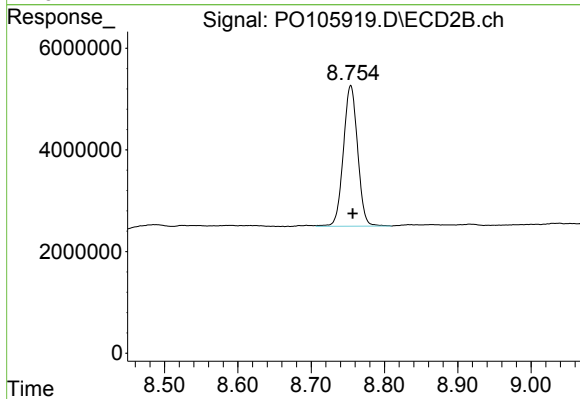

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: -0.003 min
Response: 37374075
Conc: 17.12 ng/ml