

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0082818\
Data File : P0048585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2018 10:26
Operator : SM/SJ
Sample : J4673-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SOUTH-PATERSON-PILE

Manual Integrations
APPROVED

Sohil
8/29/2018 1:44:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 10:41:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.622	4701321	5440108	24.818m	20.094
2) SA Decachlor...	10.070	8.600	2998444	2652420	17.413	15.838

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082818\
Data File : P0048585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2018 10:26
Operator : SM/SJ
Sample : J4673-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOUTH-PATERSON-PILE


Manual Integrations
APPROVED

Sohil
8/29/2018 1:44:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 10:41:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

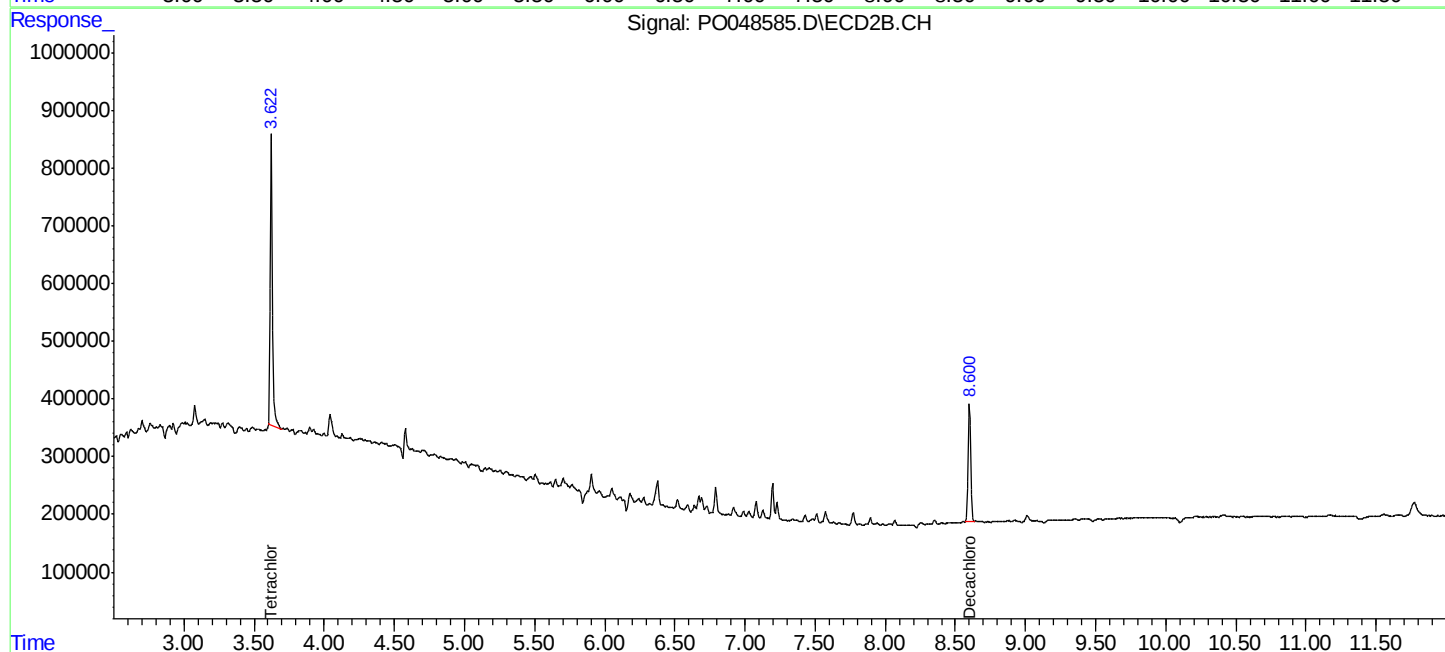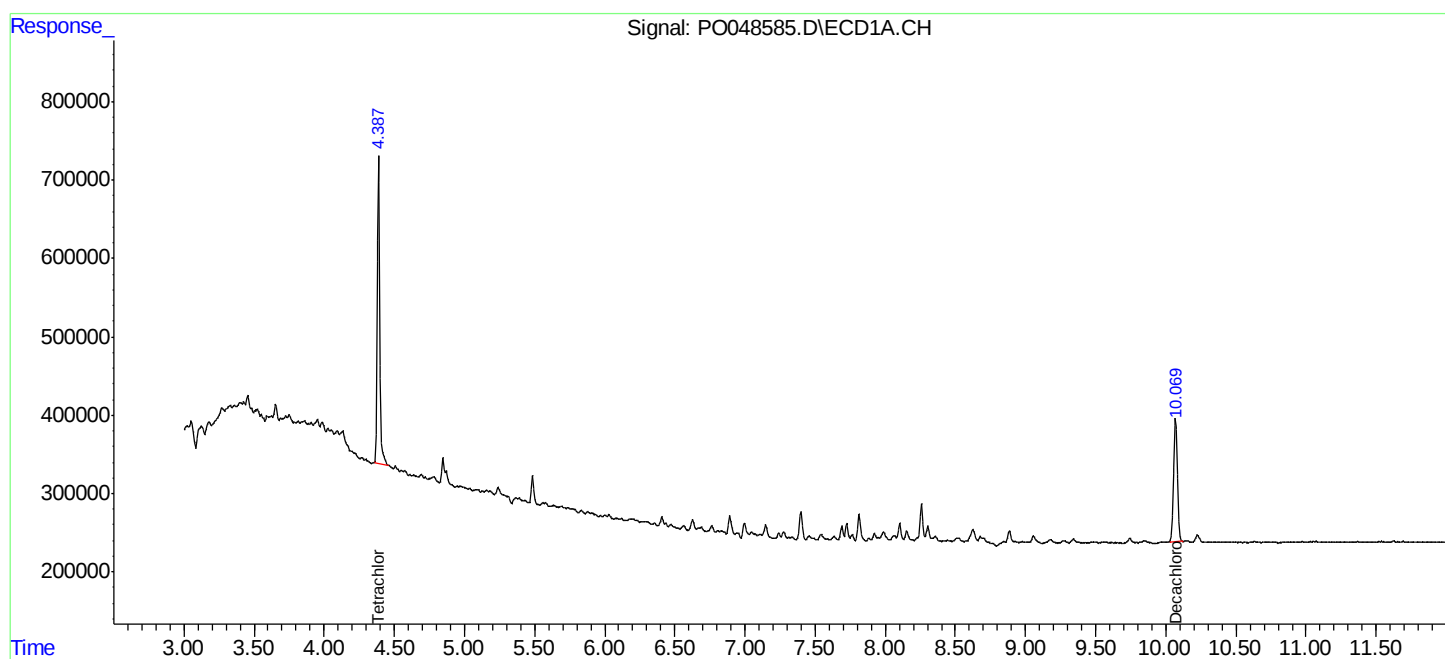

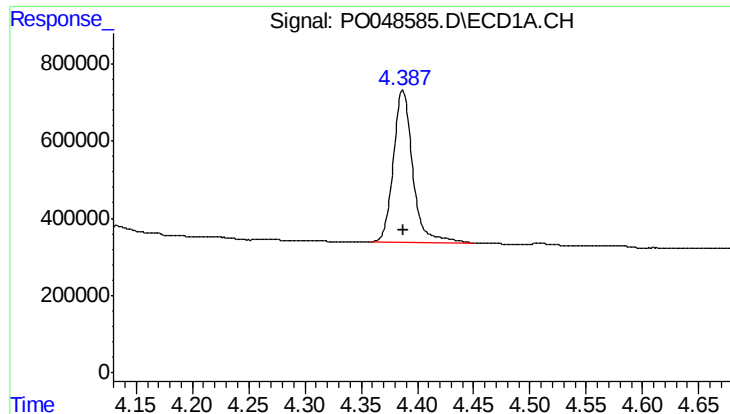


#1 Tetrachloro-m-xylene

R.T.: 4.387 min
Delta R.T.: -0.001 min
Response: 4701321
Conc: 24.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOUTH-PATERSON-PILE


Manual Integrations
APPROVED

Sohil
8/29/2018 1:44:07 PM

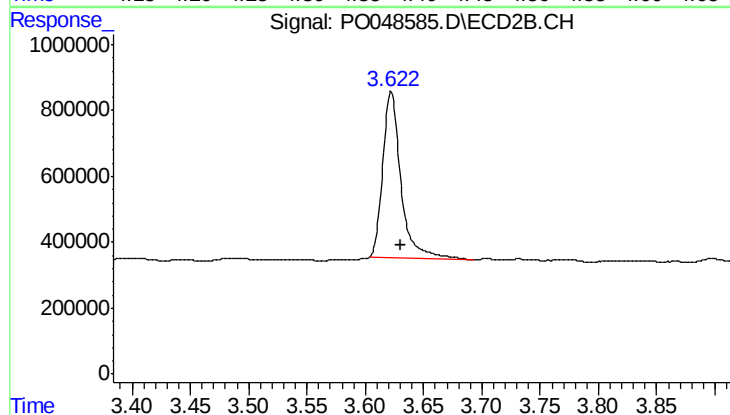


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.008 min
Response: 5440108
Conc: 20.09 ng/ml

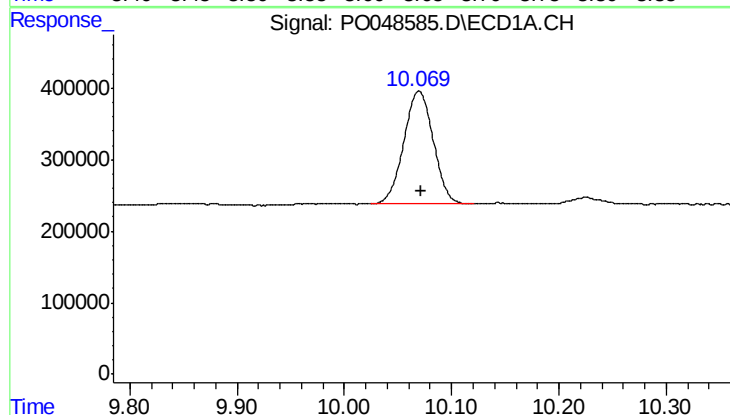

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: -0.002 min
Response: 2998444
Conc: 17.41 ng/ml

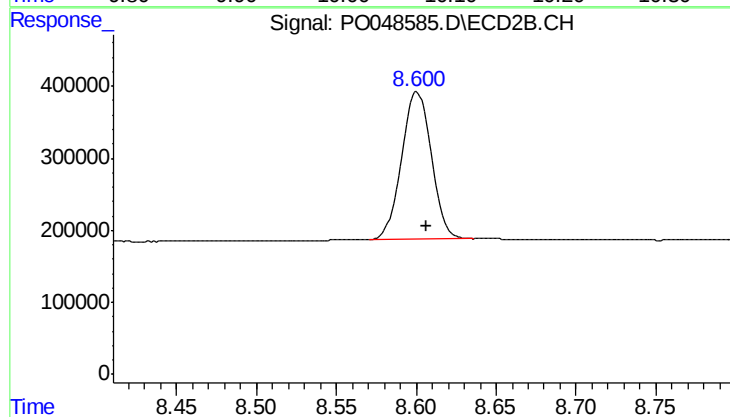

#2 Decachlorobiphenyl

R.T.: 8.600 min
Delta R.T.: -0.006 min
Response: 2652420
Conc: 15.84 ng/ml