

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082819\
Data File : P0059960.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 14:08
Operator : SM/AJ
Sample : K4551-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S401-K1-1.0-1.5-082619-FDRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 14:40:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.130	3.501	772467	609612	22.063	16.936
2)	SA Decachlor...	9.601	8.361	543286	413300	10.212	10.250

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082819\
Data File : PO059960.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 14:08
Operator : SM/AJ
Sample : K4551-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S401-K1-1.0-1.5-082619-FDRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 14:40:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

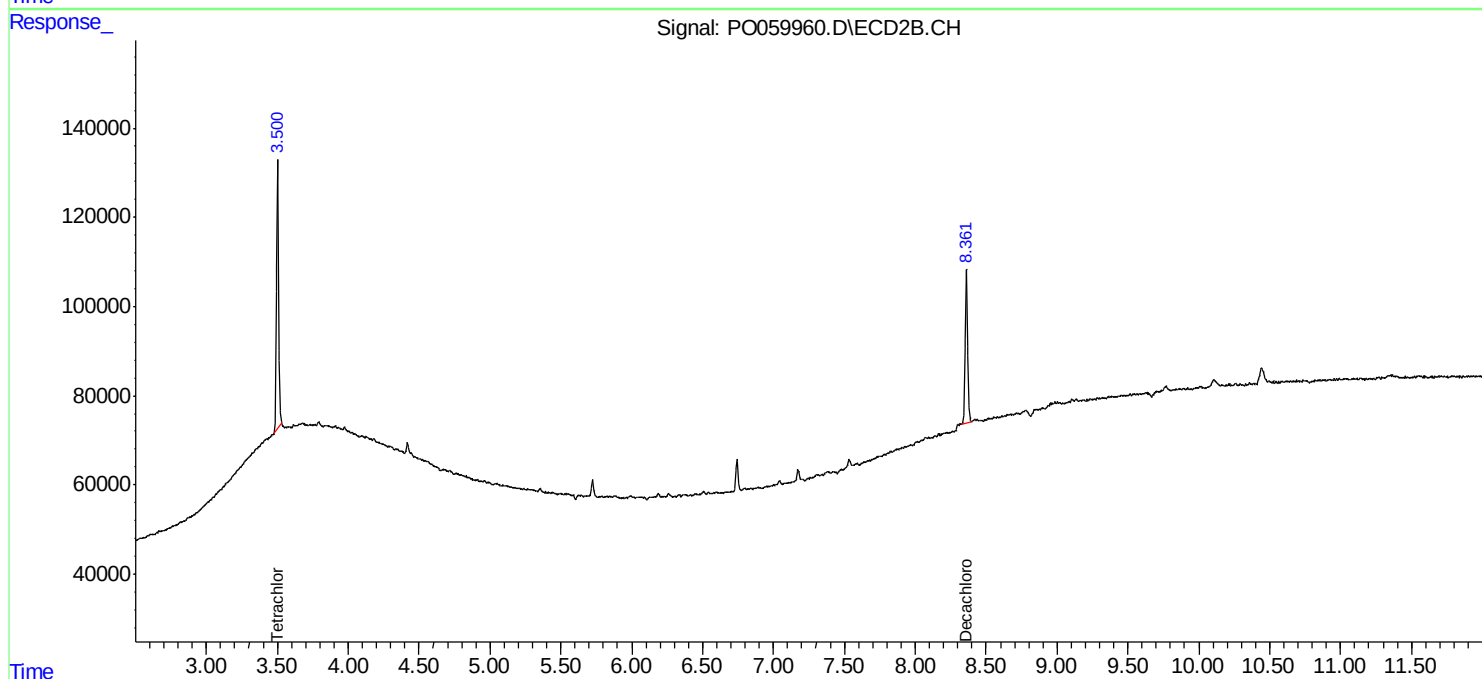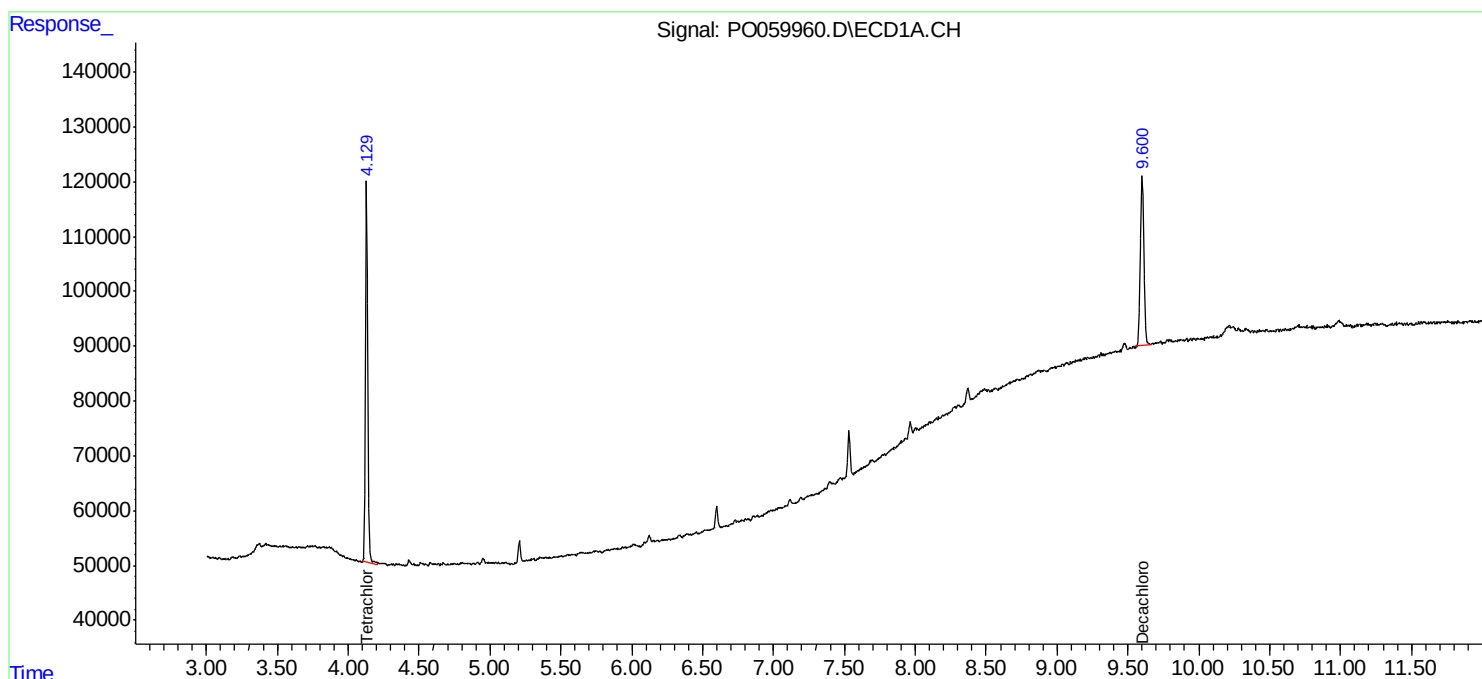


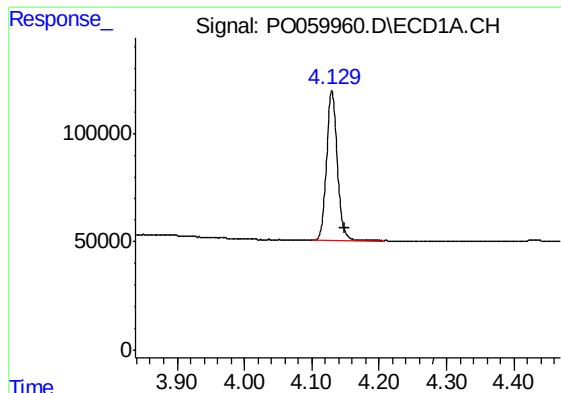

#1 Tetrachloro-m-xylene


R.T.: 4.130 min
Delta R.T.: -0.019 min
Response: 772467
Conc: 22.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
S401-K1-1.0-1.5-082619-FDRE

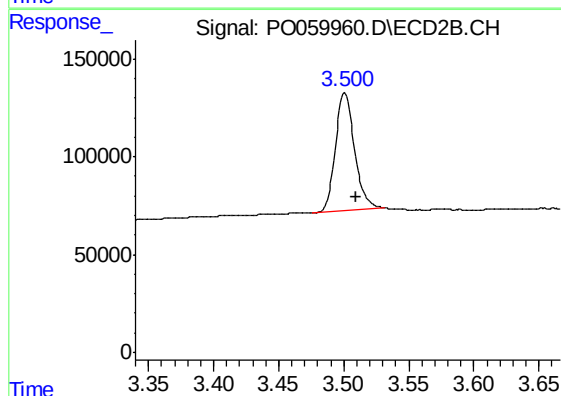


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.009 min
Response: 609612
Conc: 16.94 ng/ml

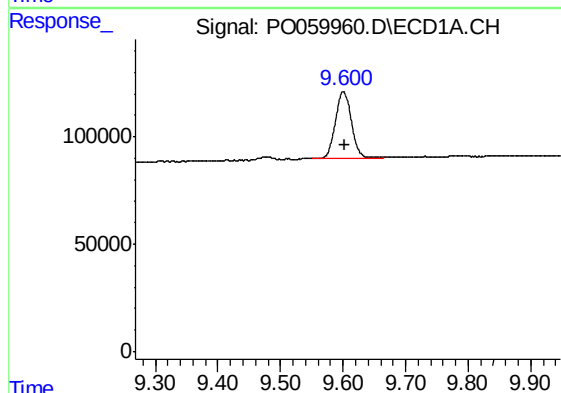

#2 Decachlorobiphenyl

R.T.: 9.601 min
Delta R.T.: -0.002 min
Response: 543286
Conc: 10.21 ng/ml

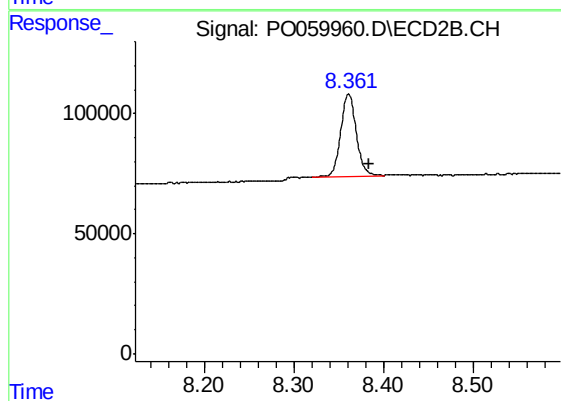

#2 Decachlorobiphenyl

R.T.: 8.361 min
Delta R.T.: -0.022 min
Response: 413300
Conc: 10.25 ng/ml