

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082819\
 Data File : P0059964.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2019 15:17
 Operator : SM/AJ
 Sample : K4560-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S404-K1-1.0-1.5-082619

Manual Integrations
 APPROVED

Ankita
 8/29/2019 2:01:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 15:58:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.128	3.500	720454	620616	20.577	17.241m
2) SA Decachlor...	9.600	8.361	577740	489044	10.860	12.129

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082819\
Data File : P0059964.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 15:17
Operator : SM/AJ
Sample : K4560-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S404-K1-1.0-1.5-082619


Manual Integrations
APPROVED

Ankita
8/29/2019 2:01:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 15:58:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

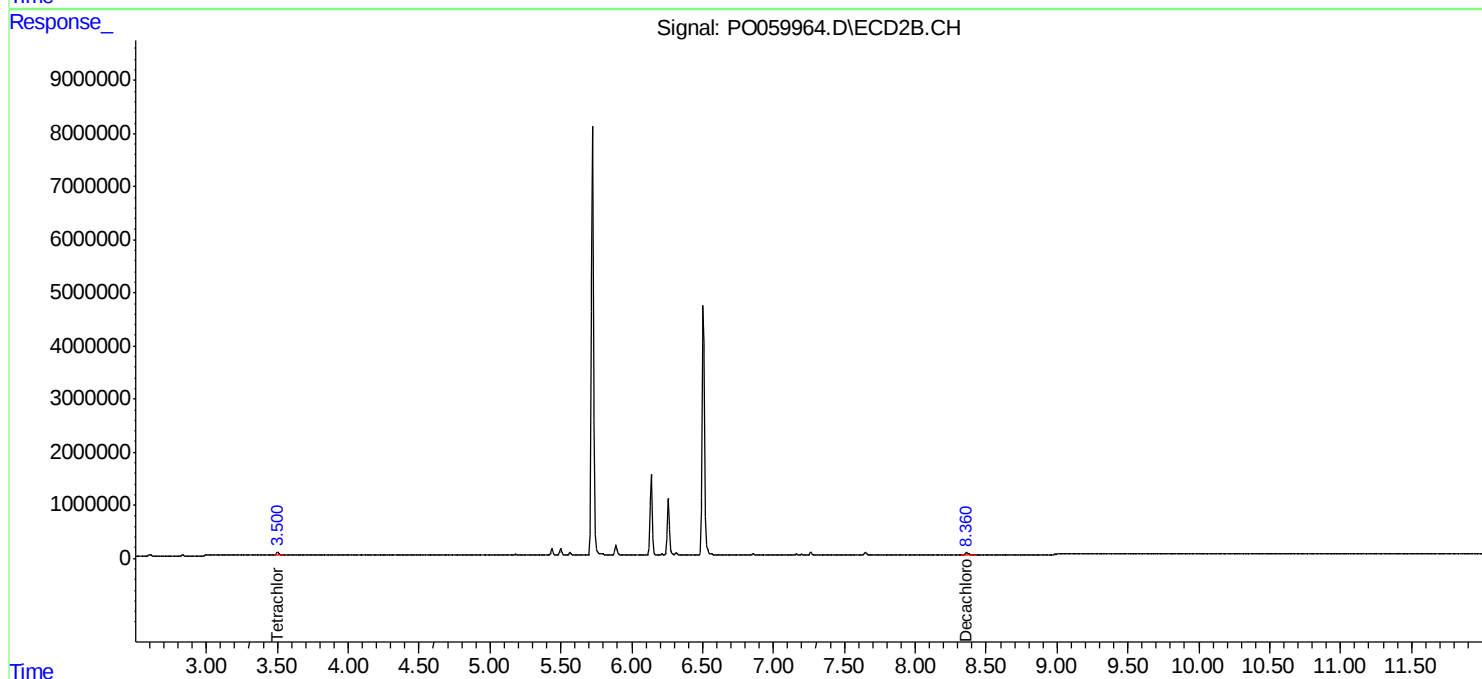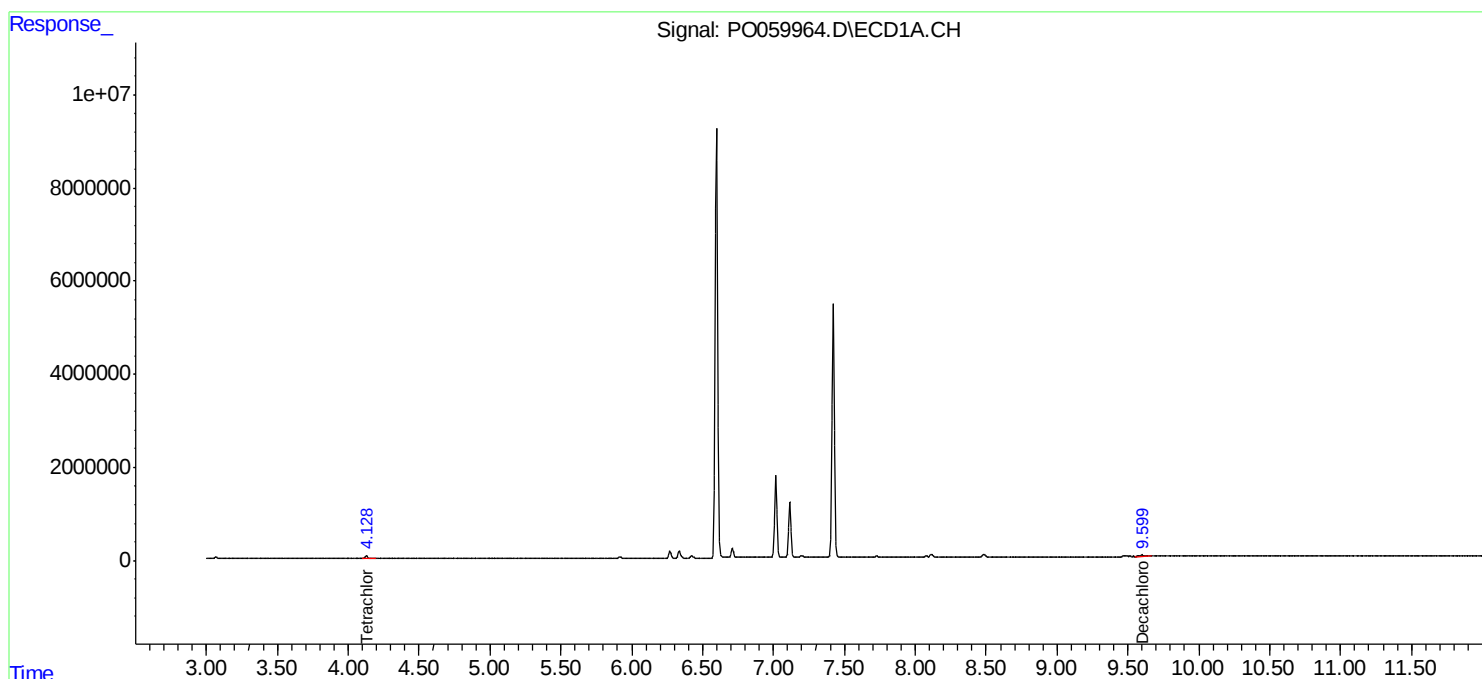

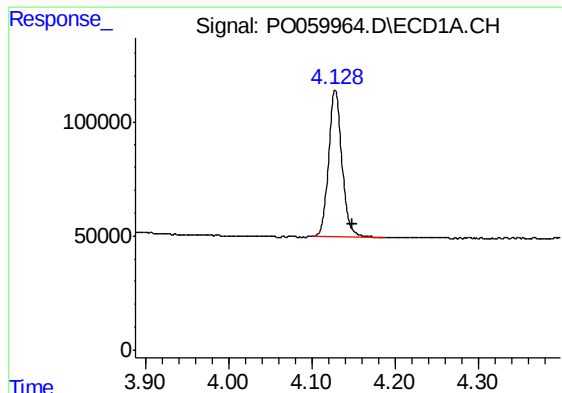


#1 Tetrachloro-m-xylene

R.T.: 4.128 min
Delta R.T.: -0.021 min
Response: 720454
Conc: 20.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
S404-K1-1.0-1.5-082619


Manual Integrations
APPROVED

Ankita
8/29/2019 2:01:37 PM

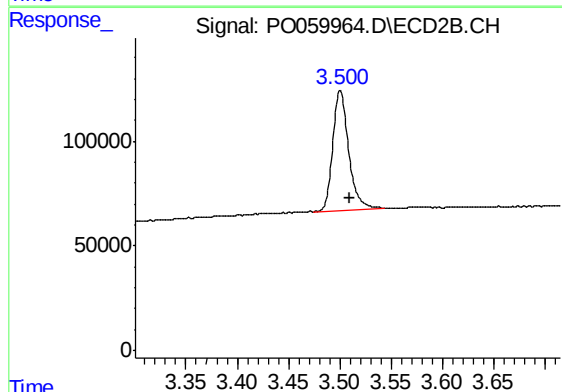


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 620616
Conc: 17.24 ng/ml m

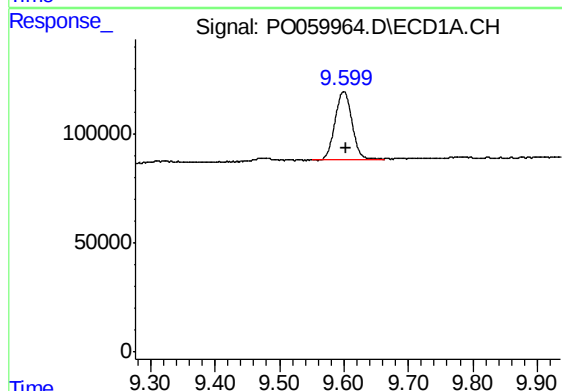

#2 Decachlorobiphenyl

R.T.: 9.600 min
Delta R.T.: -0.003 min
Response: 577740
Conc: 10.86 ng/ml

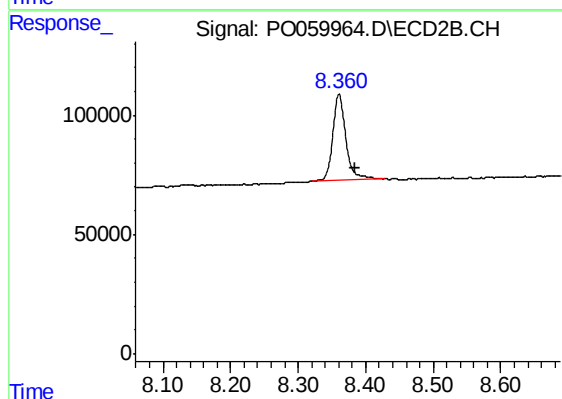

#2 Decachlorobiphenyl

R.T.: 8.361 min
Delta R.T.: -0.023 min
Response: 489044
Conc: 12.13 ng/ml