

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082819\
 Data File : P0059965.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2019 15:34
 Operator : SM/AJ
 Sample : K4560-10RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S401-K1-1.0-1.5-082619RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 15:59:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.128	3.499	694261	573868	19.829	15.943
2)	SA Decachlor...	9.598	8.360	605685	460487	11.385	11.421

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082819\
Data File : PO059965.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 15:34
Operator : SM/AJ
Sample : K4560-10RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S401-K1-1.0-1.5-082619RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 15:59:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

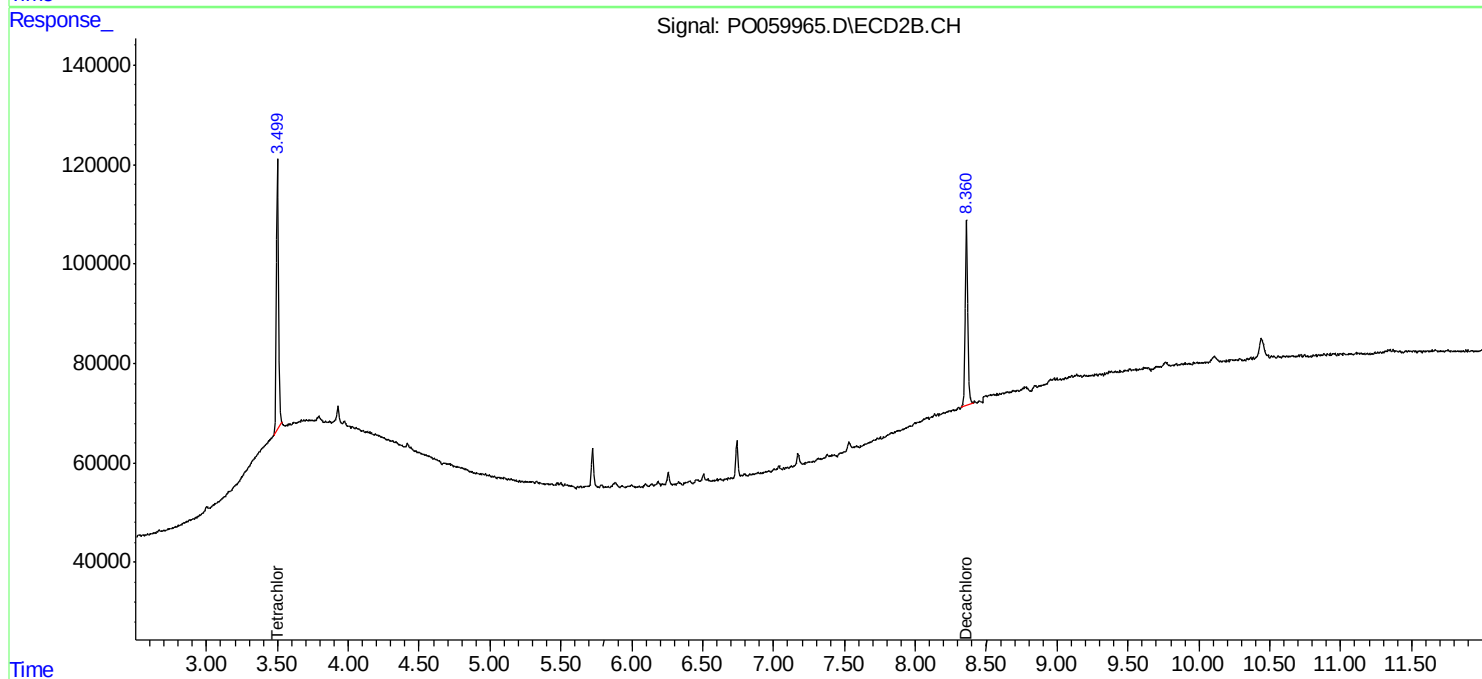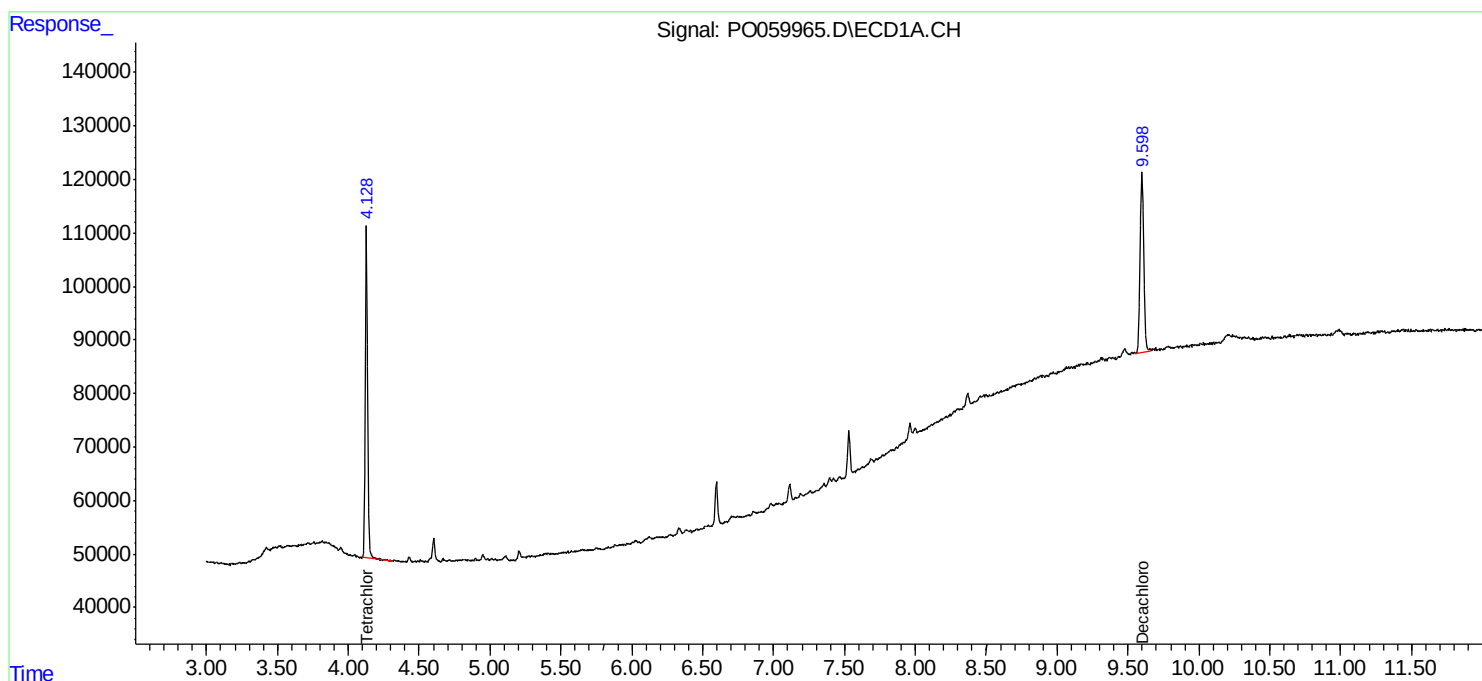


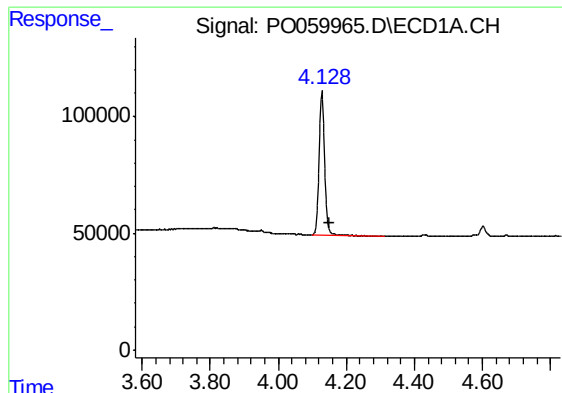

#1 Tetrachloro-m-xylene


R.T.: 4.128 min
Delta R.T.: -0.021 min
Response: 694261
Conc: 19.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
S401-K1-1.0-1.5-082619RE

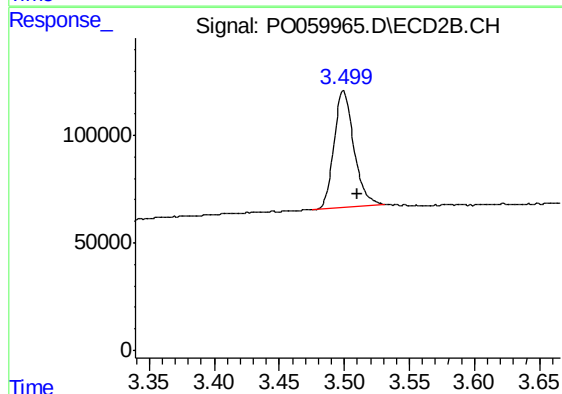


#1 Tetrachloro-m-xylene

R.T.: 3.499 min
Delta R.T.: -0.011 min
Response: 573868
Conc: 15.94 ng/ml

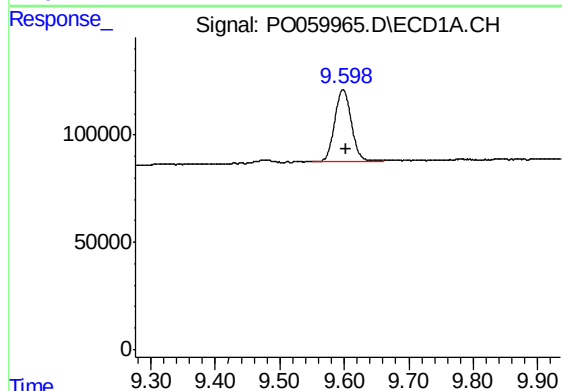

#2 Decachlorobiphenyl

R.T.: 9.598 min
Delta R.T.: -0.005 min
Response: 605685
Conc: 11.39 ng/ml

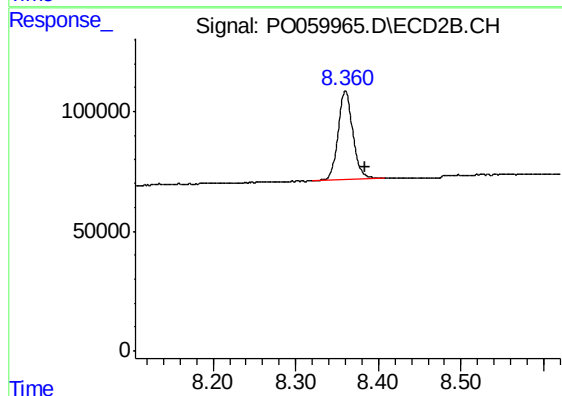

#2 Decachlorobiphenyl

R.T.: 8.360 min
Delta R.T.: -0.023 min
Response: 460487
Conc: 11.42 ng/ml