

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082819\
 Data File : P0059983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2019 20:30
 Operator : SM/AJ
 Sample : K4567-11
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-7-D

Manual Integrations
 APPROVED

Ankita
 8/29/2019 2:02:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 04:09:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.123	3.499	1085798	941413	31.012m	26.154m
2)	SA Decachlor...	9.592	8.358	1118956	857068	21.033	21.256

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082819\
Data File : PO059983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 20:30
Operator : SM/AJ
Sample : K4567-11
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-7-D


Manual Integrations
APPROVED

Ankita
8/29/2019 2:02:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 04:09:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

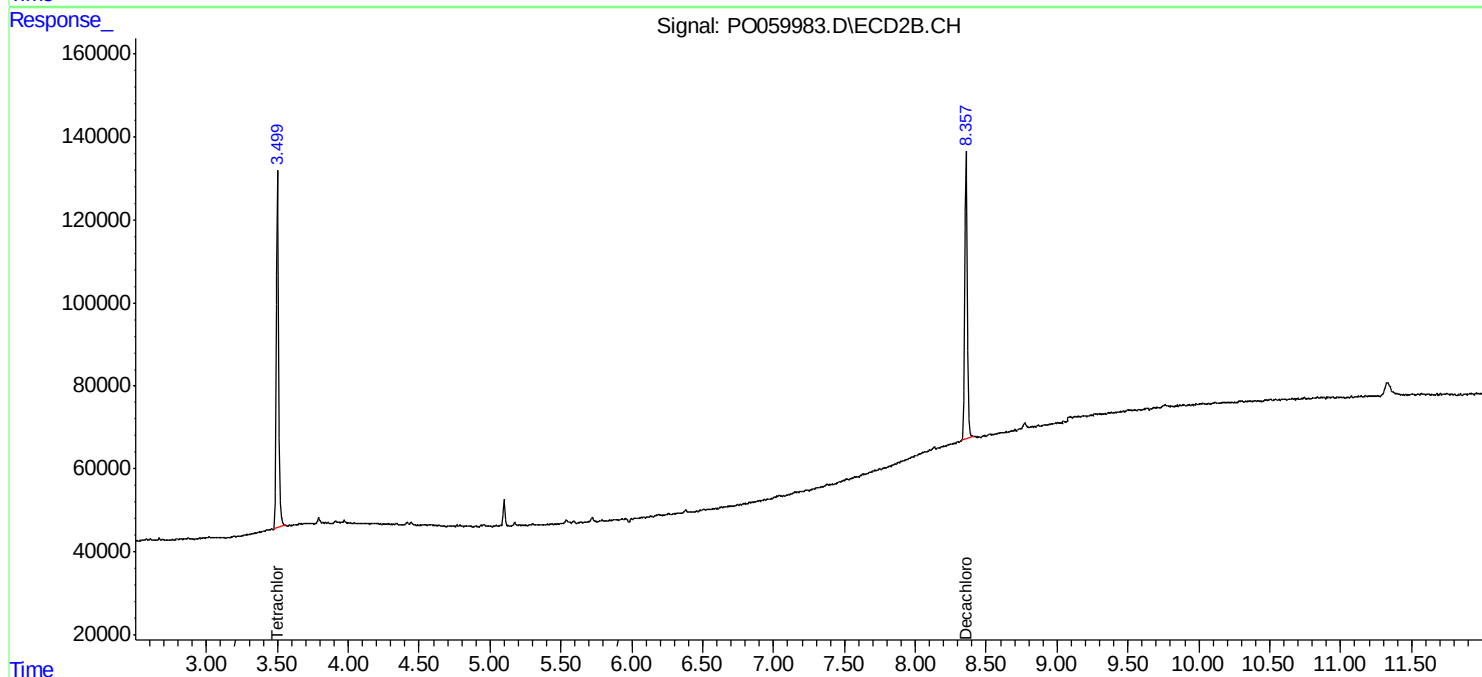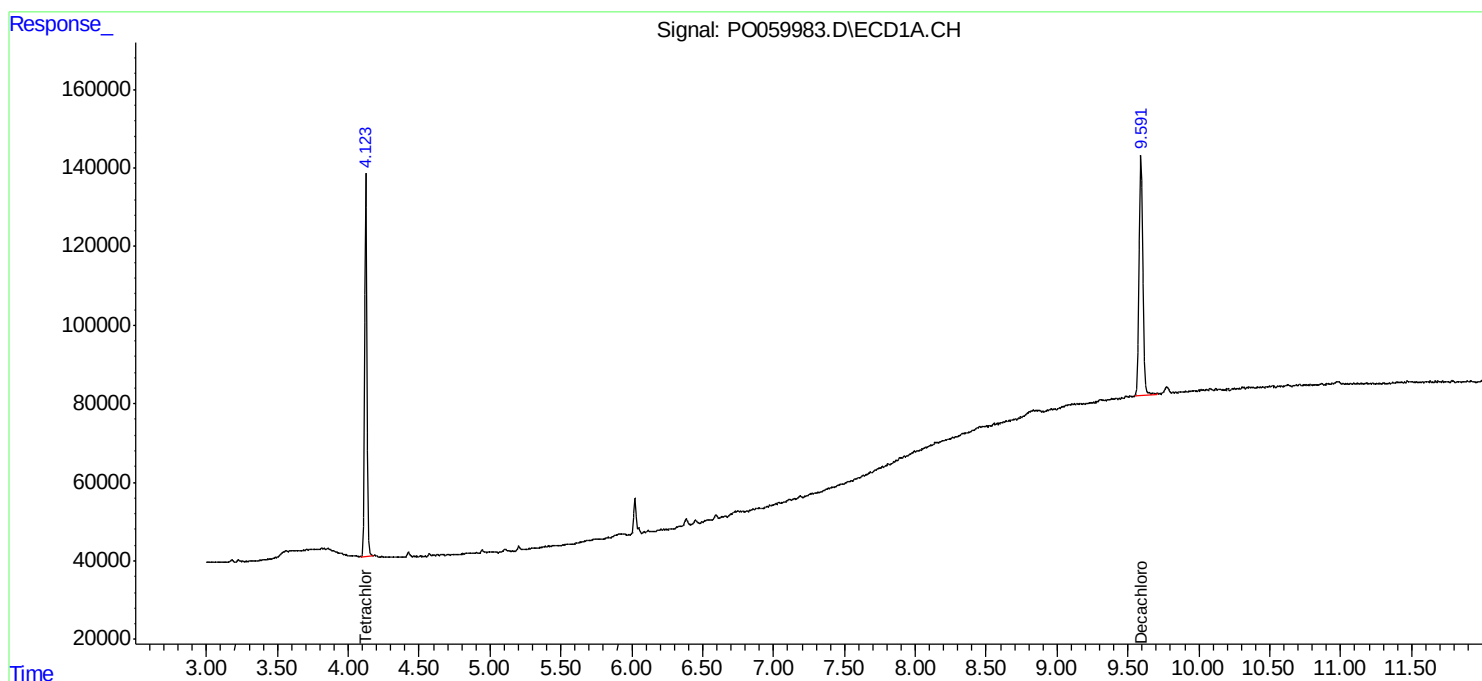

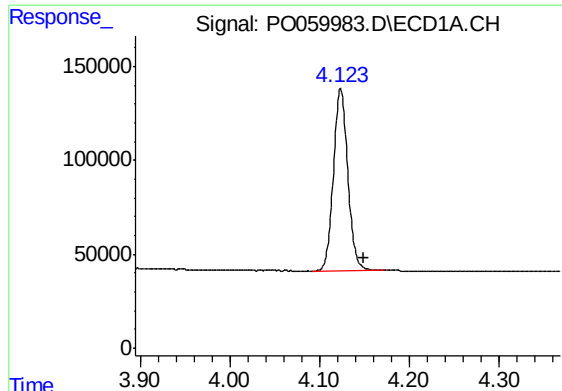


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: -0.026 min
Response: 1085798
Conc: 31.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-7-D


Manual Integrations
APPROVED

Ankita
8/29/2019 2:02:36 PM

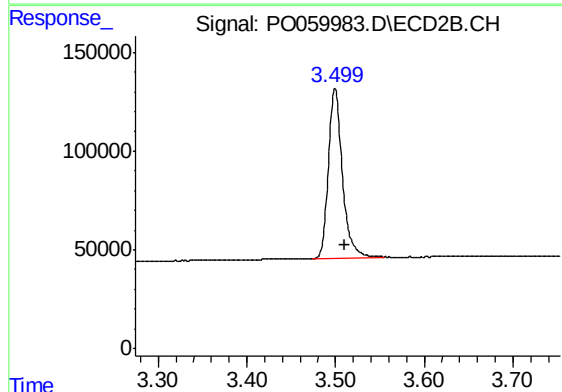


#1 Tetrachloro-m-xylene

R.T.: 3.499 min
Delta R.T.: -0.011 min
Response: 941413
Conc: 26.15 ng/ml m

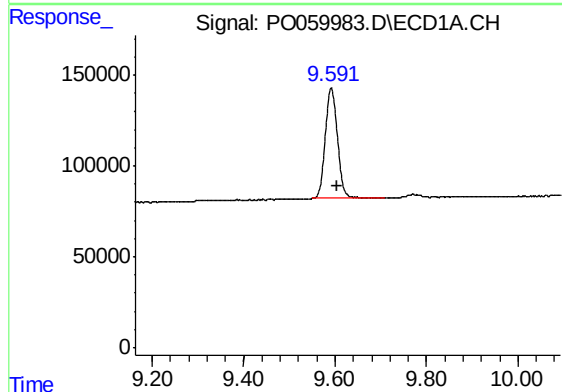

#2 Decachlorobiphenyl

R.T.: 9.592 min
Delta R.T.: -0.011 min
Response: 1118956
Conc: 21.03 ng/ml

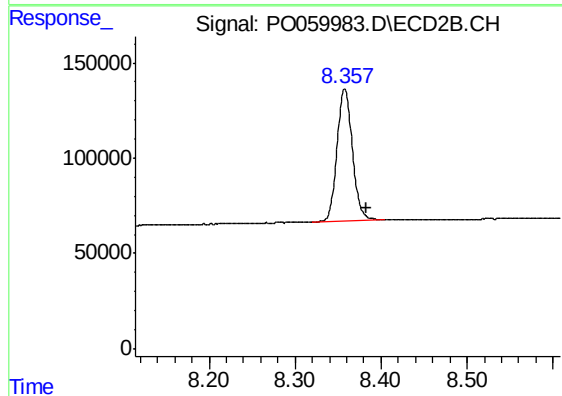

#2 Decachlorobiphenyl

R.T.: 8.358 min
Delta R.T.: -0.026 min
Response: 857068
Conc: 21.26 ng/ml