

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082819\
 Data File : P0059986.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Aug 2019 21:18
 Operator : SM/AJ
 Sample : K4569-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-39-COMP

Manual Integrations
 APPROVED

Ankita
 8/29/2019 2:02:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 04:10:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.123	3.498	952412	882255	27.202m	24.510m
2)	SA Decachlor...	9.591	8.357	1045002	805016	19.643	19.965

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082819\
Data File : PO059986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Aug 2019 21:18
Operator : SM/AJ
Sample : K4569-02
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-39-COMP


Manual Integrations
APPROVED

Ankita
8/29/2019 2:02:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 04:10:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

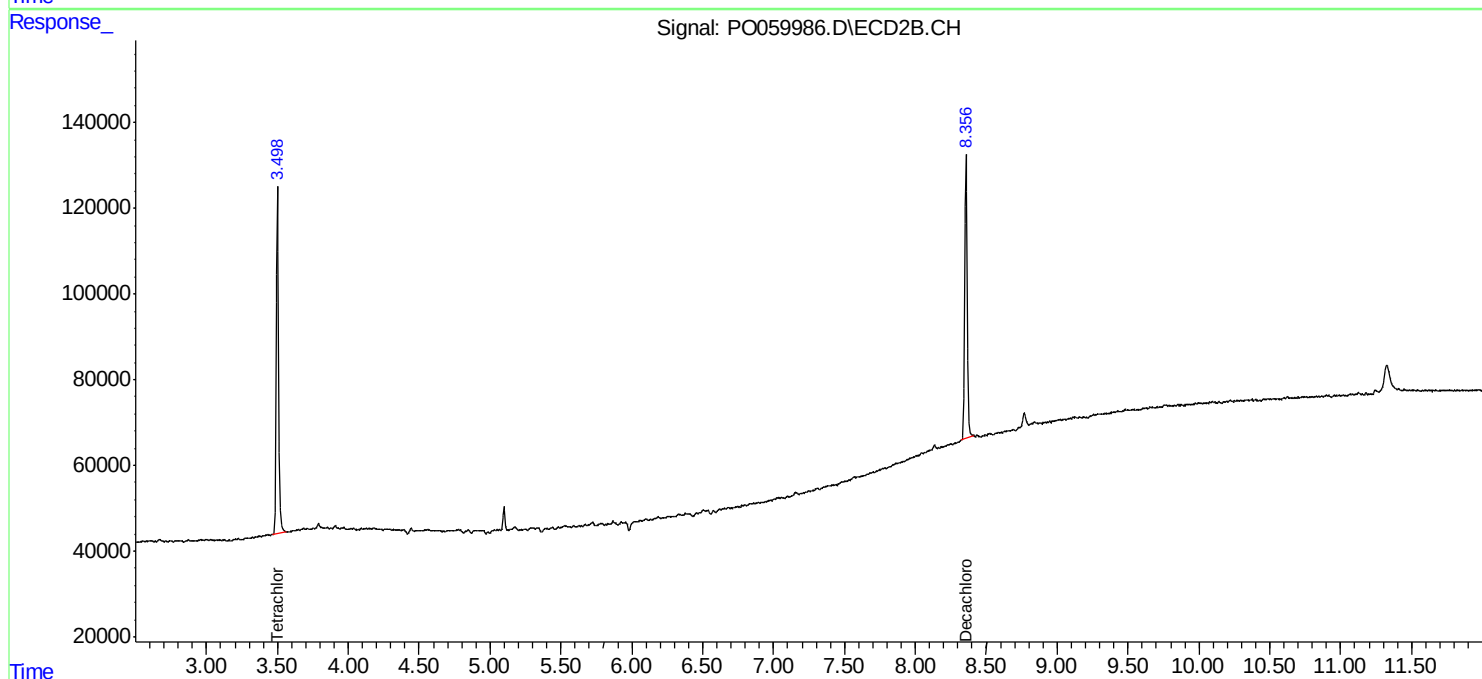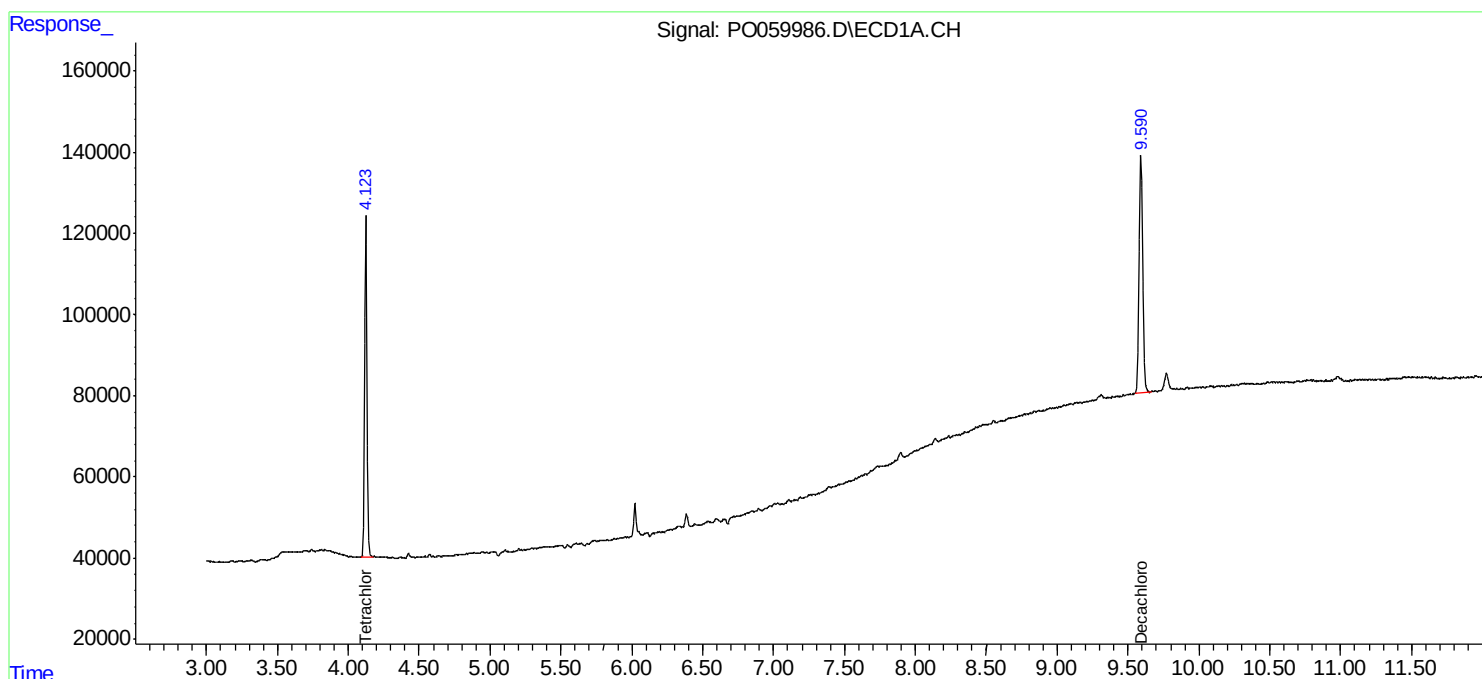

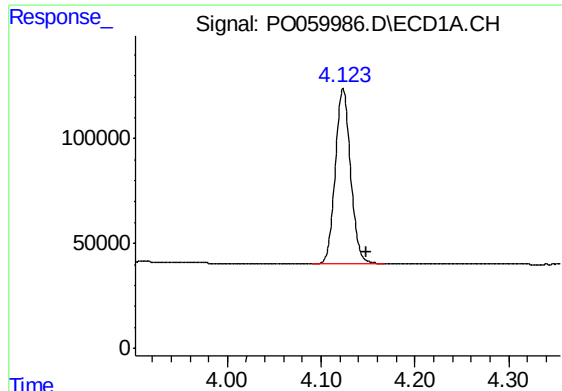


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: -0.026 min
Response: 952412
Conc: 27.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-39-COMP


Manual Integrations
APPROVED

Ankita
8/29/2019 2:02:41 PM

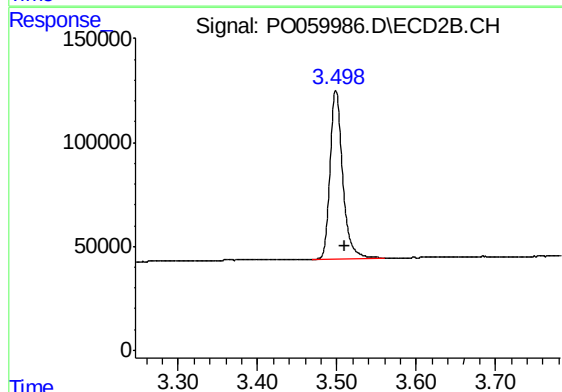


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.012 min
Response: 882255
Conc: 24.51 ng/ml m

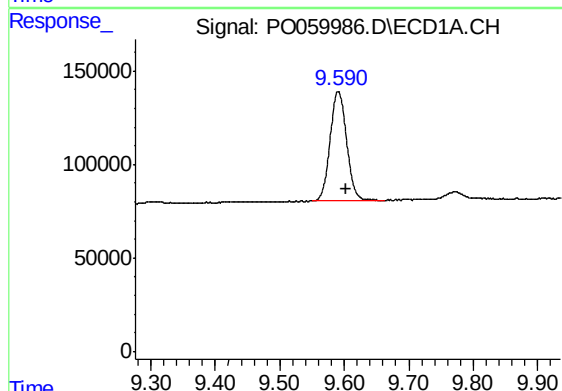

#2 Decachlorobiphenyl

R.T.: 9.591 min
Delta R.T.: -0.012 min
Response: 1045002
Conc: 19.64 ng/ml

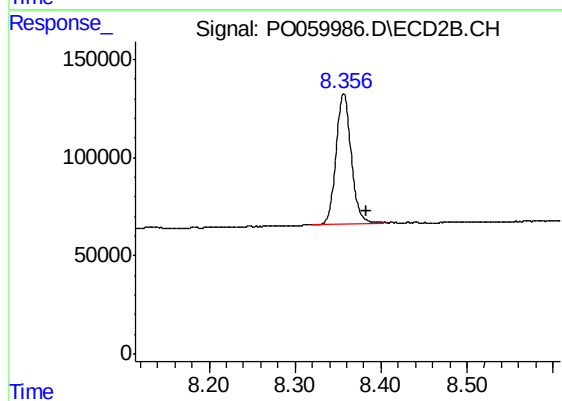

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.027 min
Response: 805016
Conc: 19.97 ng/ml