

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0082918\
Data File : P0048607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Aug 2018 12:10
Operator : SM/SJ
Sample : J4671-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TL-SPEEDY-DRY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 01:01:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.624	4666957	5065635	24.637	18.711
2) SA Decachlor...	10.064	8.601	3053874	2458556	17.734m	14.680

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082918\
Data File : P0048607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Aug 2018 12:10
Operator : SM/SJ
Sample : J4671-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TL-SPEEDY-DRY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 01:01:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

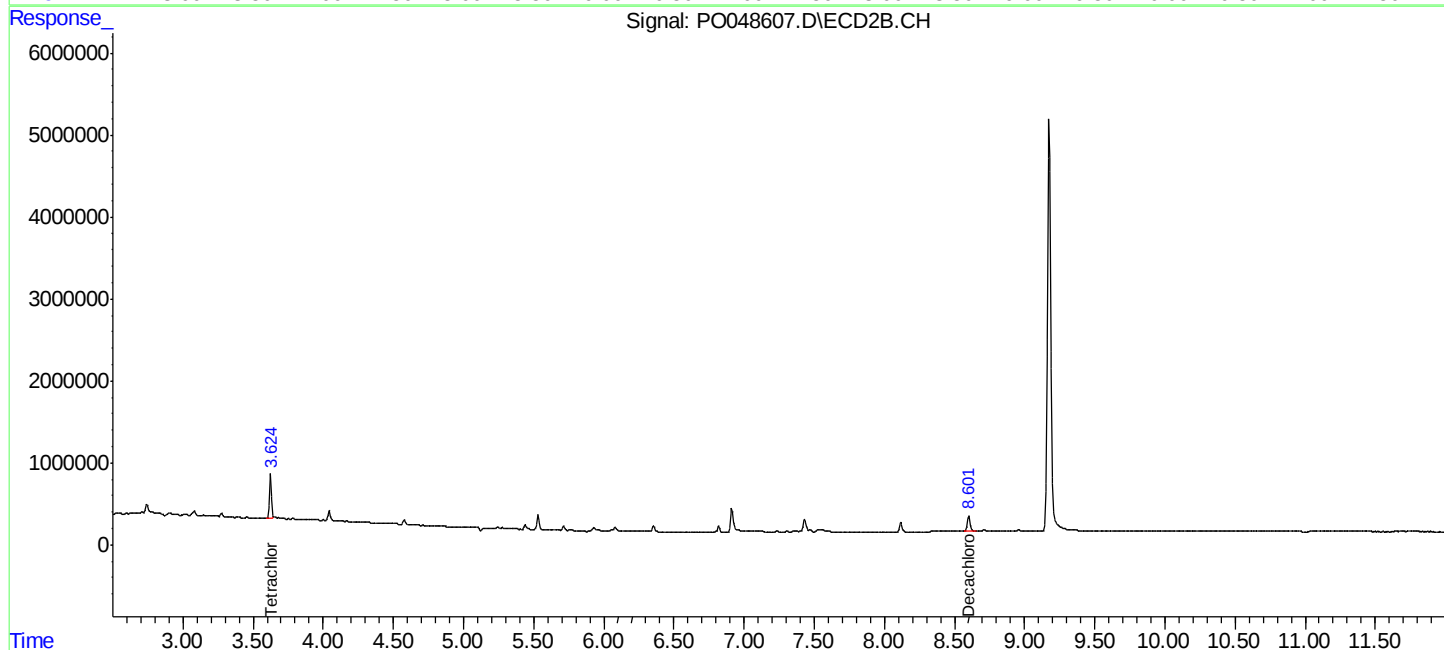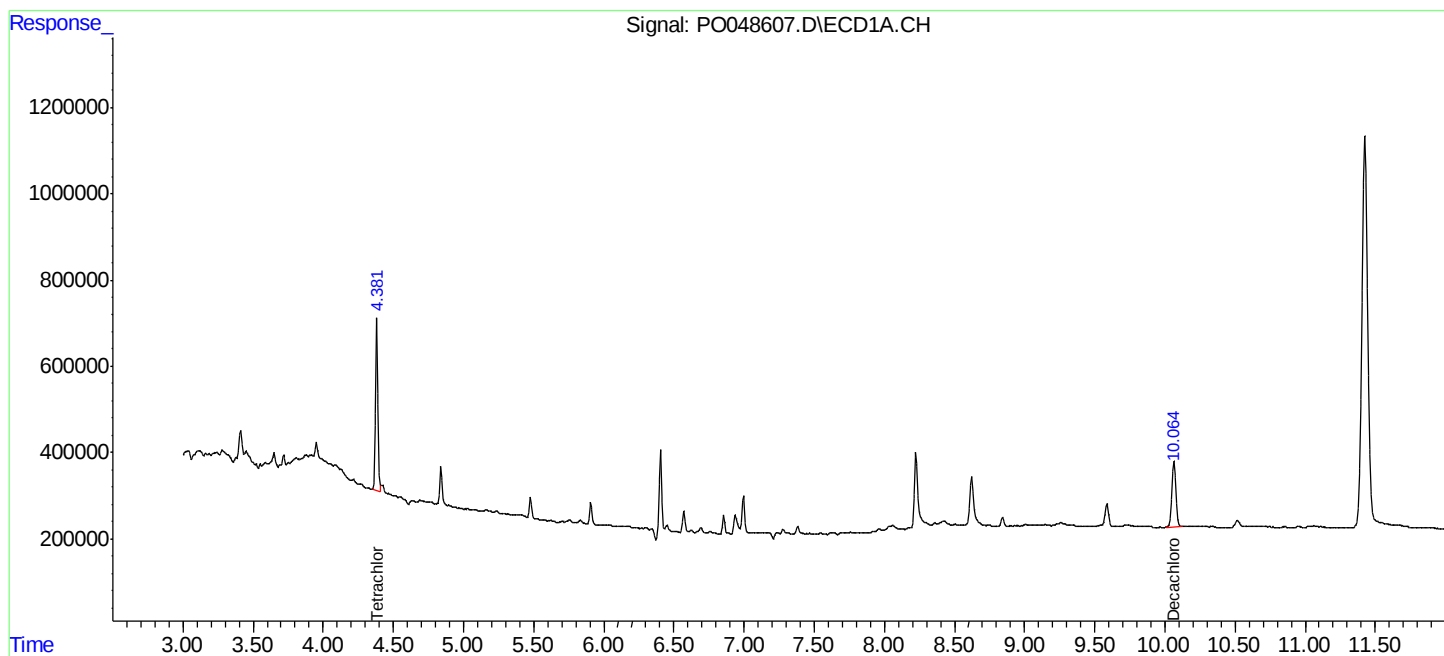


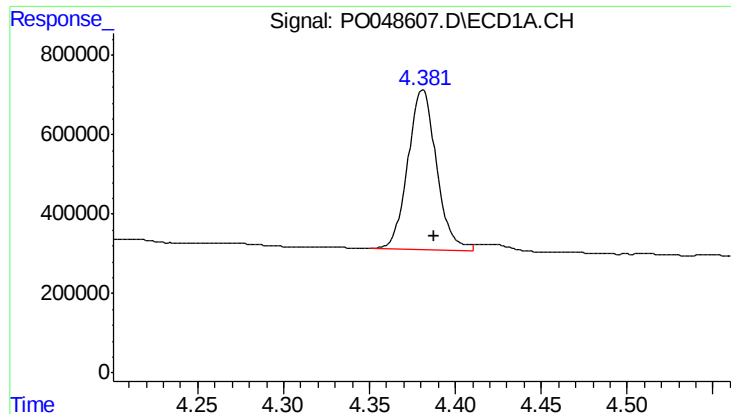

#1 Tetrachloro-m-xylene


R.T.: 4.381 min
Delta R.T.: -0.007 min
Response: 4666957
Conc: 24.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
TL-SPEEDY-DRY

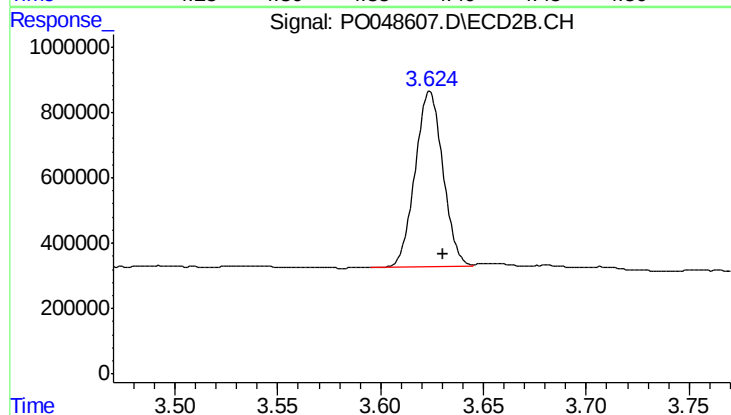


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.006 min
Response: 5065635
Conc: 18.71 ng/ml

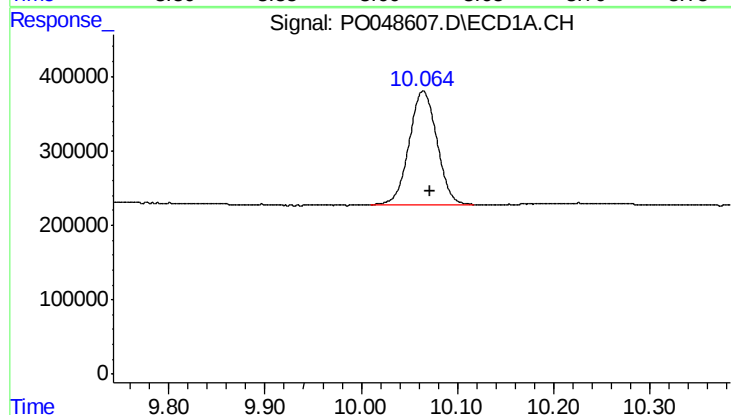

#2 Decachlorobiphenyl

R.T.: 10.064 min
Delta R.T.: -0.008 min
Response: 3053874
Conc: 17.73 ng/ml m

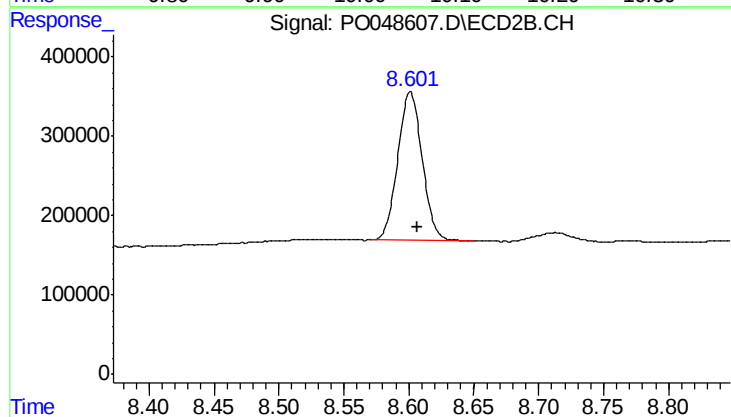

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: -0.005 min
Response: 2458556
Conc: 14.68 ng/ml