

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082919\
 Data File : P0060008.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Aug 2019 12:26
 Operator : SM/AJ
 Sample : K4546-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 T3-S-A

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:48:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 01:26:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.127	3.500	891328	830750	25.457	23.079
2)	SA Decachlor...	9.591	8.358	905871	688444	17.028	17.074
Target Compounds							
31)	L7 AR-1260-1	6.851	5.996	203232	140978	75.388	61.862
32)	L7 AR-1260-2	7.106	6.183	239681	156406	64.596	53.383
33)	L7 AR-1260-3	7.459	6.331	160010	141431	48.838	53.387
34)	L7 AR-1260-4	7.683	6.794	161081	83127	52.447m	36.740 #
35)	L7 AR-1260-5	7.992	7.037	248959	229024	35.159m	41.616

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082919\
Data File : PO060008.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Aug 2019 12:26
Operator : SM/AJ
Sample : K4546-12
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:48:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 01:26:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

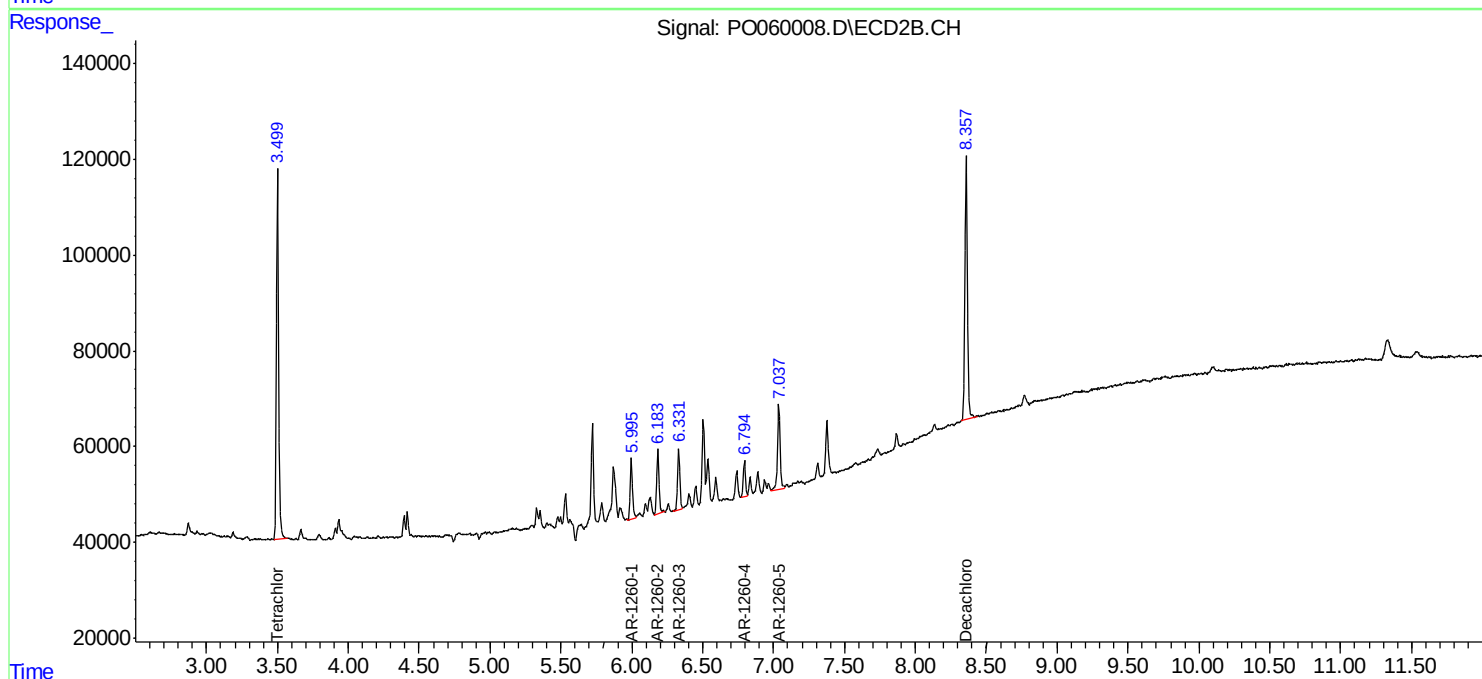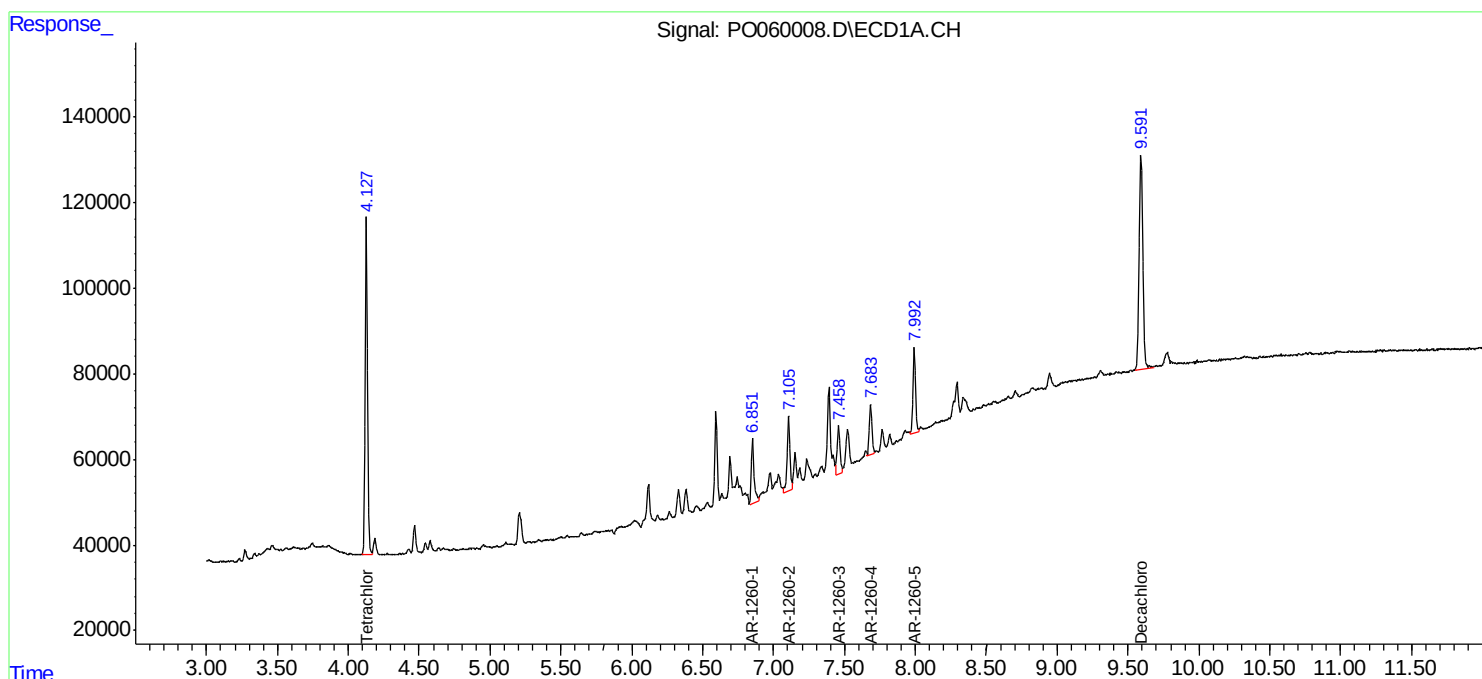

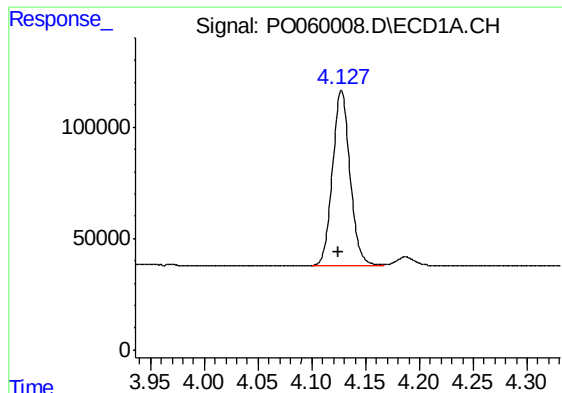


#1 Tetrachloro-m-xylene

R.T.: 4.127 min
Delta R.T.: 0.003 min
Response: 891328
Conc: 25.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:48:29 PM

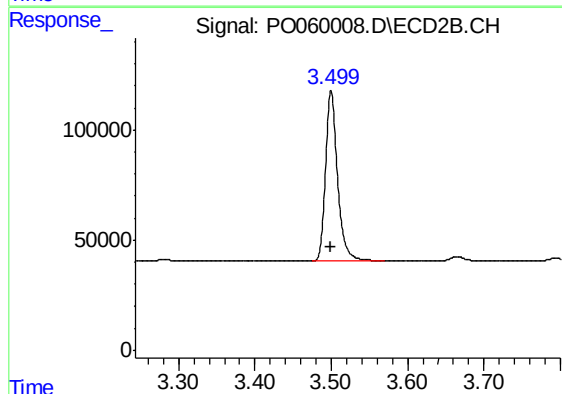


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 830750
Conc: 23.08 ng/ml

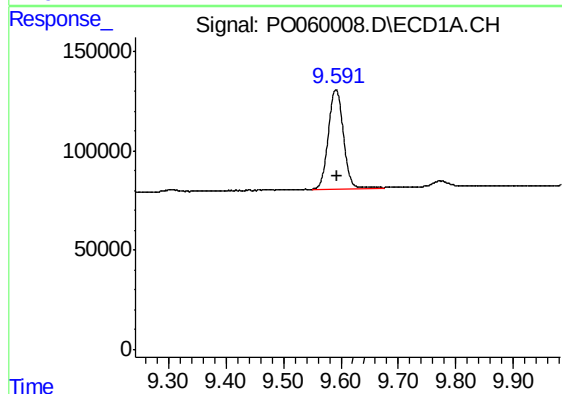


#2 Decachlorobiphenyl

R.T.: 9.591 min
Delta R.T.: -0.002 min
Response: 905871
Conc: 17.03 ng/ml

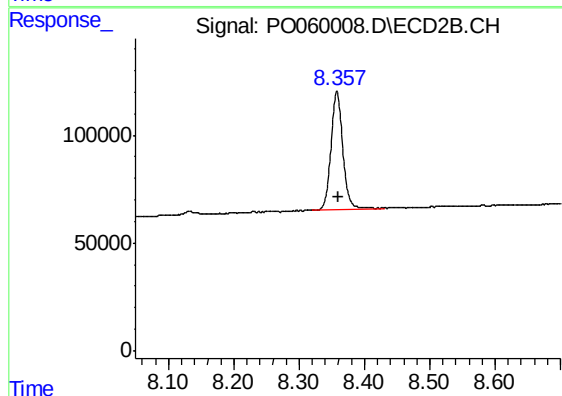

#2 Decachlorobiphenyl

R.T.: 8.358 min
Delta R.T.: -0.001 min
Response: 688444
Conc: 17.07 ng/ml

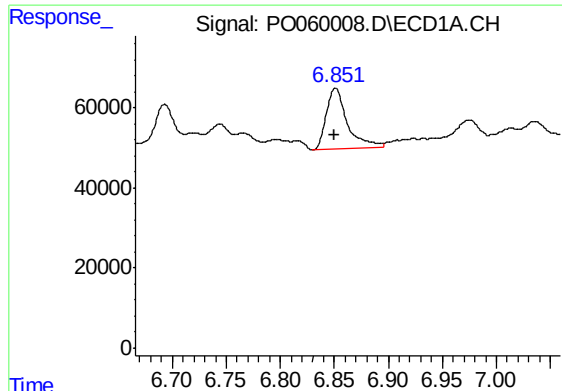


#31 AR-1260-1

R.T.: 6.851 min
Delta R.T.: 0.001 min
Response: 203232
Conc: 75.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:48:29 PM

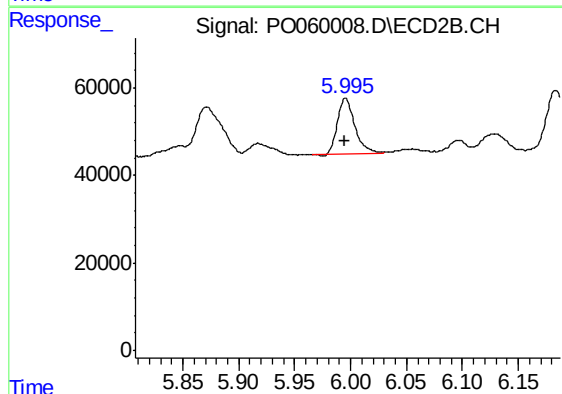


#31 AR-1260-1

R.T.: 5.996 min
Delta R.T.: 0.000 min
Response: 140978
Conc: 61.86 ng/ml

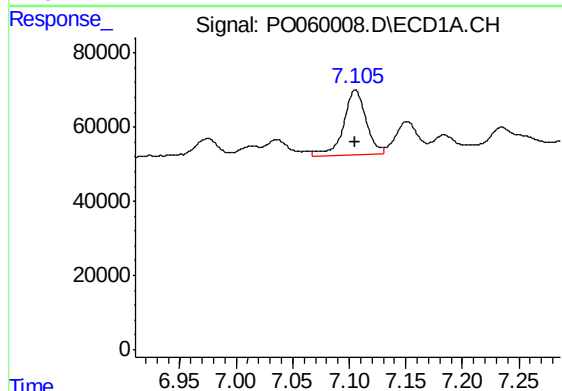


#32 AR-1260-2

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 239681
Conc: 64.60 ng/ml

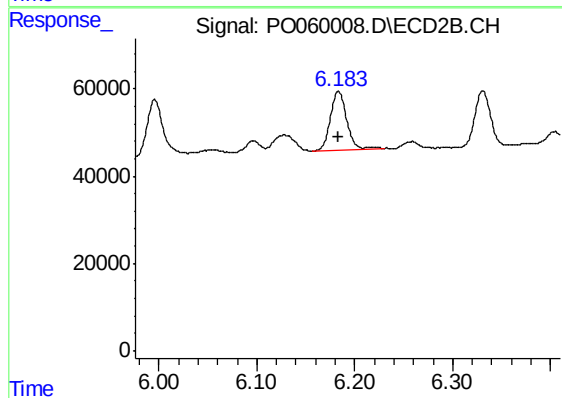

#32 AR-1260-2

R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 156406
Conc: 53.38 ng/ml

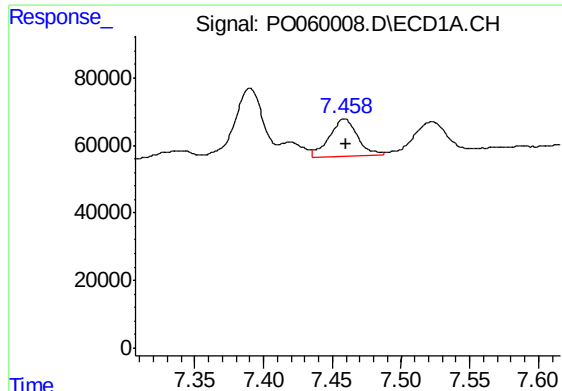


#33 AR-1260-3

R.T.: 7.459 min
Delta R.T.: 0.000 min
Response: 160010
Conc: 48.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:48:29 PM

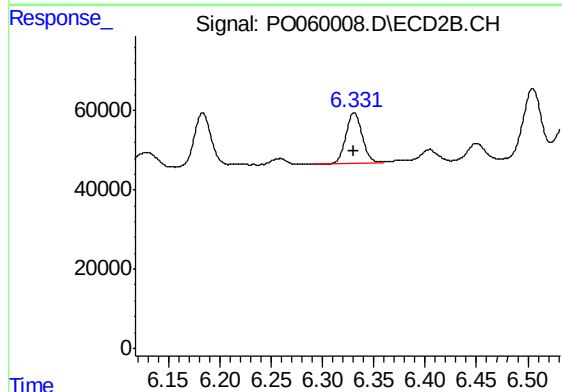


#33 AR-1260-3

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 141431
Conc: 53.39 ng/ml

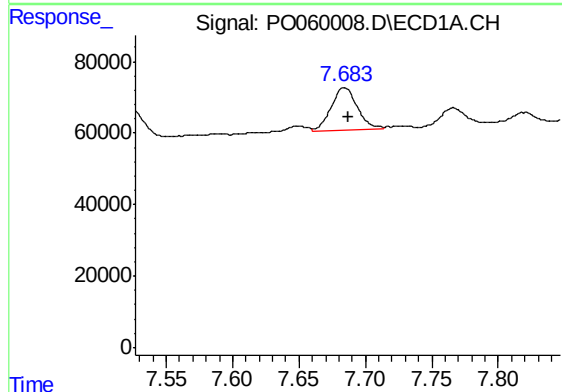


#34 AR-1260-4

R.T.: 7.683 min
Delta R.T.: -0.004 min
Response: 161081
Conc: 52.45 ng/ml m

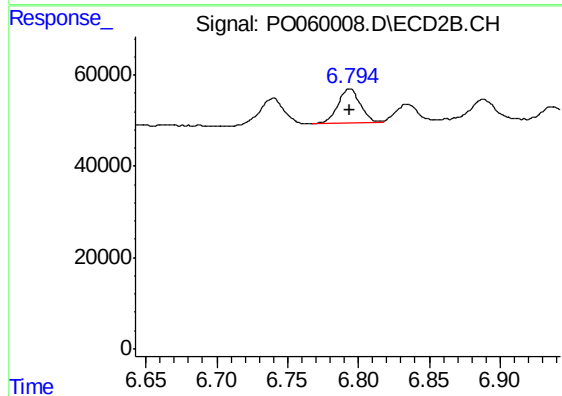

#34 AR-1260-4

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 83127
Conc: 36.74 ng/ml

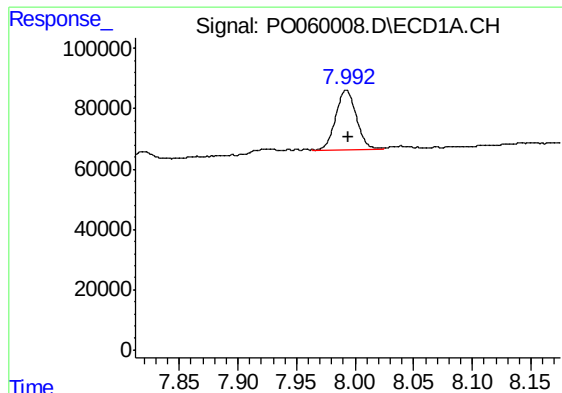


#35 AR-1260-5

R.T.: 7.992 min
Delta R.T.: -0.002 min
Response: 248959
Conc: 35.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
T3-S-A

Manual Integrations
APPROVED

Ankita
8/30/2019 5:48:29 PM

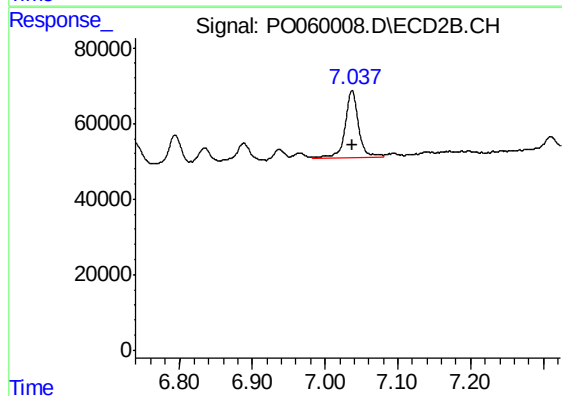

#35 AR-1260-5

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 229024
Conc: 41.62 ng/ml