

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082919\
Data File : P0060041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Aug 2019 22:19
Operator : SM/AJ
Sample : K4439-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S-4A-(1-3)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:23:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.122	3.500	1017441	860144	29.059	23.896
2)	SA Decachlor...	9.583	8.355	795519	581580	14.953	14.424

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082919\
Data File : PO060041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Aug 2019 22:19
Operator : SM/AJ
Sample : K4439-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S-4A-(1-3)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:23:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

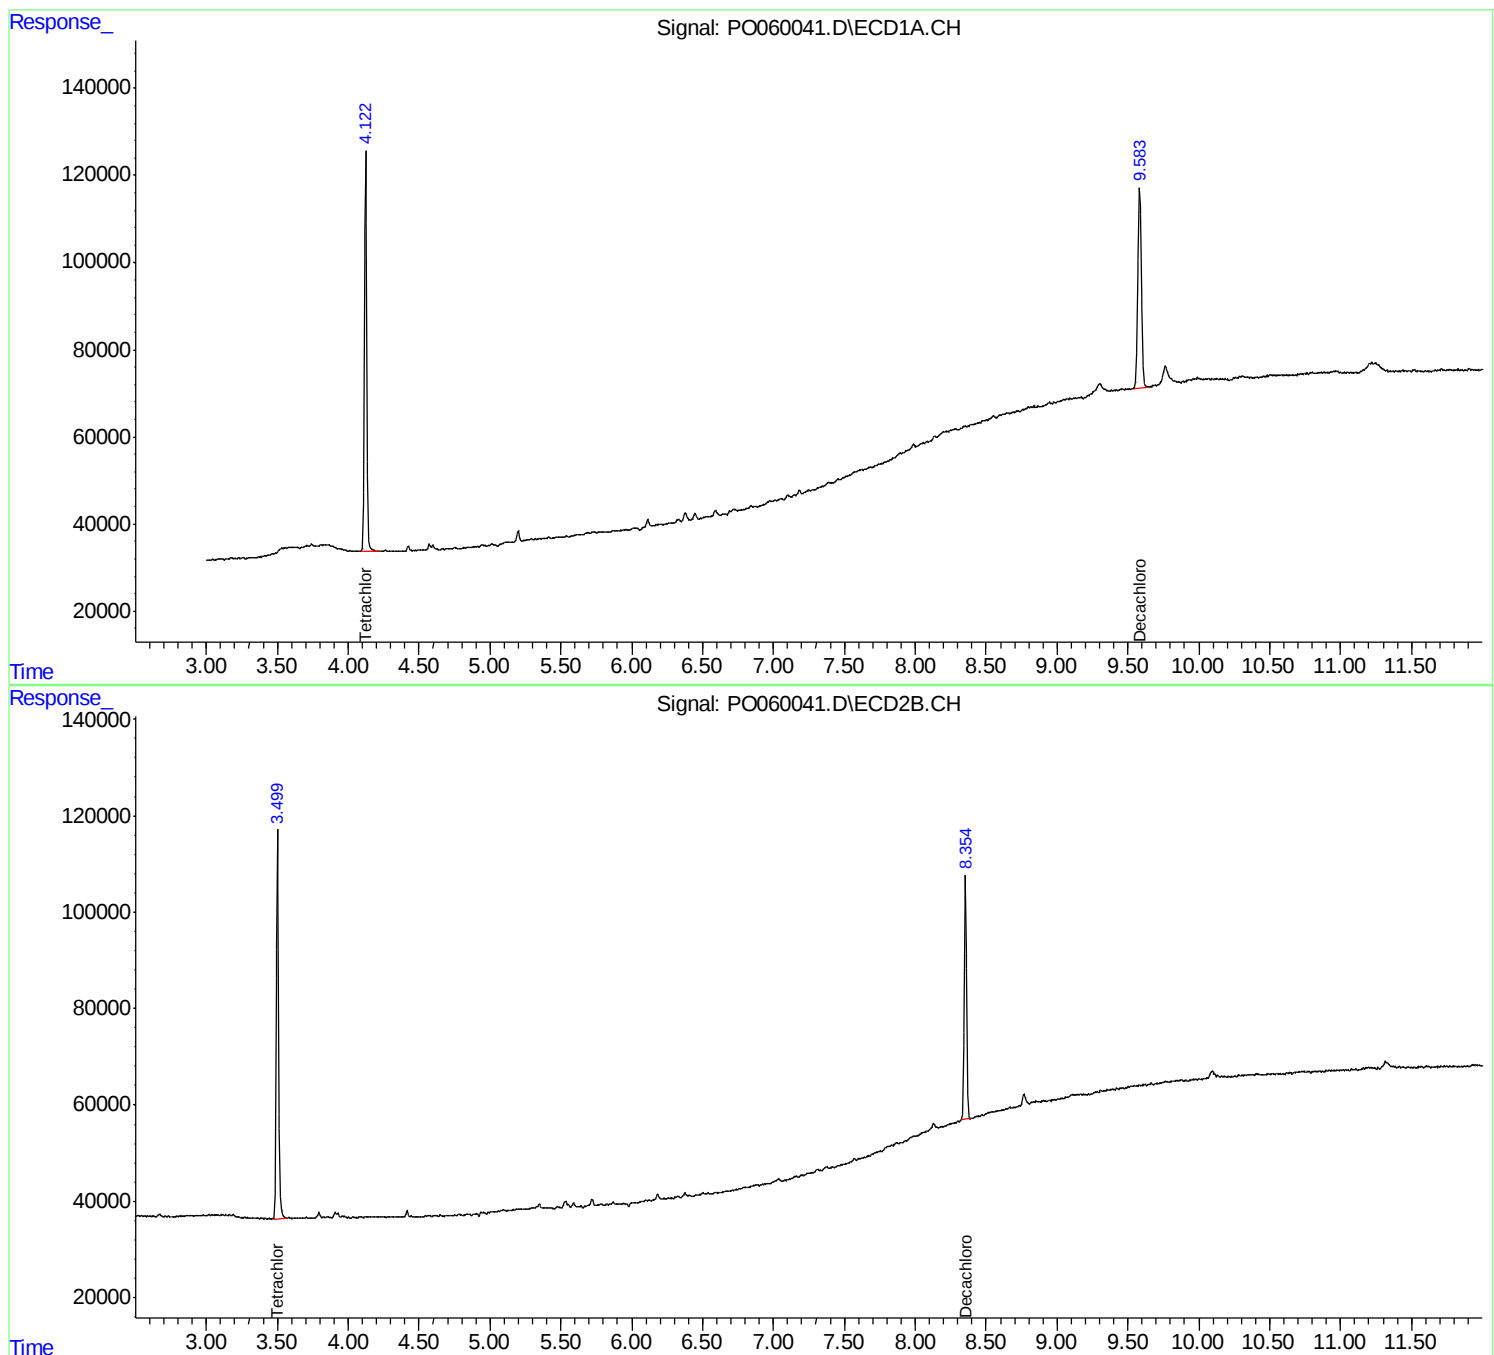


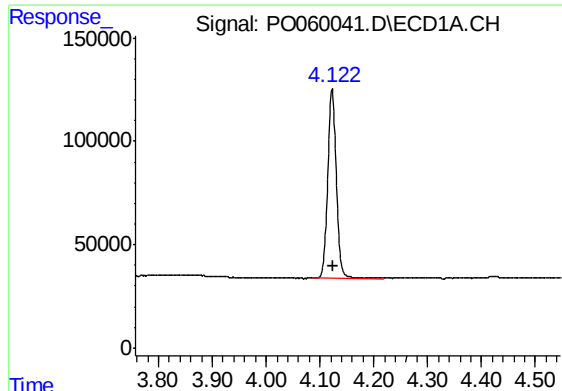

#1 Tetrachloro-m-xylene


R.T.: 4.122 min
Delta R.T.: -0.002 min
Response: 1017441
Conc: 29.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-4A-(1-3)

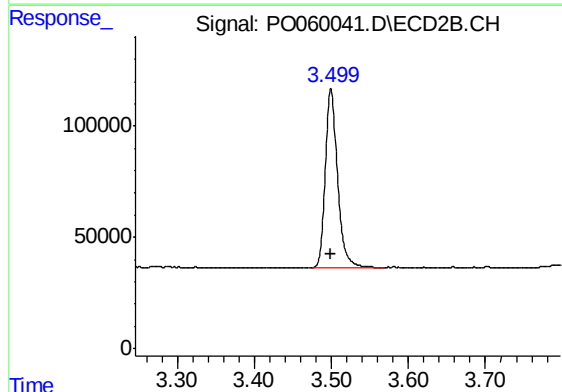


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 860144
Conc: 23.90 ng/ml

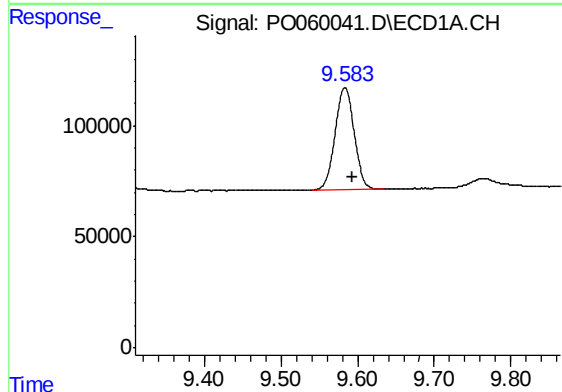

#2 Decachlorobiphenyl

R.T.: 9.583 min
Delta R.T.: -0.010 min
Response: 795519
Conc: 14.95 ng/ml

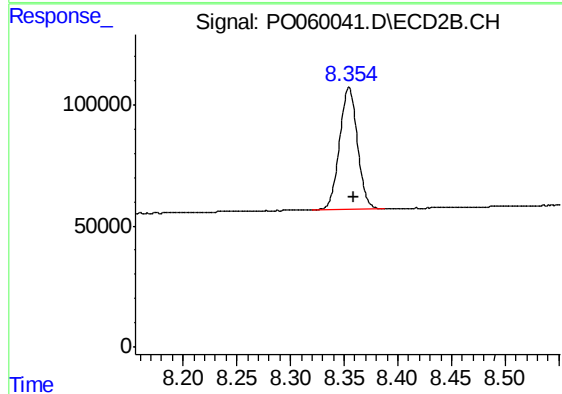

#2 Decachlorobiphenyl

R.T.: 8.355 min
Delta R.T.: -0.005 min
Response: 581580
Conc: 14.42 ng/ml