

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082919\
 Data File : P0060043.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Aug 2019 22:51
 Operator : SM/AJ
 Sample : K4439-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-5-(1-3)

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:49:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 03:26:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.121	3.499	1093482	926865	31.231	25.749
2)	SA Decachlor...	9.581	8.353	861107	629545	16.186	15.613
Target Compounds							
26)	L6 AR-1254-1	6.110	5.327	148460	143017	71.156m	60.299
27)	L6 AR-1254-2	6.325	5.472	188154	75839	56.397	36.143 #
28)	L6 AR-1254-3	6.685	5.866	124092	94482	34.971	28.099
29)	L6 AR-1254-4	6.967	6.093	95856	44100	32.543	21.389m#
30)	L6 AR-1254-5	7.382	6.500	141502	87635	45.758	28.224 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082919\
Data File : PO060043.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Aug 2019 22:51
Operator : SM/AJ
Sample : K4439-07
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S-5-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:49:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:26:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

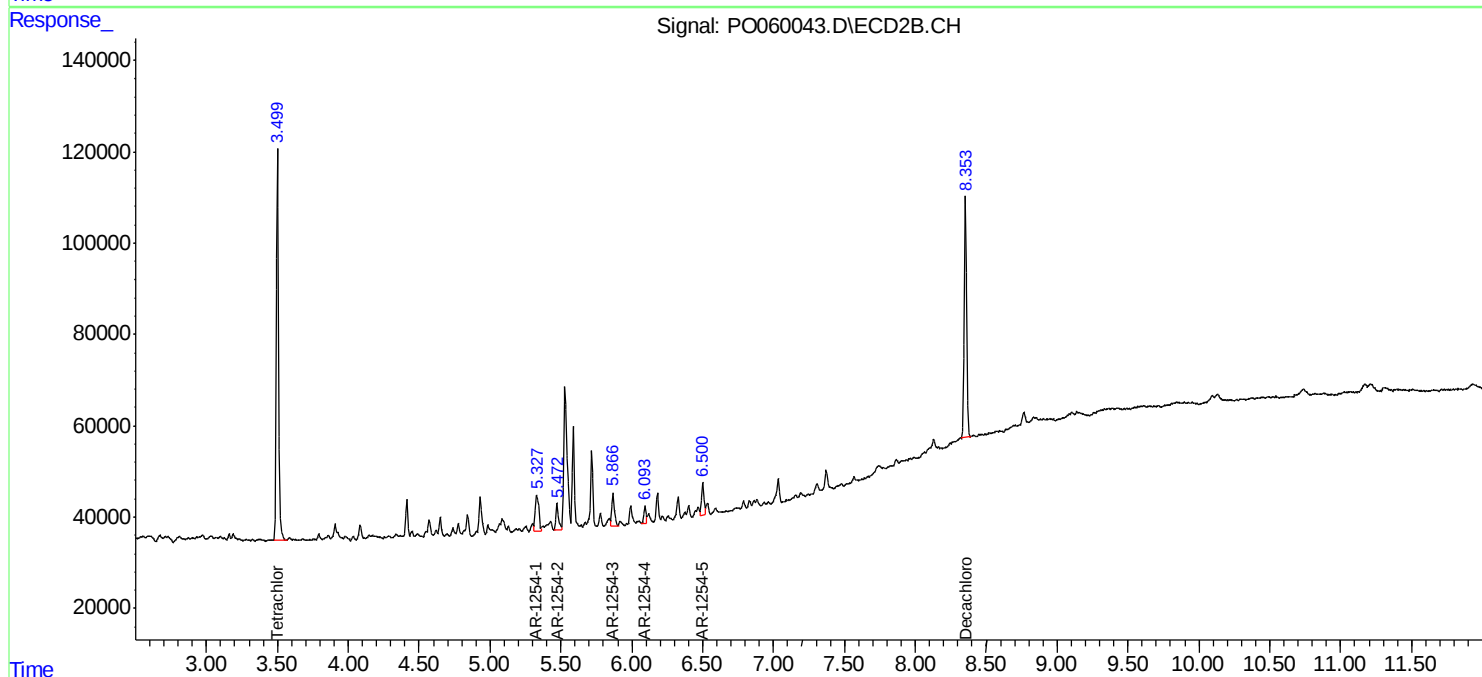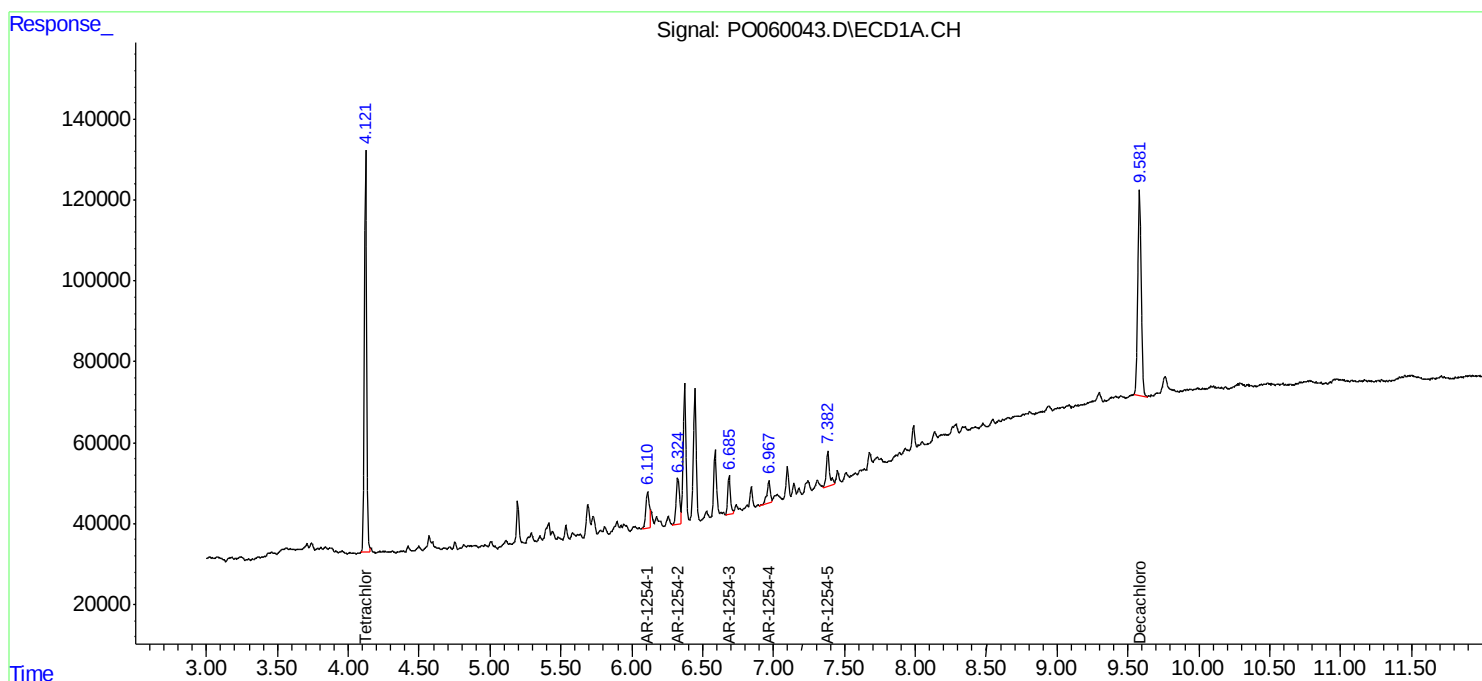

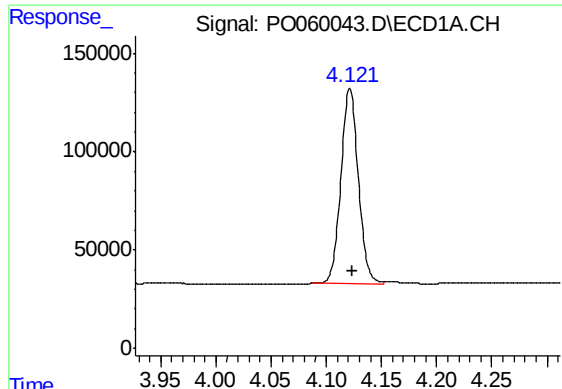


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: -0.003 min
Response: 1093482
Conc: 31.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-5-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:49:48 PM

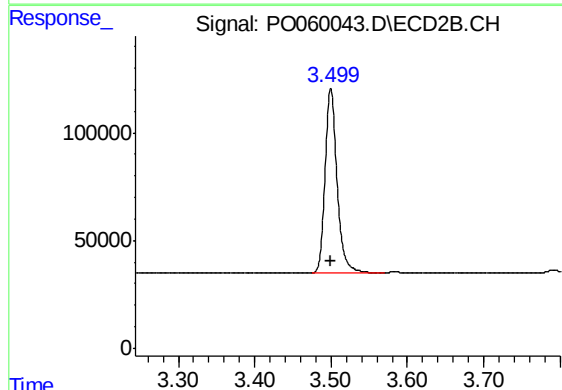


#1 Tetrachloro-m-xylene

R.T.: 3.499 min
Delta R.T.: 0.000 min
Response: 926865
Conc: 25.75 ng/ml

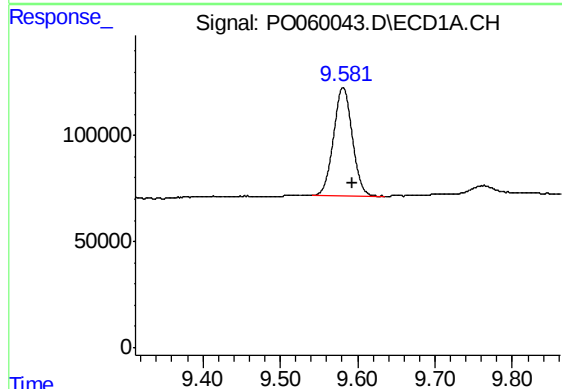


#2 Decachlorobiphenyl

R.T.: 9.581 min
Delta R.T.: -0.012 min
Response: 861107
Conc: 16.19 ng/ml

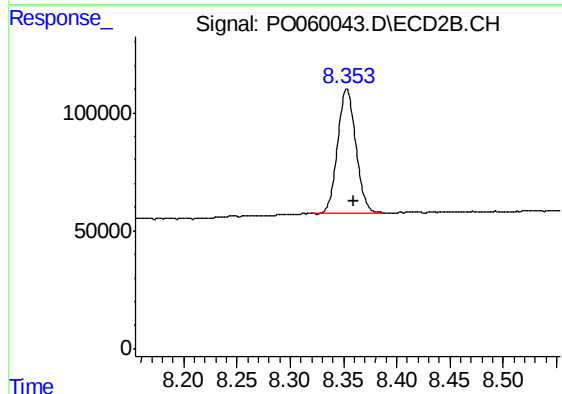

#2 Decachlorobiphenyl

R.T.: 8.353 min
Delta R.T.: -0.006 min
Response: 629545
Conc: 15.61 ng/ml

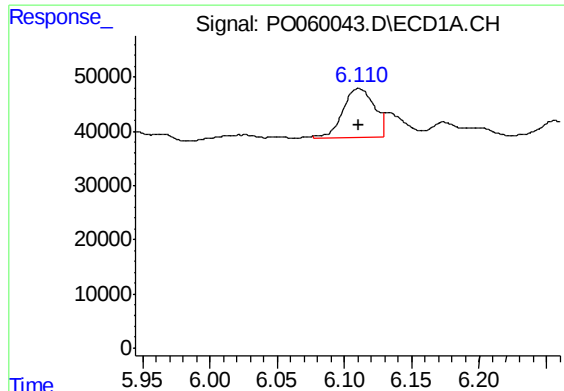


#26 AR-1254-1

R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 148460
Conc: 71.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S-5-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:49:48 PM

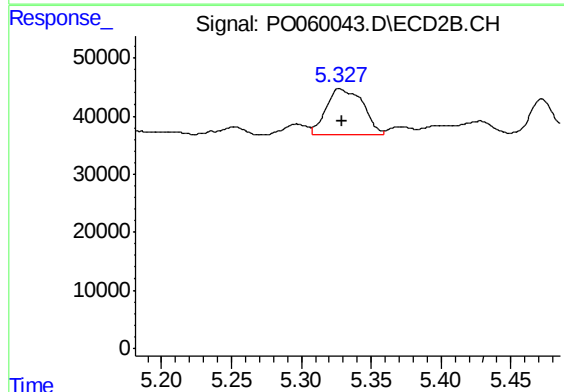


#26 AR-1254-1

R.T.: 5.327 min
Delta R.T.: -0.002 min
Response: 143017
Conc: 60.30 ng/ml

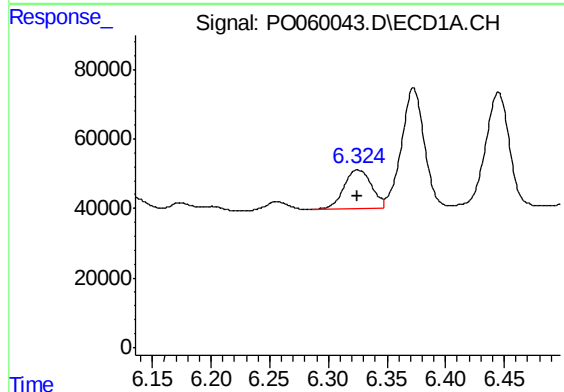


#27 AR-1254-2

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 188154
Conc: 56.40 ng/ml

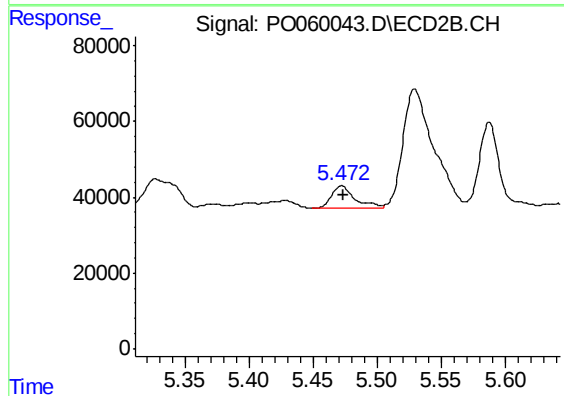

#27 AR-1254-2

R.T.: 5.472 min
Delta R.T.: -0.002 min
Response: 75839
Conc: 36.14 ng/ml

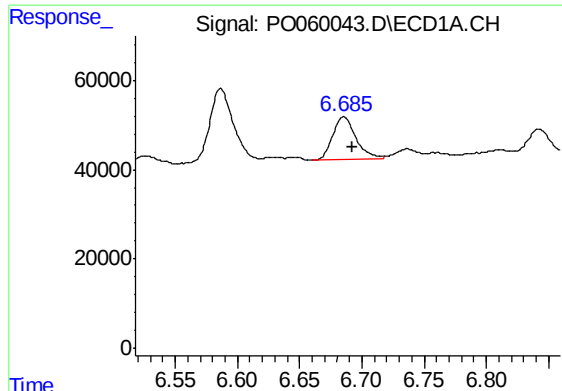


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.007 min
Response: 124092
Conc: 34.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-5-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:49:48 PM

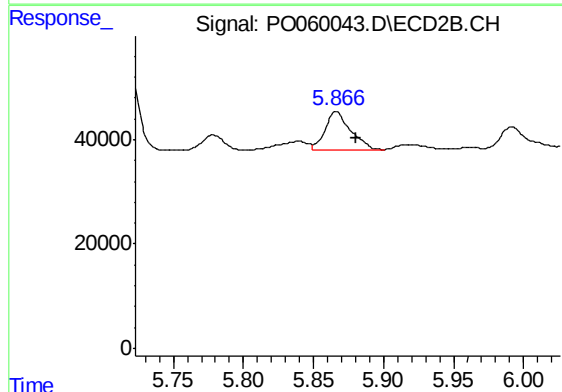


#28 AR-1254-3

R.T.: 5.866 min
Delta R.T.: -0.015 min
Response: 94482
Conc: 28.10 ng/ml

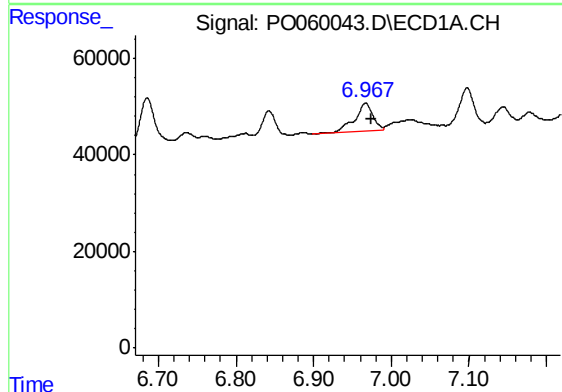


#29 AR-1254-4

R.T.: 6.967 min
Delta R.T.: -0.007 min
Response: 95856
Conc: 32.54 ng/ml

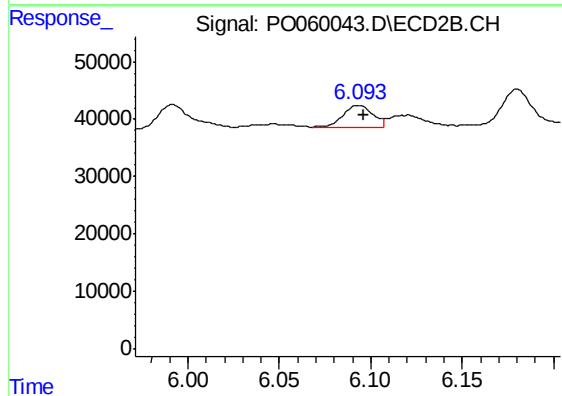

#29 AR-1254-4

R.T.: 6.093 min
Delta R.T.: -0.004 min
Response: 44100
Conc: 21.39 ng/ml m

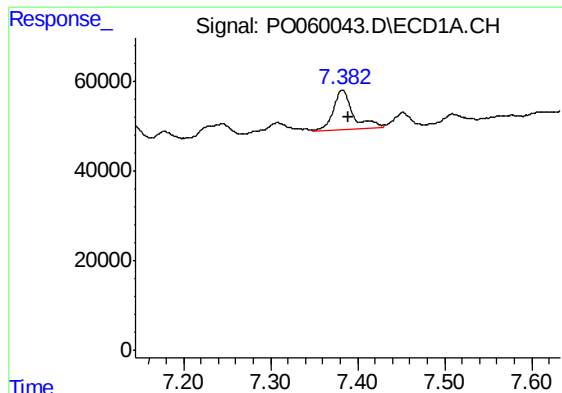


#30 AR-1254-5

R.T.: 7.382 min
Delta R.T.: -0.008 min
Response: 141502
Conc: 45.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-5-(1-3)

Manual Integrations
APPROVED

Ankita
8/30/2019 5:49:48 PM

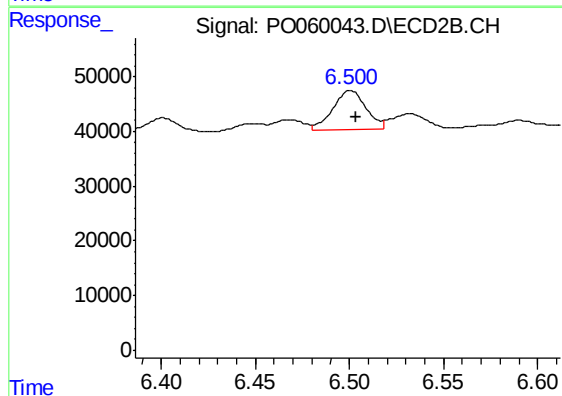

#30 AR-1254-5

R.T.: 6.500 min
Delta R.T.: -0.003 min
Response: 87635
Conc: 28.22 ng/ml