

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082919\
 Data File : P0060063.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 5:02
 Operator : SM/AJ
 Sample : K4568-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-15-COMP

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:50:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 07:06:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.121	3.498	1028335	912482	29.370	25.350
2)	SA Decachlor...	9.580	8.352	1036753	810339	19.488	20.097
Target Compounds							
31)	L7 AR-1260-1	6.840	5.997	73087	83409	27.111m	36.600 #
32)	L7 AR-1260-2	7.099	6.181	100865	55508	27.184m	18.946m#
33)	L7 AR-1260-3	7.451	6.326	62059	45333	18.942m	17.112
34)	L7 AR-1260-4	7.679	6.788	75453	33682	24.567m	14.886 #
35)	L7 AR-1260-5	7.985	7.032	93901	134828	13.261m	24.499 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082919\
Data File : PO060063.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 5:02
Operator : SM/AJ
Sample : K4568-04
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-15-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 07:06:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

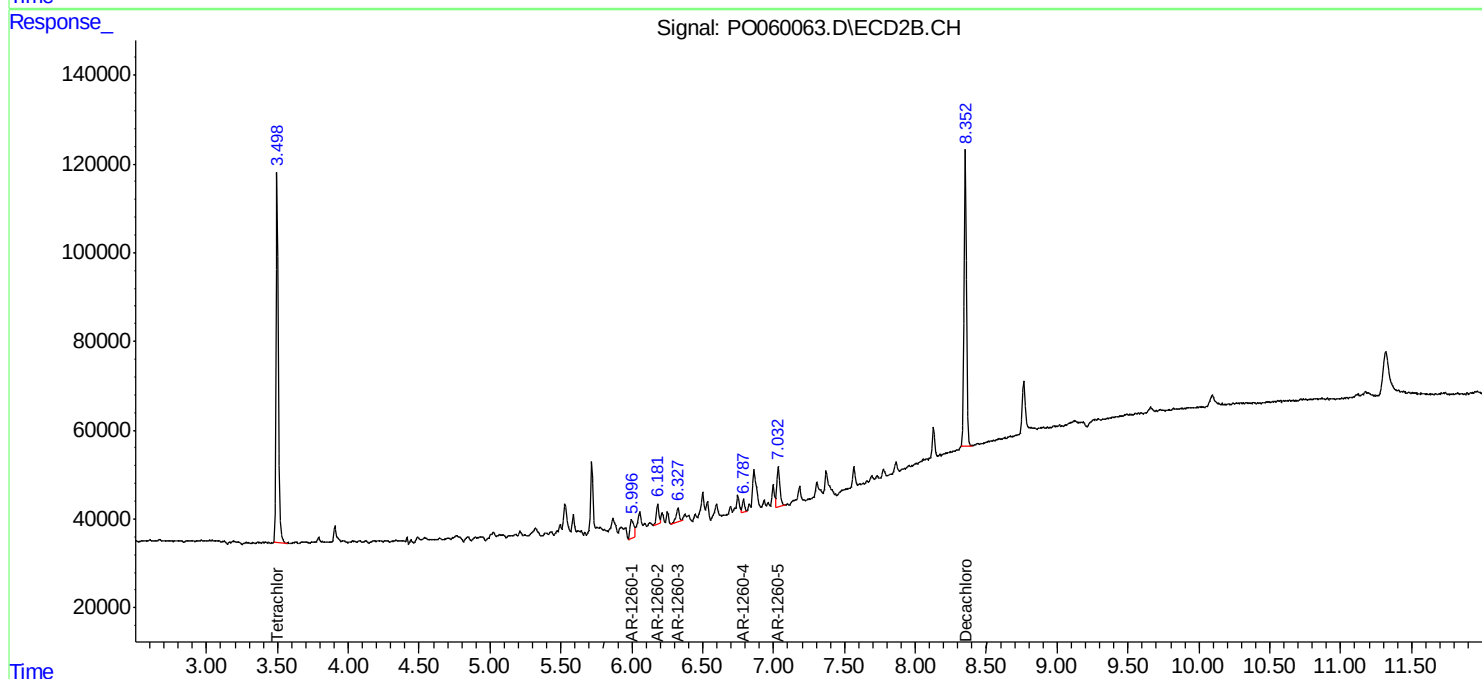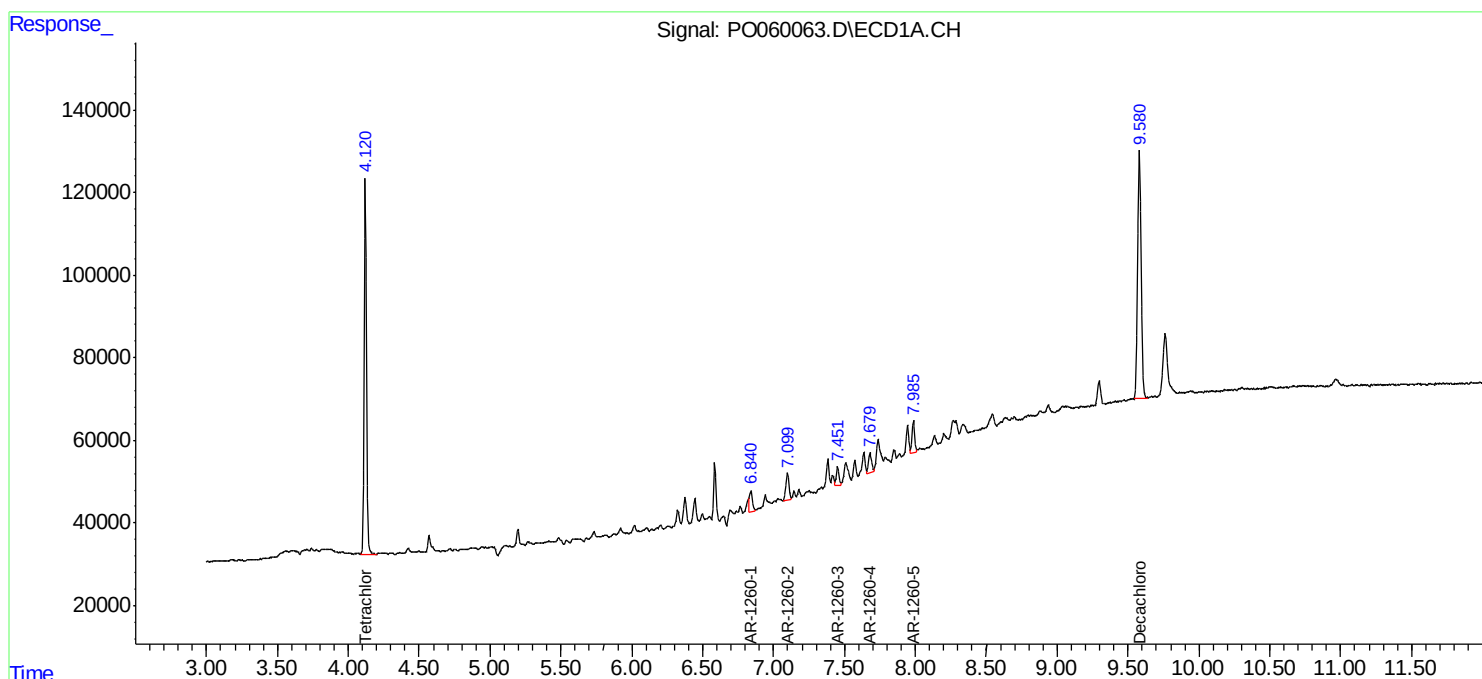

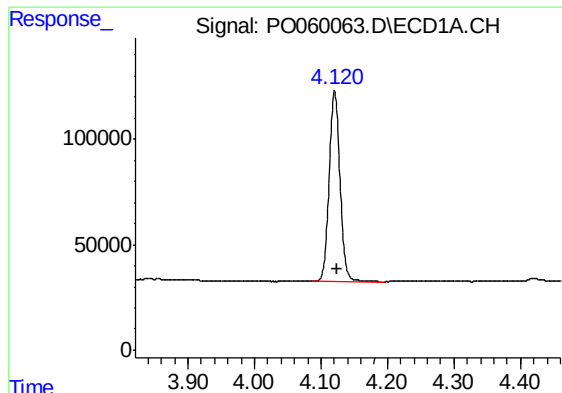


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: -0.003 min
Response: 1028335
Conc: 29.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-15-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:13 PM

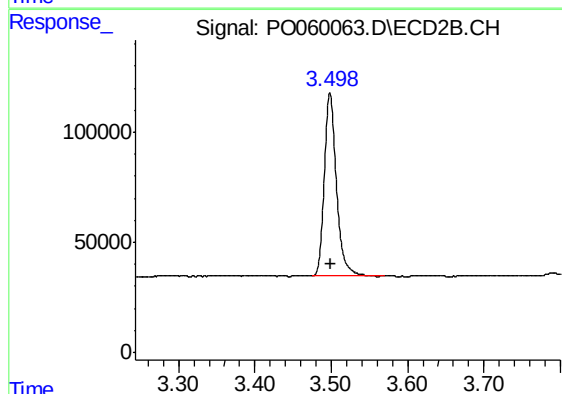


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.001 min
Response: 912482
Conc: 25.35 ng/ml

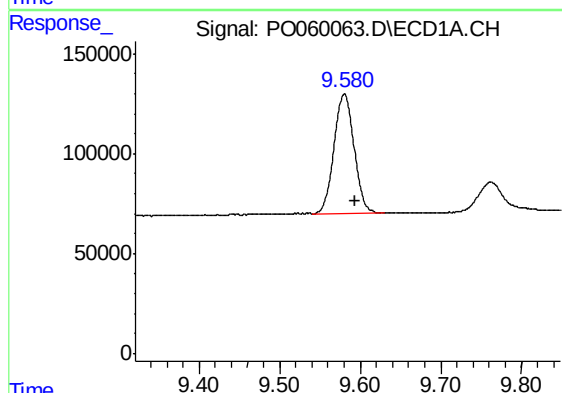


#2 Decachlorobiphenyl

R.T.: 9.580 min
Delta R.T.: -0.013 min
Response: 1036753
Conc: 19.49 ng/ml

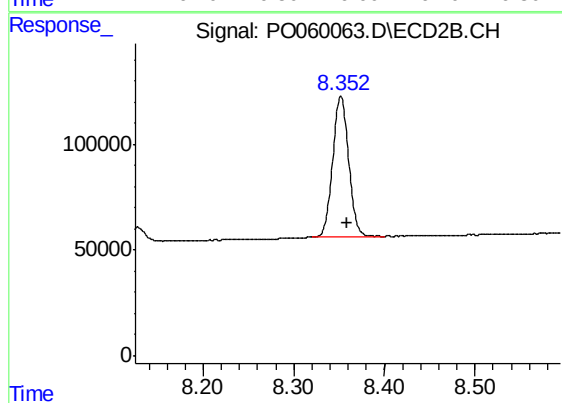

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: -0.007 min
Response: 810339
Conc: 20.10 ng/ml

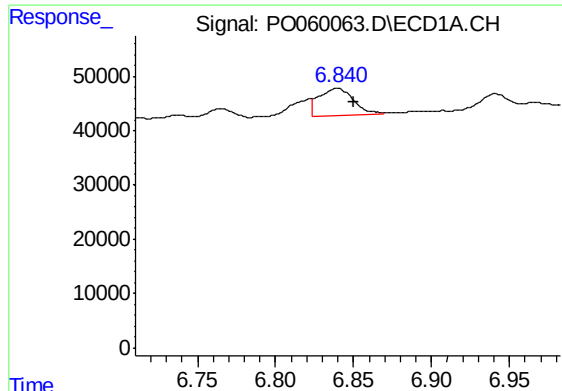


#31 AR-1260-1

R.T.: 6.840 min
Delta R.T.: -0.010 min
Response: 73087
Conc: 27.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-15-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:13 PM

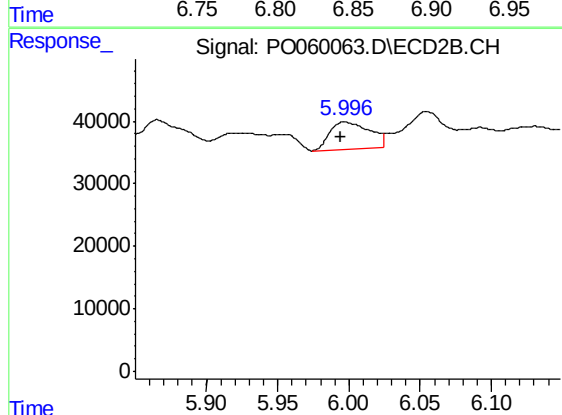


#31 AR-1260-1

R.T.: 5.997 min
Delta R.T.: 0.002 min
Response: 83409
Conc: 36.60 ng/ml

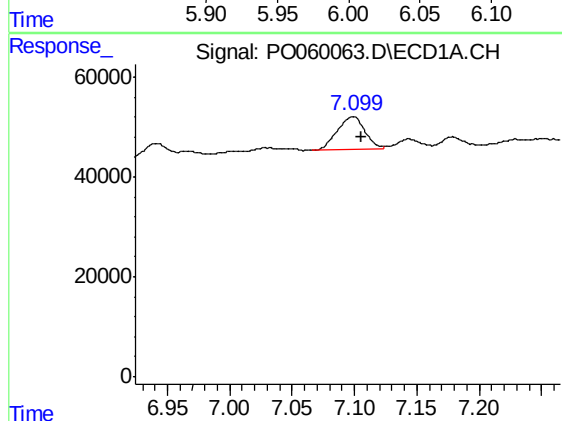


#32 AR-1260-2

R.T.: 7.099 min
Delta R.T.: -0.006 min
Response: 100865
Conc: 27.18 ng/ml m

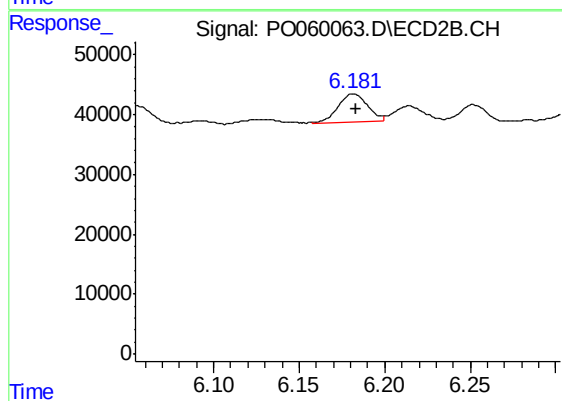

#32 AR-1260-2

R.T.: 6.181 min
Delta R.T.: -0.002 min
Response: 55508
Conc: 18.95 ng/ml m

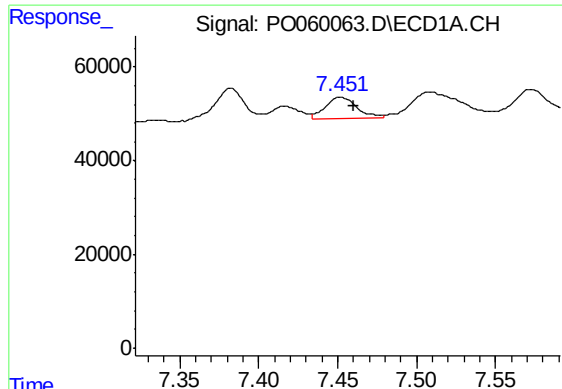


#33 AR-1260-3

R.T.: 7.451 min
Delta R.T.: -0.008 min
Response: 62059
Conc: 18.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-15-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:13 PM

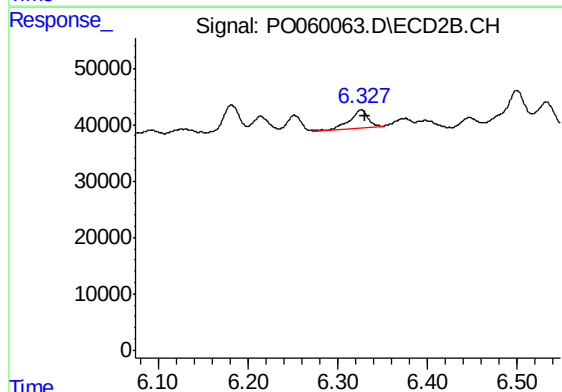


#33 AR-1260-3

R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 45333
Conc: 17.11 ng/ml

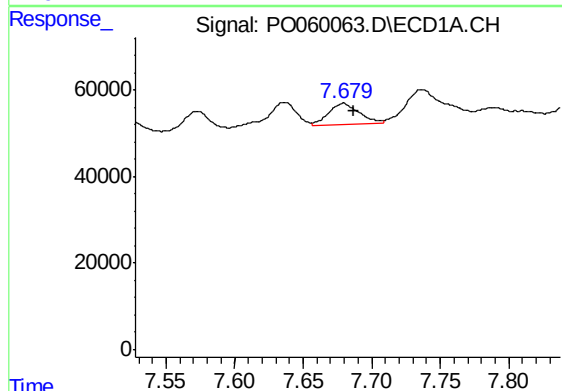


#34 AR-1260-4

R.T.: 7.679 min
Delta R.T.: -0.008 min
Response: 75453
Conc: 24.57 ng/ml m

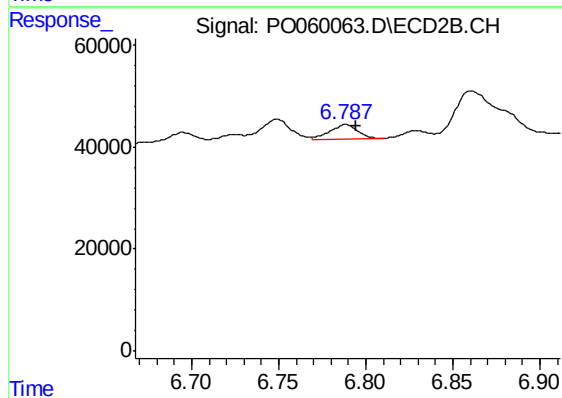

#34 AR-1260-4

R.T.: 6.788 min
Delta R.T.: -0.006 min
Response: 33682
Conc: 14.89 ng/ml

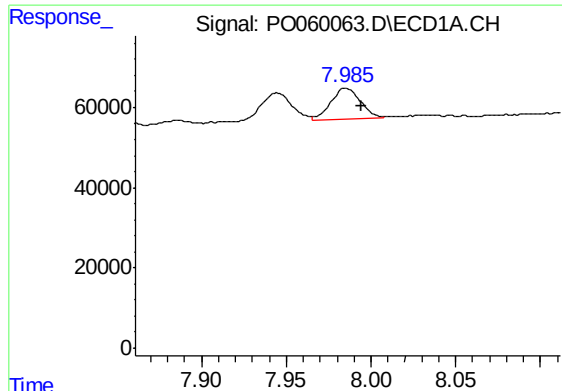


#35 AR-1260-5

R.T.: 7.985 min
Delta R.T.: -0.009 min
Response: 93901
Conc: 13.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-15-COMP

Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:13 PM

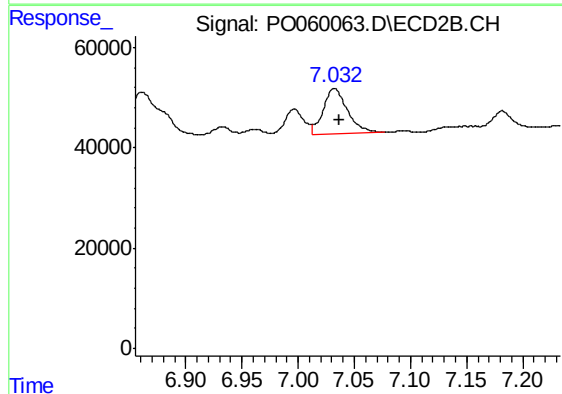

#35 AR-1260-5

R.T.: 7.032 min
Delta R.T.: -0.005 min
Response: 134828
Conc: 24.50 ng/ml