

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082919\
 Data File : P0060064.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 5:18
 Operator : SM/AJ
 Sample : K4568-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-16-COMP

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:50:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 07:07:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.120	3.497	1095978	986961	31.302	27.419
2)	SA Decachlor...	9.580	8.351	1049022	825481	19.718	20.473
Target Compounds							
31)	L7 AR-1260-1	6.837	5.994	51994	53794	19.287m	23.605
32)	L7 AR-1260-2	7.099	6.182	65442	23429	17.637	7.997 #
33)	L7 AR-1260-3	7.451	6.326	35527	22034	10.844m	8.318
34)	L7 AR-1260-4	7.678	6.788	47222	23268	15.375m	10.284 #
35)	L7 AR-1260-5	7.984	7.033	62307	80693	8.799m	14.663 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082919\
Data File : PO060064.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 5:18
Operator : SM/AJ
Sample : K4568-06
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-16-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 07:07:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

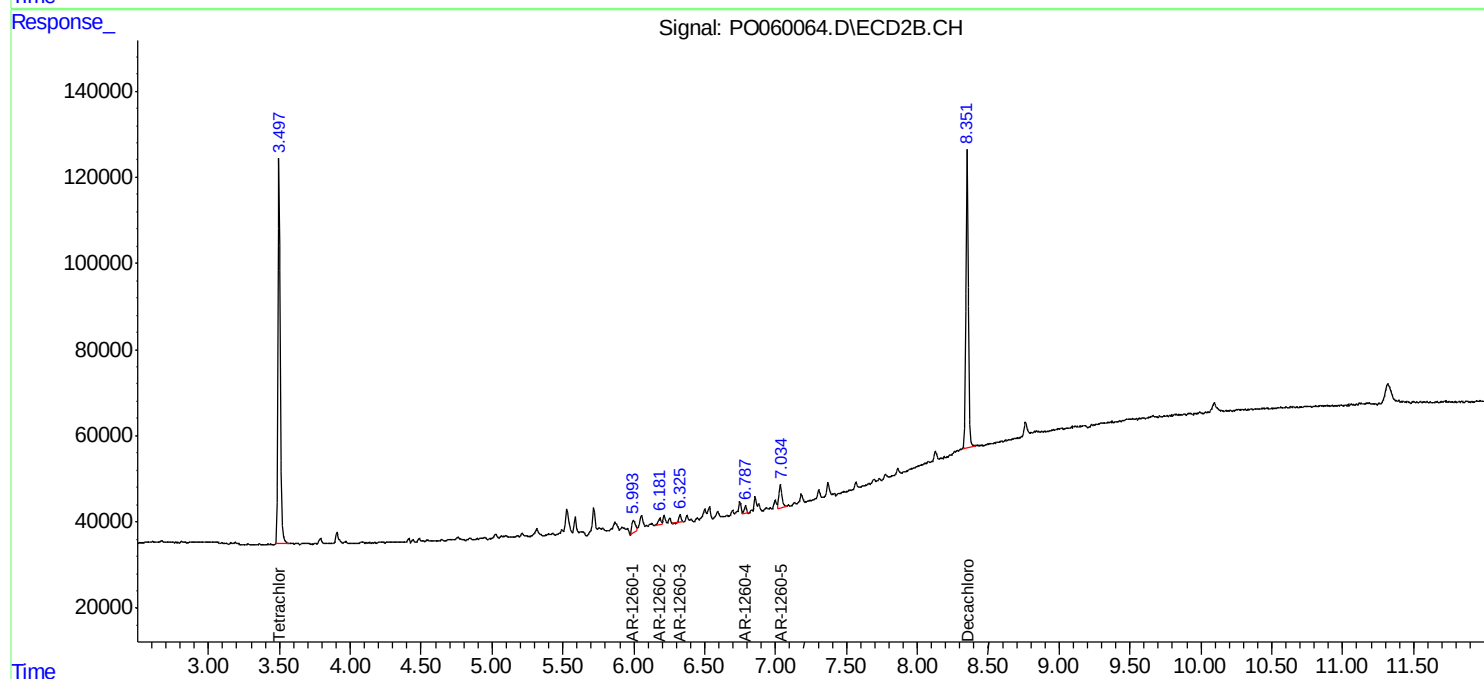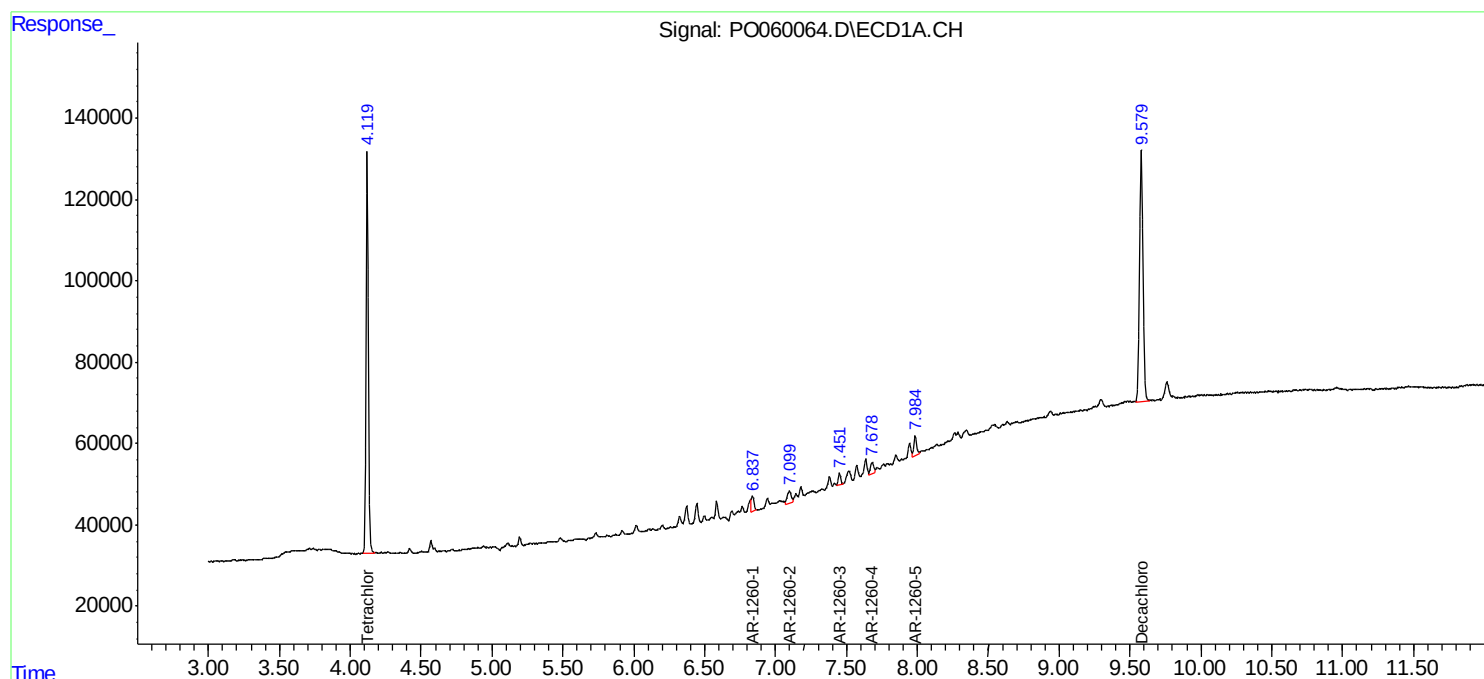

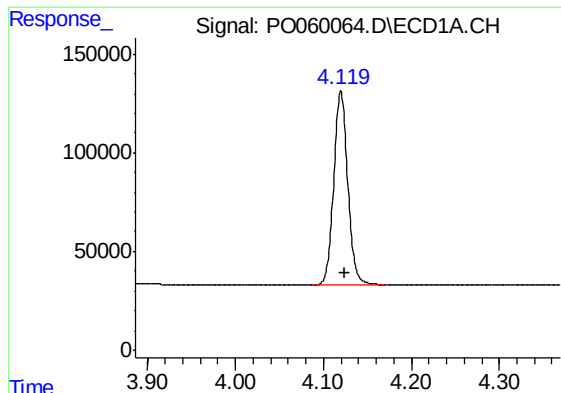


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: -0.004 min
Response: 1095978
Conc: 31.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-16-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:15 PM

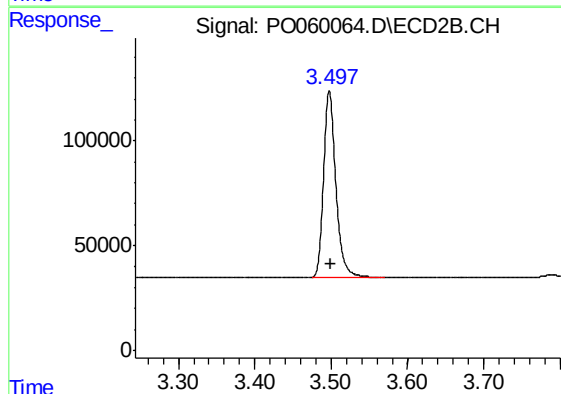


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.002 min
Response: 986961
Conc: 27.42 ng/ml

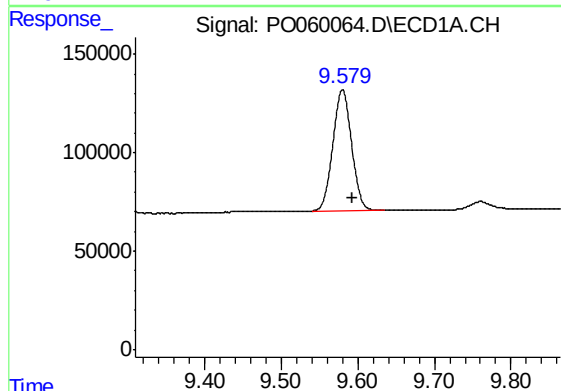


#2 Decachlorobiphenyl

R.T.: 9.580 min
Delta R.T.: -0.014 min
Response: 1049022
Conc: 19.72 ng/ml

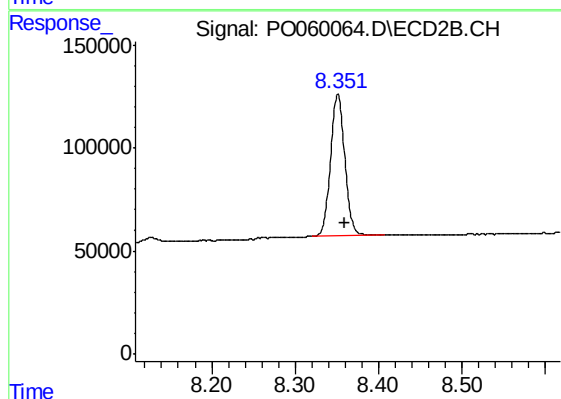

#2 Decachlorobiphenyl

R.T.: 8.351 min
Delta R.T.: -0.008 min
Response: 825481
Conc: 20.47 ng/ml

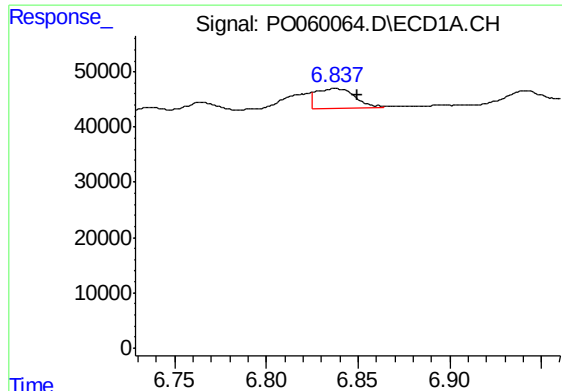


#31 AR-1260-1

R.T.: 6.837 min
Delta R.T.: -0.013 min
Response: 51994
Conc: 19.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-16-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:15 PM

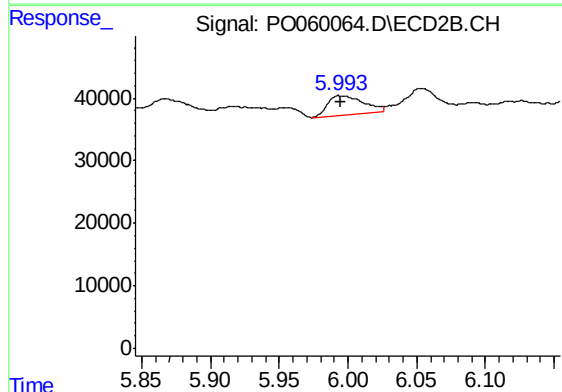


#31 AR-1260-1

R.T.: 5.994 min
Delta R.T.: -0.001 min
Response: 53794
Conc: 23.61 ng/ml

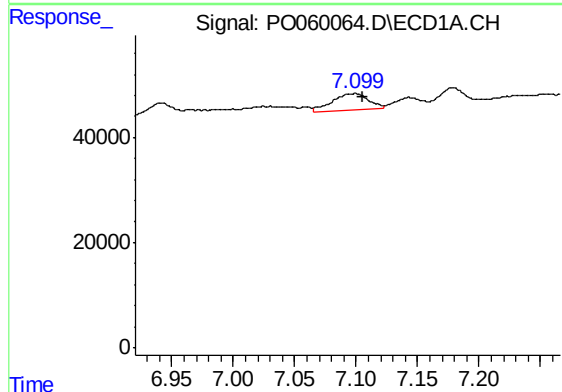


#32 AR-1260-2

R.T.: 7.099 min
Delta R.T.: -0.006 min
Response: 65442
Conc: 17.64 ng/ml

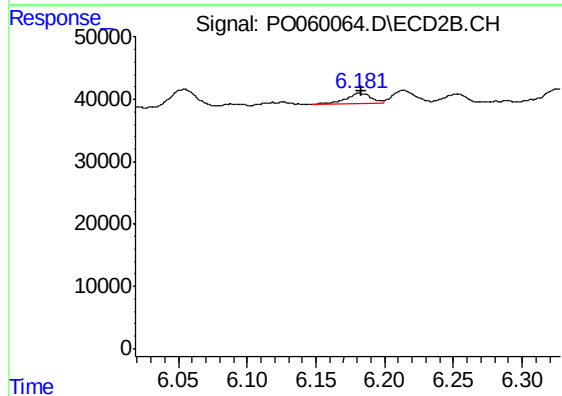

#32 AR-1260-2

R.T.: 6.182 min
Delta R.T.: -0.001 min
Response: 23429
Conc: 8.00 ng/ml

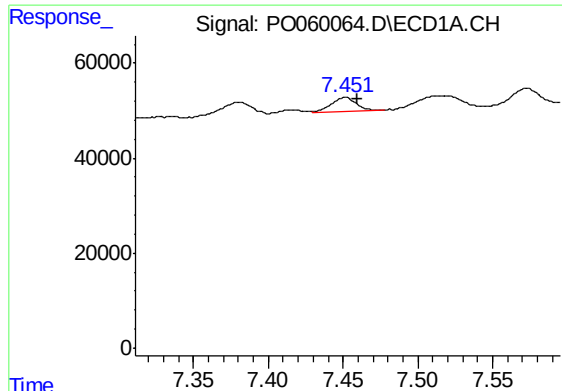


#33 AR-1260-3

R.T.: 7.451 min
Delta R.T.: -0.009 min
Response: 35527
Conc: 10.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-16-COMP


Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:15 PM

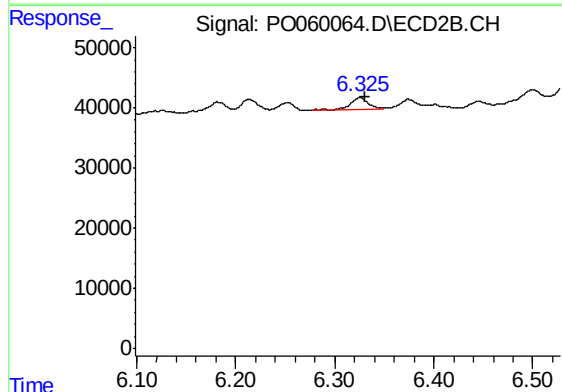


#33 AR-1260-3

R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 22034
Conc: 8.32 ng/ml

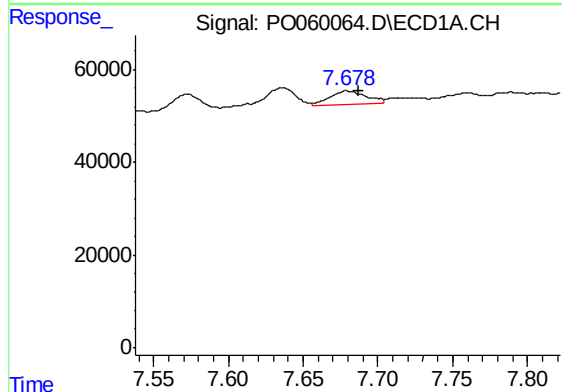


#34 AR-1260-4

R.T.: 7.678 min
Delta R.T.: -0.008 min
Response: 47222
Conc: 15.38 ng/ml m

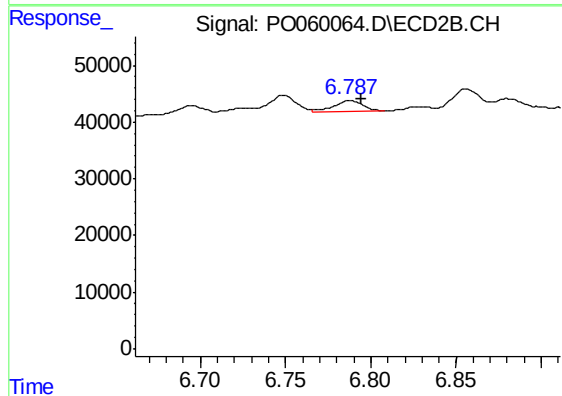

#34 AR-1260-4

R.T.: 6.788 min
Delta R.T.: -0.006 min
Response: 23268
Conc: 10.28 ng/ml

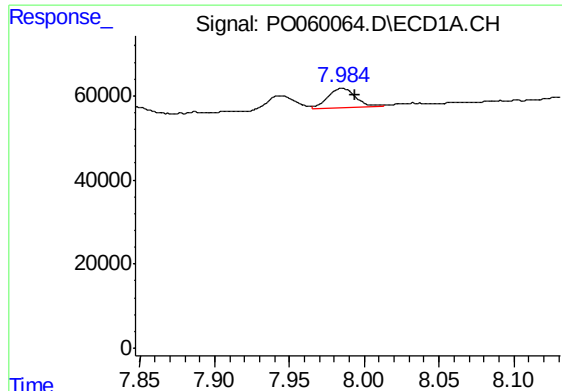


#35 AR-1260-5

R.T.: 7.984 min
Delta R.T.: -0.010 min
Response: 62307
Conc: 8.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-16-COMP

Manual Integrations
APPROVED

Ankita
8/30/2019 5:50:15 PM

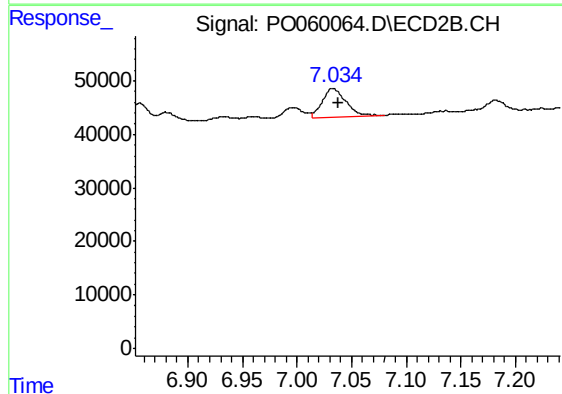

#35 AR-1260-5

R.T.: 7.033 min
Delta R.T.: -0.004 min
Response: 80693
Conc: 14.66 ng/ml