

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082922\
 Data File : P0089140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2022 01:55
 Operator : YP/AJ
 Sample : N4401-10 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 64A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/30/2022
 Supervised By :Ankita Jodhani 08/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 03:15:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.588	6160856	1812520	1.643	1.878
2) SA Decachlor...	10.260	8.570	4497875	1614145	1.954	1.825m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082922\
Data File : PO089140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2022 01:55
Operator : YP/AJ
Sample : N4401-10 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
64A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2022
Supervised By :Ankita Jodhani 08/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:15:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

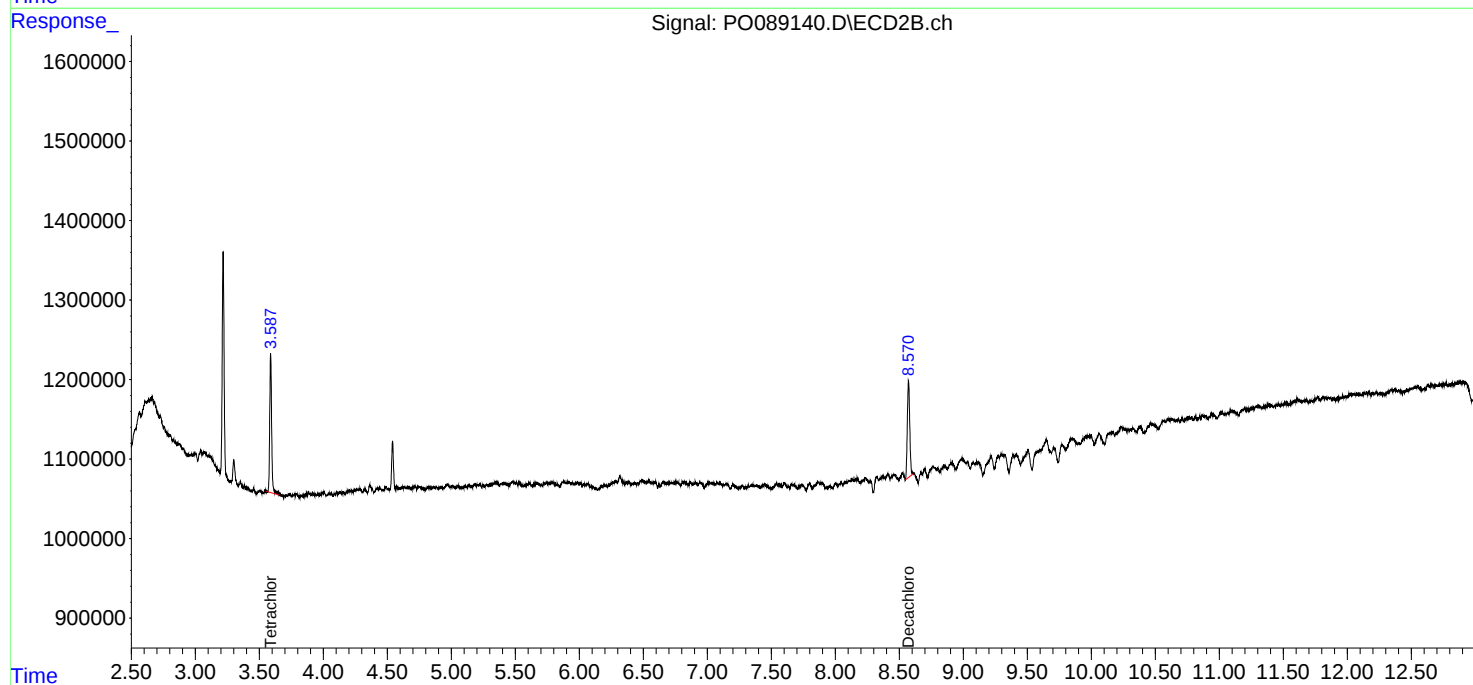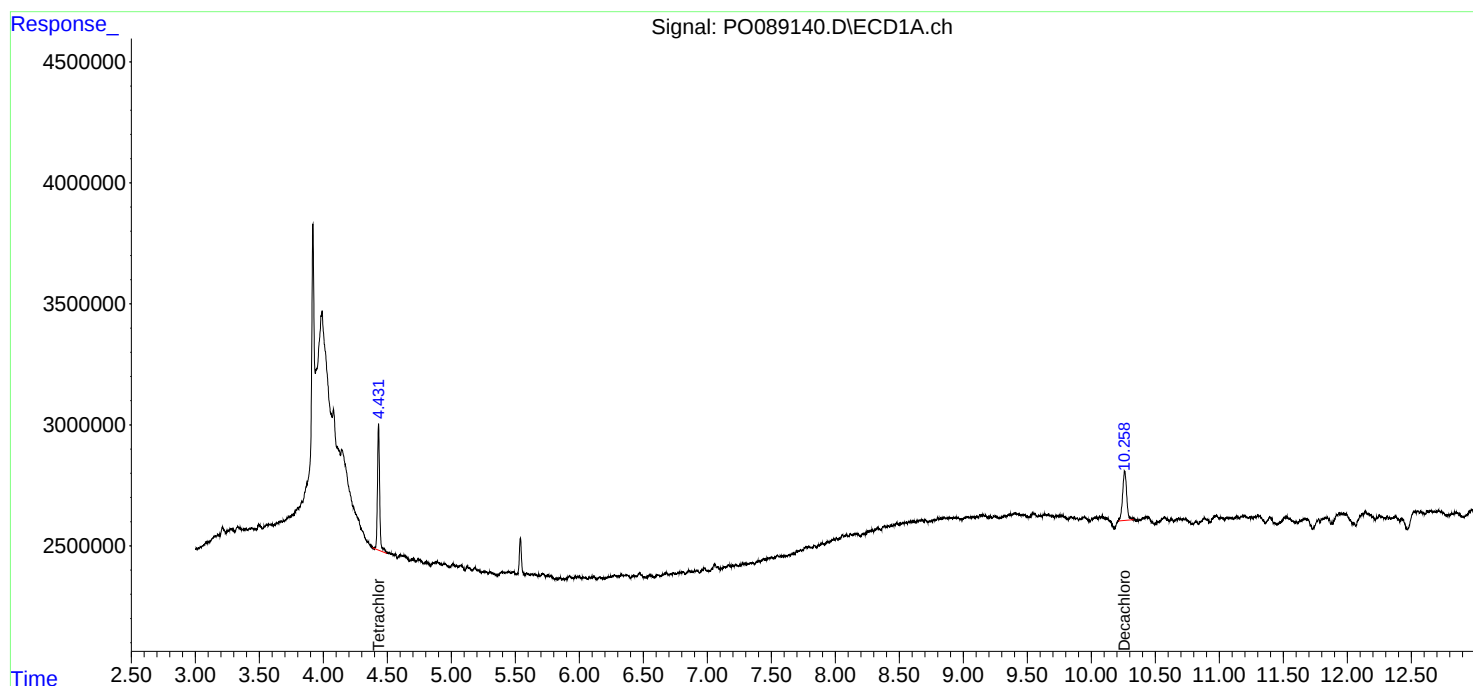

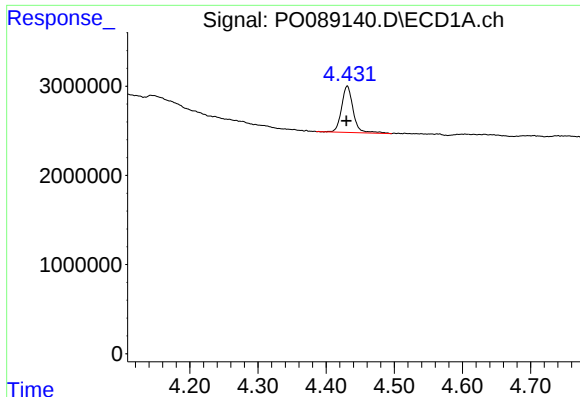


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: 0.000 min
Response: 6160856
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
64A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2022
Supervised By :Ankita Jodhani 08/30/2022

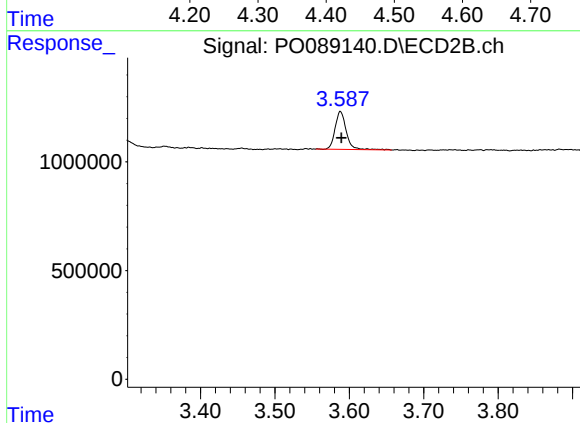


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.001 min
Response: 1812520
Conc: 1.88 ng/ml

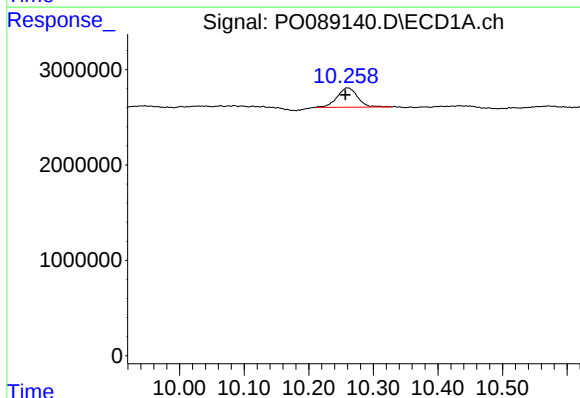

#2 Decachlorobiphenyl

R.T.: 10.260 min
Delta R.T.: 0.003 min
Response: 4497875
Conc: 1.95 ng/ml

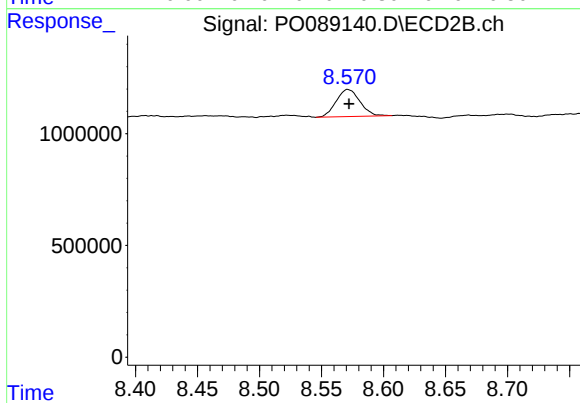

#2 Decachlorobiphenyl

R.T.: 8.570 min
Delta R.T.: -0.002 min
Response: 1614145
Conc: 1.83 ng/ml m