

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082923\
 Data File : P0097501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2023 19:26
 Operator : YP/AJ
 Sample : 04196-29
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-345-COMP-05

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/30/2023
 Supervised By :Ankita Jodhani 08/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 20:46:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.628	73120236	15415736	21.908	22.851
2) SA Decachlor...	10.302	8.675	36039805	12179674	19.636	21.218m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082923\
Data File : PO097501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2023 19:26
Operator : YP/AJ
Sample : 04196-29
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-345-COMP-05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 20:46:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

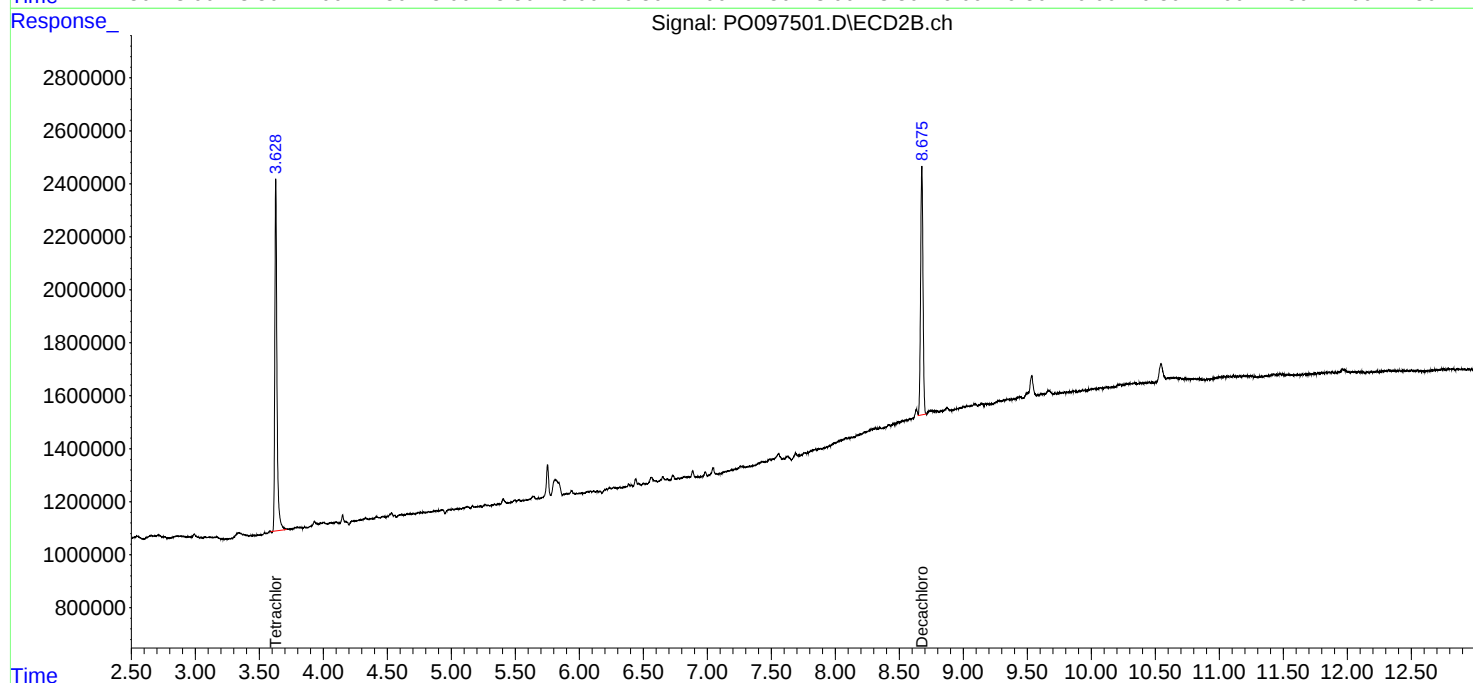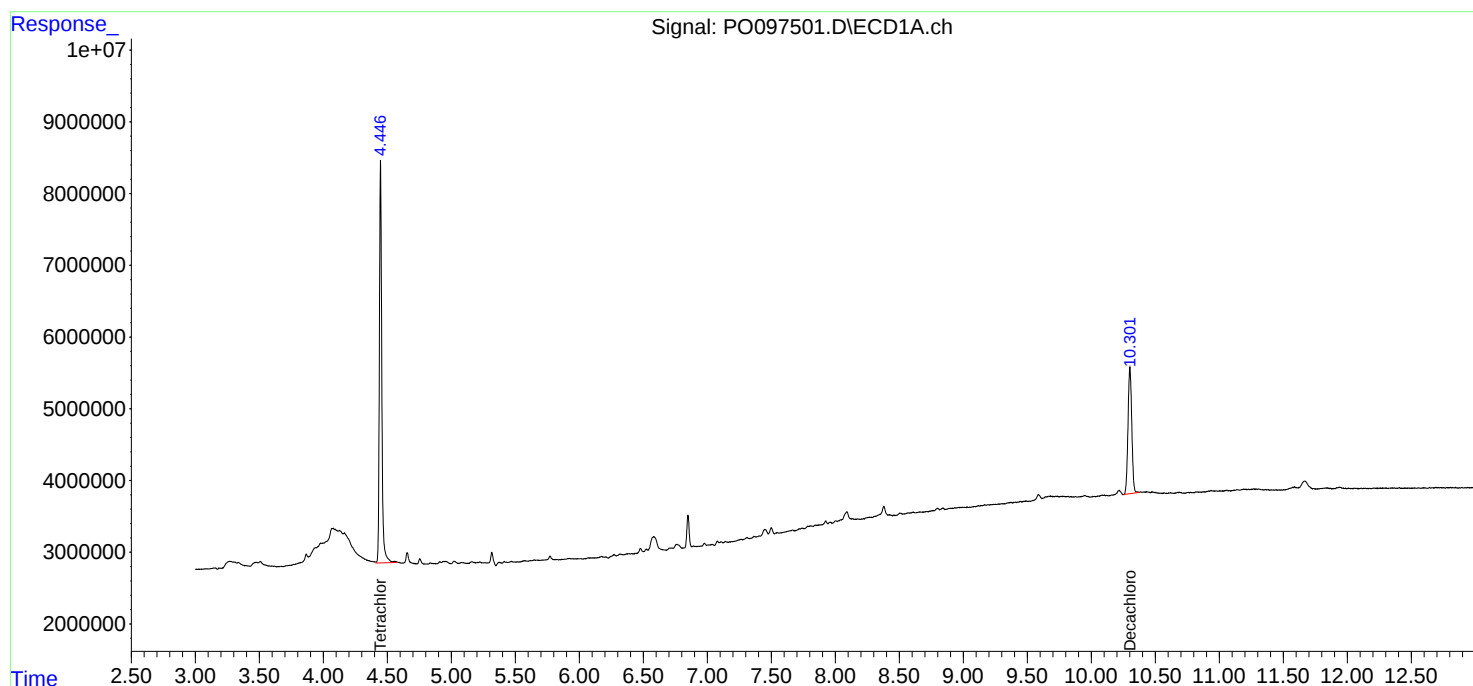

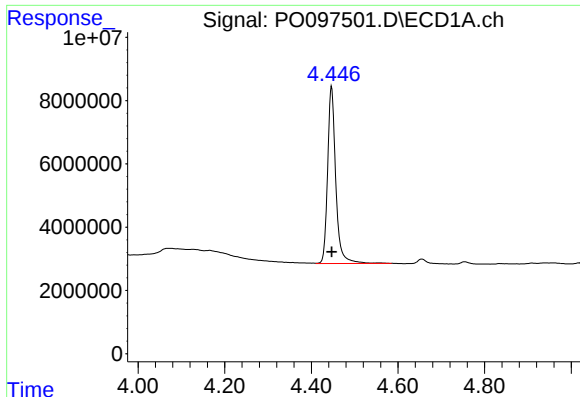


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 73120236
Conc: 21.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-345-COMP-05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

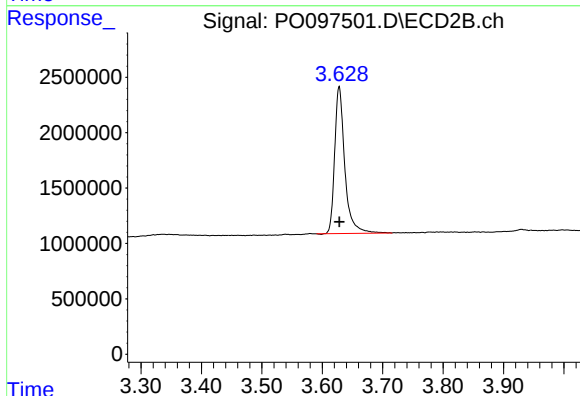


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 15415736
Conc: 22.85 ng/ml

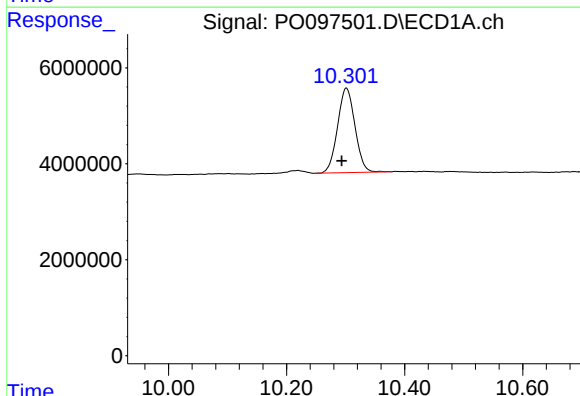

#2 Decachlorobiphenyl

R.T.: 10.302 min
Delta R.T.: 0.008 min
Response: 36039805
Conc: 19.64 ng/ml

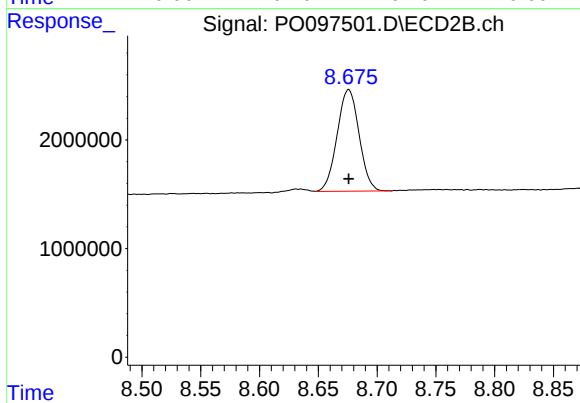

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: 0.000 min
Response: 12179674
Conc: 21.22 ng/ml m