

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082923\
 Data File : P0097503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2023 20:00
 Operator : YP/AJ
 Sample : 04197-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-309-OK-370-COMP-21

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/30/2023
 Supervised By :Ankita Jodhani 08/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 20:47:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.628	65272512	13563091	19.557	20.104
2) SA Decachlor...	10.300	8.676	35137105	12132384	19.144m	21.135

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082923\
Data File : PO097503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2023 20:00
Operator : YP/AJ
Sample : 04197-08
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-309-OK-370-COMP-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 20:47:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

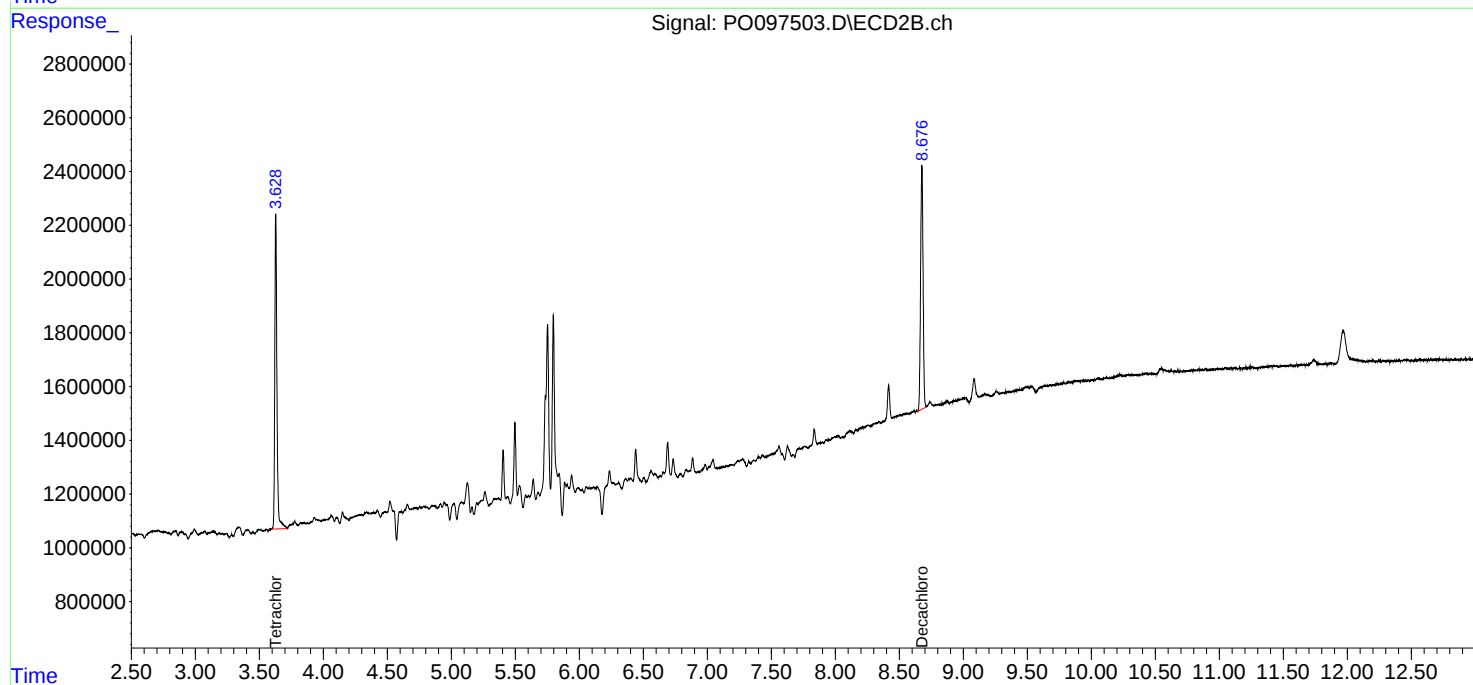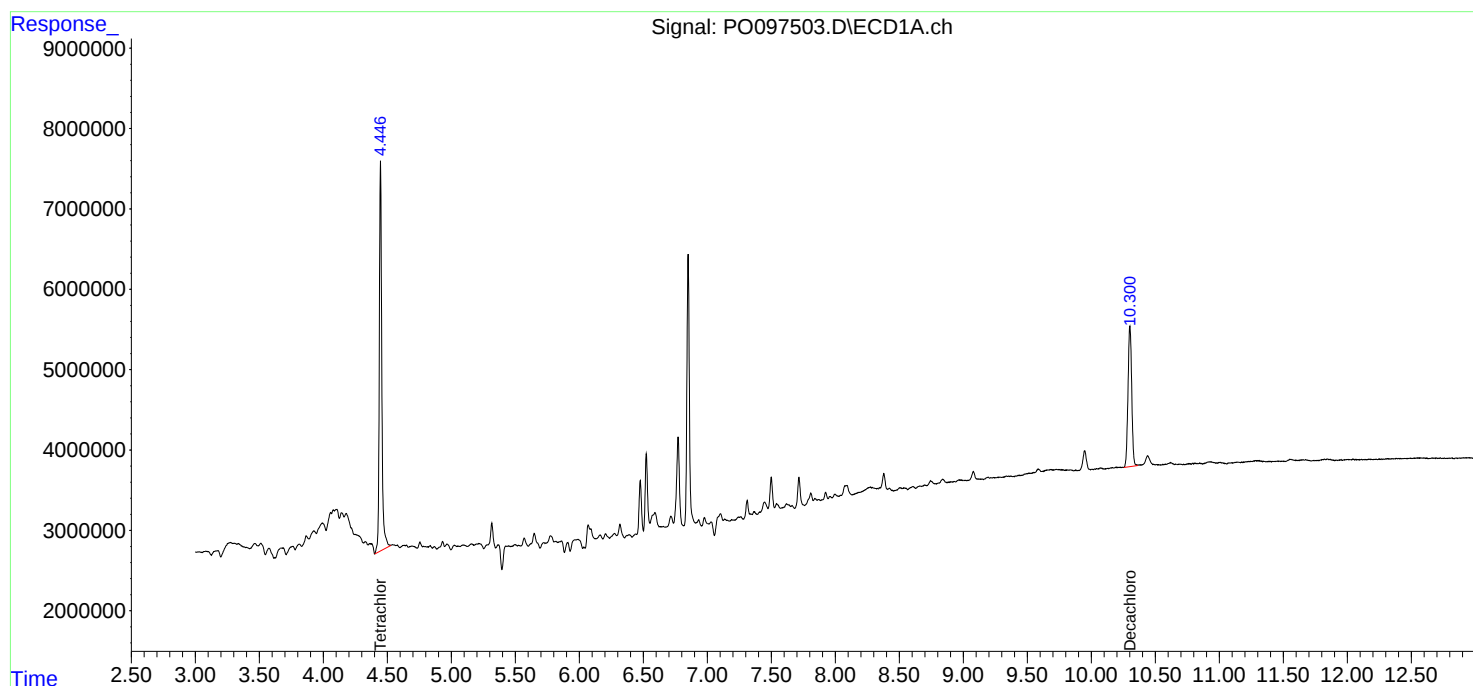

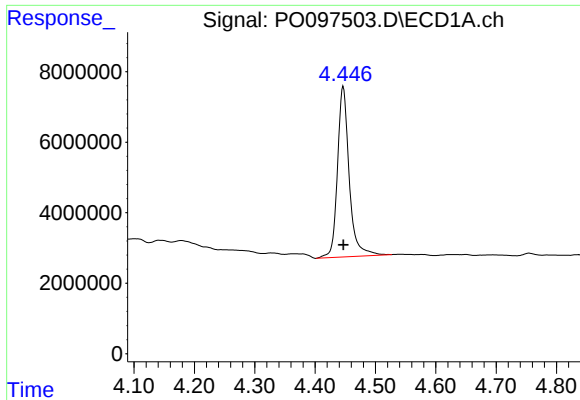


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 65272512
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-309-OK-370-COMP-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

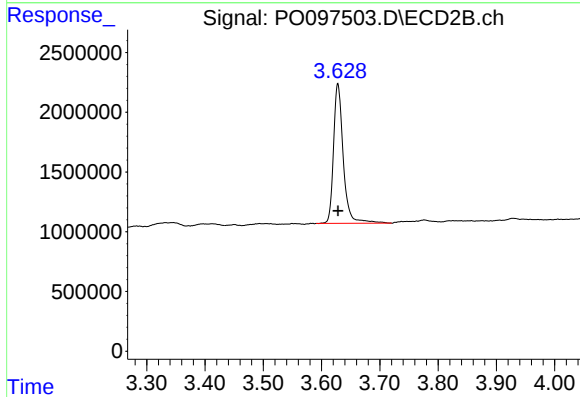


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 13563091
Conc: 20.10 ng/ml

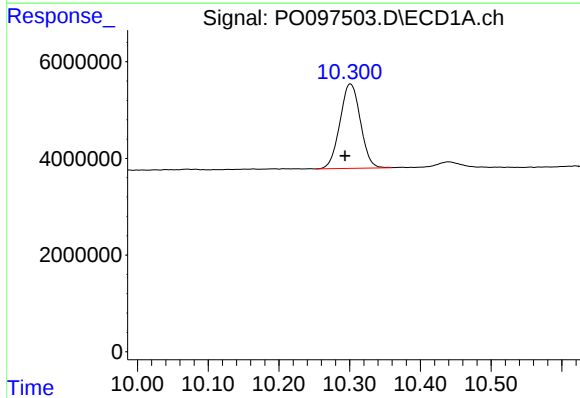

#2 Decachlorobiphenyl

R.T.: 10.300 min
Delta R.T.: 0.007 min
Response: 35137105
Conc: 19.14 ng/ml m

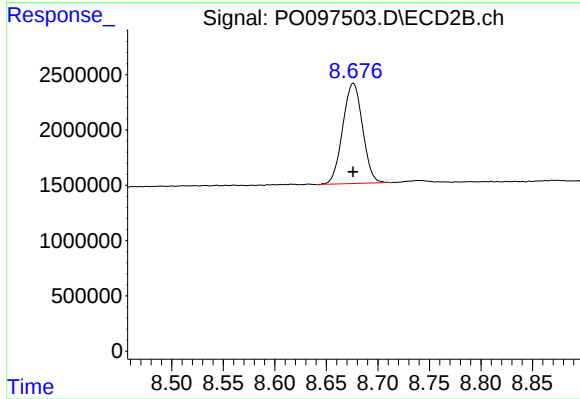

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: 0.000 min
Response: 12132384
Conc: 21.14 ng/ml