

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082923\
 Data File : P0097508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2023 21:24
 Operator : YP/AJ
 Sample : 04198-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-309-OK-370-COMP-26

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/30/2023
 Supervised By :Ankita Jodhani 08/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 22:06:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.628	79176121	16457446	23.723	24.395
2) SA Decachlor...	10.303	8.675	40824948	14061536	22.243m	24.496

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082923\
Data File : PO097508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2023 21:24
Operator : YP/AJ
Sample : 04198-14
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-309-OK-370-COMP-26


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 22:06:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

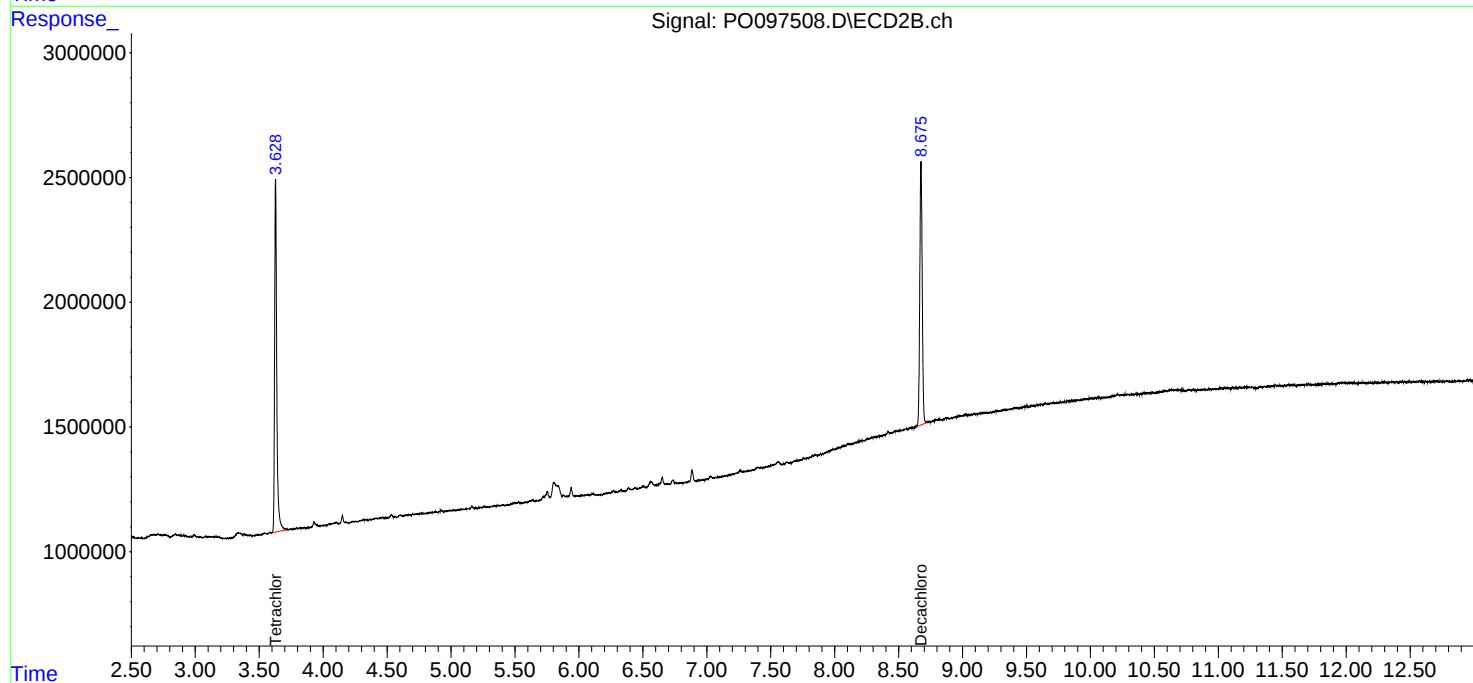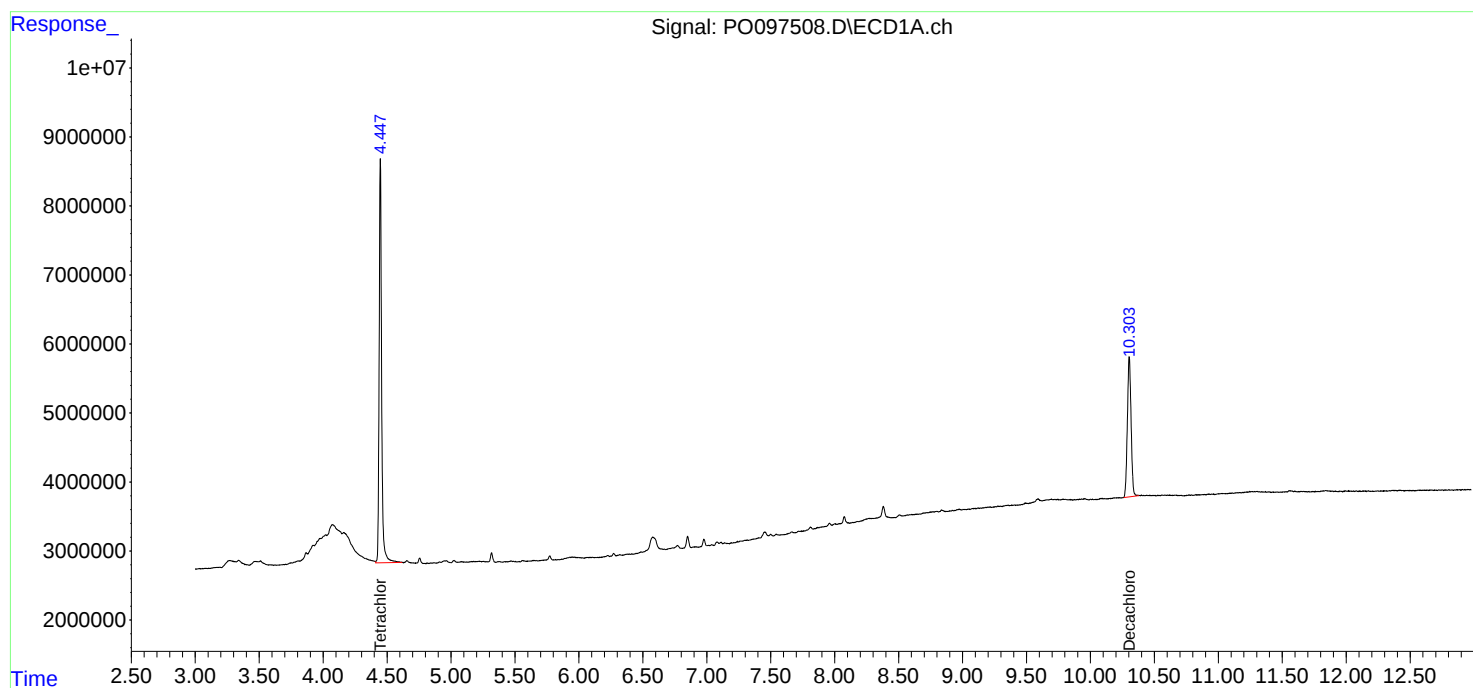

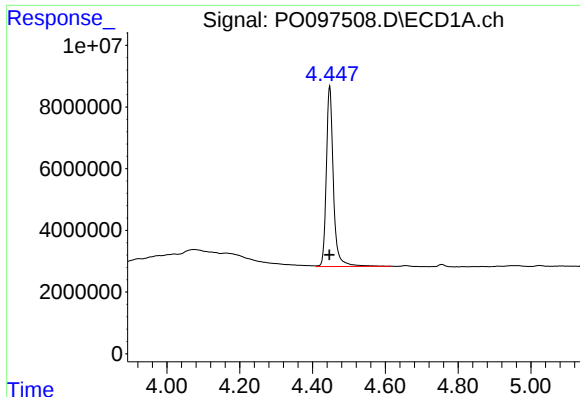


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 79176121
Conc: 23.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-309-OK-370-COMP-26


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

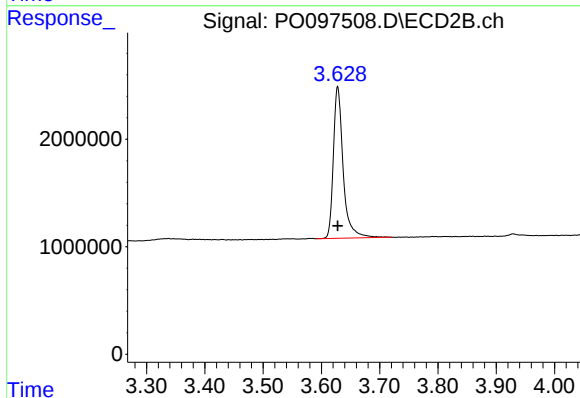


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 16457446
Conc: 24.39 ng/ml

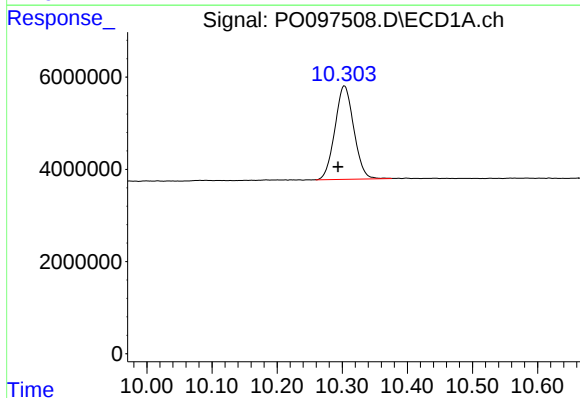

#2 Decachlorobiphenyl

R.T.: 10.303 min
Delta R.T.: 0.009 min
Response: 40824948
Conc: 22.24 ng/ml m

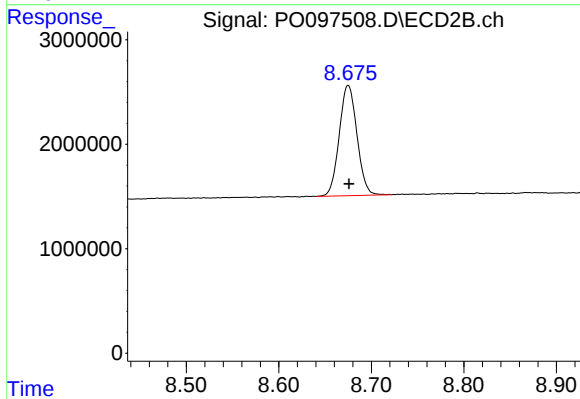

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: 0.000 min
Response: 14061536
Conc: 24.50 ng/ml