

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082925\
 Data File : P0113366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2025 19:02
 Operator : YP/AJ
 Sample : Q2982-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-25-0249-0253

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/03/2025
 Supervised By :mohammad ahmed 09/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 23:28:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.661	3.654	129.8E6	86767724	15.861m	17.146
2) SA Decachlor...	8.676	8.622	135.2E6	43889974	19.508	23.163

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082925\
Data File : PO113366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2025 19:02
Operator : YP/AJ
Sample : Q2982-05
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-25-0249-0253


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/03/2025
Supervised By :mohammad ahmed 09/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 23:28:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

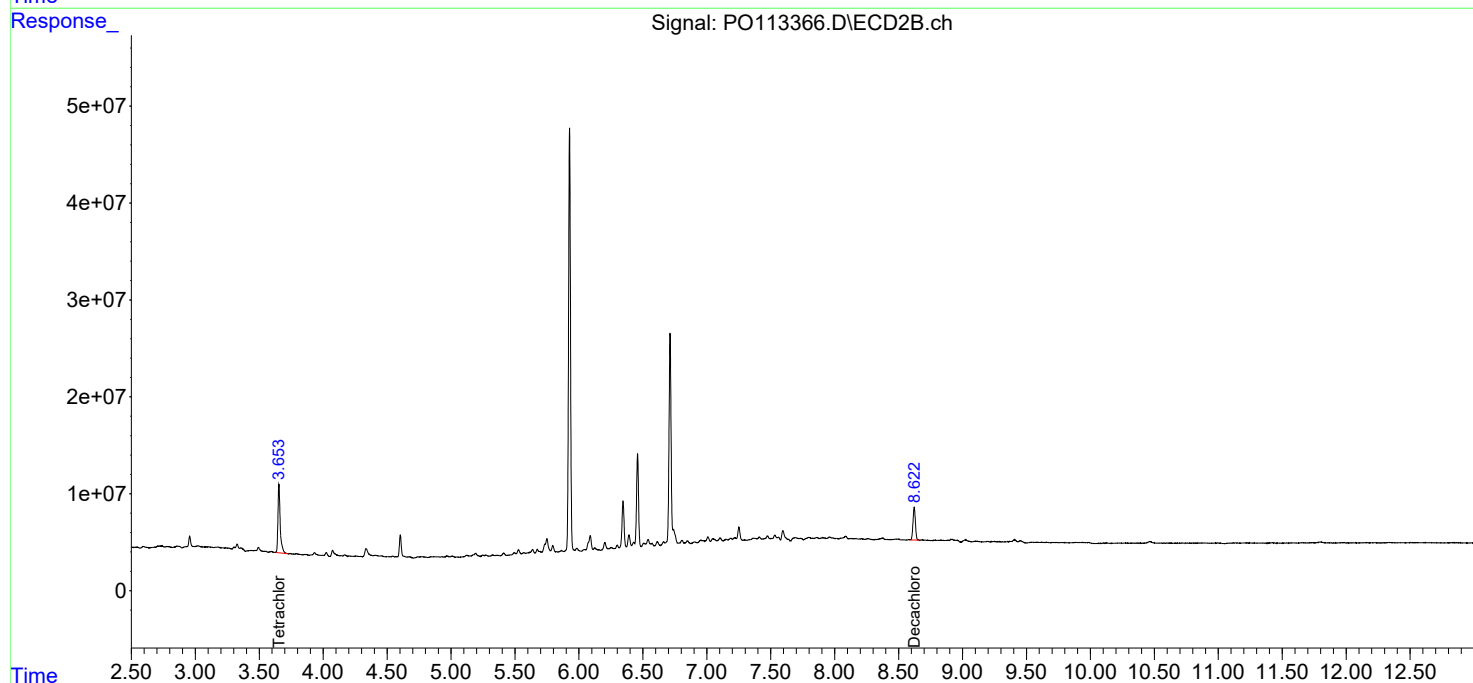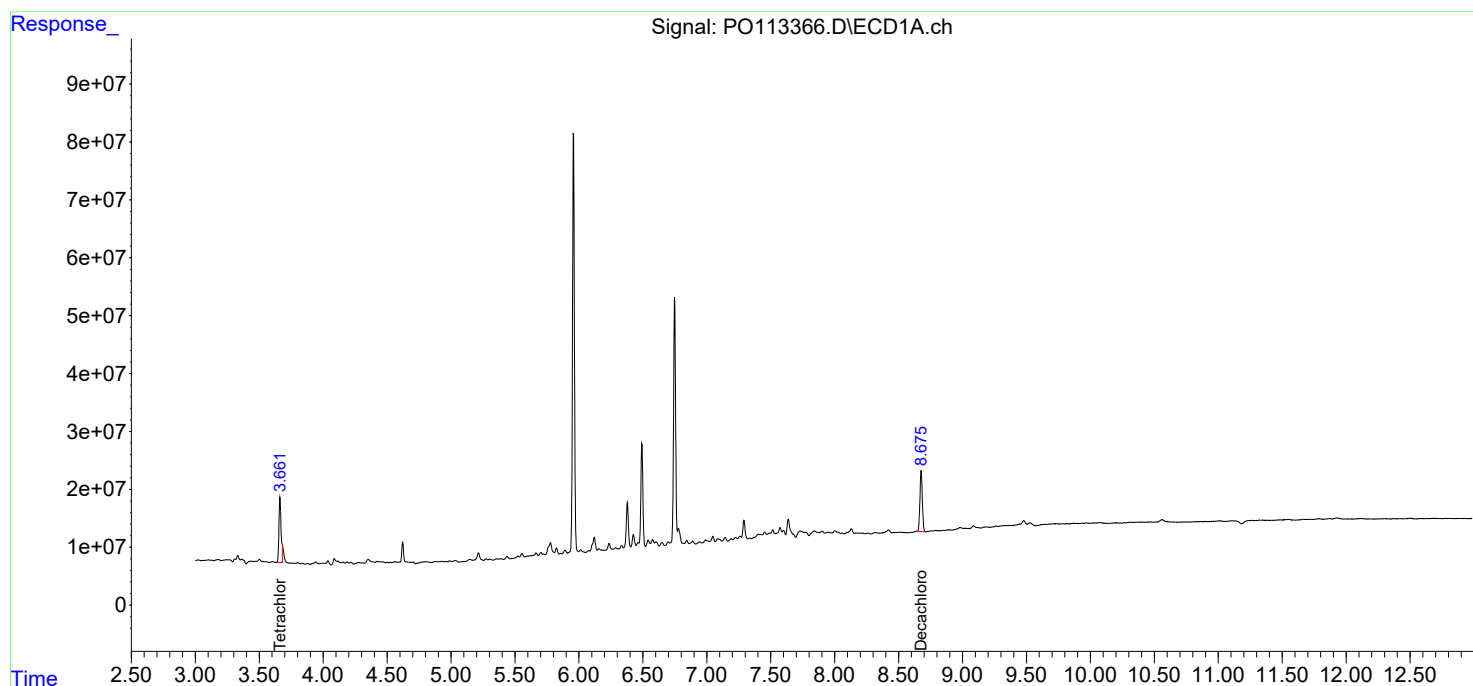

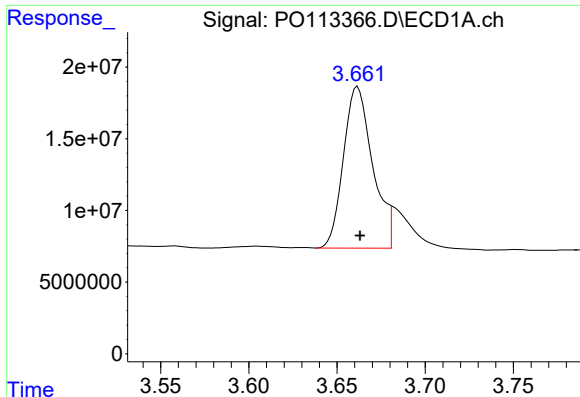


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.002 min
Response: 129846835
Conc: 15.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-25-0249-0253


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/03/2025
Supervised By :mohammad ahmed 09/04/2025

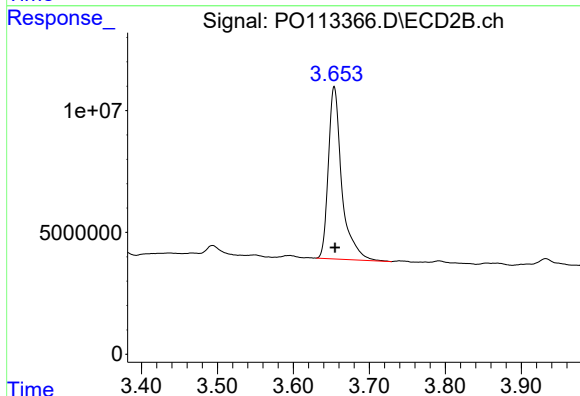


#1 Tetrachloro-m-xylene

R.T.: 3.654 min
Delta R.T.: -0.001 min
Response: 86767724
Conc: 17.15 ng/ml

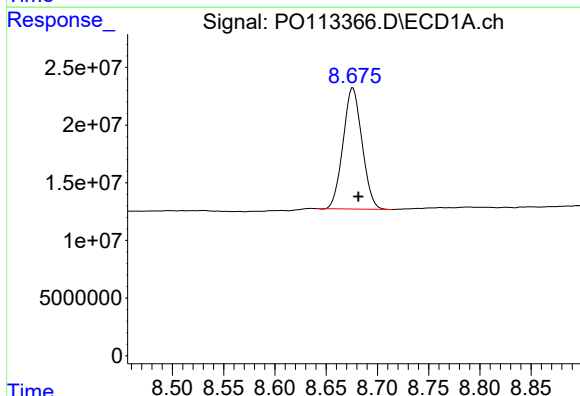

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.005 min
Response: 135217955
Conc: 19.51 ng/ml

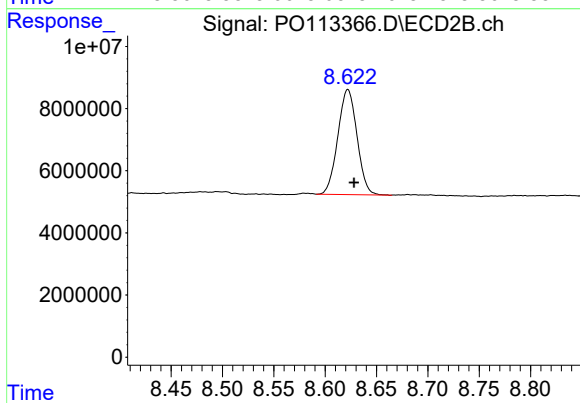

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.006 min
Response: 43889974
Conc: 23.16 ng/ml