

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0083018\
Data File : P0048624.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2018 13:19
Operator : SM/SJ
Sample : J4656-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082418-SIDI-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:31:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.380	3.621	3589985	4283965	18.951	15.824
2)	SA Decachlor...	10.059	8.596	2252313	2045406	13.080	12.213

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083018\
Data File : P0048624.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2018 13:19
Operator : SM/SJ
Sample : J4656-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082418-SIDI-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:31:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

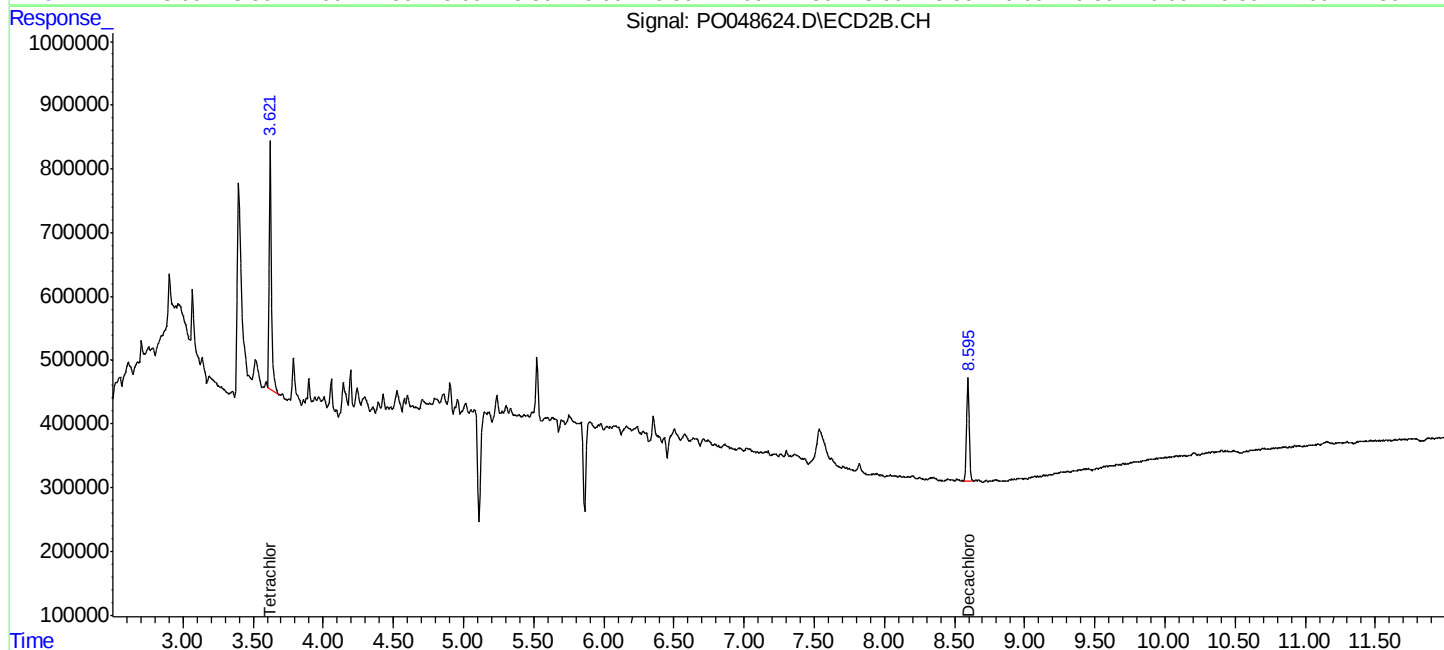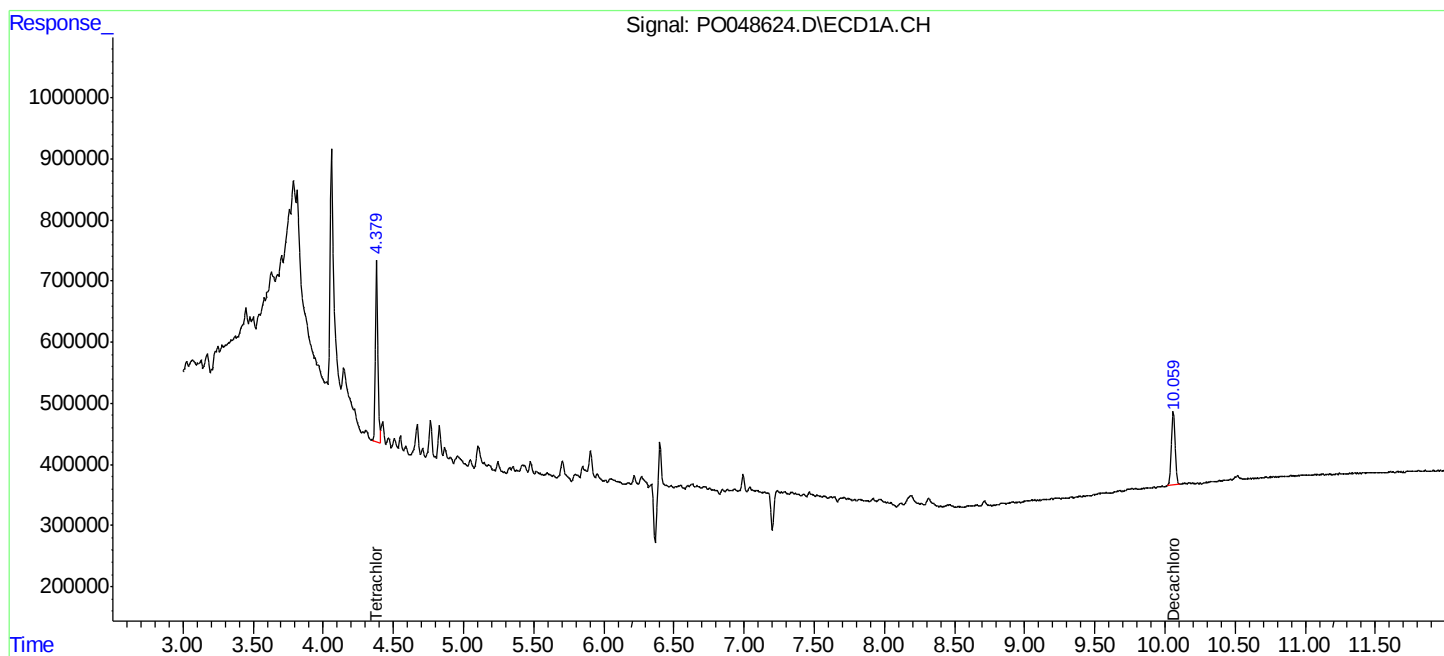


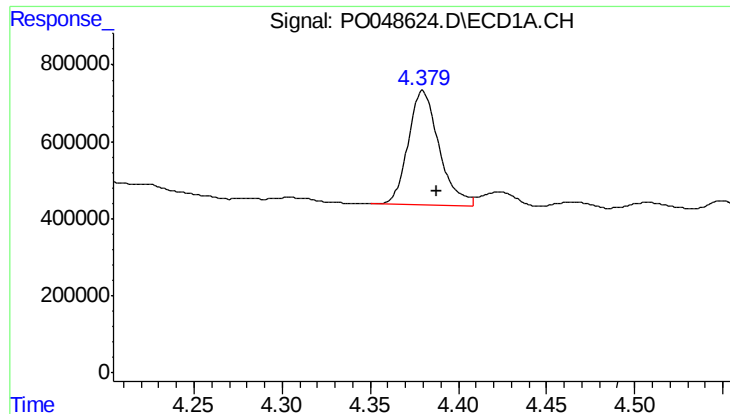

#1 Tetrachloro-m-xylene


R.T.: 4.380 min
Delta R.T.: -0.008 min
Response: 3589985
Conc: 18.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
082418-SIDI-F-D-S

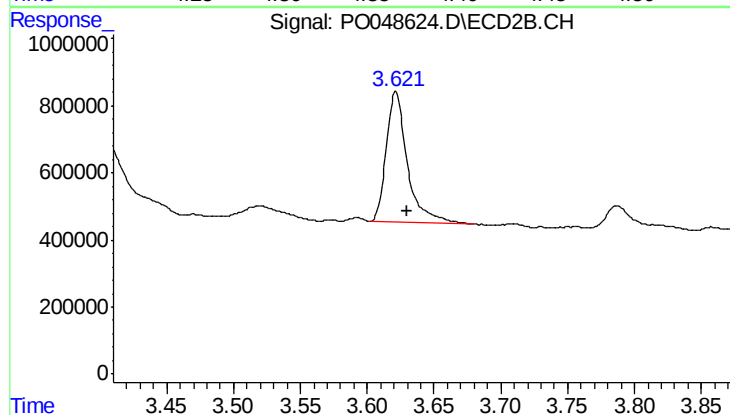


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.009 min
Response: 4283965
Conc: 15.82 ng/ml

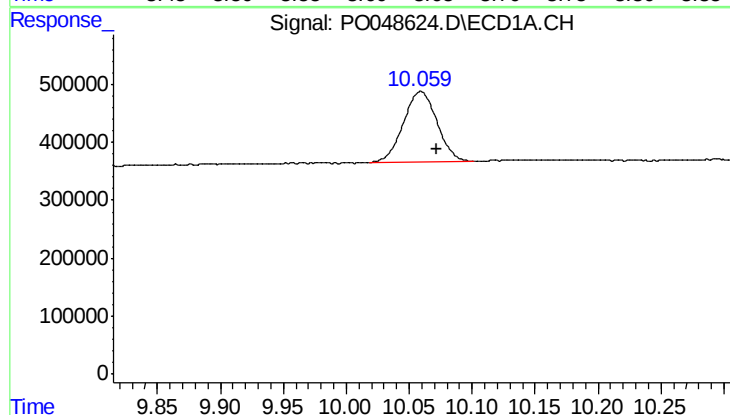

#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: -0.013 min
Response: 2252313
Conc: 13.08 ng/ml

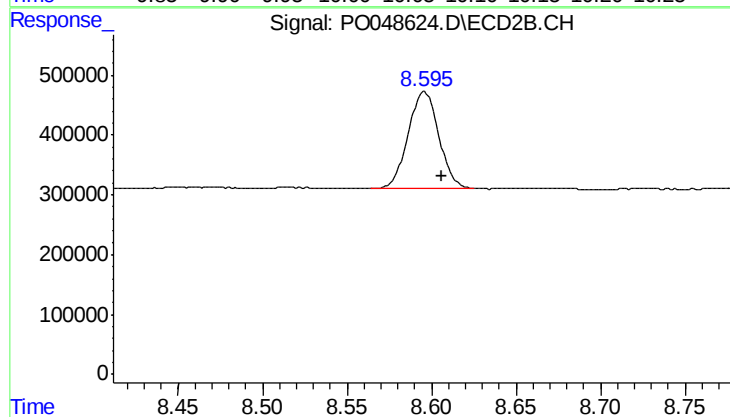

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.011 min
Response: 2045406
Conc: 12.21 ng/ml