

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0083018\
 Data File : P0048626.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2018 13:51
 Operator : SM/SJ
 Sample : J4656-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 082418-SIDI-F-U-M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:33:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.622	4239181	5012400	22.378	18.515
2) SA Decachlor...	10.061	8.596	2094715	1919165	12.164	11.459

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083018\
Data File : P0048626.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2018 13:51
Operator : SM/SJ
Sample : J4656-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082418-SIDI-F-U-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:33:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

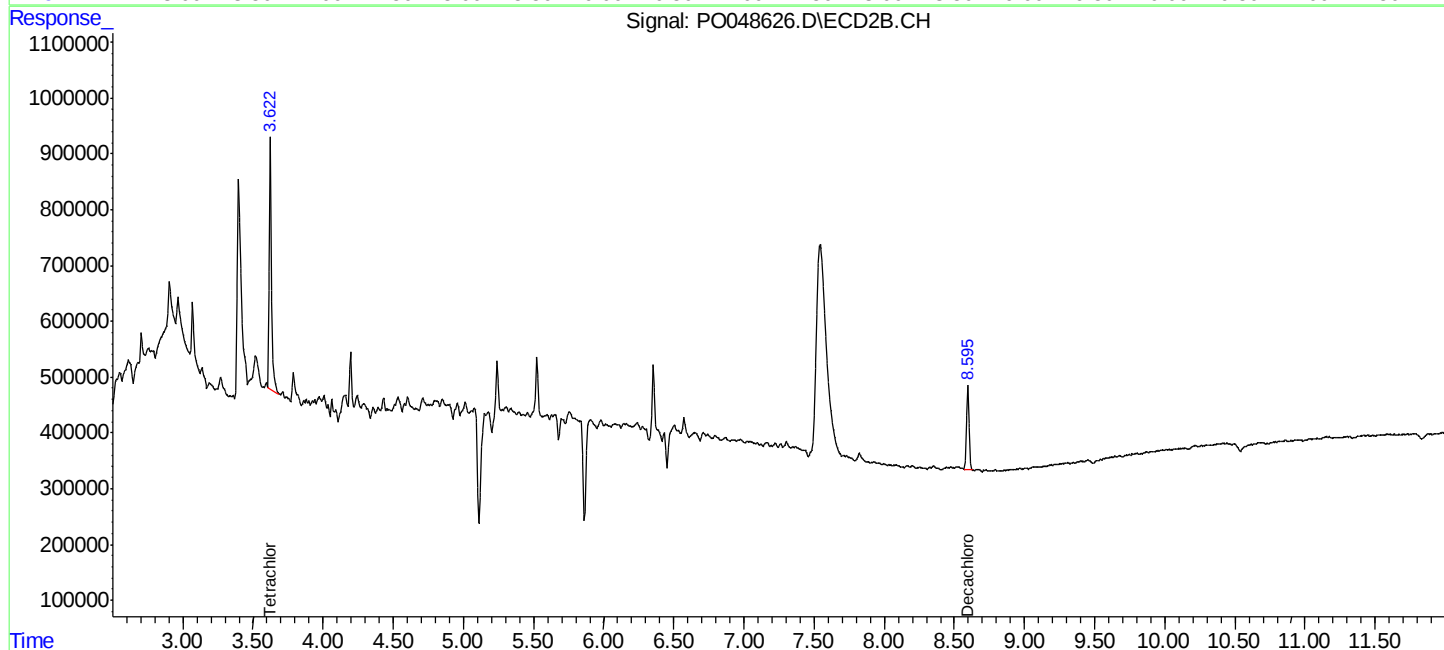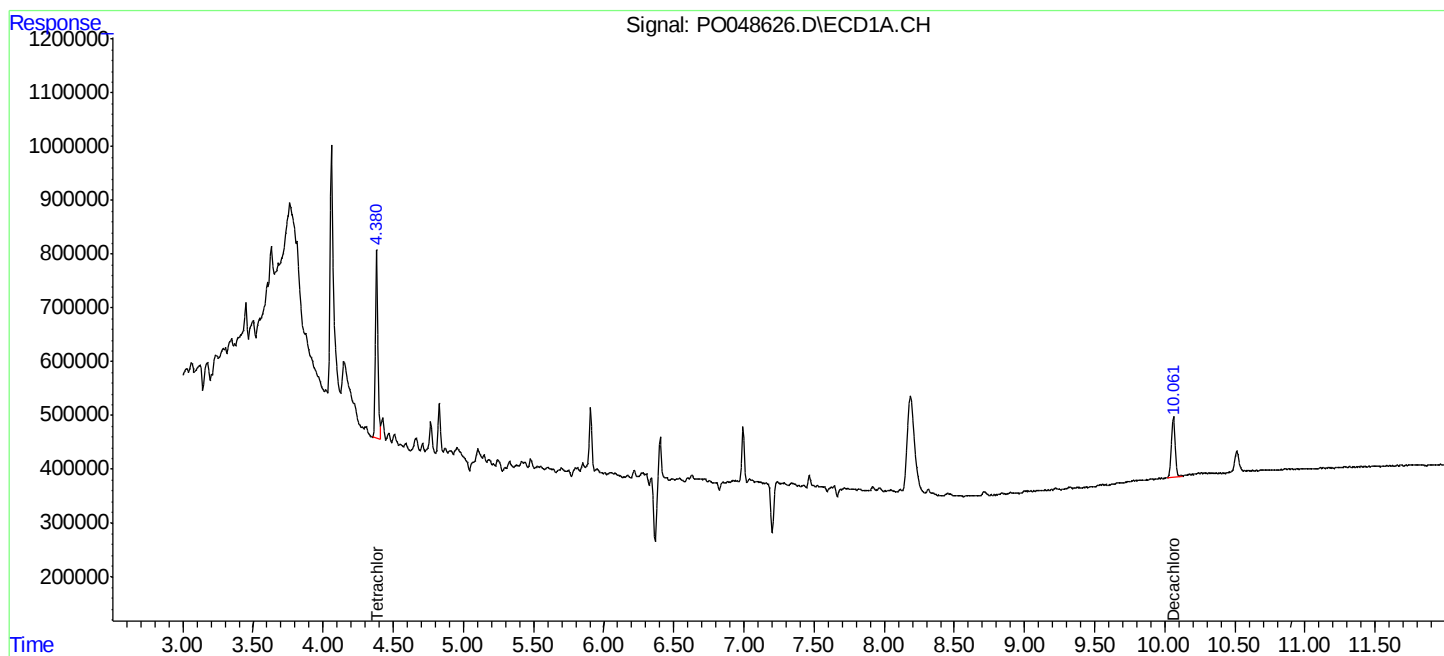


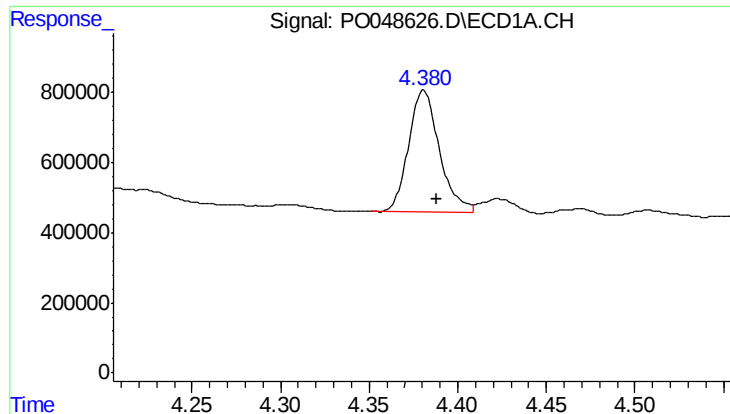

#1 Tetrachloro-m-xylene


R.T.: 4.381 min
Delta R.T.: -0.007 min
Response: 4239181
Conc: 22.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
082418-SIDI-F-U-M

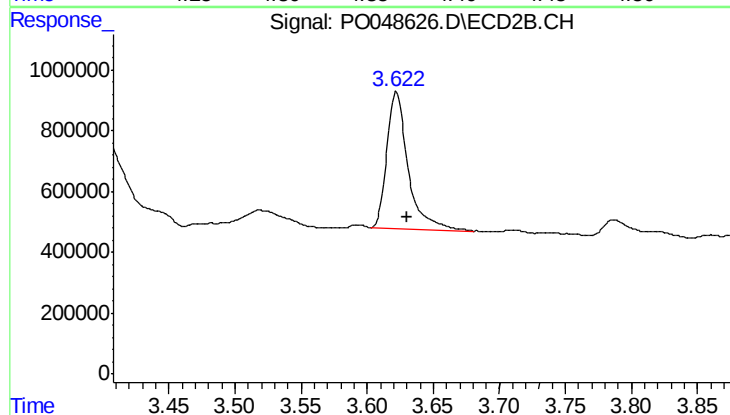


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.008 min
Response: 5012400
Conc: 18.51 ng/ml

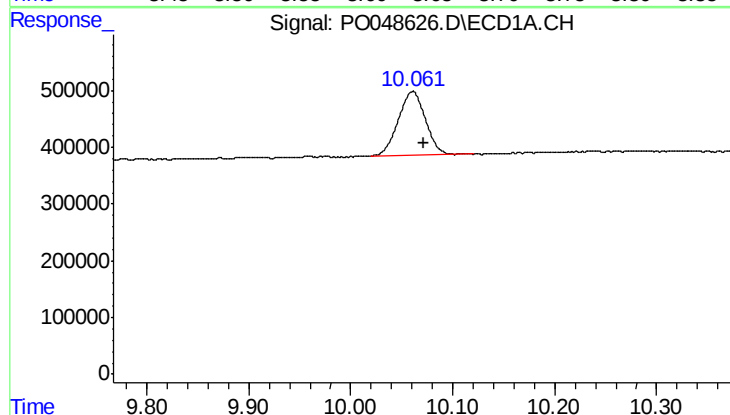

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: -0.011 min
Response: 2094715
Conc: 12.16 ng/ml

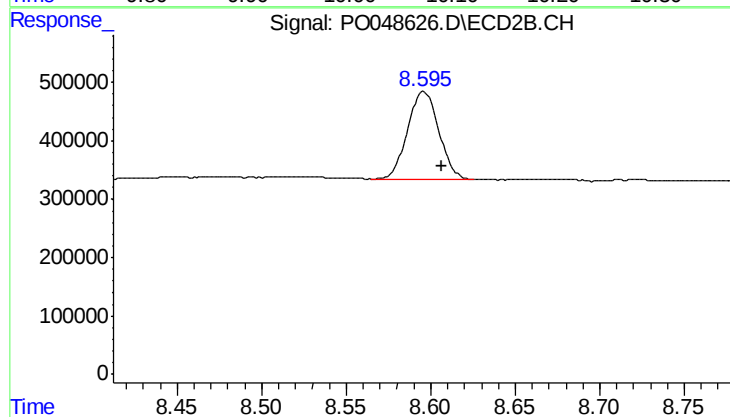

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.011 min
Response: 1919165
Conc: 11.46 ng/ml