

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 17:37
 Operator : SM/AJ
 Sample : K4587-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-057

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 23:21:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.123	3.496	870261	772351	24.856	21.457
2)	SA Decachlor...	9.584	8.353	632994	494330	11.898	12.260
Target Compounds							
3)	L1 AR-1016-1	5.282	0.000	1878	0	1.171	N.D. #
4)	L1 AR-1016-2	5.282	0.000	1878	0	0.785	N.D. #
5)	L1 AR-1016-3	5.339	0.000	8360	0	5.612	N.D. #
6)	L1 AR-1016-4	5.482	0.000	2901	0	2.398	N.D. #
7)	L1 AR-1016-5	5.737	0.000	2115	0	1.647	N.D. #
8)	L2 AR-1221-1	4.338	0.000	3604	0	8.510	N.D. #
9)	L2 AR-1221-2	4.422	0.000	14386	0	44.293	N.D. #
10)	L2 AR-1221-3	4.504	3.924	18906	31127	17.974	31.812 #
11)	L3 AR-1232-1	4.504	3.924	18906	31127	15.168	27.301 #
12)	L3 AR-1232-2	5.006	0.000	1249	0	1.768	N.D. #
13)	L3 AR-1232-3	5.282	0.000	1878	0	1.226	N.D. #
14)	L3 AR-1232-4	5.526	0.000	13177	0	16.853	N.D. #
15)	L3 AR-1232-5	5.564	0.000	8609	0	14.321	N.D. #
16)	L4 AR-1242-1	5.282	0.000	1878	0	1.479	N.D. #
17)	L4 AR-1242-2	5.282	0.000	1878	0	1.012	N.D. #
18)	L4 AR-1242-3	5.339	0.000	8360	0	7.152	N.D. #
19)	L4 AR-1242-4	5.526	0.000	13177	0	13.615	N.D. #
20)	L4 AR-1242-5	6.215	5.341	5372	37627	4.275	33.638 #
21)	L5 AR-1248-1	5.282	0.000	1878	0	1.873	N.D. #
22)	L5 AR-1248-2	5.526	0.000	13177	0	9.082	N.D. #
23)	L5 AR-1248-3	5.691	0.000	21246	0	12.783	N.D. #
24)	L5 AR-1248-4	6.120	0.000	66193	0	32.382	N.D. #
25)	L5 AR-1248-5	6.181	5.341	7564	37627	3.814	26.289 #
26)	L6 AR-1254-1	6.120	5.341	66193	37627	31.725	15.864 #
27)	L6 AR-1254-2	6.333	5.533	42786	421247	12.825	200.756 #
28)	L6 AR-1254-3	6.686	0.000	19583	0	5.519	N.D. #
29)	L6 AR-1254-4	6.974	0.000	5873	0	1.994	N.D. #
30)	L6 AR-1254-5	7.391	0.000	13463	0	4.354	N.D. #
31)	L7 AR-1260-1	6.845	0.000	9434	0	3.499	N.D. #
32)	L7 AR-1260-2	7.091	6.216	74062	45560	19.960	15.550
33)	L7 AR-1260-3	7.455	0.000	20664	0	6.307	N.D. #
34)	L7 AR-1260-4	7.690	0.000	52608	0	17.129	N.D. #
35)	L7 AR-1260-5	7.987	0.000	59800	0	8.445	N.D. #
36)	L8 AR-1262-1	7.523	0.000	26590	0	5.479	N.D. #
37)	L8 AR-1262-2	8.057	0.000	114289	0	14.812	N.D. #
38)	L8 AR-1262-3	8.350	0.000	346594	0	67.929	N.D. #
39)	L8 AR-1262-4	8.350	0.000	346594	0	89.914	N.D. #
40)	L8 AR-1262-5	8.942	0.000	75155	0	29.282	N.D. #
41)	L9 AR-1268-1	8.350	0.000	346594	0	36.830	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 17:37
Operator : SM/AJ
Sample : K4587-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 23:21:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.350	0.000	346594	0	43.969	N.D. #
43)	L9 AR-1268-3	8.601	0.000	20286	0	2.878	N.D. #
44)	L9 AR-1268-4	8.942	0.000	75155	0	27.034	N.D. #
45)	L9 AR-1268-5	9.383	8.132	47829	28934	2.593	1.991


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 17:37
Operator : SM/AJ
Sample : K4587-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 23:21:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

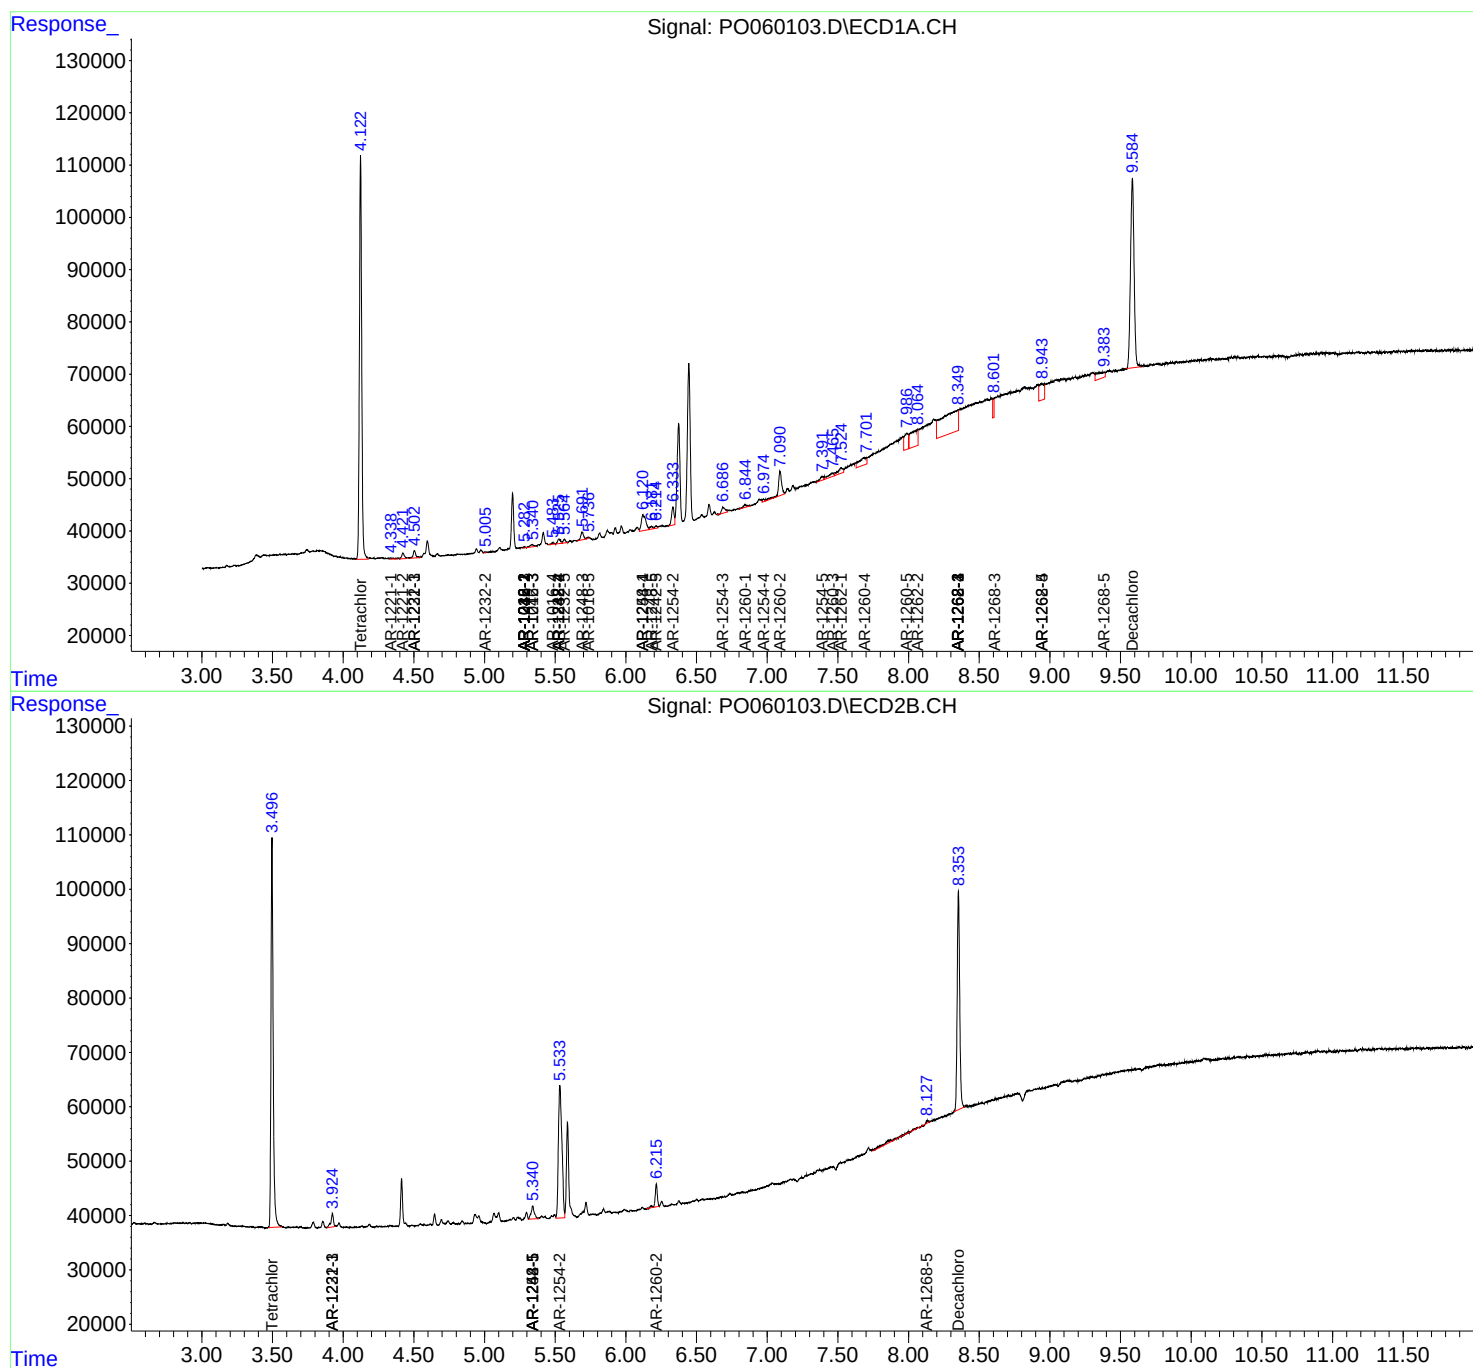


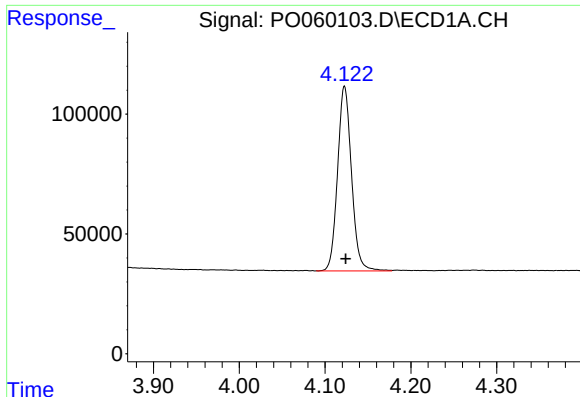

#1 Tetrachloro-m-xylene


R.T.: 4.123 min
Delta R.T.: -0.001 min
Response: 870261
Conc: 24.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

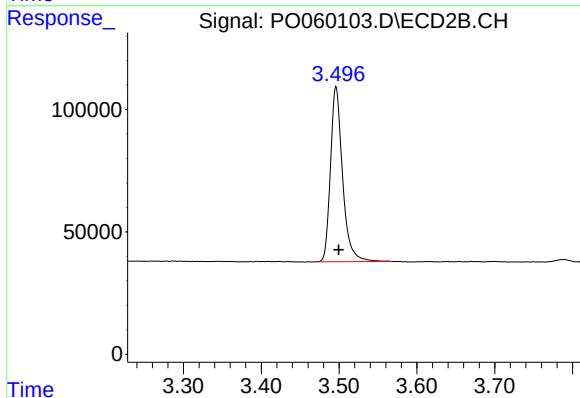


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.003 min
Response: 772351
Conc: 21.46 ng/ml

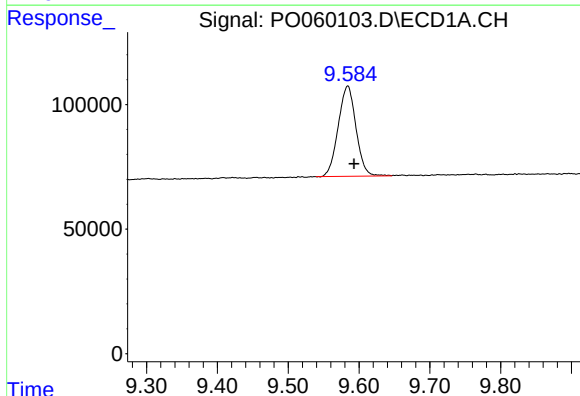


#2 Decachlorobiphenyl

R.T.: 9.584 min
Delta R.T.: -0.009 min
Response: 632994
Conc: 11.90 ng/ml

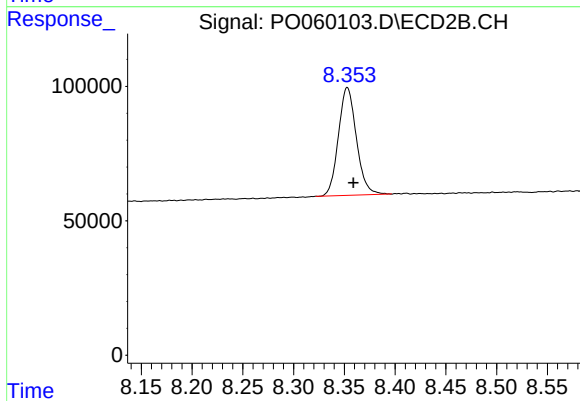

#2 Decachlorobiphenyl


R.T.: 8.353 min
Delta R.T.: -0.006 min
Response: 494330
Conc: 12.26 ng/ml

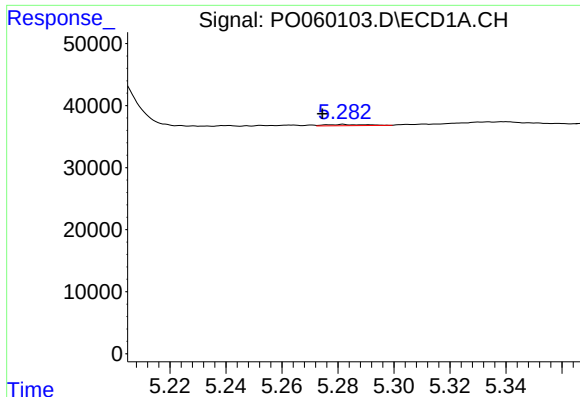

#3 AR-1016-1


R.T.: 5.282 min
Delta R.T.: 0.007 min
Response: 1878
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

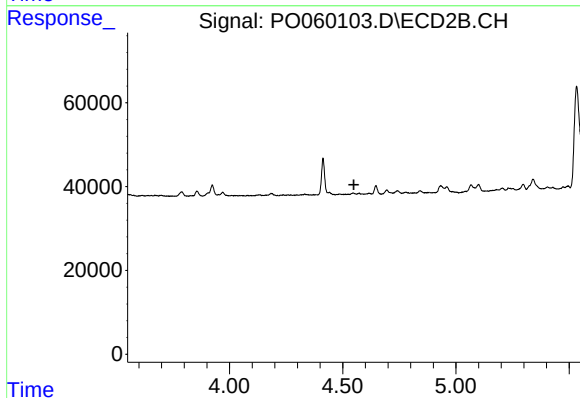


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

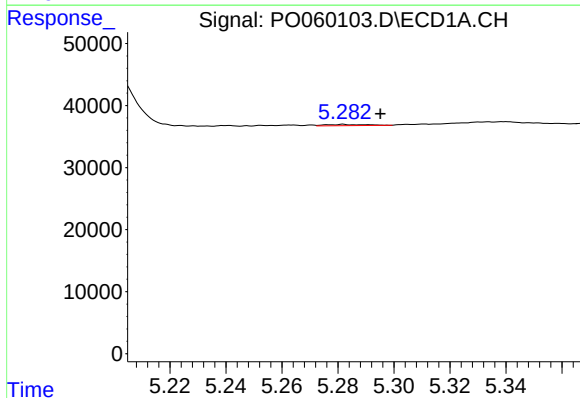


#4 AR-1016-2

R.T.: 5.282 min
Delta R.T.: -0.013 min
Response: 1878
Conc: 0.79 ng/ml

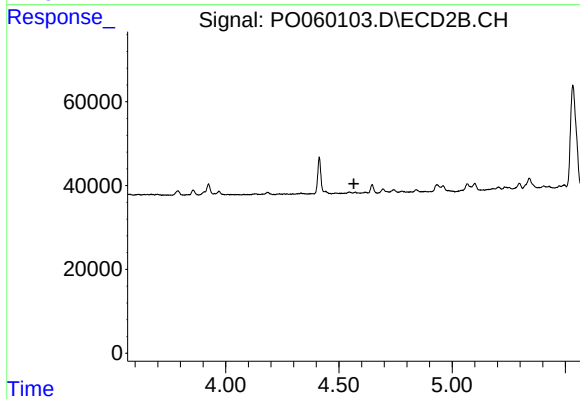

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

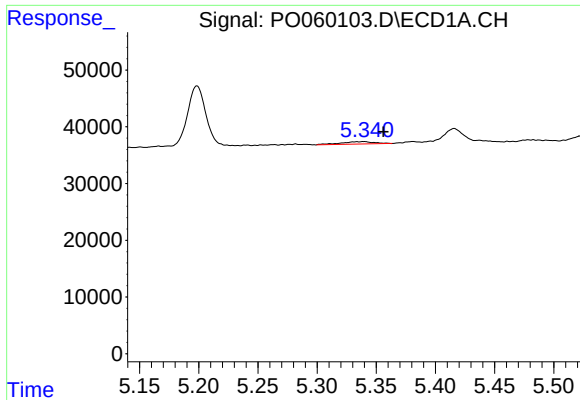

#5 AR-1016-3


R.T.: 5.339 min
Delta R.T.: -0.017 min
Response: 8360
Conc: 5.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

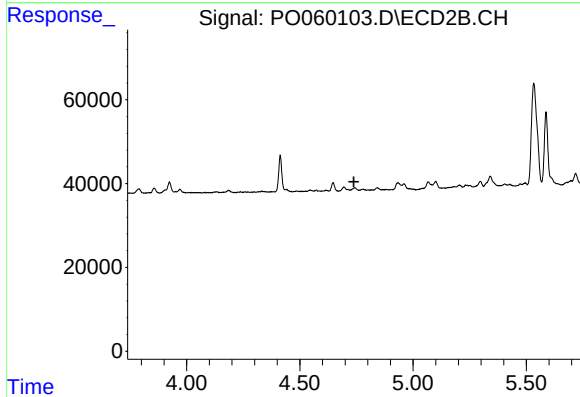


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

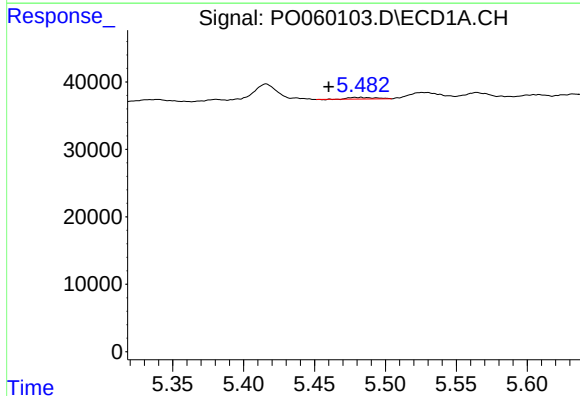


#6 AR-1016-4

R.T.: 5.482 min
Delta R.T.: 0.022 min
Response: 2901
Conc: 2.40 ng/ml

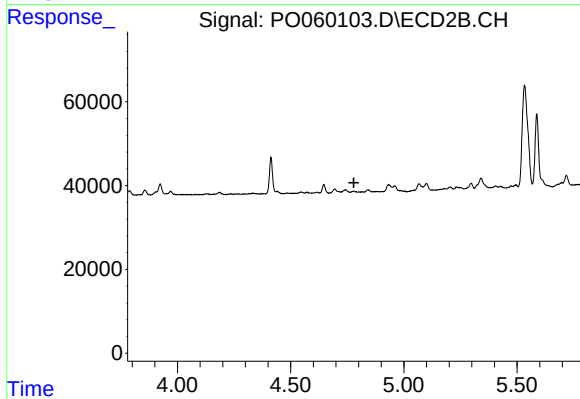

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

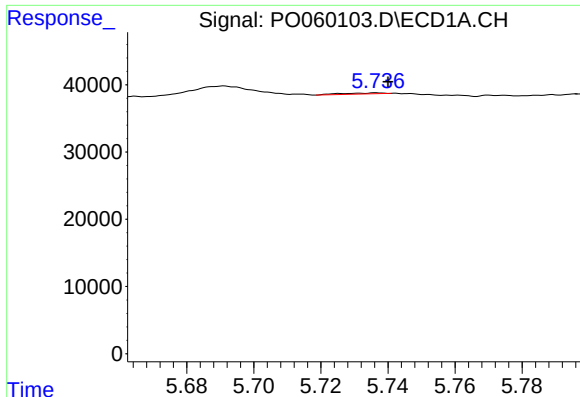

#7 AR-1016-5


R.T.: 5.737 min
Delta R.T.: -0.003 min
Response: 2115
Conc: 1.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

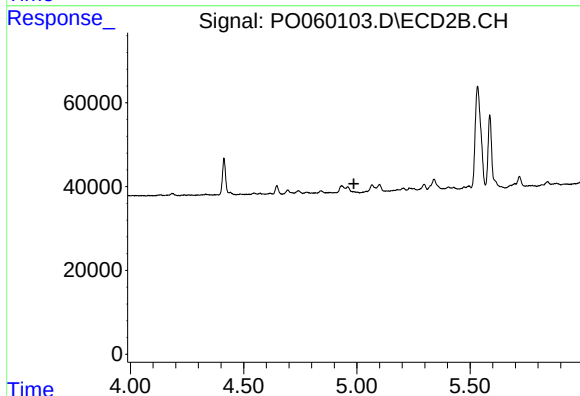


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

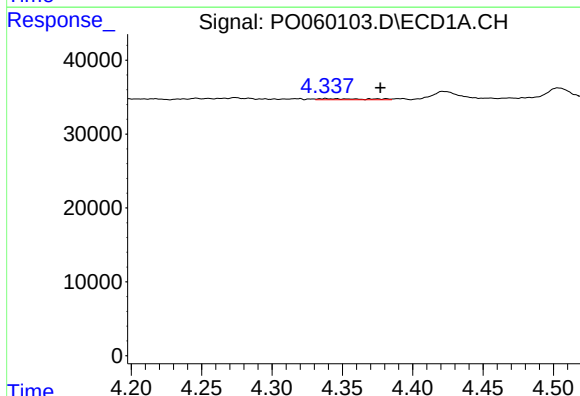


#8 AR-1221-1

R.T.: 4.338 min
Delta R.T.: -0.039 min
Response: 3604
Conc: 8.51 ng/ml

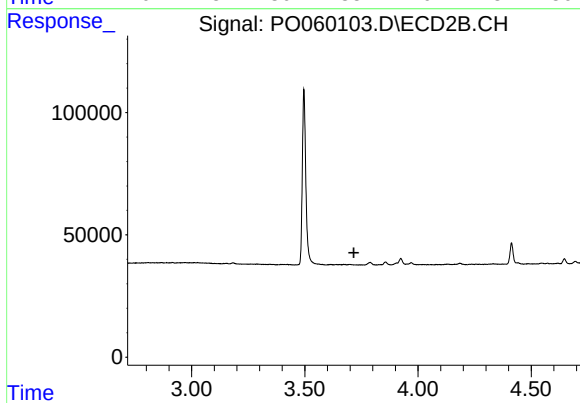

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.717 min
Response: 0
Conc: N.D.

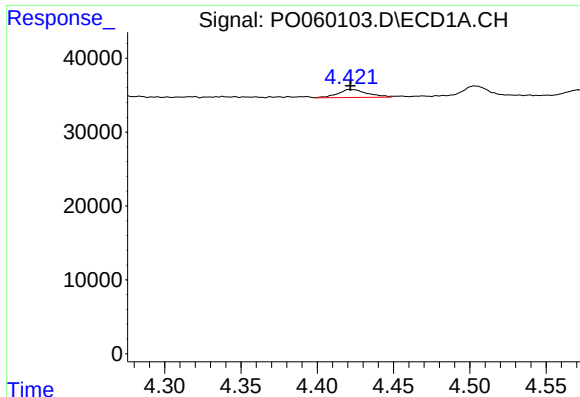

#9 AR-1221-2


R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 14386
Conc: 44.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

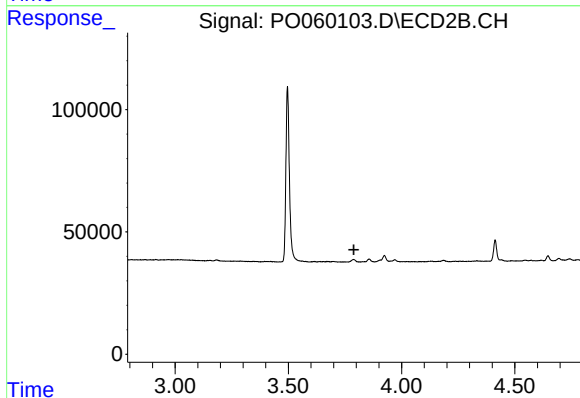


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.789 min
Response: 0
Conc: N.D.

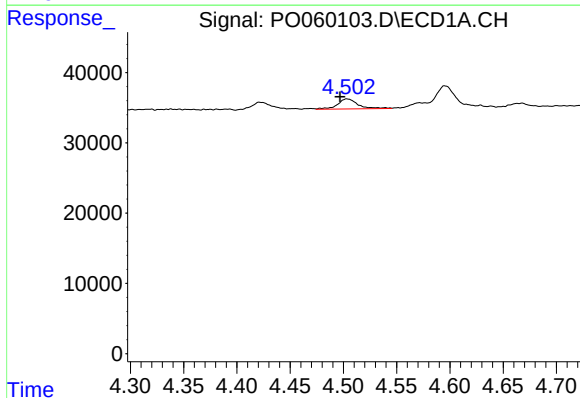


#10 AR-1221-3

R.T.: 4.504 min
Delta R.T.: 0.007 min
Response: 18906
Conc: 17.97 ng/ml

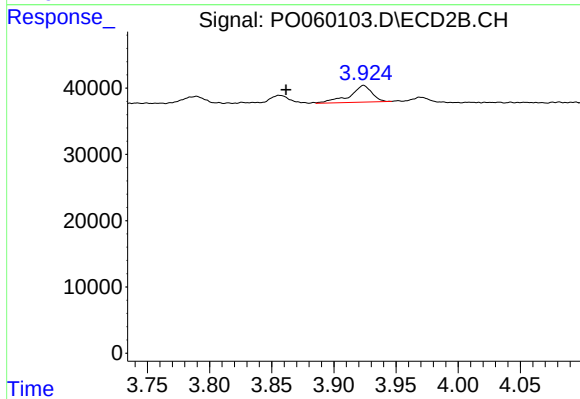

#10 AR-1221-3


R.T.: 3.924 min
Delta R.T.: 0.062 min
Response: 31127
Conc: 31.81 ng/ml

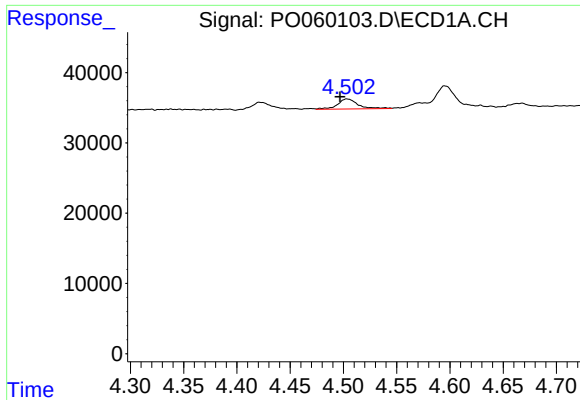

#11 AR-1232-1


R.T.: 4.504 min
Delta R.T.: 0.007 min
Response: 18906
Conc: 15.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

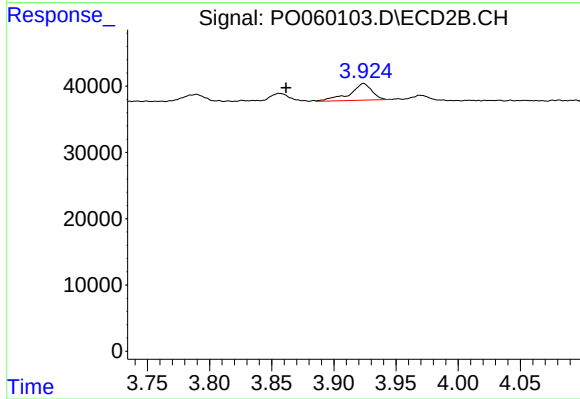


#11 AR-1232-1

R.T.: 3.924 min
Delta R.T.: 0.062 min
Response: 31127
Conc: 27.30 ng/ml

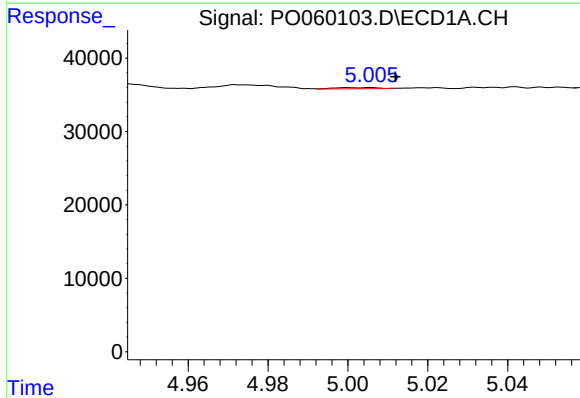


#12 AR-1232-2

R.T.: 5.006 min
Delta R.T.: -0.006 min
Response: 1249
Conc: 1.77 ng/ml

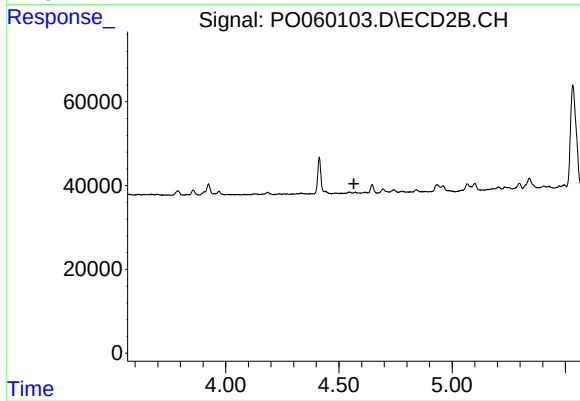

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

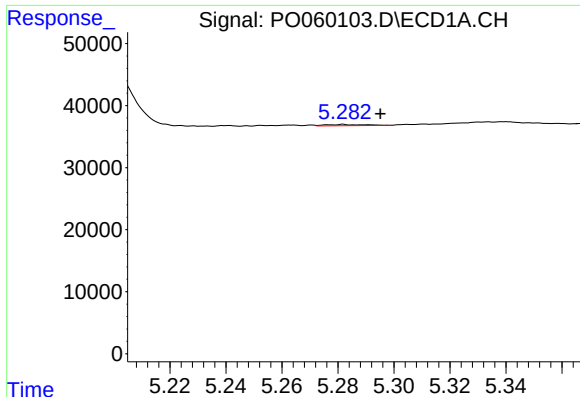

#13 AR-1232-3


R.T.: 5.282 min
Delta R.T.: -0.013 min
Response: 1878
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

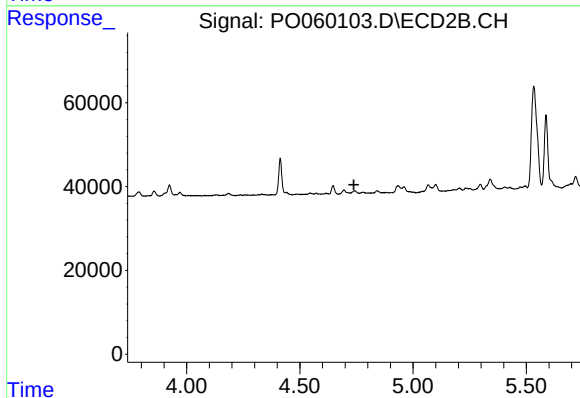


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

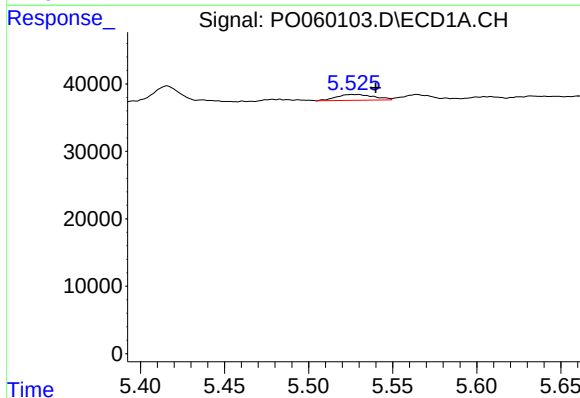


#14 AR-1232-4

R.T.: 5.526 min
Delta R.T.: -0.014 min
Response: 13177
Conc: 16.85 ng/ml

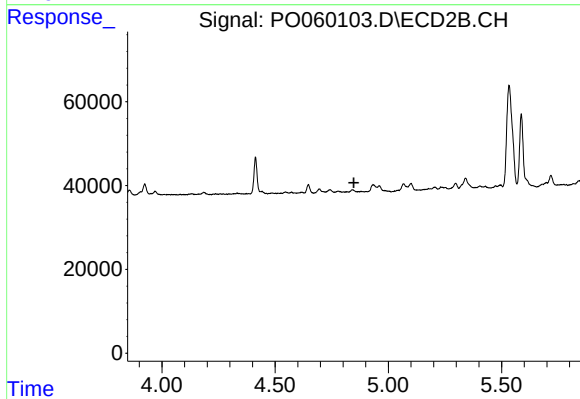

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

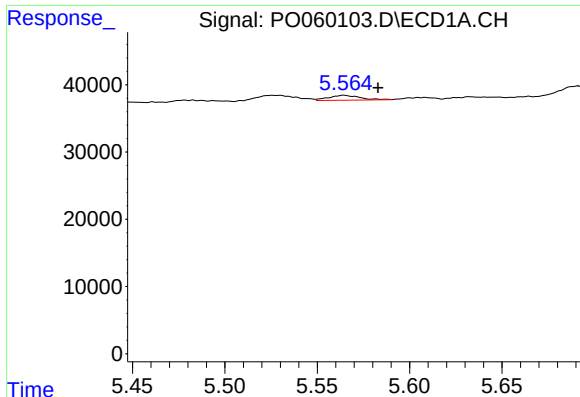

#15 AR-1232-5


R.T.: 5.564 min
Delta R.T.: -0.019 min
Response: 8609
Conc: 14.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

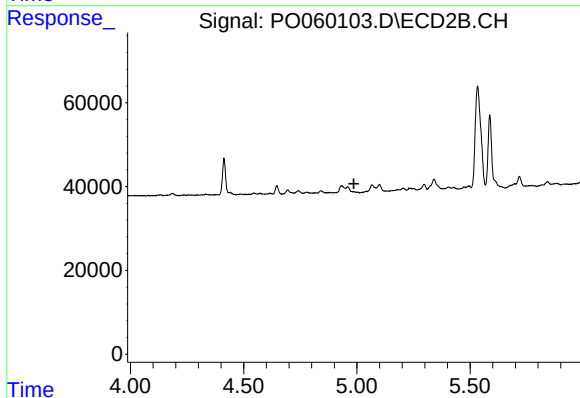


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

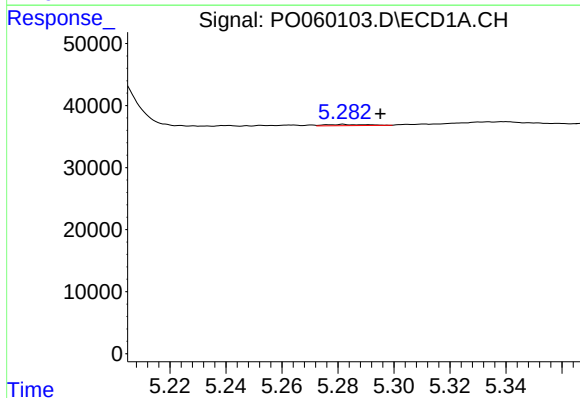


#16 AR-1242-1

R.T.: 5.282 min
Delta R.T.: -0.013 min
Response: 1878
Conc: 1.48 ng/ml

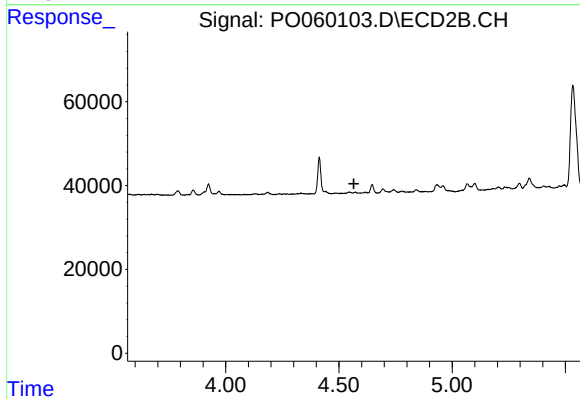

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

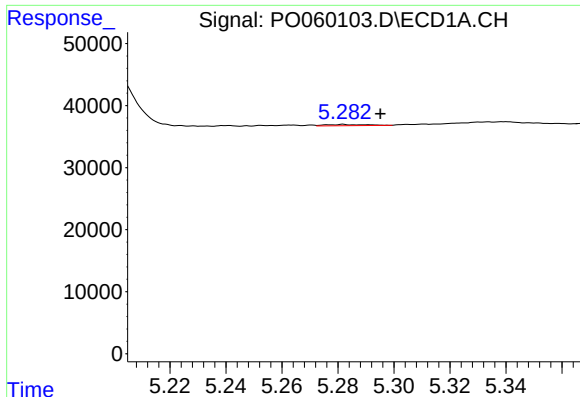

#17 AR-1242-2


R.T.: 5.282 min
Delta R.T.: -0.013 min
Response: 1878
Conc: 1.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

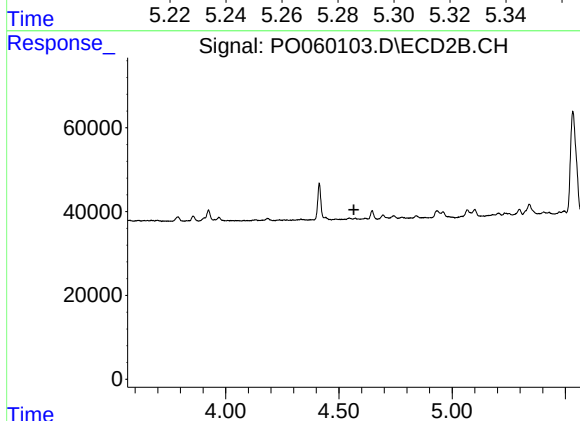


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

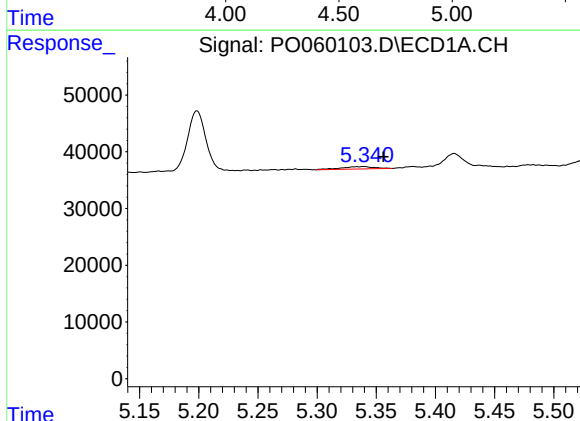


#18 AR-1242-3

R.T.: 5.339 min
Delta R.T.: -0.017 min
Response: 8360
Conc: 7.15 ng/ml

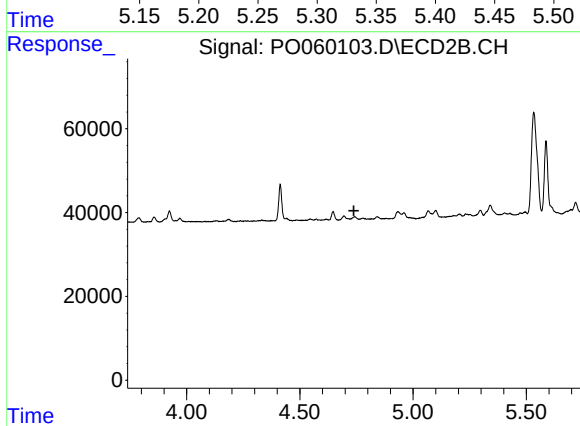

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

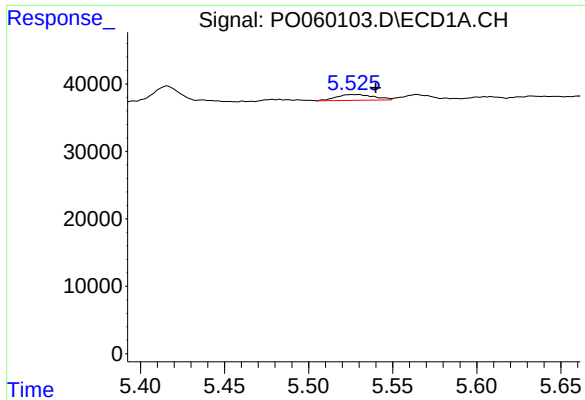

#19 AR-1242-4


R.T.: 5.526 min
Delta R.T.: -0.014 min
Response: 13177
Conc: 13.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

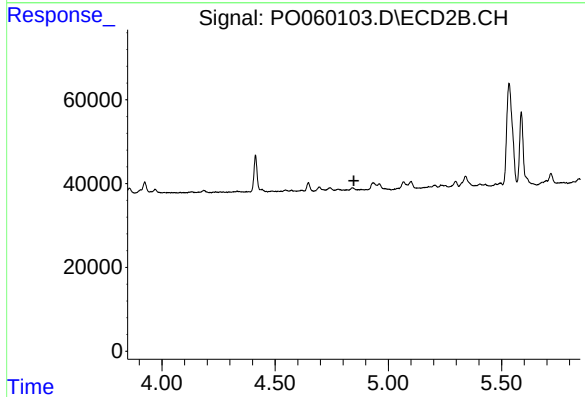


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

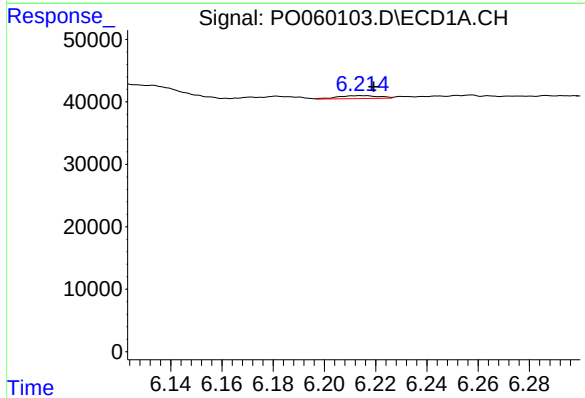


#20 AR-1242-5

R.T.: 6.215 min
Delta R.T.: -0.005 min
Response: 5372
Conc: 4.27 ng/ml

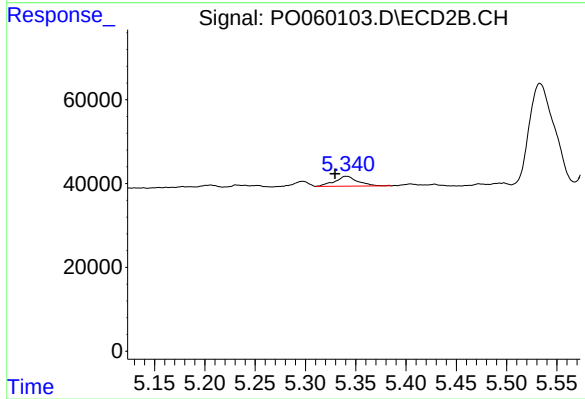

#20 AR-1242-5


R.T.: 5.341 min
Delta R.T.: 0.011 min
Response: 37627
Conc: 33.64 ng/ml

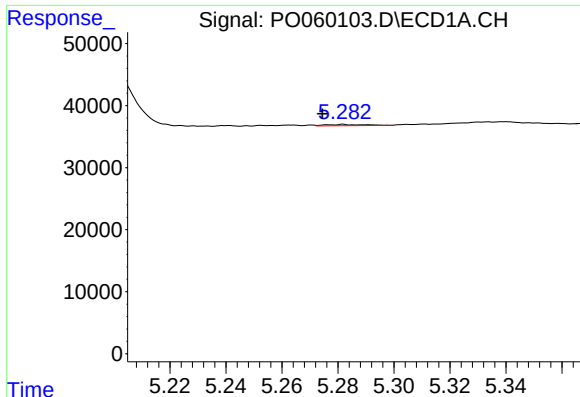

#21 AR-1248-1


R.T.: 5.282 min
Delta R.T.: 0.007 min
Response: 1878
Conc: 1.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

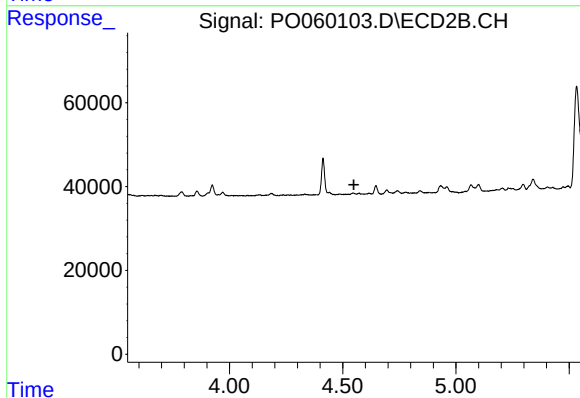


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

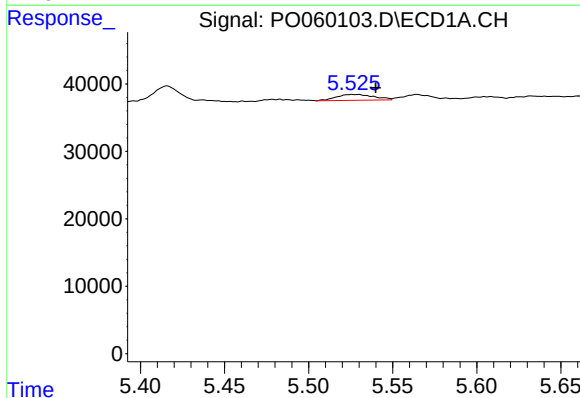


#22 AR-1248-2

R.T.: 5.526 min
Delta R.T.: -0.014 min
Response: 13177
Conc: 9.08 ng/ml

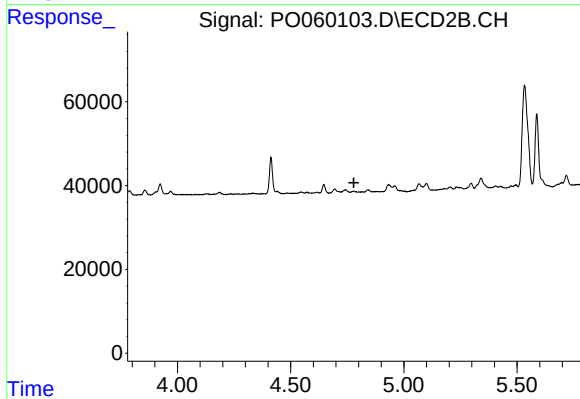

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

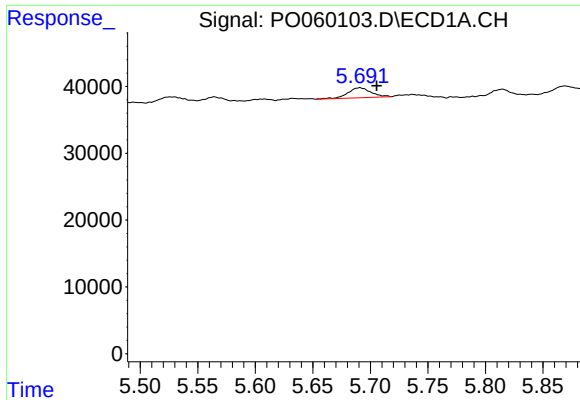

#23 AR-1248-3


R.T.: 5.691 min
Delta R.T.: -0.015 min
Response: 21246
Conc: 12.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

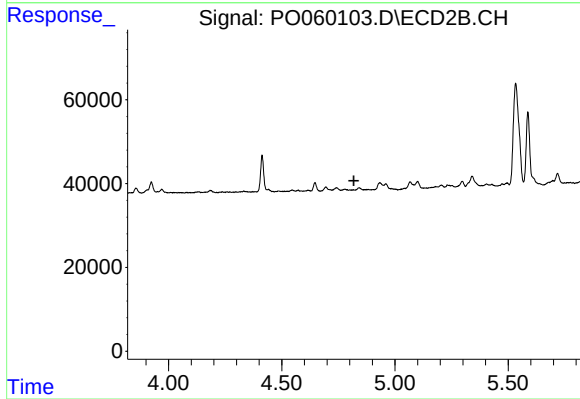


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

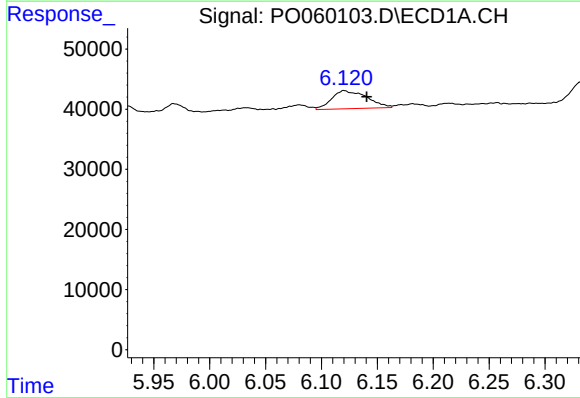


#24 AR-1248-4

R.T.: 6.120 min
Delta R.T.: -0.020 min
Response: 66193
Conc: 32.38 ng/ml

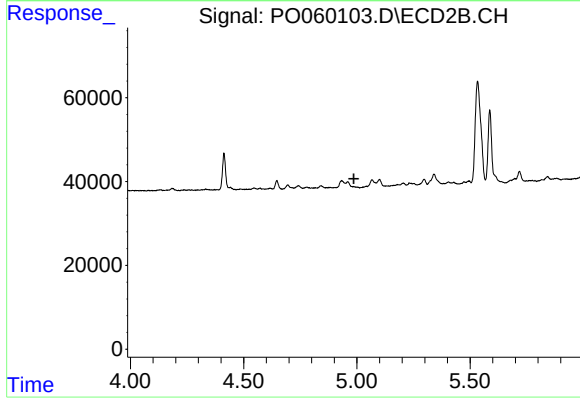

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

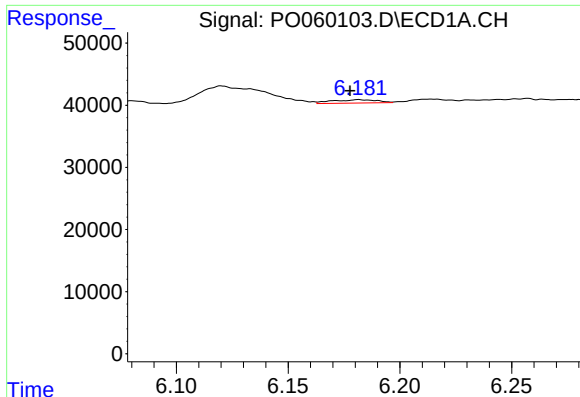

#25 AR-1248-5


R.T.: 6.181 min
Delta R.T.: 0.004 min
Response: 7564
Conc: 3.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

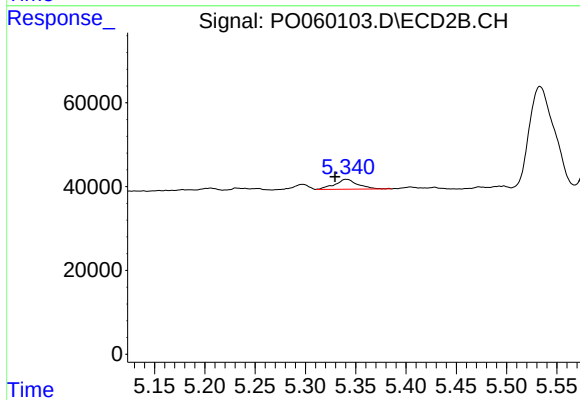


#25 AR-1248-5

R.T.: 5.341 min
Delta R.T.: 0.011 min
Response: 37627
Conc: 26.29 ng/ml

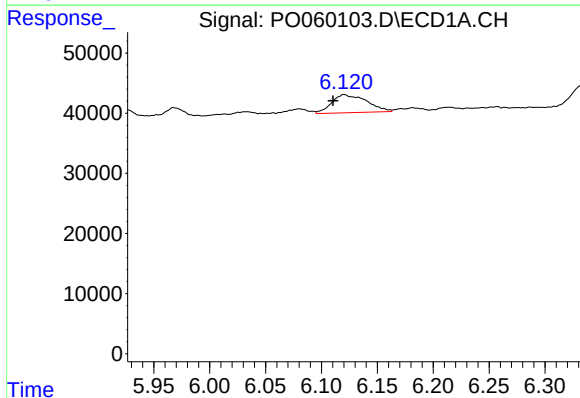


#26 AR-1254-1

R.T.: 6.120 min
Delta R.T.: 0.010 min
Response: 66193
Conc: 31.73 ng/ml

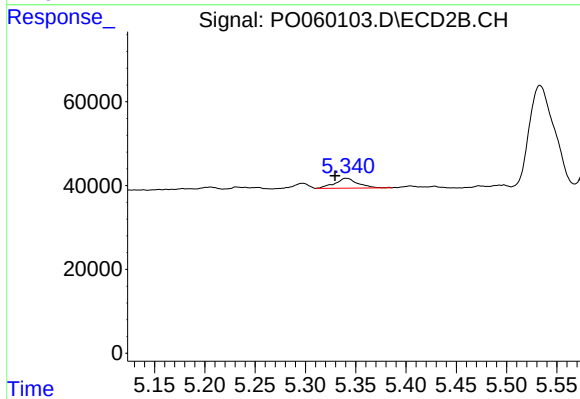

#26 AR-1254-1


R.T.: 5.341 min
Delta R.T.: 0.011 min
Response: 37627
Conc: 15.86 ng/ml

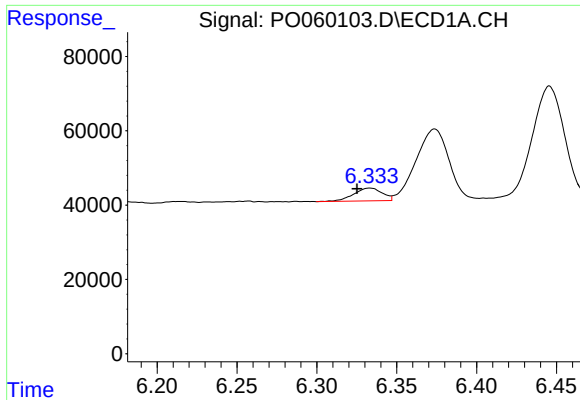

#27 AR-1254-2


R.T.: 6.333 min
Delta R.T.: 0.008 min
Response: 42786
Conc: 12.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

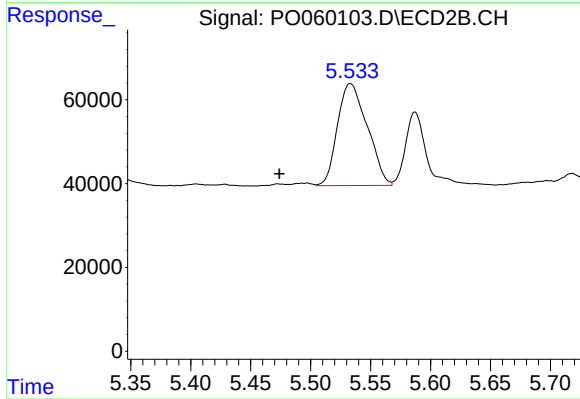


#27 AR-1254-2

R.T.: 5.533 min
Delta R.T.: 0.059 min
Response: 421247
Conc: 200.76 ng/ml

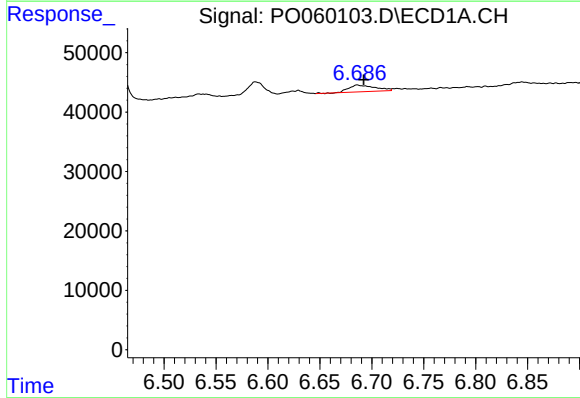


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 19583
Conc: 5.52 ng/ml

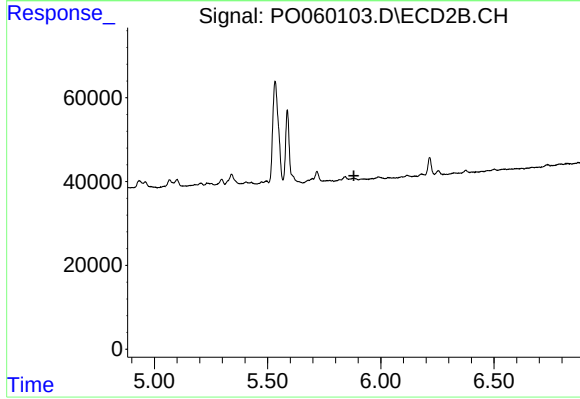

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 5.881 min
Response: 0
Conc: N.D.

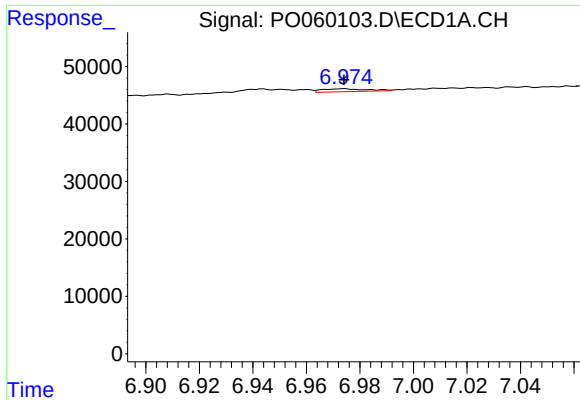

#29 AR-1254-4


R.T.: 6.974 min
Delta R.T.: 0.000 min
Response: 5873
Conc: 1.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

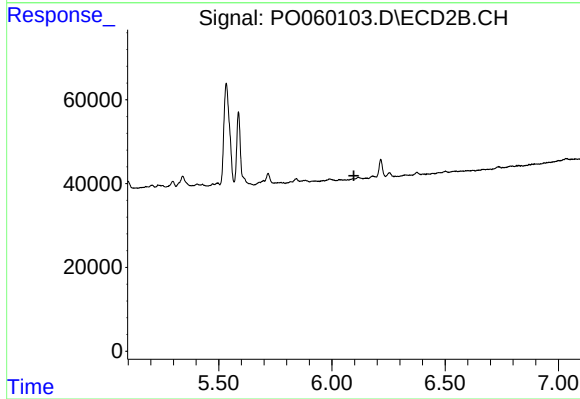


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

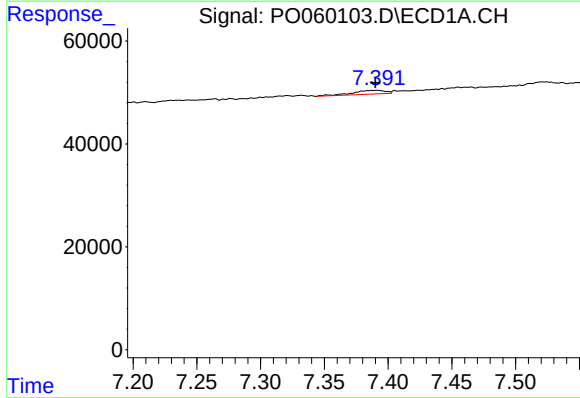


#30 AR-1254-5

R.T.: 7.391 min
Delta R.T.: 0.000 min
Response: 13463
Conc: 4.35 ng/ml

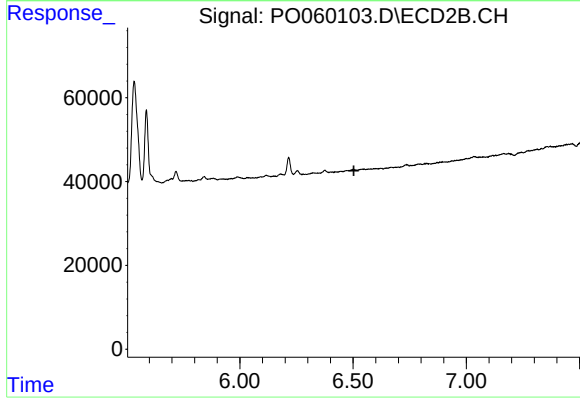

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.503 min
Response: 0
Conc: N.D.

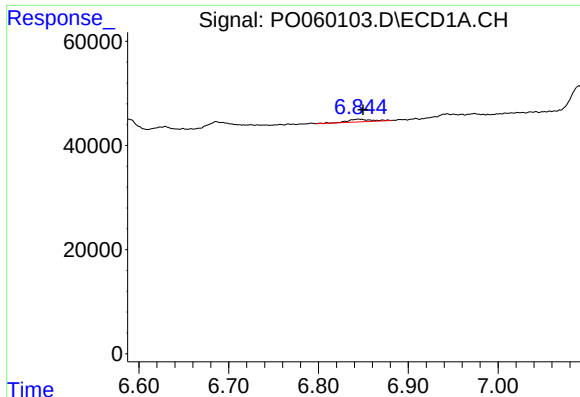

#31 AR-1260-1


R.T.: 6.845 min
Delta R.T.: -0.005 min
Response: 9434
Conc: 3.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

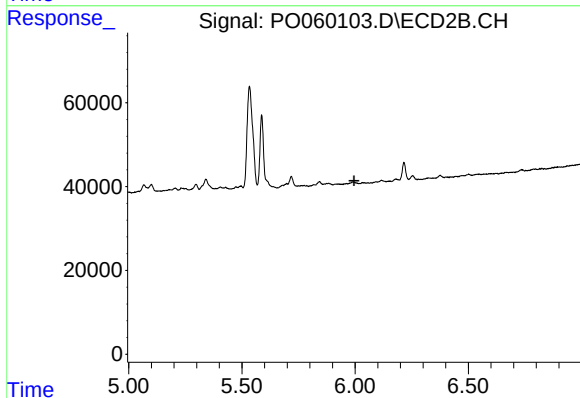


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.

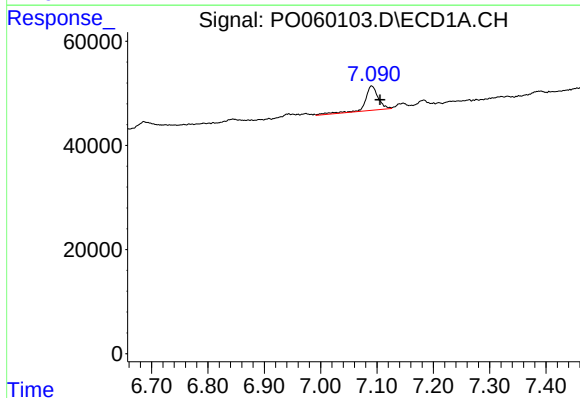


#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.015 min
Response: 74062
Conc: 19.96 ng/ml

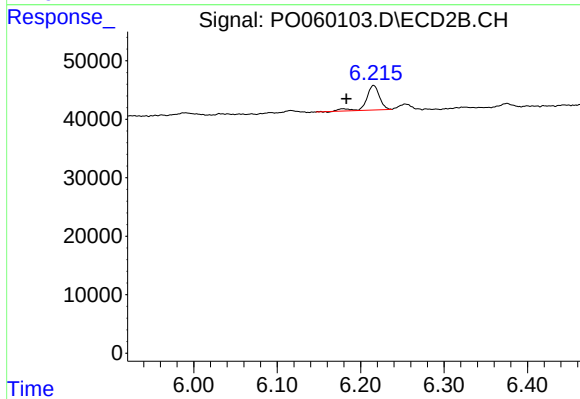

#32 AR-1260-2


R.T.: 6.216 min
Delta R.T.: 0.033 min
Response: 45560
Conc: 15.55 ng/ml

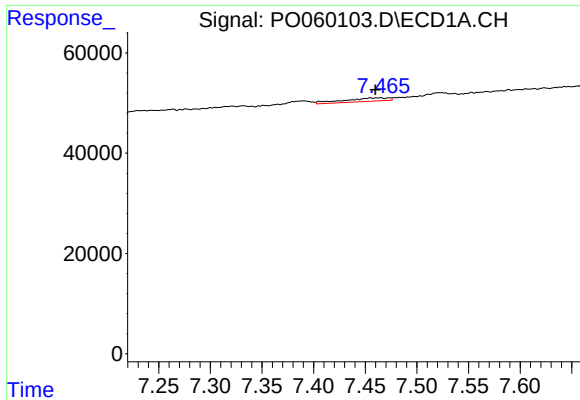

#33 AR-1260-3


R.T.: 7.455 min
Delta R.T.: -0.004 min
Response: 20664
Conc: 6.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

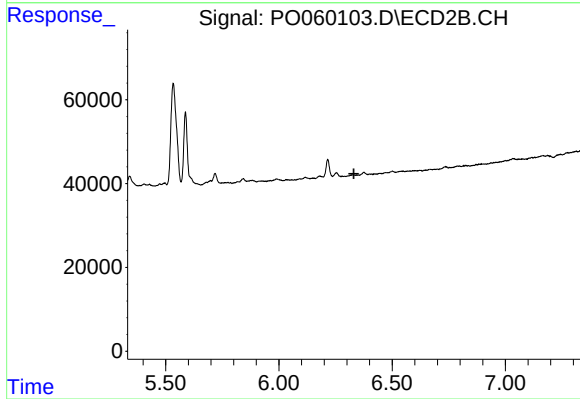


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

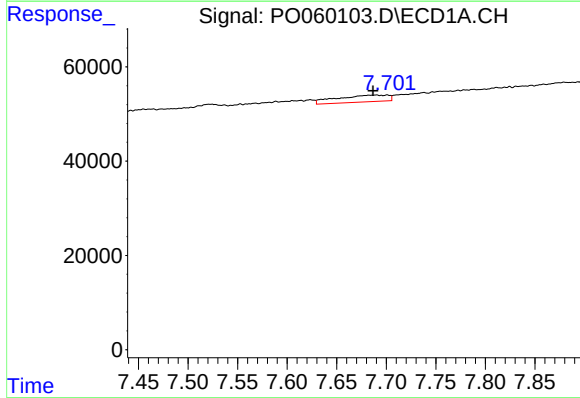


#34 AR-1260-4

R.T.: 7.690 min
Delta R.T.: 0.003 min
Response: 52608
Conc: 17.13 ng/ml

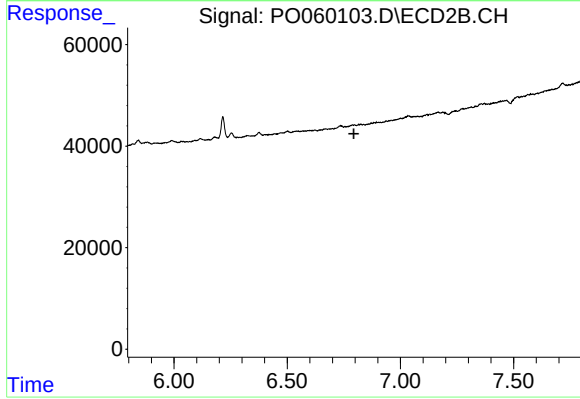

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

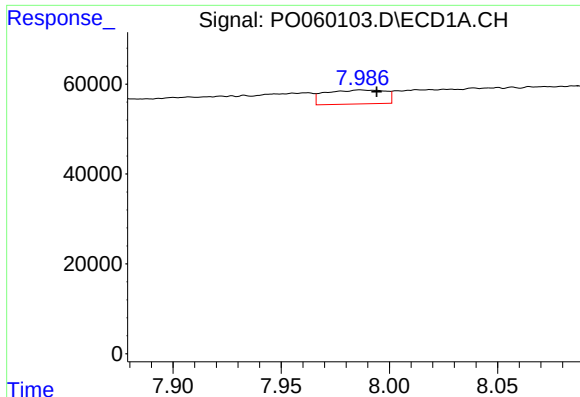

#35 AR-1260-5


R.T.: 7.987 min
Delta R.T.: -0.007 min
Response: 59800
Conc: 8.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

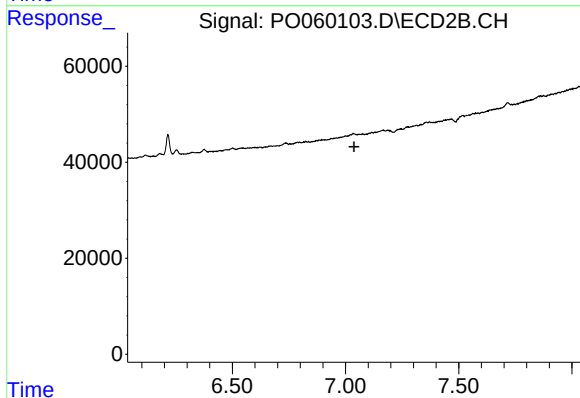


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

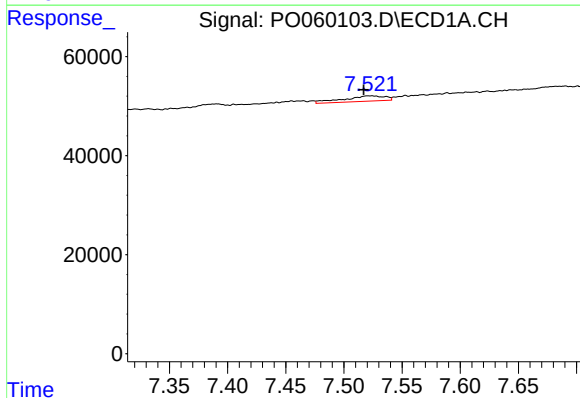


#36 AR-1262-1

R.T.: 7.523 min
Delta R.T.: 0.006 min
Response: 26590
Conc: 5.48 ng/ml

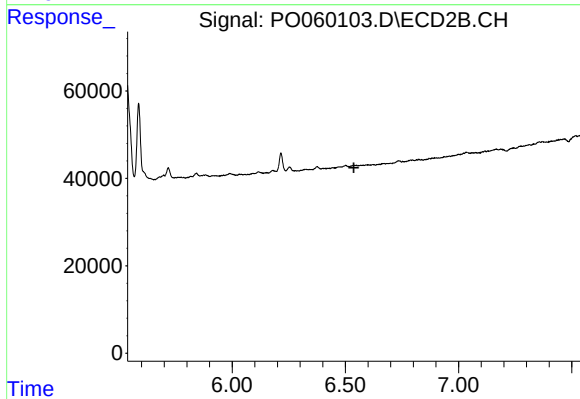

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.538 min
Response: 0
Conc: N.D.

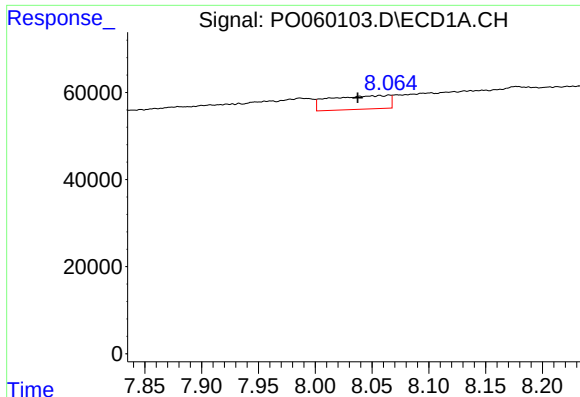

#37 AR-1262-2


R.T.: 8.057 min
Delta R.T.: 0.019 min
Response: 114289
Conc: 14.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

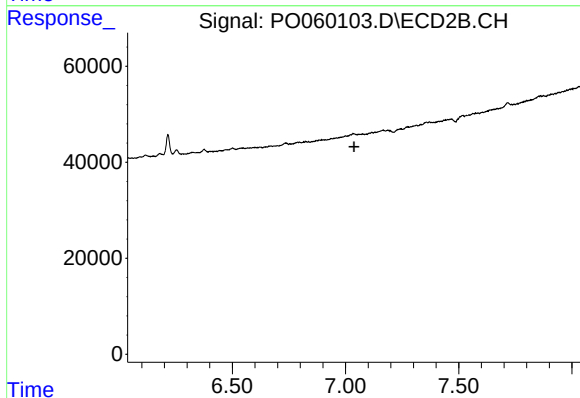


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

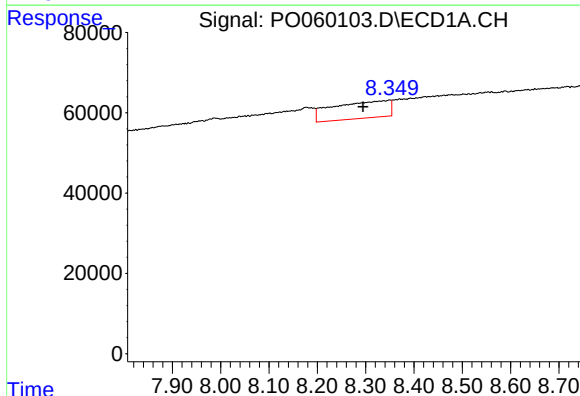


#38 AR-1262-3

R.T.: 8.350 min
Delta R.T.: 0.055 min
Response: 346594
Conc: 67.93 ng/ml

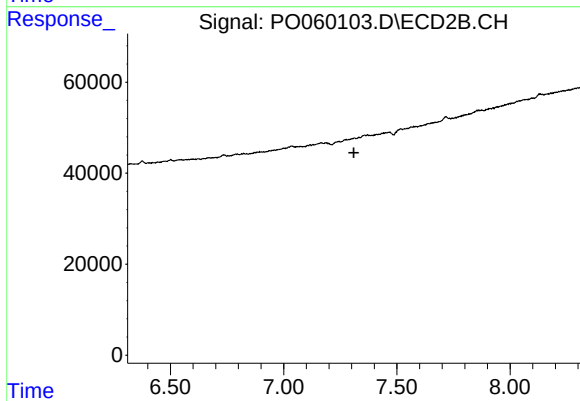

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

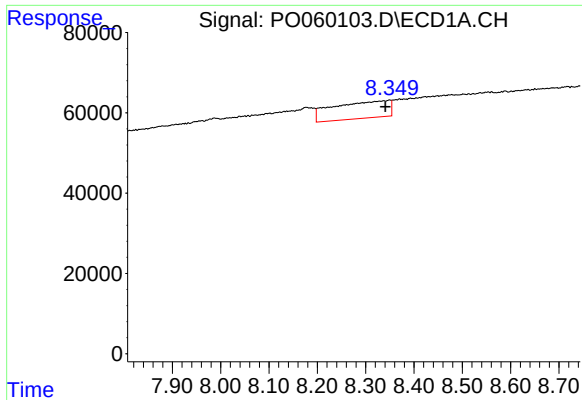

#39 AR-1262-4


R.T.: 8.350 min
Delta R.T.: 0.009 min
Response: 346594
Conc: 89.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

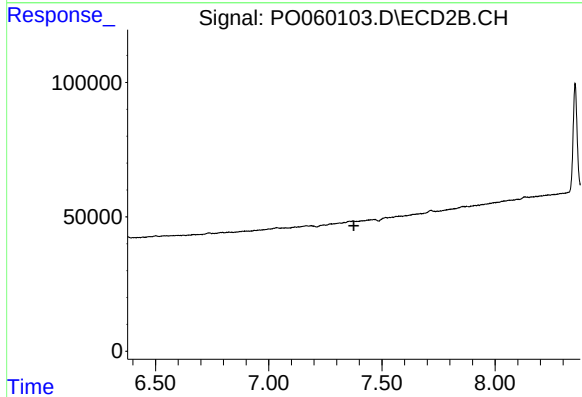


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.376 min
Response: 0
Conc: N.D.

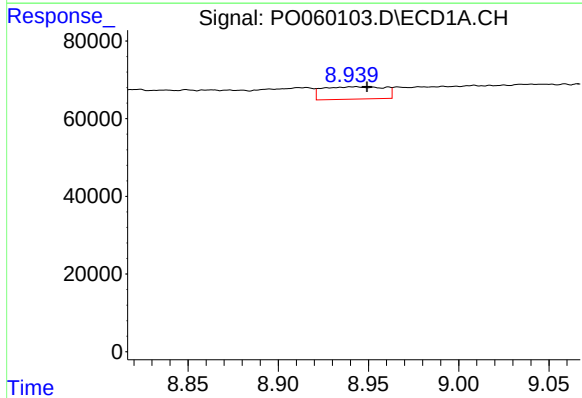


#40 AR-1262-5

R.T.: 8.942 min
Delta R.T.: -0.007 min
Response: 75155
Conc: 29.28 ng/ml

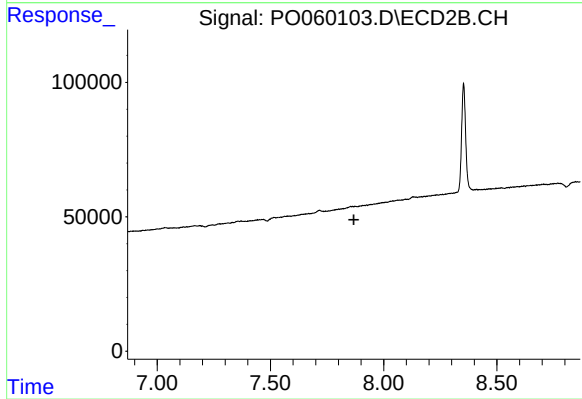

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 7.868 min
Response: 0
Conc: N.D.

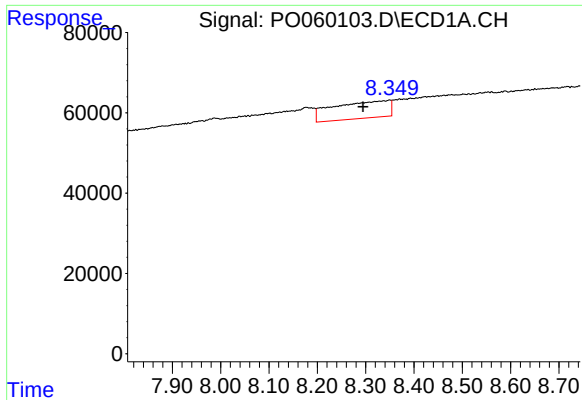

#41 AR-1268-1


R.T.: 8.350 min
Delta R.T.: 0.055 min
Response: 346594
Conc: 36.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

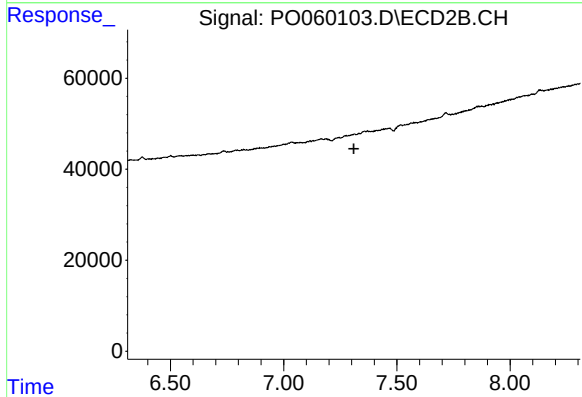


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

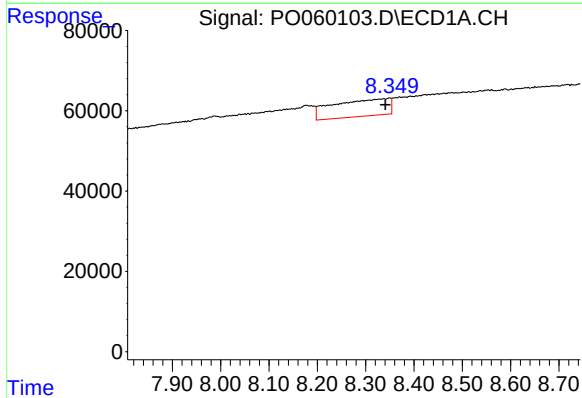


#42 AR-1268-2

R.T.: 8.350 min
Delta R.T.: 0.009 min
Response: 346594
Conc: 43.97 ng/ml

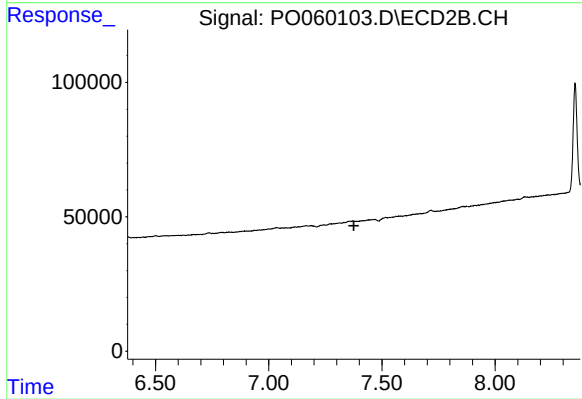

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.376 min
Response: 0
Conc: N.D.

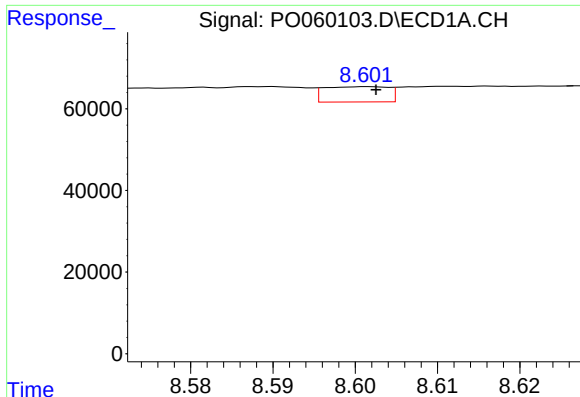

#43 AR-1268-3


R.T.: 8.601 min
Delta R.T.: -0.001 min
Response: 20286
Conc: 2.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

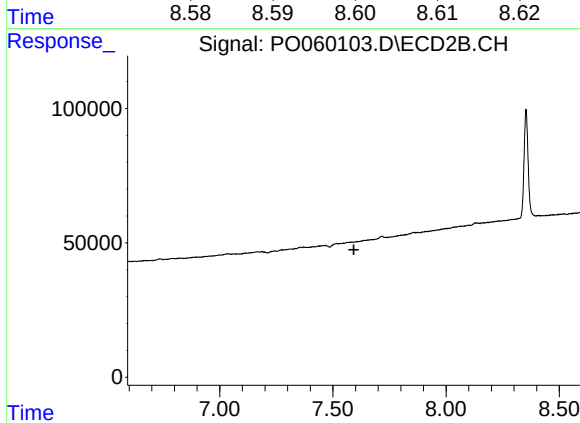


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

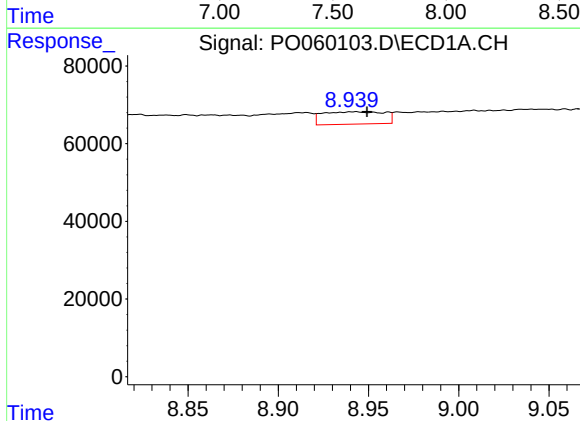


#44 AR-1268-4

R.T.: 8.942 min
Delta R.T.: -0.007 min
Response: 75155
Conc: 27.03 ng/ml

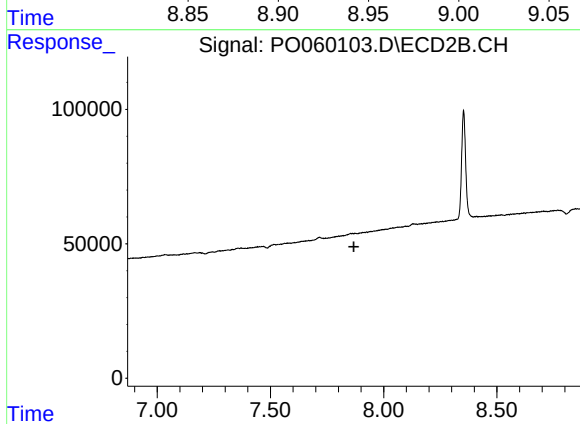

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.868 min
Response: 0
Conc: N.D.

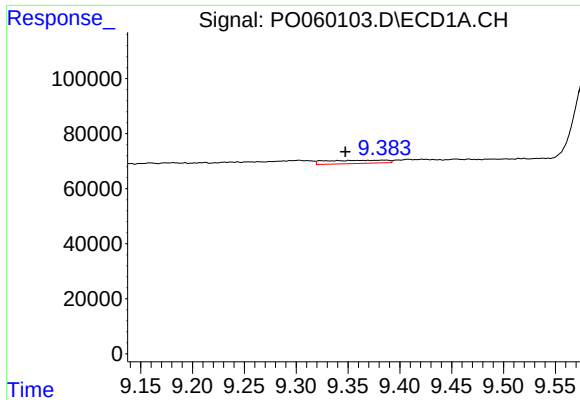

#45 AR-1268-5

R.T.: 9.383 min
Delta R.T.: 0.036 min
Response: 47829
Conc: 2.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

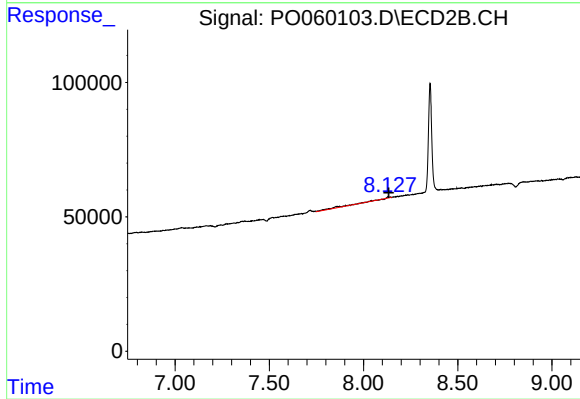

#45 AR-1268-5

R.T.: 8.132 min
Delta R.T.: -0.003 min
Response: 28934
Conc: 1.99 ng/ml