

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060129.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 1:19
 Operator : SM/AJ
 Sample : K4619-18
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP6-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 01:46:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.120	3.495	972394	925673	27.773	25.716
2)	SA Decachlor...	9.578	8.350	993251	802373	18.670	19.900
Target Compounds							
3)	L1 AR-1016-1	5.253	0.000	2947	0	1.837	N.D. #
4)	L1 AR-1016-2	5.298	0.000	2929	0	1.224	N.D. #
5)	L1 AR-1016-3	5.344	0.000	4016	0	2.696	N.D. #
6)	L1 AR-1016-4	5.462	0.000	480	0	0.397	N.D. #
7)	L1 AR-1016-5	5.731	0.000	1523	0	1.186	N.D. #
8)	L2 AR-1221-1	4.376	3.686	445	19867	1.050	49.497 #
9)	L2 AR-1221-2	4.423	0.000	21959	0	67.610	N.D. #
10)	L2 AR-1221-3	4.494	3.922	24385	22365	23.182	22.857
11)	L3 AR-1232-1	4.494	3.922	24385	22365	19.564	19.616
12)	L3 AR-1232-2	5.010	0.000	1549	0	2.194	N.D. #
13)	L3 AR-1232-3	5.298	0.000	2929	0	1.912	N.D. #
14)	L3 AR-1232-4	5.541	0.000	2124	0	2.717	N.D. #
15)	L3 AR-1232-5	5.569	0.000	675	0	1.122	N.D. #
16)	L4 AR-1242-1	5.298	0.000	2929	0	2.307	N.D. #
17)	L4 AR-1242-2	5.298	0.000	2929	0	1.578	N.D. #
18)	L4 AR-1242-3	5.344	0.000	4016	0	3.436	N.D. #
19)	L4 AR-1242-4	5.541	0.000	2124	0	2.195	N.D. #
20)	L4 AR-1242-5	6.221	0.000	1386	0	1.103	N.D. #
21)	L5 AR-1248-1	5.253	0.000	2947	0	2.940	N.D. #
22)	L5 AR-1248-2	5.541	0.000	2124	0	1.464	N.D. #
23)	L5 AR-1248-3	5.731	0.000	1523	0	0.917	N.D. #
24)	L5 AR-1248-4	6.133	0.000	3604	0	1.763	N.D. #
25)	L5 AR-1248-5	6.179	0.000	2827	0	1.425	N.D. #
26)	L6 AR-1254-1	6.133	0.000	3604	0	1.727	N.D. #
27)	L6 AR-1254-2	6.324	0.000	4892	0	1.466	N.D. #
28)	L6 AR-1254-3	6.723	0.000	5529	0	1.558	N.D. #
29)	L6 AR-1254-4	6.943	0.000	1652	0	0.561	N.D. #
30)	L6 AR-1254-5	7.336	0.000	5851	0	1.892	N.D. #
31)	L7 AR-1260-1	6.861	0.000	4542	0	1.685	N.D. #
32)	L7 AR-1260-2	7.107	0.000	4266	0	1.150	N.D. #
33)	L7 AR-1260-3	7.463	0.000	20036	0	6.115	N.D. #
34)	L7 AR-1260-4	7.703	0.000	38941	0	12.679	N.D. #
35)	L7 AR-1260-5	7.990	0.000	247372	0	34.935	N.D. #
36)	L8 AR-1262-1	7.524	0.000	14935	0	3.077	N.D. #
37)	L8 AR-1262-2	7.990	0.000	247372	0	32.060	N.D. #
38)	L8 AR-1262-3	8.296	0.000	244447	0	47.909	N.D. #
39)	L8 AR-1262-4	8.331	0.000	70660	0	18.331	N.D. #
40)	L8 AR-1262-5	8.952	0.000	103313	0	40.254	N.D. #
41)	L9 AR-1268-1	8.296	0.000	244447	0	25.976	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060129.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 1:19
 Operator : SM/AJ
 Sample : K4619-18
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP6-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 01:46:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
42)	L9 AR-1268-2	8.331	0.000	70660	0	8.964	N.D.	#
43)	L9 AR-1268-3	8.590	0.000	284658	0	40.384	N.D.	#
44)	L9 AR-1268-4	8.952	0.000	103313	0	37.162	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083019\
Data File : PO060129.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 1:19
Operator : SM/AJ
Sample : K4619-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 01:46:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

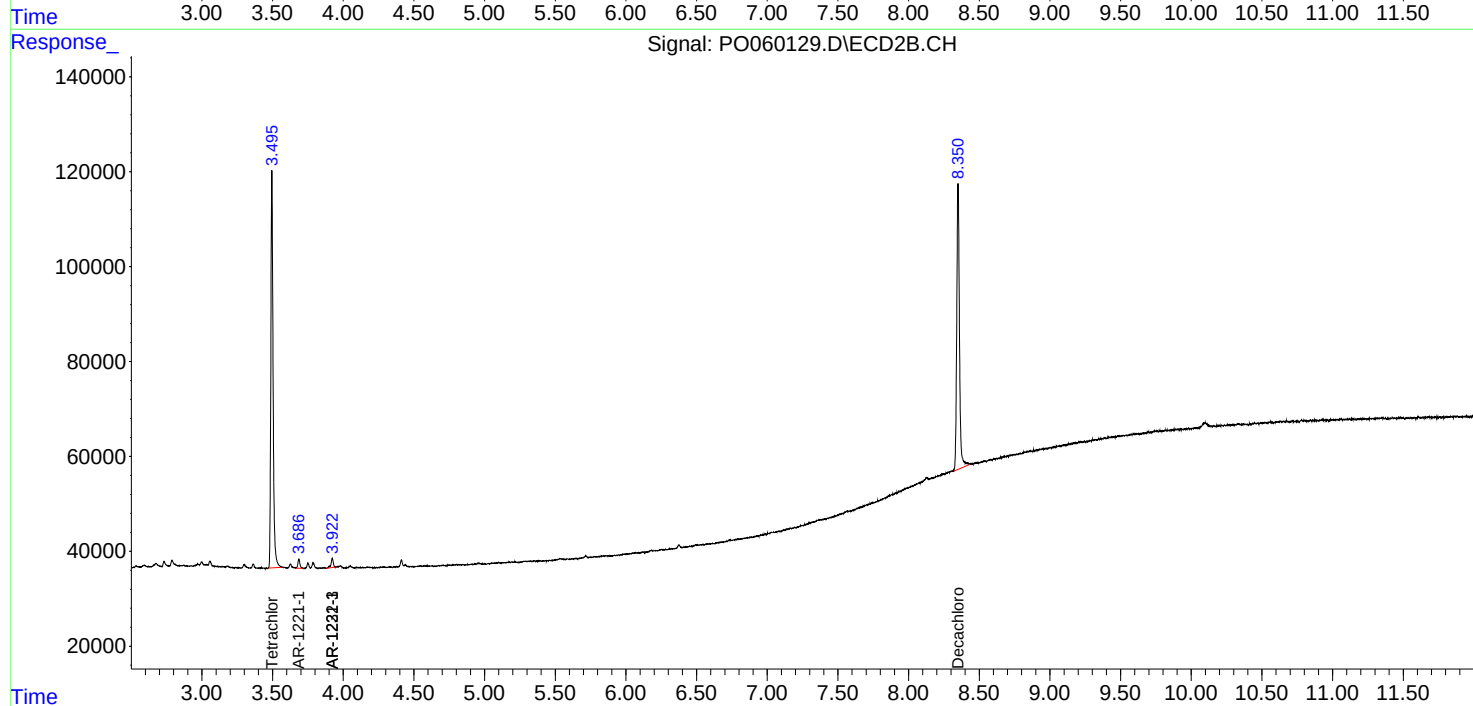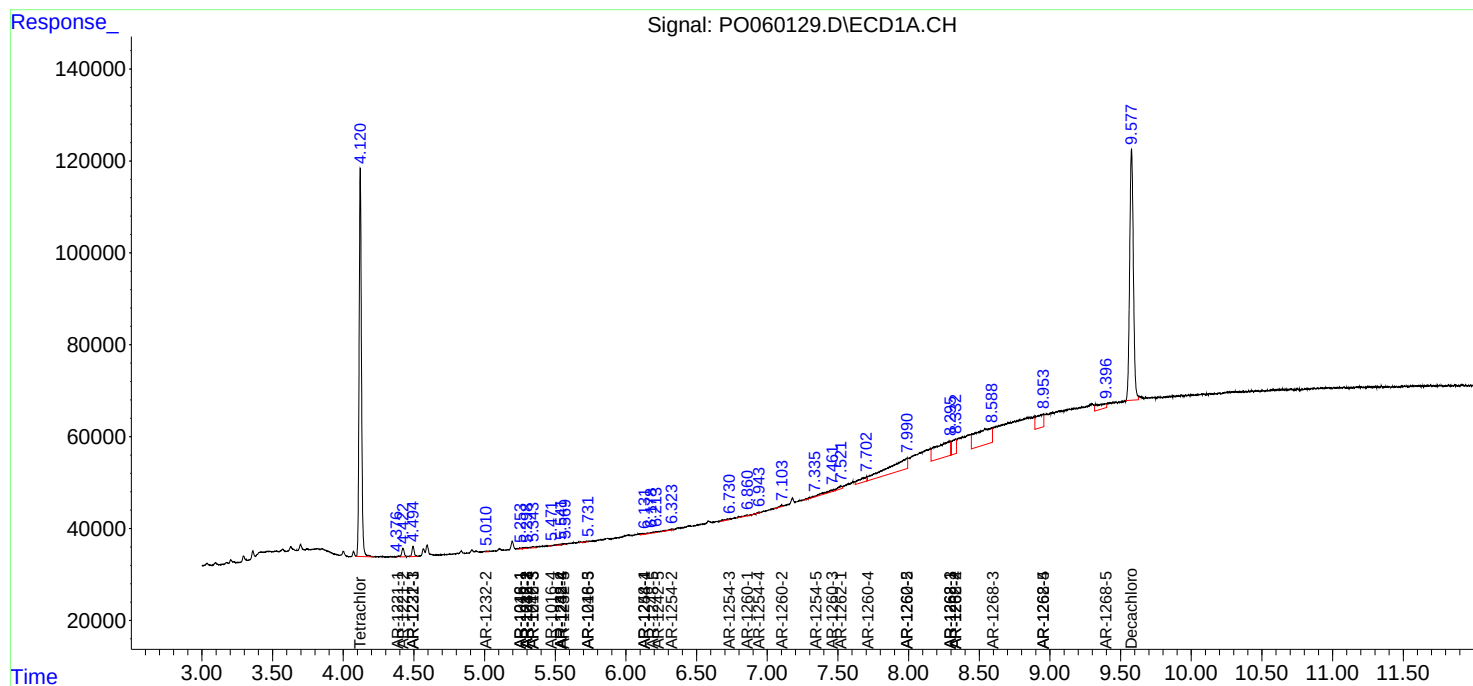


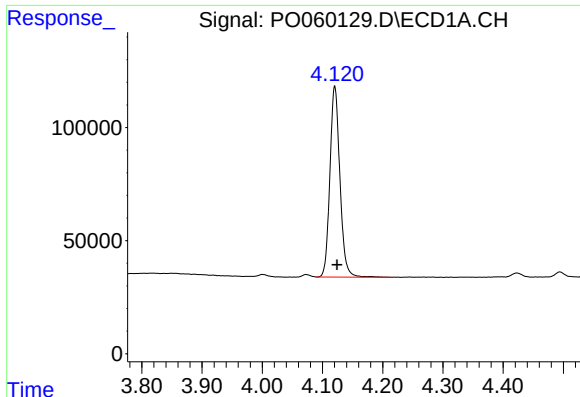

#1 Tetrachloro-m-xylene


R.T.: 4.120 min
Delta R.T.: -0.004 min
Response: 972394
Conc: 27.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

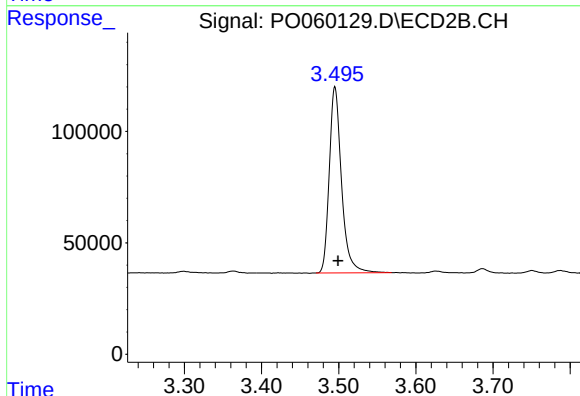


#1 Tetrachloro-m-xylene

R.T.: 3.495 min
Delta R.T.: -0.004 min
Response: 925673
Conc: 25.72 ng/ml

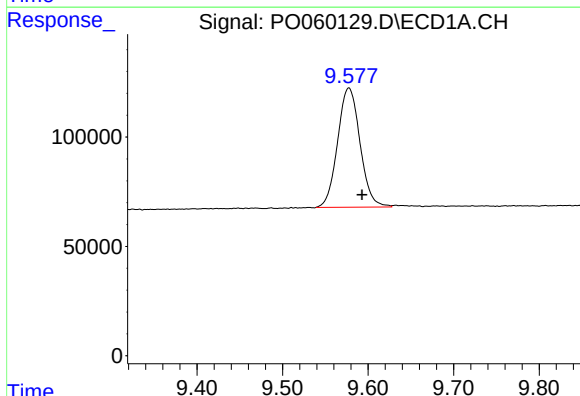


#2 Decachlorobiphenyl

R.T.: 9.578 min
Delta R.T.: -0.016 min
Response: 993251
Conc: 18.67 ng/ml

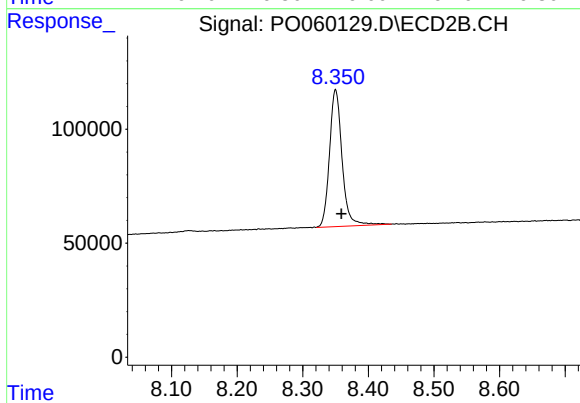

#2 Decachlorobiphenyl


R.T.: 8.350 min
Delta R.T.: -0.009 min
Response: 802373
Conc: 19.90 ng/ml

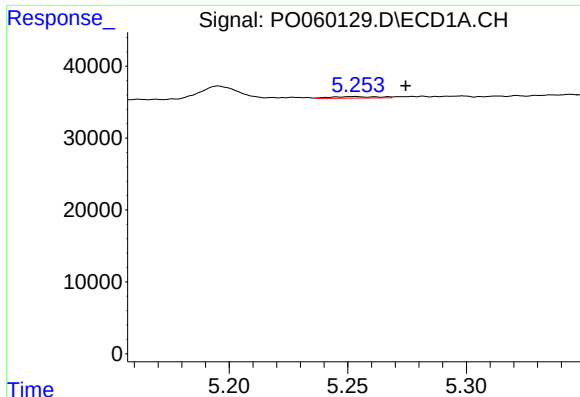

#3 AR-1016-1


R.T.: 5.253 min
Delta R.T.: -0.022 min
Response: 2947
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

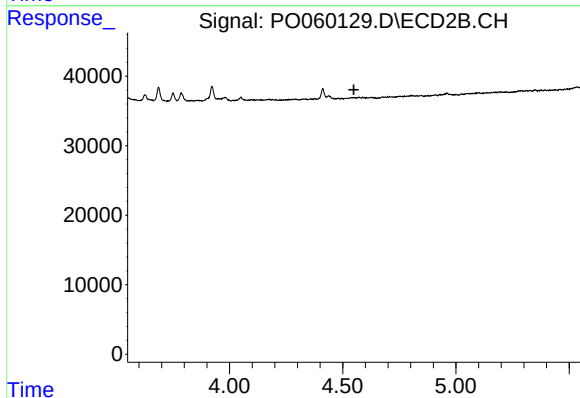


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

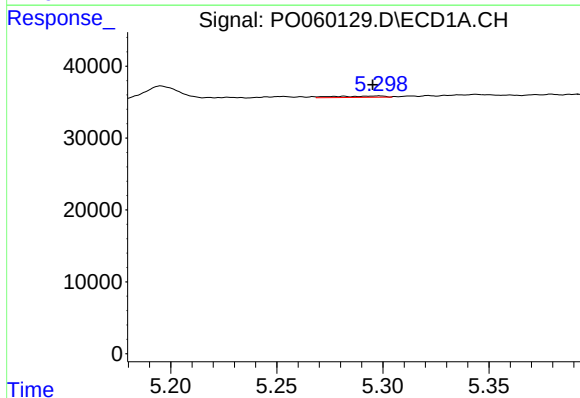


#4 AR-1016-2

R.T.: 5.298 min
Delta R.T.: 0.003 min
Response: 2929
Conc: 1.22 ng/ml

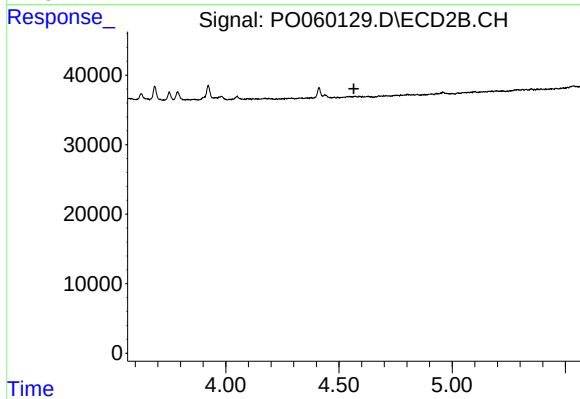

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

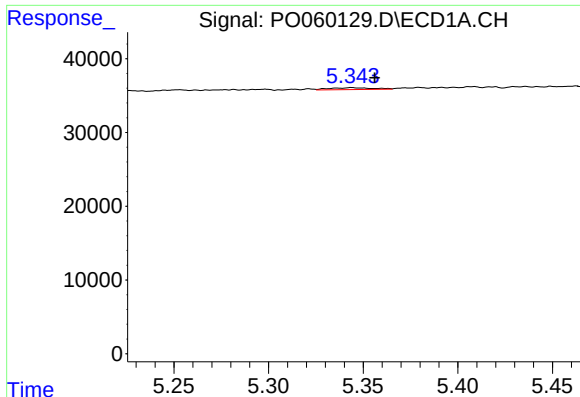

#5 AR-1016-3


R.T.: 5.344 min
Delta R.T.: -0.012 min
Response: 4016
Conc: 2.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

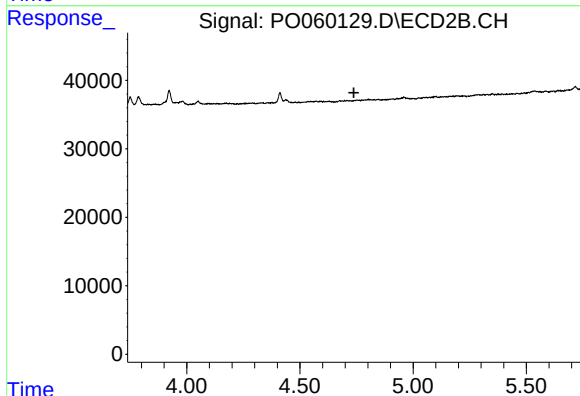


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

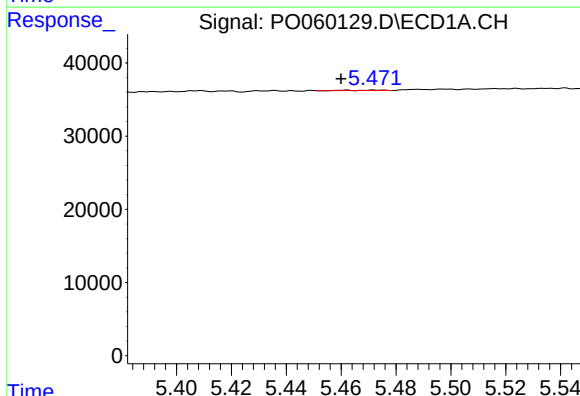


#6 AR-1016-4

R.T.: 5.462 min
Delta R.T.: 0.002 min
Response: 480
Conc: 0.40 ng/ml

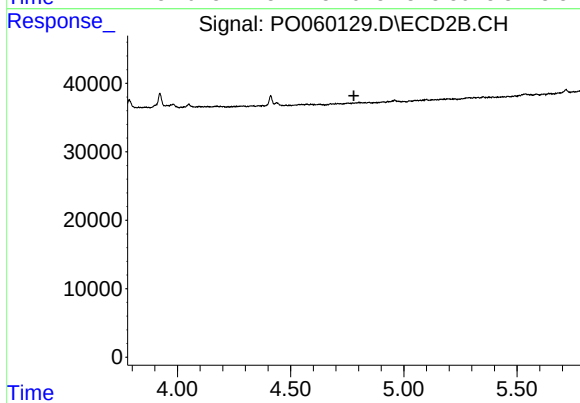

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

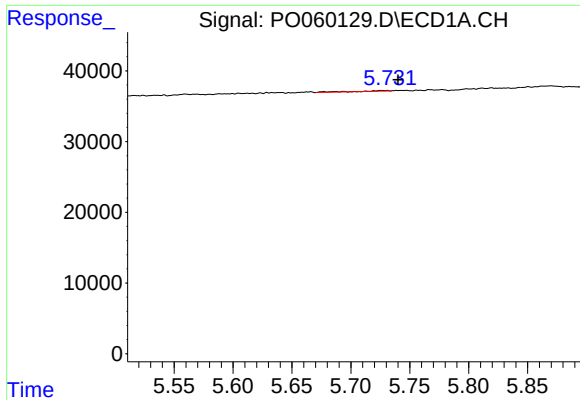

#7 AR-1016-5


R.T.: 5.731 min
Delta R.T.: -0.009 min
Response: 1523
Conc: 1.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

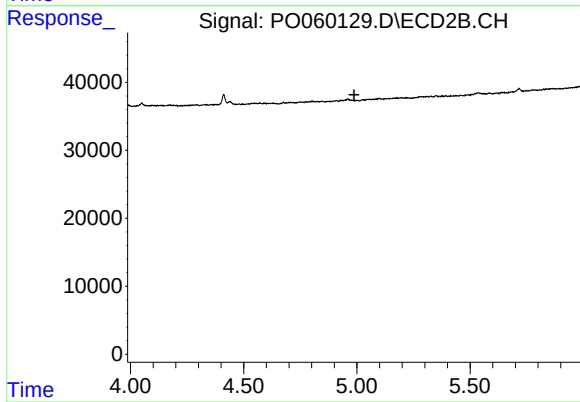


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

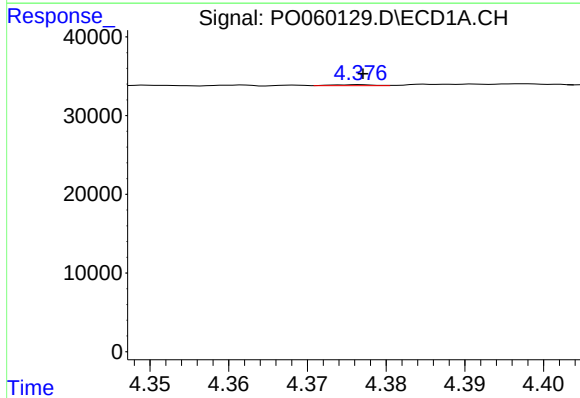


#8 AR-1221-1

R.T.: 4.376 min
Delta R.T.: 0.000 min
Response: 445
Conc: 1.05 ng/ml

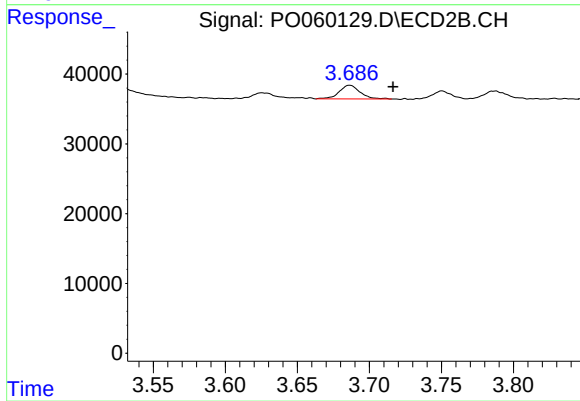

#8 AR-1221-1


R.T.: 3.686 min
Delta R.T.: -0.030 min
Response: 19867
Conc: 49.50 ng/ml

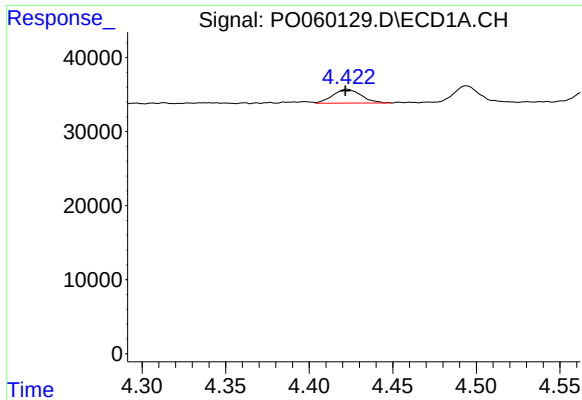

#9 AR-1221-2


R.T.: 4.423 min
Delta R.T.: 0.000 min
Response: 21959
Conc: 67.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

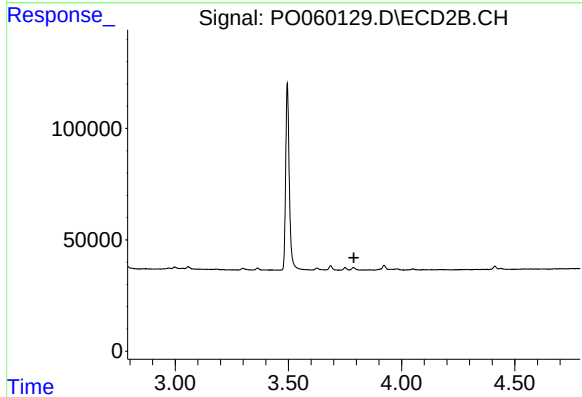


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.789 min
Response: 0
Conc: N.D.

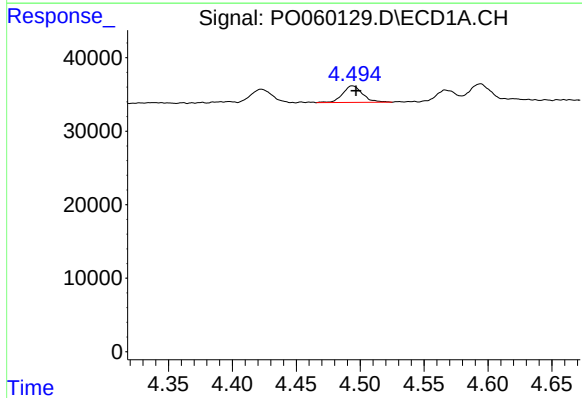


#10 AR-1221-3

R.T.: 4.494 min
Delta R.T.: -0.003 min
Response: 24385
Conc: 23.18 ng/ml

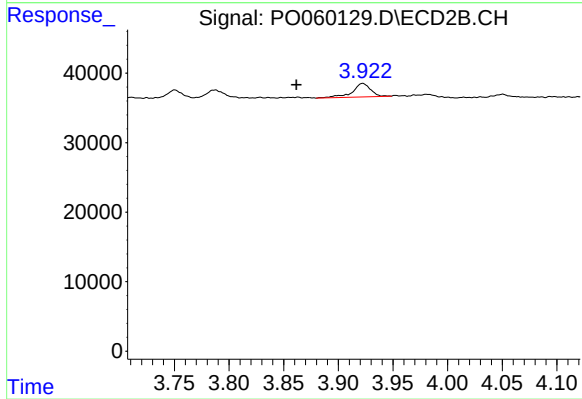

#10 AR-1221-3


R.T.: 3.922 min
Delta R.T.: 0.061 min
Response: 22365
Conc: 22.86 ng/ml

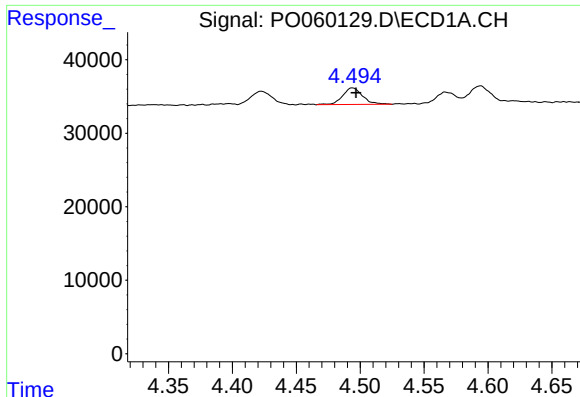

#11 AR-1232-1


R.T.: 4.494 min
Delta R.T.: -0.003 min
Response: 24385
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

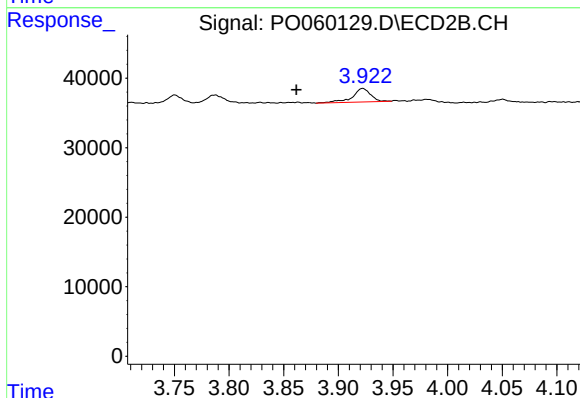


#11 AR-1232-1

R.T.: 3.922 min
Delta R.T.: 0.061 min
Response: 22365
Conc: 19.62 ng/ml

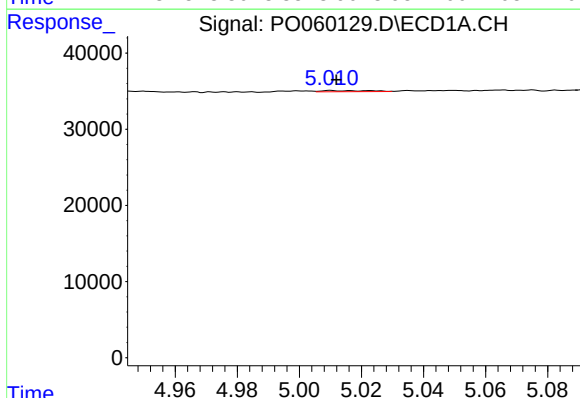


#12 AR-1232-2

R.T.: 5.010 min
Delta R.T.: -0.002 min
Response: 1549
Conc: 2.19 ng/ml

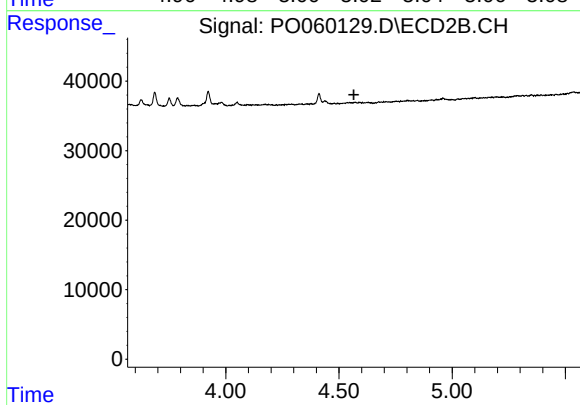

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

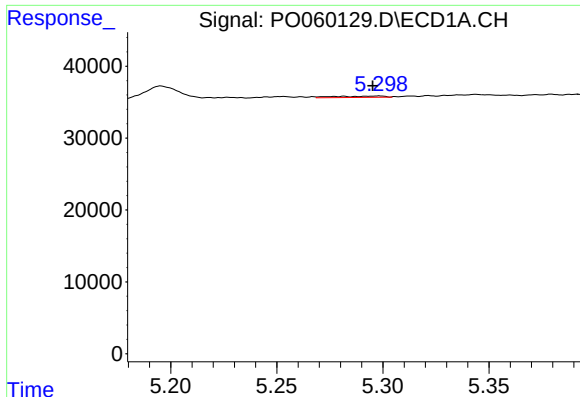

#13 AR-1232-3


R.T.: 5.298 min
Delta R.T.: 0.003 min
Response: 2929
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

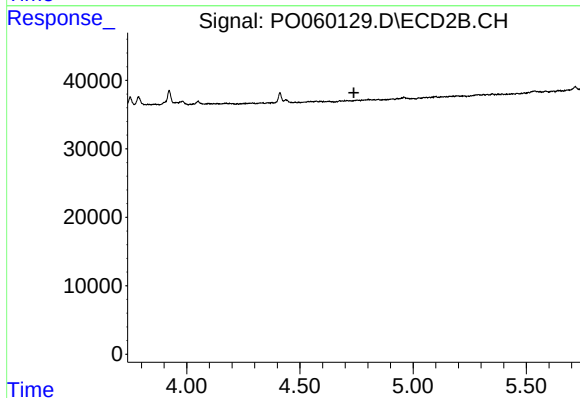


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

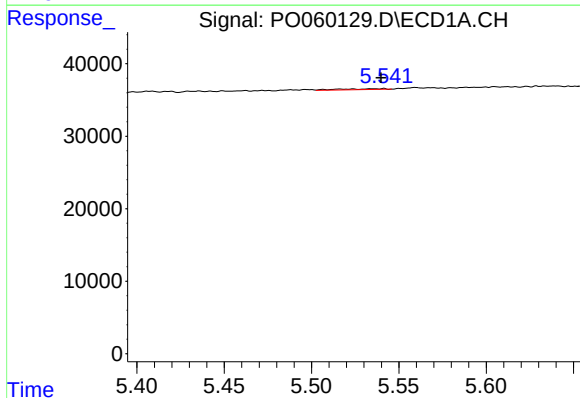


#14 AR-1232-4

R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 2124
Conc: 2.72 ng/ml

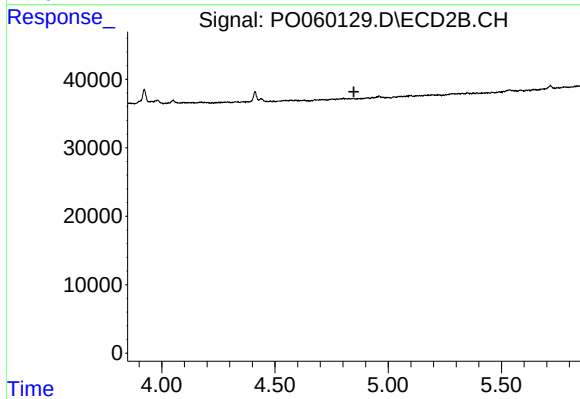

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

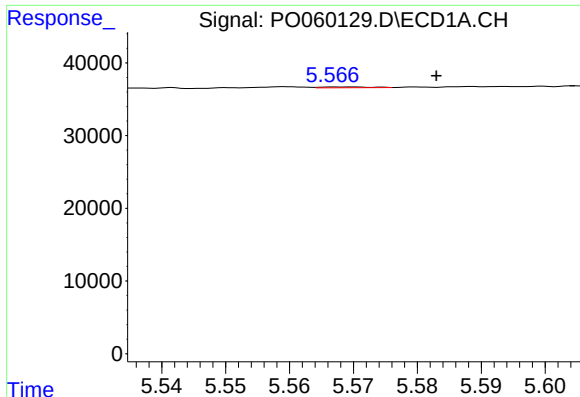

#15 AR-1232-5


R.T.: 5.569 min
Delta R.T.: -0.014 min
Response: 675
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

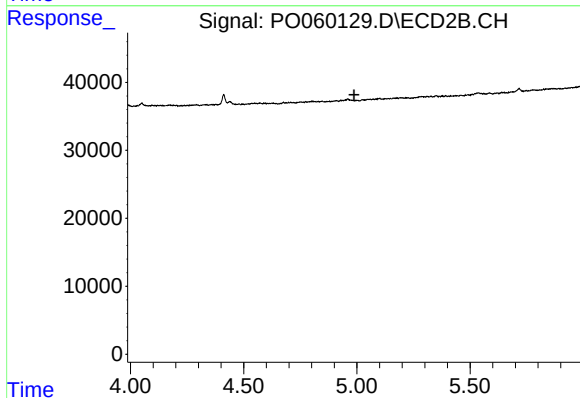


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

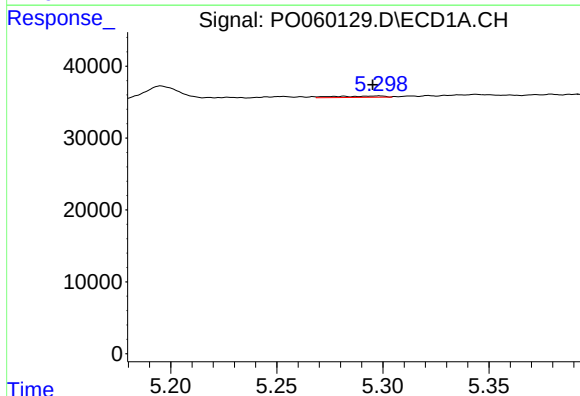


#16 AR-1242-1

R.T.: 5.298 min
Delta R.T.: 0.003 min
Response: 2929
Conc: 2.31 ng/ml

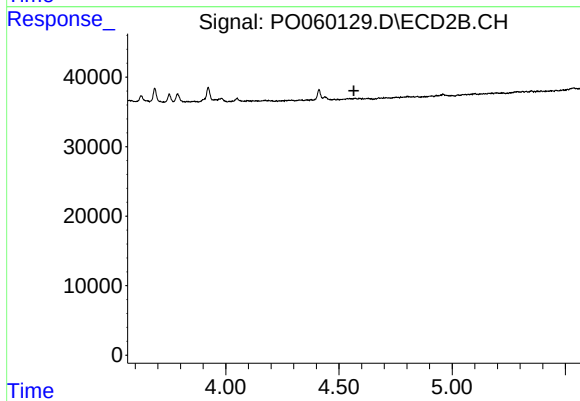

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

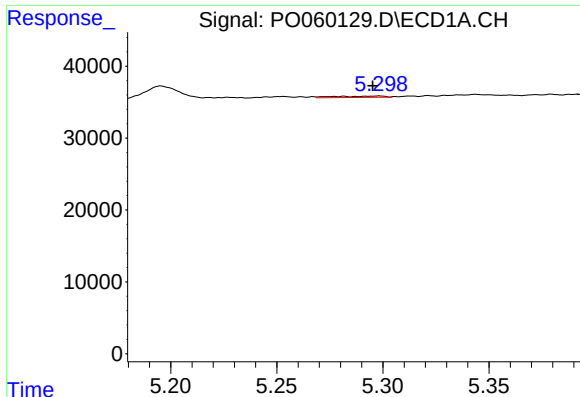

#17 AR-1242-2


R.T.: 5.298 min
Delta R.T.: 0.003 min
Response: 2929
Conc: 1.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

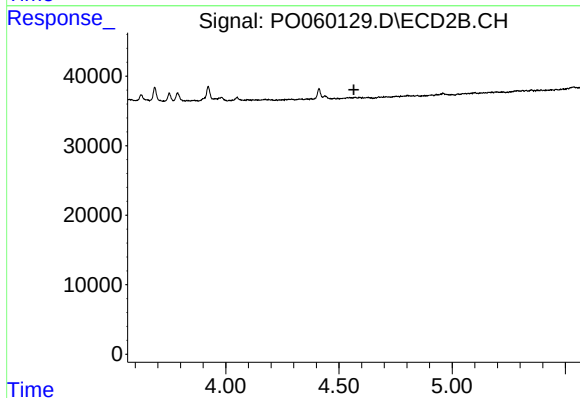


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

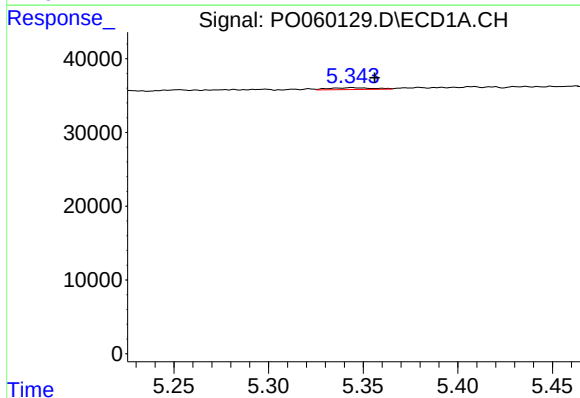


#18 AR-1242-3

R.T.: 5.344 min
Delta R.T.: -0.012 min
Response: 4016
Conc: 3.44 ng/ml

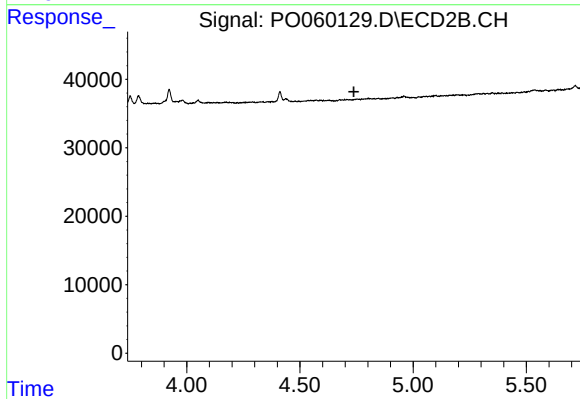

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

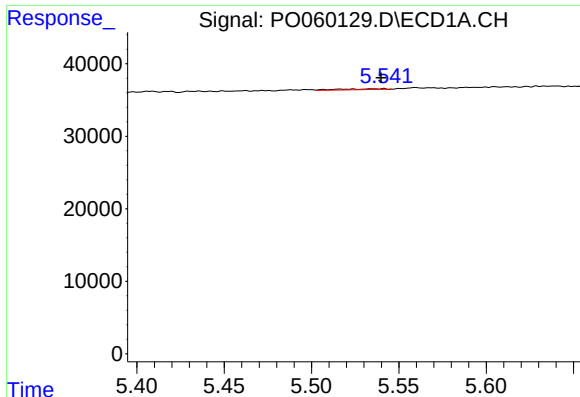

#19 AR-1242-4


R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 2124
Conc: 2.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

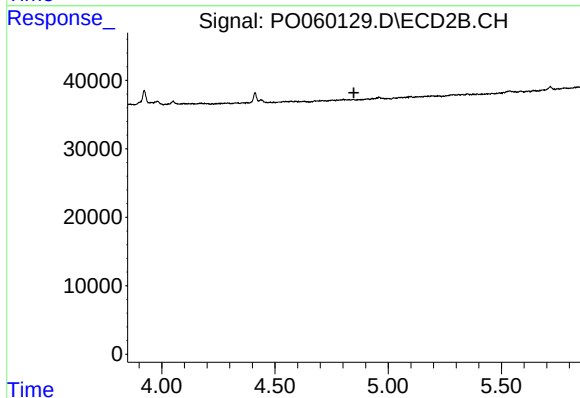


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

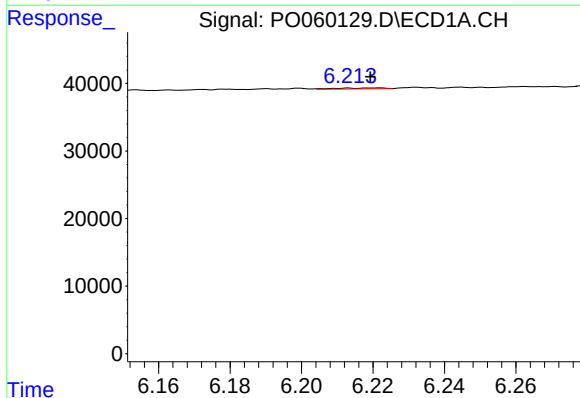


#20 AR-1242-5

R.T.: 6.221 min
Delta R.T.: 0.002 min
Response: 1386
Conc: 1.10 ng/ml

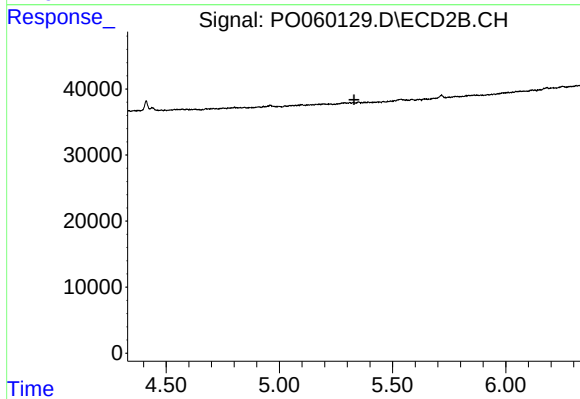

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

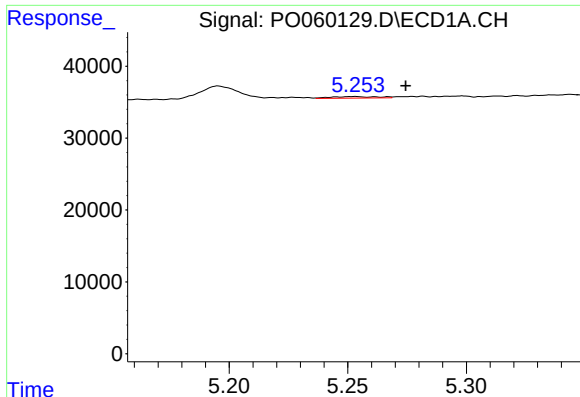

#21 AR-1248-1


R.T.: 5.253 min
Delta R.T.: -0.022 min
Response: 2947
Conc: 2.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

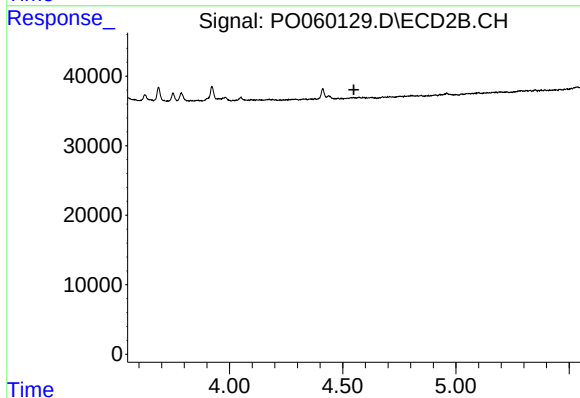


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

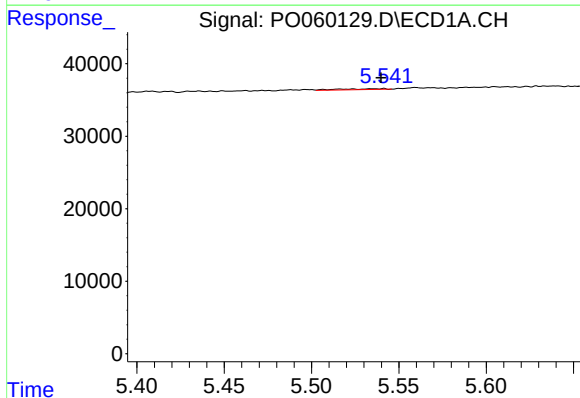


#22 AR-1248-2

R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 2124
Conc: 1.46 ng/ml

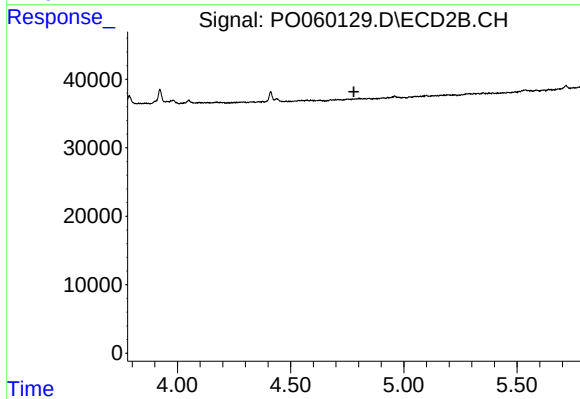

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

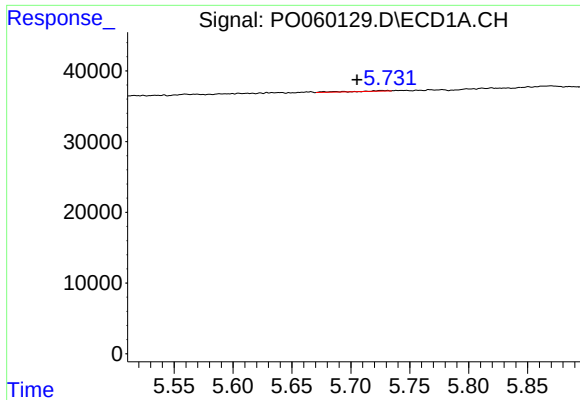

#23 AR-1248-3


R.T.: 5.731 min
Delta R.T.: 0.025 min
Response: 1523
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

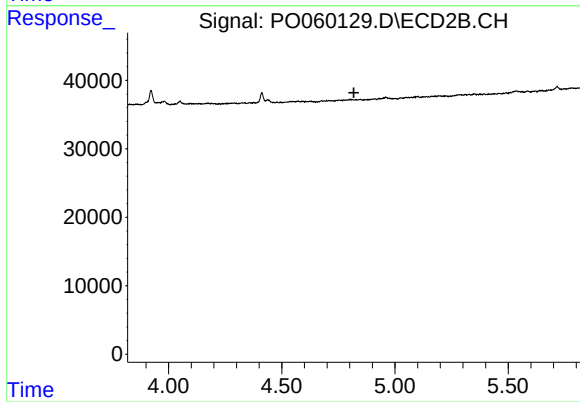


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

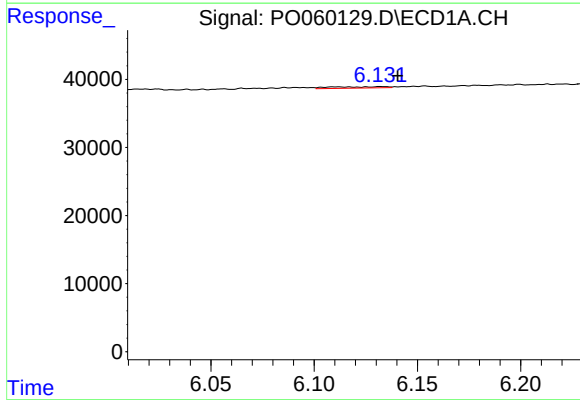


#24 AR-1248-4

R.T.: 6.133 min
Delta R.T.: -0.008 min
Response: 3604
Conc: 1.76 ng/ml

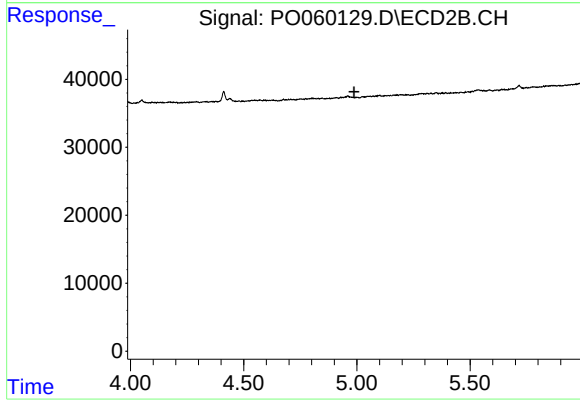

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

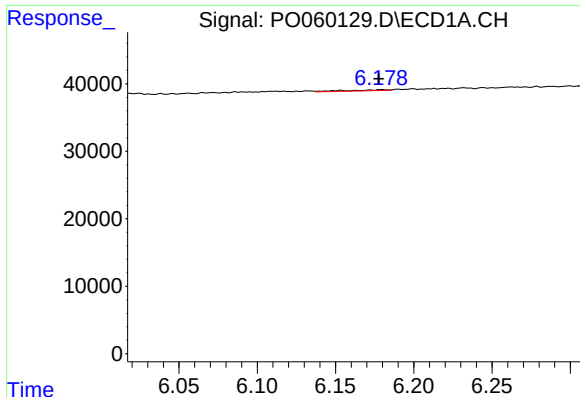

#25 AR-1248-5


R.T.: 6.179 min
Delta R.T.: 0.002 min
Response: 2827
Conc: 1.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

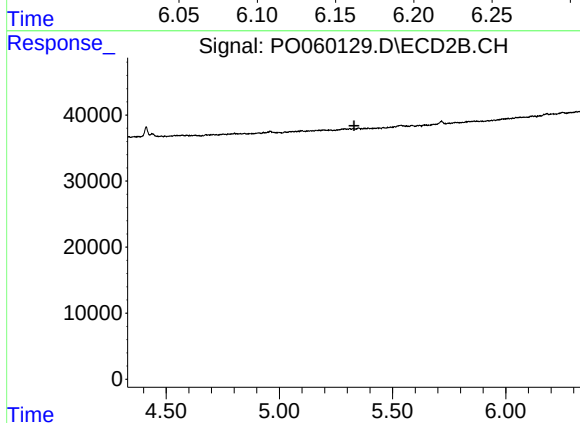


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

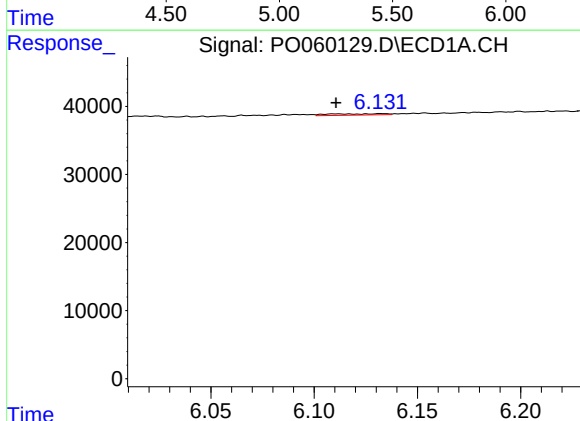


#26 AR-1254-1

R.T.: 6.133 min
Delta R.T.: 0.022 min
Response: 3604
Conc: 1.73 ng/ml

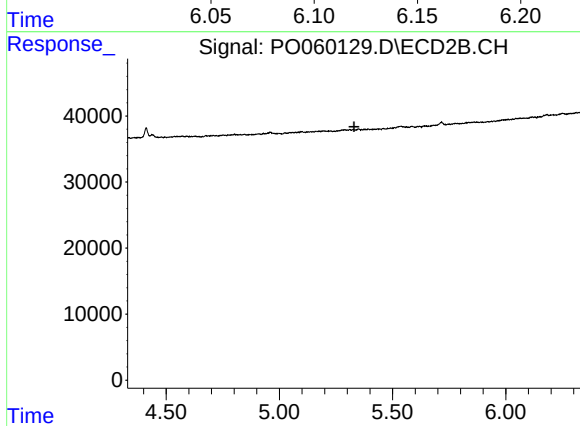

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

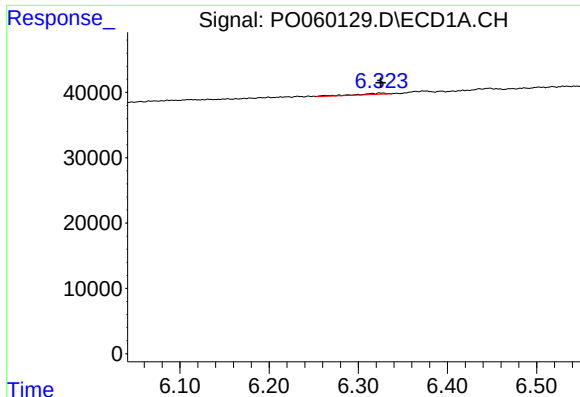

#27 AR-1254-2


R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 4892
Conc: 1.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

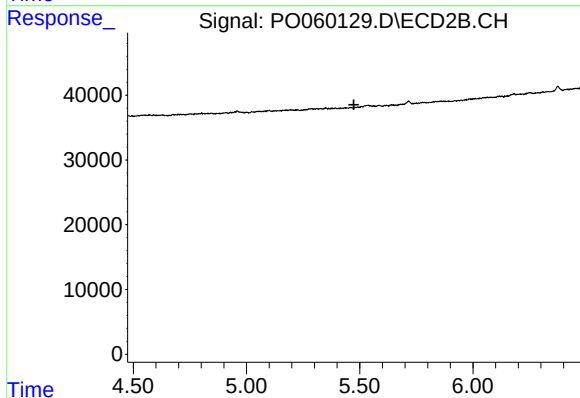


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.474 min
Response: 0
Conc: N.D.

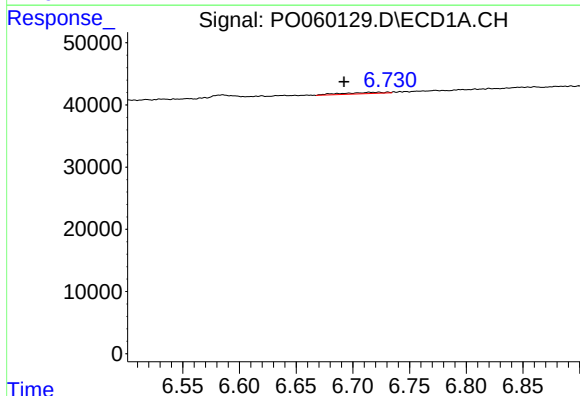


#28 AR-1254-3

R.T.: 6.723 min
Delta R.T.: 0.031 min
Response: 5529
Conc: 1.56 ng/ml

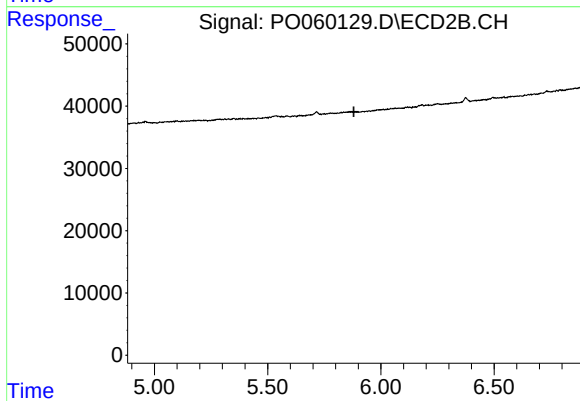

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.881 min
Response: 0
Conc: N.D.

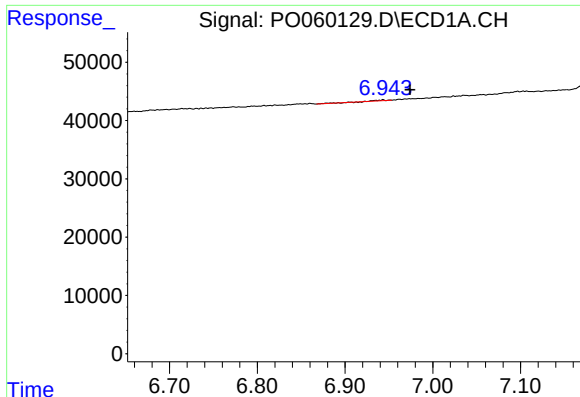

#29 AR-1254-4


R.T.: 6.943 min
Delta R.T.: -0.031 min
Response: 1652
Conc: 0.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

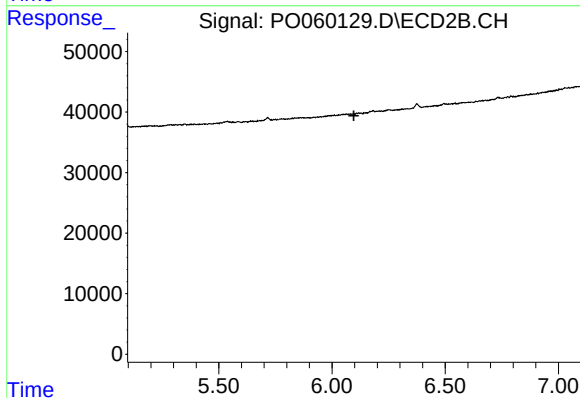


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

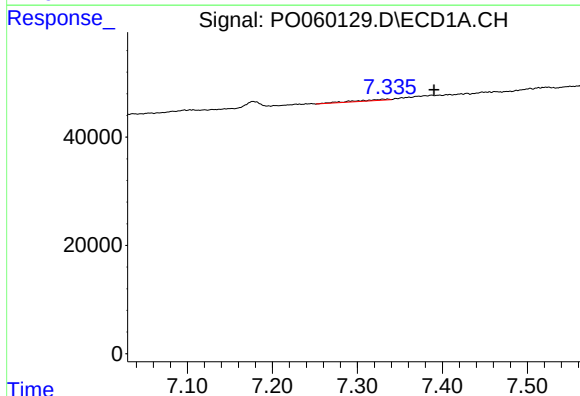


#30 AR-1254-5

R.T.: 7.336 min
Delta R.T.: -0.054 min
Response: 5851
Conc: 1.89 ng/ml

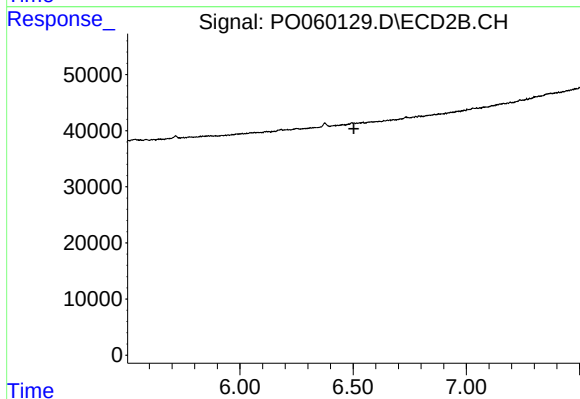

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.503 min
Response: 0
Conc: N.D.

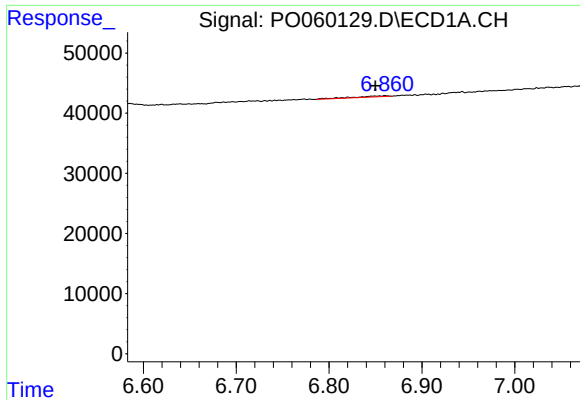

#31 AR-1260-1


R.T.: 6.861 min
Delta R.T.: 0.011 min
Response: 4542
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

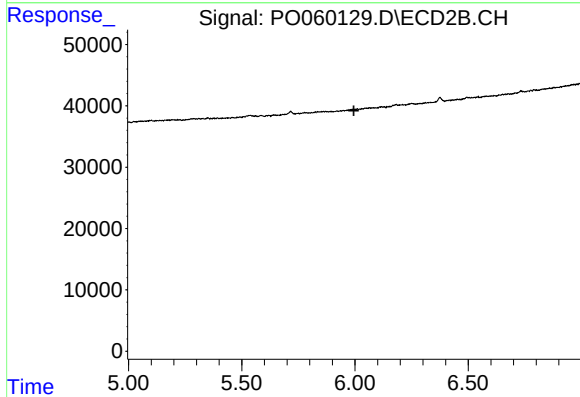


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.

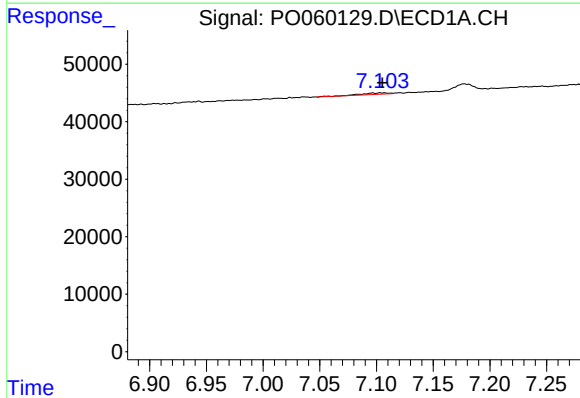


#32 AR-1260-2

R.T.: 7.107 min
Delta R.T.: 0.002 min
Response: 4266
Conc: 1.15 ng/ml

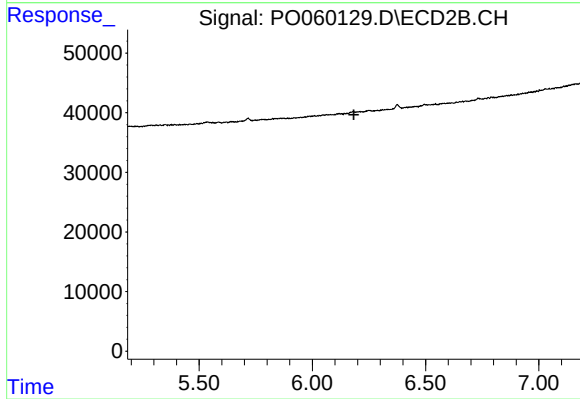

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.183 min
Response: 0
Conc: N.D.

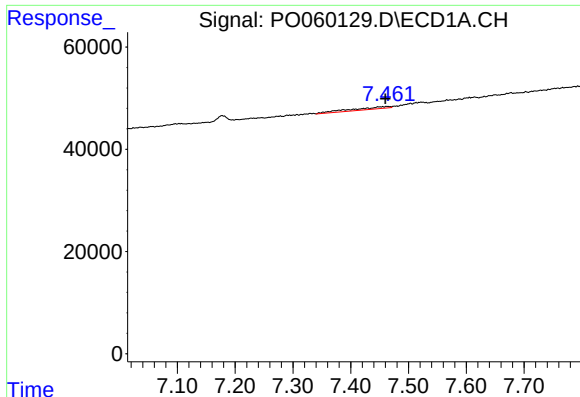

#33 AR-1260-3


R.T.: 7.463 min
Delta R.T.: 0.003 min
Response: 20036
Conc: 6.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

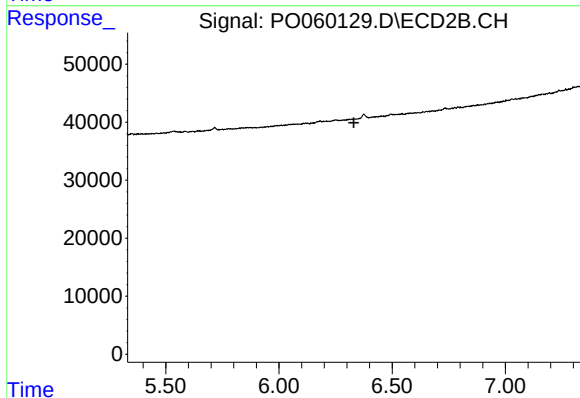


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

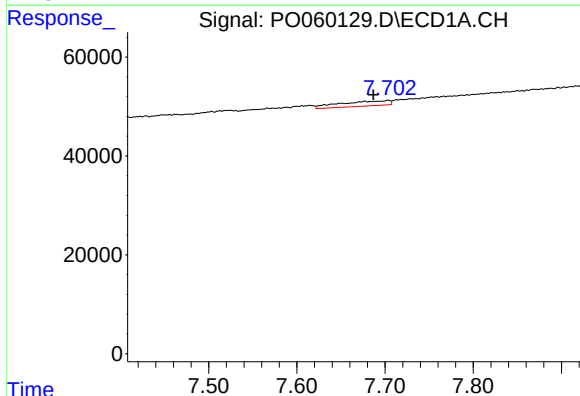


#34 AR-1260-4

R.T.: 7.703 min
Delta R.T.: 0.016 min
Response: 38941
Conc: 12.68 ng/ml

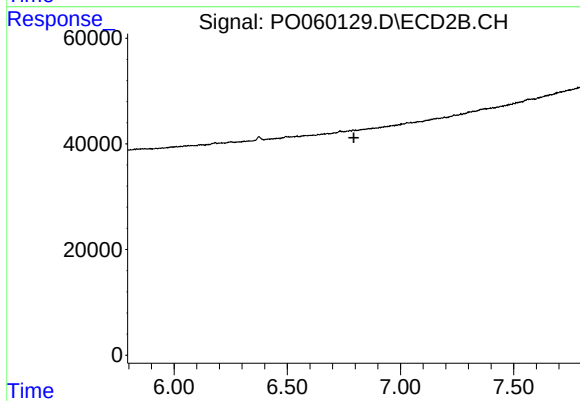

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

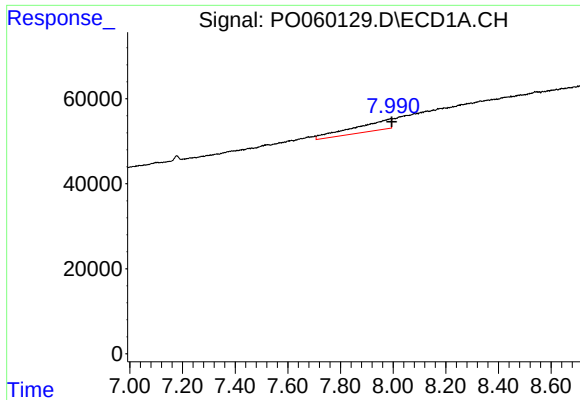

#35 AR-1260-5


R.T.: 7.990 min
Delta R.T.: -0.004 min
Response: 247372
Conc: 34.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

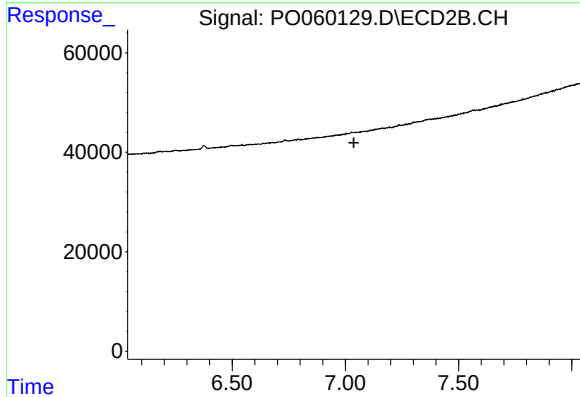


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

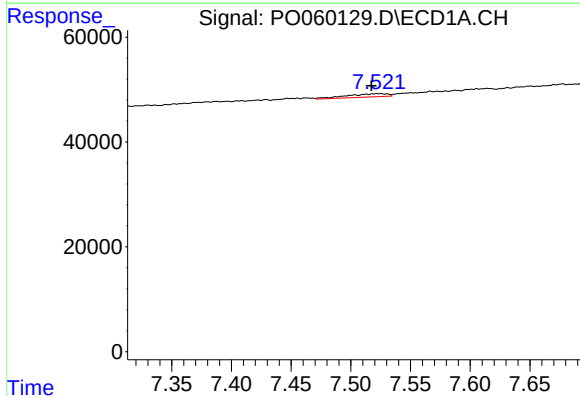


#36 AR-1262-1

R.T.: 7.524 min
Delta R.T.: 0.007 min
Response: 14935
Conc: 3.08 ng/ml

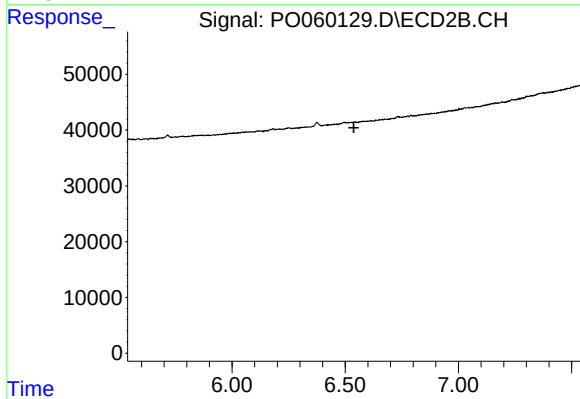

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.538 min
Response: 0
Conc: N.D.

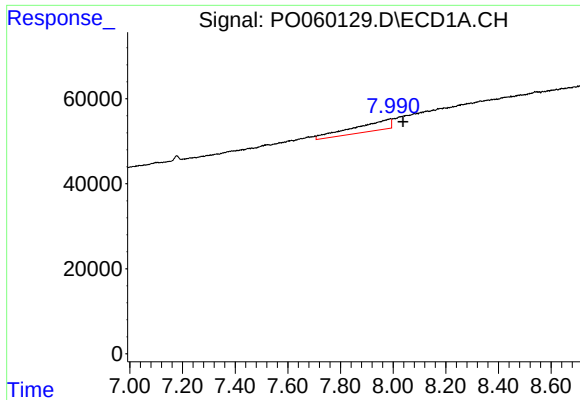

#37 AR-1262-2


R.T.: 7.990 min
Delta R.T.: -0.048 min
Response: 247372
Conc: 32.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

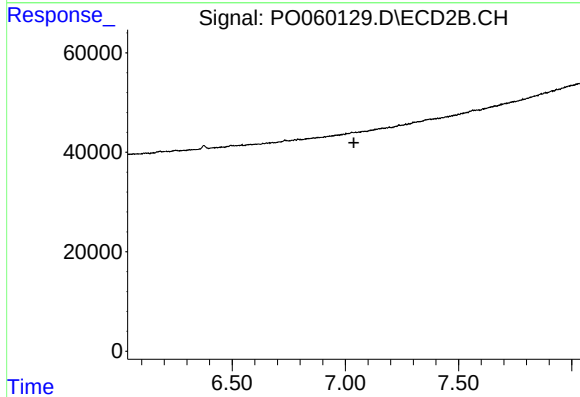


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

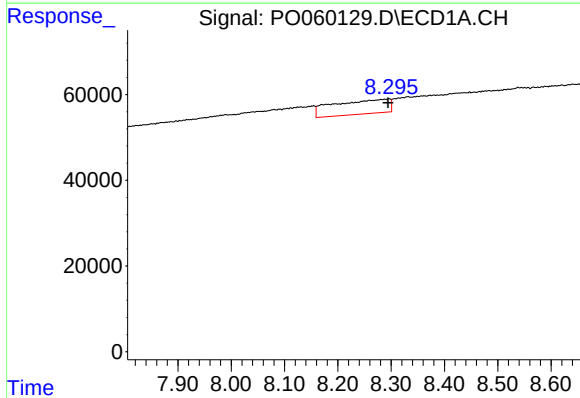


#38 AR-1262-3

R.T.: 8.296 min
Delta R.T.: 0.002 min
Response: 244447
Conc: 47.91 ng/ml

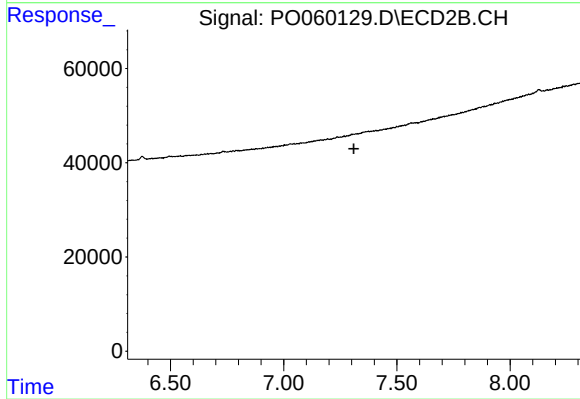

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

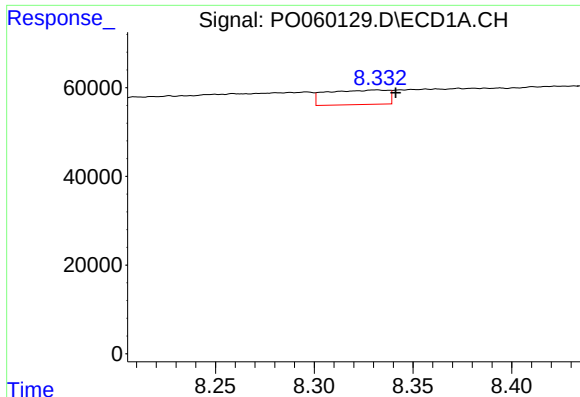

#39 AR-1262-4


R.T.: 8.331 min
Delta R.T.: -0.010 min
Response: 70660
Conc: 18.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

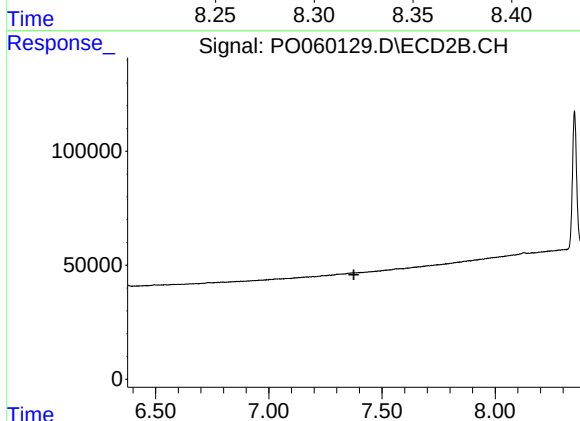


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.376 min
Response: 0
Conc: N.D.

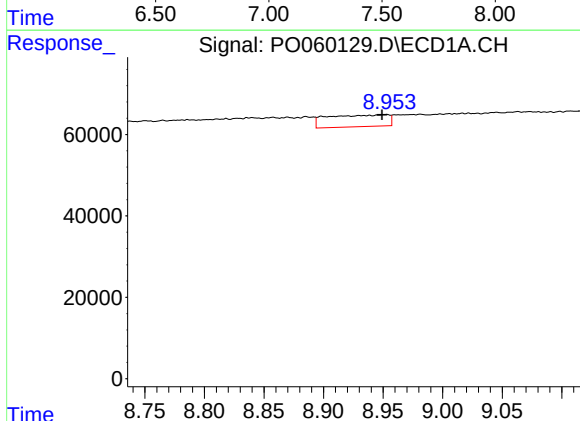


#40 AR-1262-5

R.T.: 8.952 min
Delta R.T.: 0.003 min
Response: 103313
Conc: 40.25 ng/ml

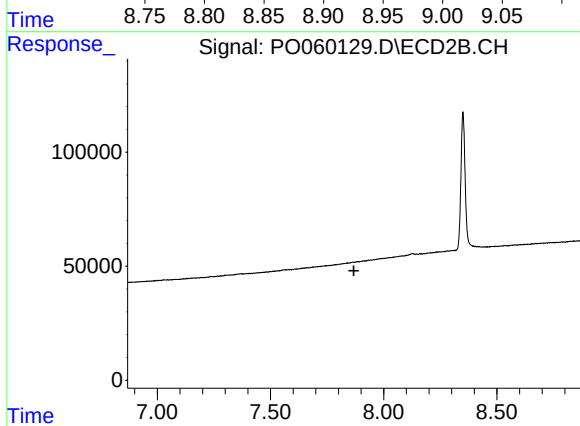

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 7.868 min
Response: 0
Conc: N.D.

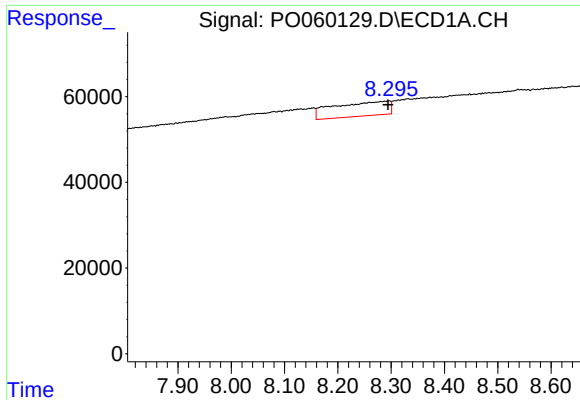

#41 AR-1268-1


R.T.: 8.296 min
Delta R.T.: 0.002 min
Response: 244447
Conc: 25.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

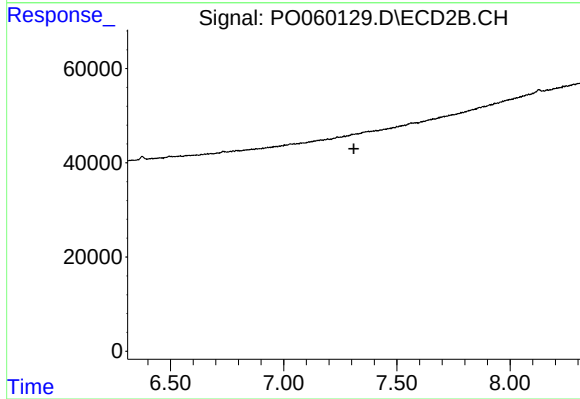


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

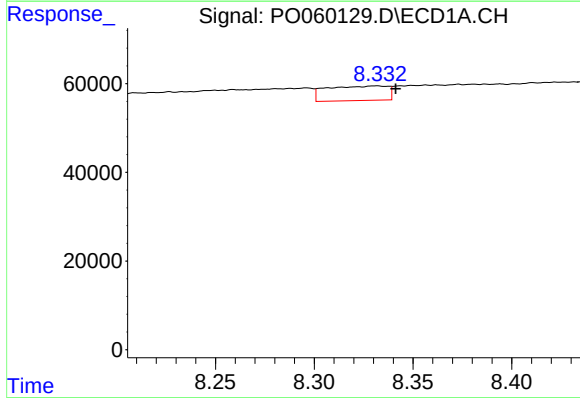


#42 AR-1268-2

R.T.: 8.331 min
Delta R.T.: -0.010 min
Response: 70660
Conc: 8.96 ng/ml

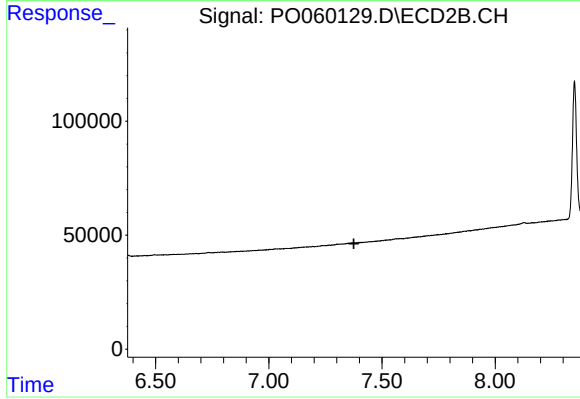

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.376 min
Response: 0
Conc: N.D.

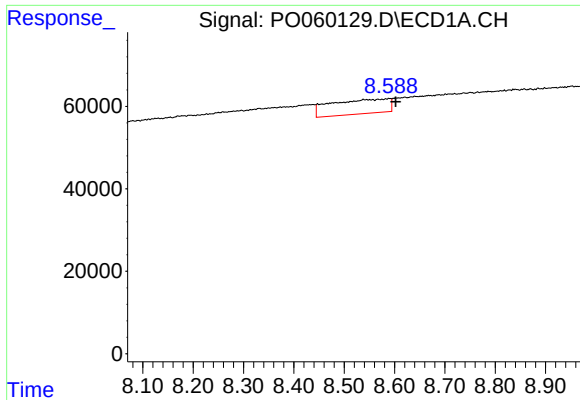

#43 AR-1268-3


R.T.: 8.590 min
Delta R.T.: -0.013 min
Response: 284658
Conc: 40.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

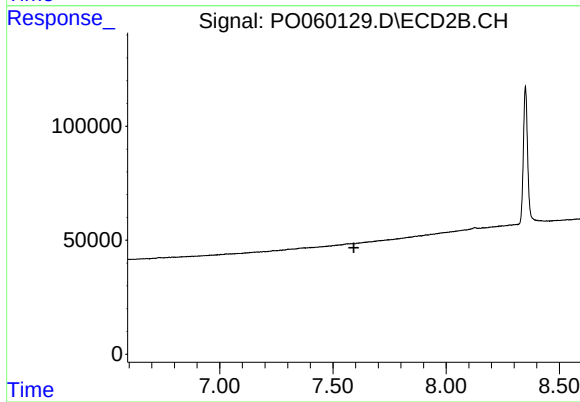


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

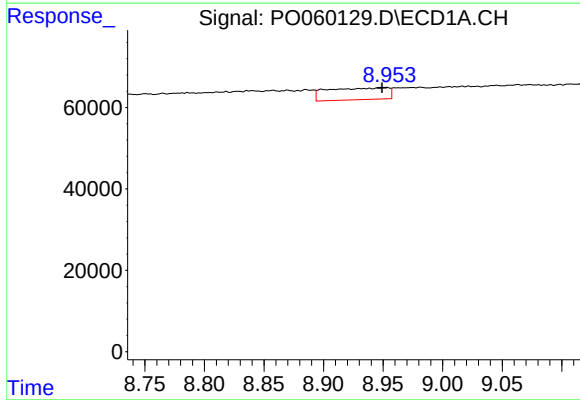


#44 AR-1268-4

R.T.: 8.952 min
Delta R.T.: 0.003 min
Response: 103313
Conc: 37.16 ng/ml

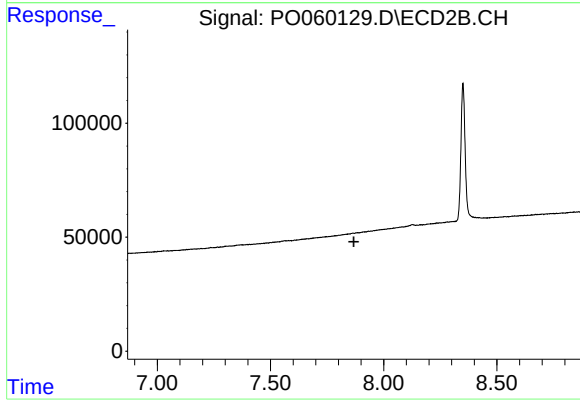

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.868 min
Response: 0
Conc: N.D.

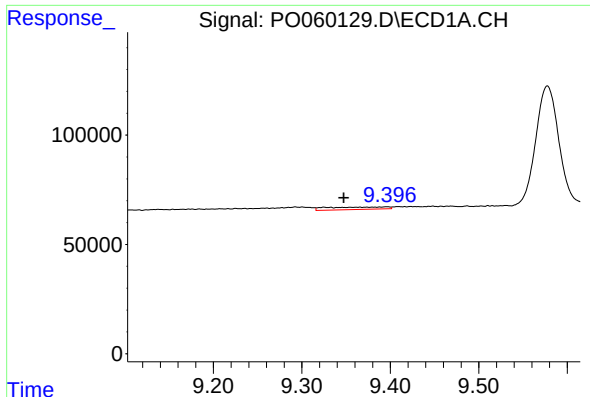

#45 AR-1268-5

R.T.: 9.396 min
Delta R.T.: 0.049 min
Response: 52075
Conc: 2.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-COMP

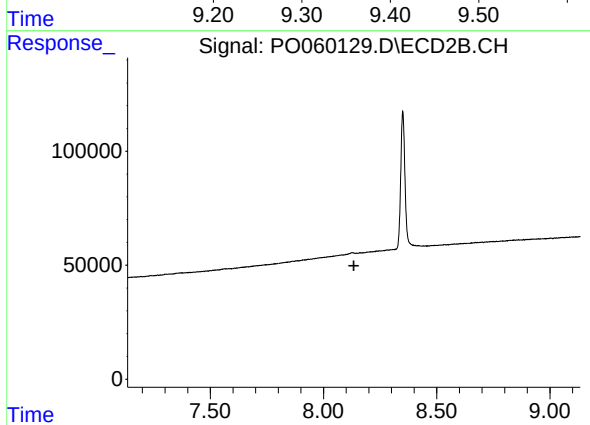

#45 AR-1268-5

R.T.: 8.127 min
Delta R.T.: -0.007 min
Response: -202021
Conc: N.D.