

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060131.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 1:53
 Operator : SM/AJ
 Sample : K4619-24
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP8-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:12:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.120	3.495	809566	765398	23.122	21.264
2)	SA Decachlor...	9.577	8.350	856012	676405	16.090	16.775
Target Compounds							
3)	L1 AR-1016-1	5.272	0.000	764	0	0.477	N.D. #
4)	L1 AR-1016-2	5.292	0.000	1278	0	0.534	N.D. #
5)	L1 AR-1016-3	5.358	0.000	540	0	0.363	N.D. #
6)	L1 AR-1016-4	5.473	0.000	735	0	0.607	N.D. #
7)	L1 AR-1016-5	5.713	0.000	649	0	0.505	N.D. #
8)	L2 AR-1221-1	4.371	0.000	466	0	1.101	N.D. #
9)	L2 AR-1221-2	4.420	0.000	12407	0	38.198	N.D. #
10)	L2 AR-1221-3	4.496	0.000	5775	0	5.491	N.D. #
11)	L3 AR-1232-1	4.496	0.000	5775	0	4.633	N.D. #
12)	L3 AR-1232-2	5.006	0.000	1100	0	1.558	N.D. #
13)	L3 AR-1232-3	5.292	0.000	1278	0	0.834	N.D. #
14)	L3 AR-1232-4	5.536	0.000	324	0	0.415	N.D. #
15)	L3 AR-1232-5	5.571	0.000	2678	0	4.454	N.D. #
16)	L4 AR-1242-1	5.292	0.000	1278	0	1.006	N.D. #
17)	L4 AR-1242-2	5.292	0.000	1278	0	0.688	N.D. #
18)	L4 AR-1242-3	5.358	0.000	540	0	0.462	N.D. #
19)	L4 AR-1242-4	5.536	0.000	324	0	0.335	N.D. #
20)	L4 AR-1242-5	6.228	0.000	2977	0	2.369	N.D. #
21)	L5 AR-1248-1	5.272	0.000	764	0	0.762	N.D. #
22)	L5 AR-1248-2	5.536	0.000	324	0	0.224	N.D. #
23)	L5 AR-1248-3	5.713	0.000	649	0	0.390	N.D. #
24)	L5 AR-1248-4	6.132	0.000	21445	0	10.491	N.D. #
25)	L5 AR-1248-5	6.173	0.000	3016	0	1.521	N.D. #
26)	L6 AR-1254-1	6.132	0.000	21445	0	10.279	N.D. #
27)	L6 AR-1254-2	6.322	0.000	10356	0	3.104	N.D. #
28)	L6 AR-1254-3	6.681	0.000	11782	0	3.320	N.D. #
29)	L6 AR-1254-4	6.968	0.000	10654	0	3.617	N.D. #
30)	L6 AR-1254-5	7.382	0.000	14215	0	4.597	N.D. #
31)	L7 AR-1260-1	6.844	0.000	6350	0	2.355	N.D. #
32)	L7 AR-1260-2	7.096	0.000	18474	0	4.979	N.D. #
33)	L7 AR-1260-3	7.448	0.000	14837	0	4.529	N.D. #
34)	L7 AR-1260-4	7.688	0.000	8603	0	2.801	N.D. #
35)	L7 AR-1260-5	7.983	0.000	122103	0	17.244	N.D. #
36)	L8 AR-1262-1	7.522	0.000	12615	0	2.599	N.D. #
37)	L8 AR-1262-2	8.038	0.000	59919	0	7.766	N.D. #
38)	L8 AR-1262-3	8.353	0.000	265419	0	52.019	N.D. #
39)	L8 AR-1262-4	8.353	0.000	265419	0	68.855	N.D. #
40)	L8 AR-1262-5	8.930	0.000	41443	0	16.147	N.D. #
41)	L9 AR-1268-1	8.353	0.000	265419	0	28.204	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060131.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 1:53
Operator : SM/AJ
Sample : K4619-24
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:12:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.353	0.000	265419	0	33.671	N.D. #
43) L9	AR-1268-3	8.597	0.000	97165	0	13.785	N.D. #
44) L9	AR-1268-4	8.930	0.000	41443	0	14.907	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083019\
Data File : PO060131.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 1:53
Operator : SM/AJ
Sample : K4619-24
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP8-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:12:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

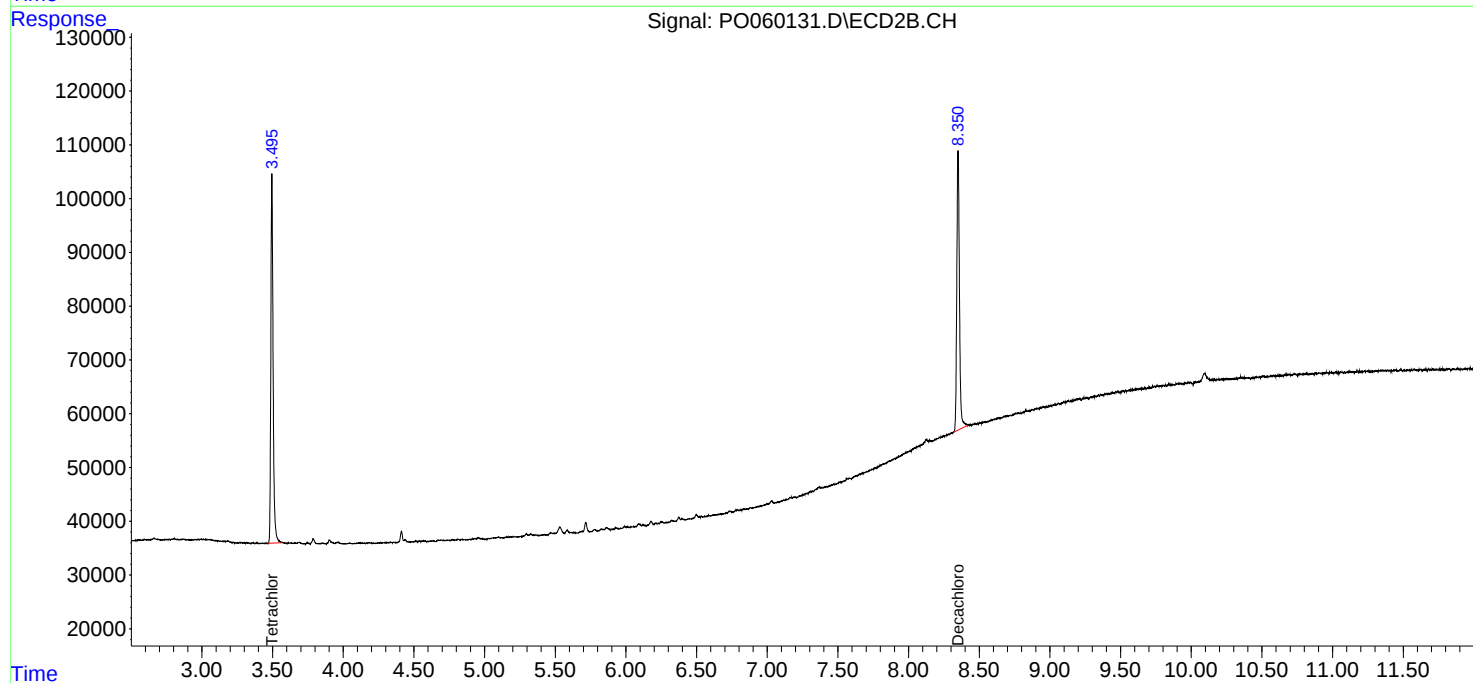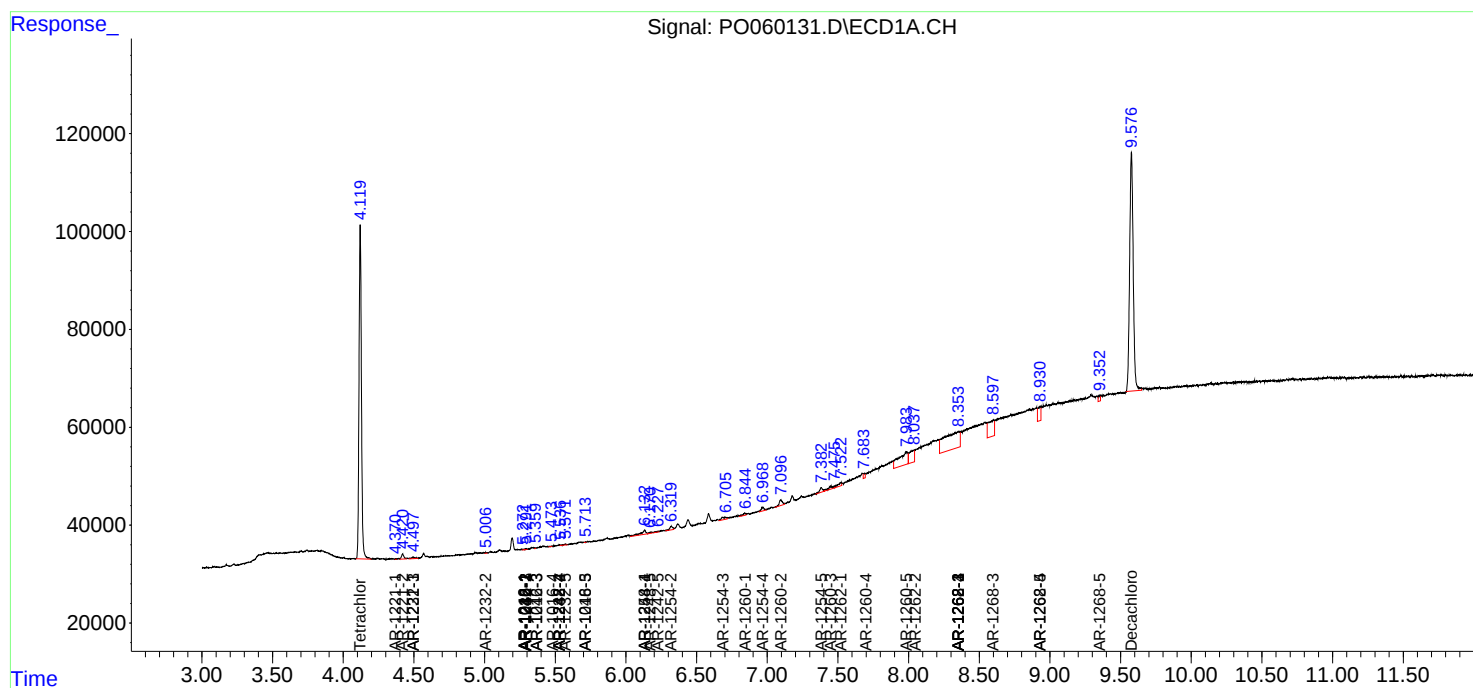


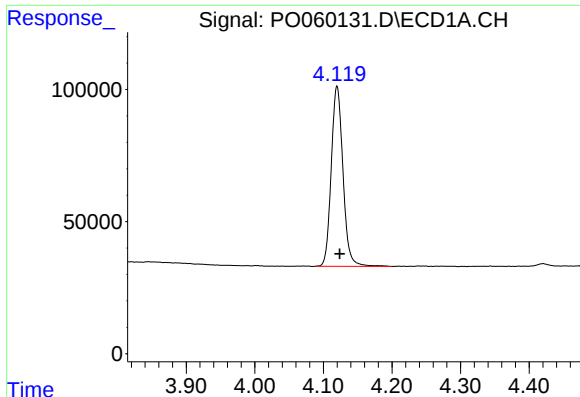

#1 Tetrachloro-m-xylene


R.T.: 4.120 min
Delta R.T.: -0.004 min
Response: 809566
Conc: 23.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

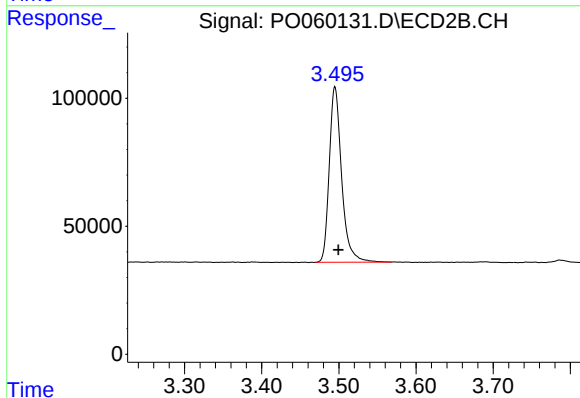


#1 Tetrachloro-m-xylene

R.T.: 3.495 min
Delta R.T.: -0.004 min
Response: 765398
Conc: 21.26 ng/ml

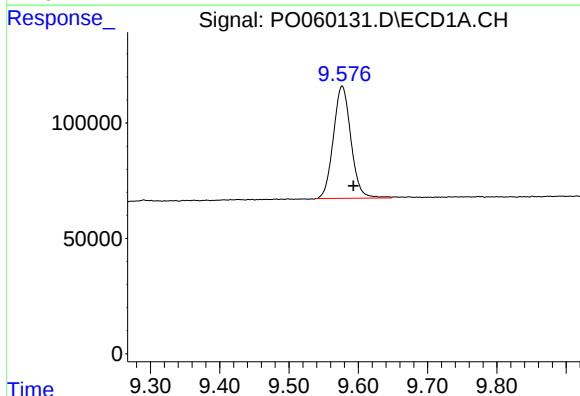


#2 Decachlorobiphenyl

R.T.: 9.577 min
Delta R.T.: -0.016 min
Response: 856012
Conc: 16.09 ng/ml

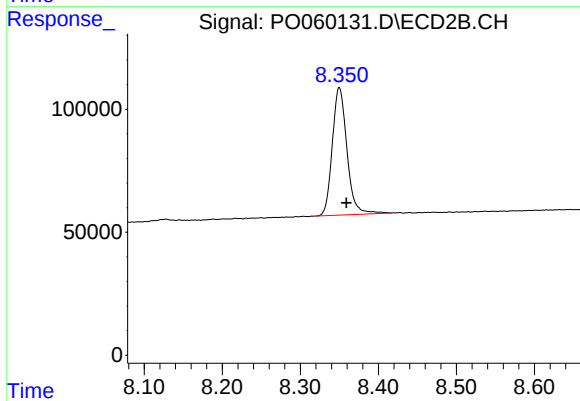

#2 Decachlorobiphenyl


R.T.: 8.350 min
Delta R.T.: -0.009 min
Response: 676405
Conc: 16.78 ng/ml

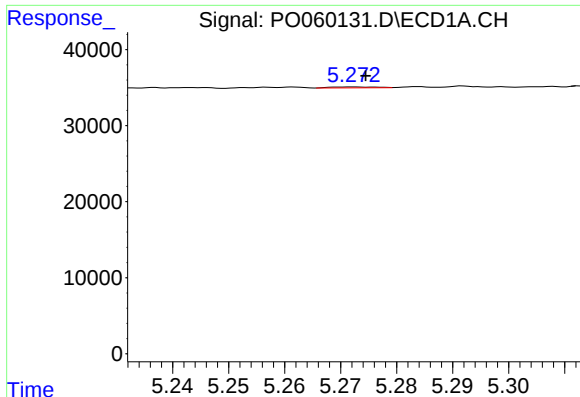

#3 AR-1016-1


R.T.: 5.272 min
Delta R.T.: -0.002 min
Response: 764
Conc: 0.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

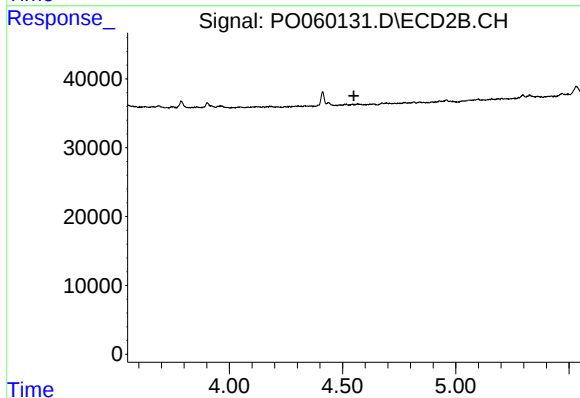


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

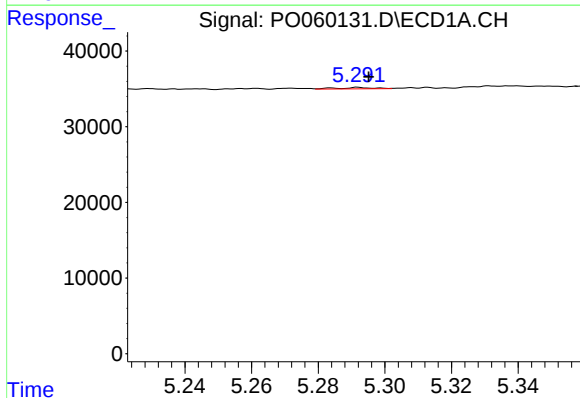


#4 AR-1016-2

R.T.: 5.292 min
Delta R.T.: -0.003 min
Response: 1278
Conc: 0.53 ng/ml

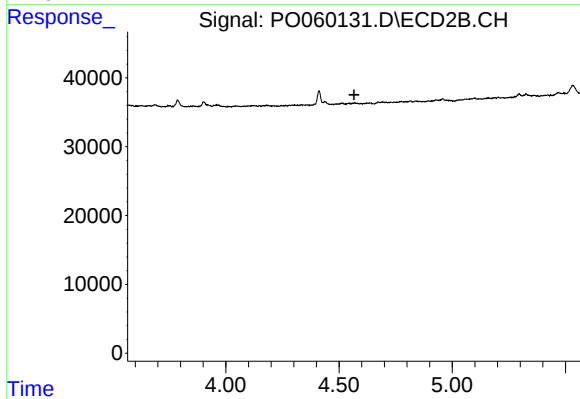

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

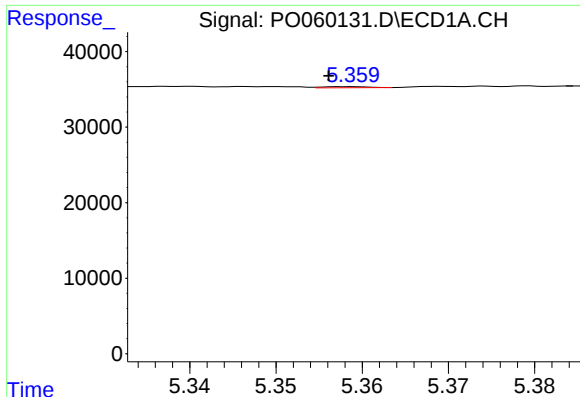

#5 AR-1016-3


R.T.: 5.358 min
Delta R.T.: 0.002 min
Response: 540
Conc: 0.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

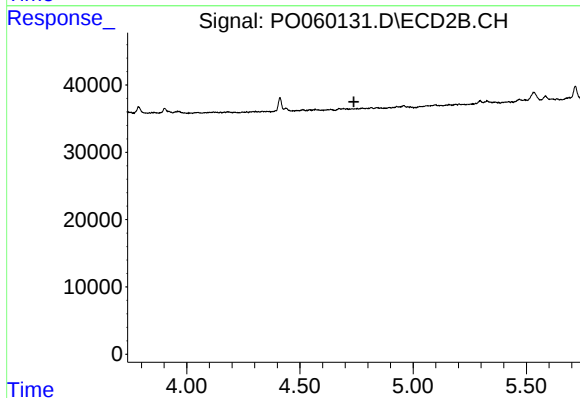


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

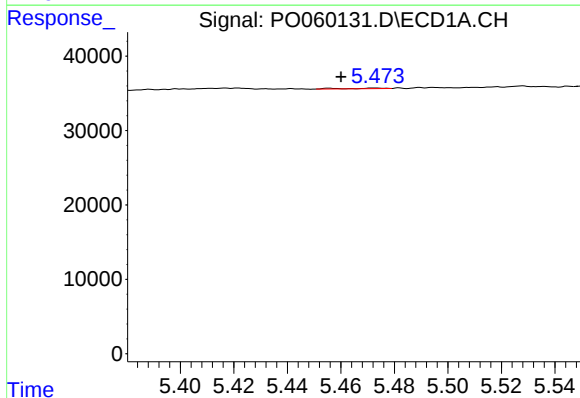


#6 AR-1016-4

R.T.: 5.473 min
Delta R.T.: 0.013 min
Response: 735
Conc: 0.61 ng/ml

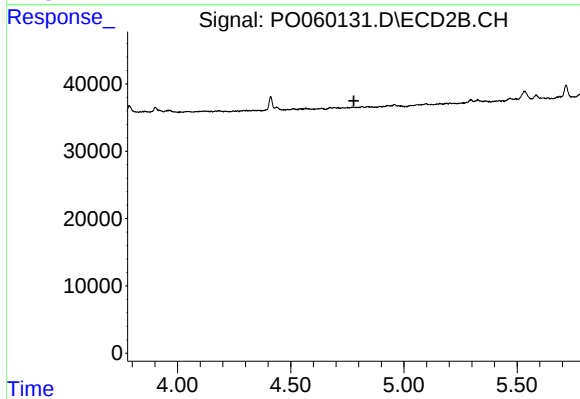

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

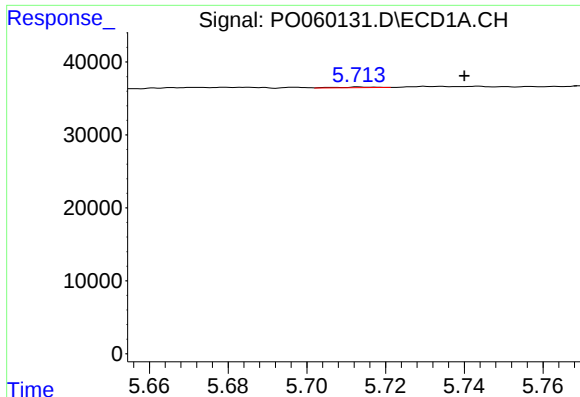

#7 AR-1016-5


R.T.: 5.713 min
Delta R.T.: -0.027 min
Response: 649
Conc: 0.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

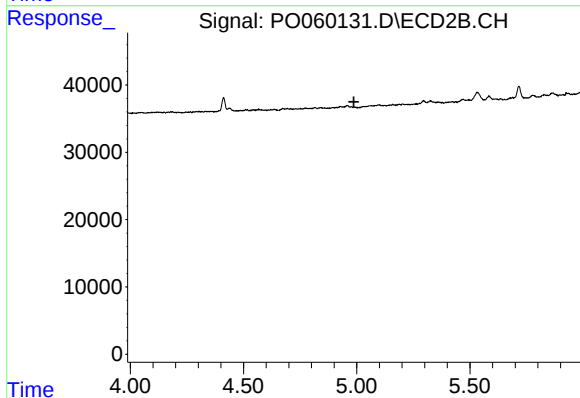


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

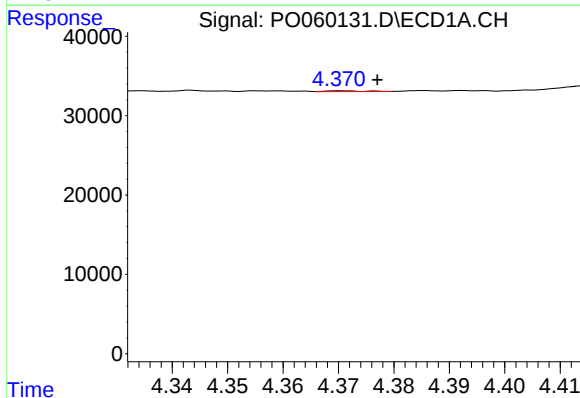


#8 AR-1221-1

R.T.: 4.371 min
Delta R.T.: -0.006 min
Response: 466
Conc: 1.10 ng/ml

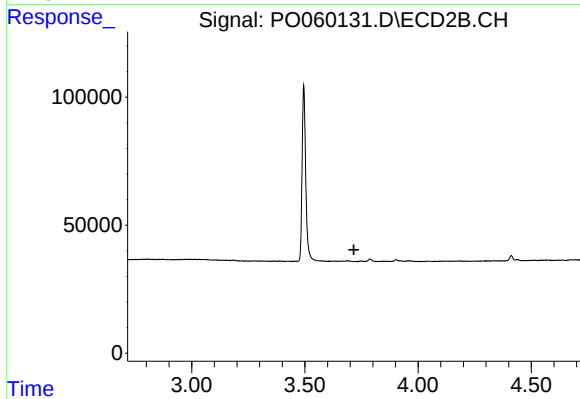

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.717 min
Response: 0
Conc: N.D.

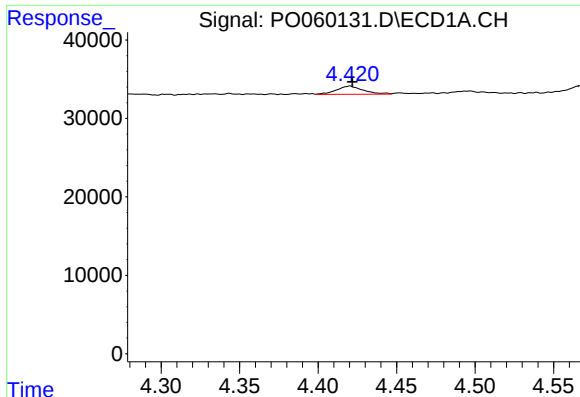

#9 AR-1221-2


R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 12407
Conc: 38.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

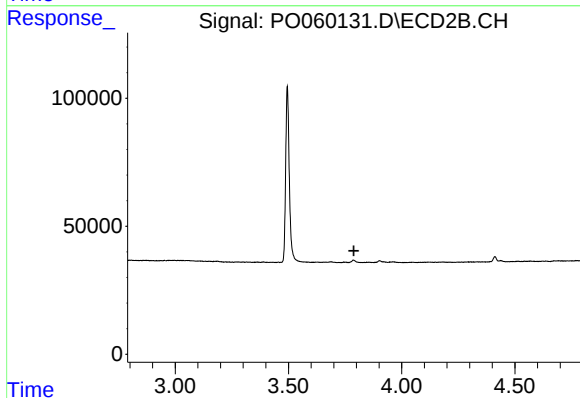


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.789 min
Response: 0
Conc: N.D.

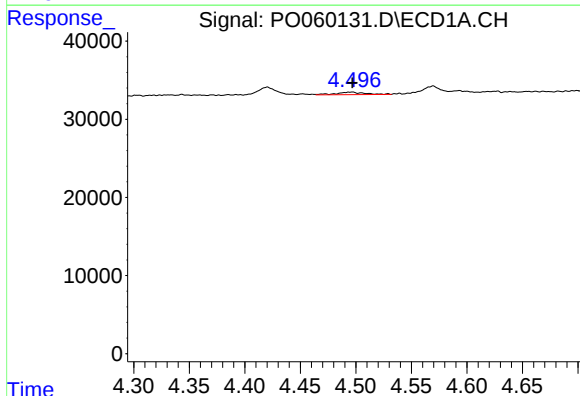


#10 AR-1221-3

R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 5775
Conc: 5.49 ng/ml

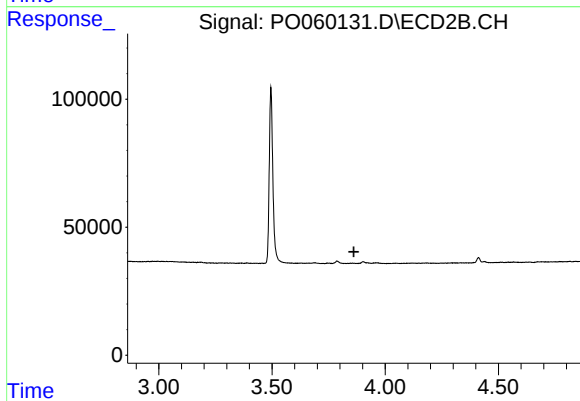

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

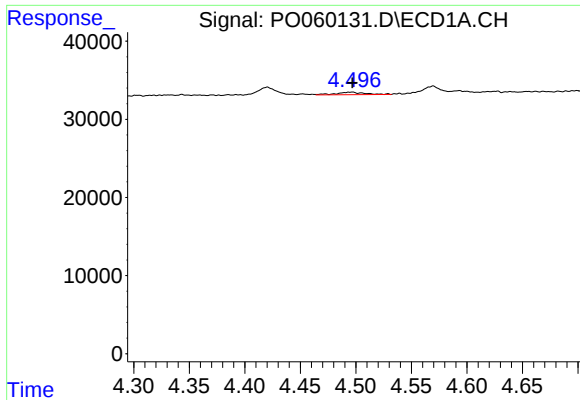

#11 AR-1232-1


R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 5775
Conc: 4.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

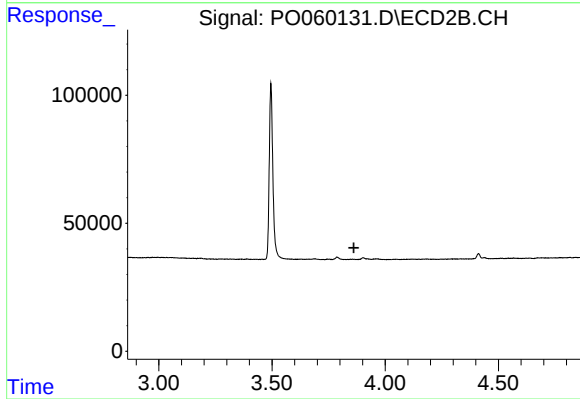


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

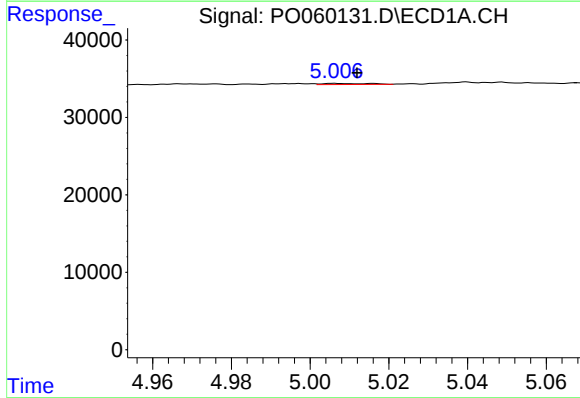


#12 AR-1232-2

R.T.: 5.006 min
Delta R.T.: -0.005 min
Response: 1100
Conc: 1.56 ng/ml

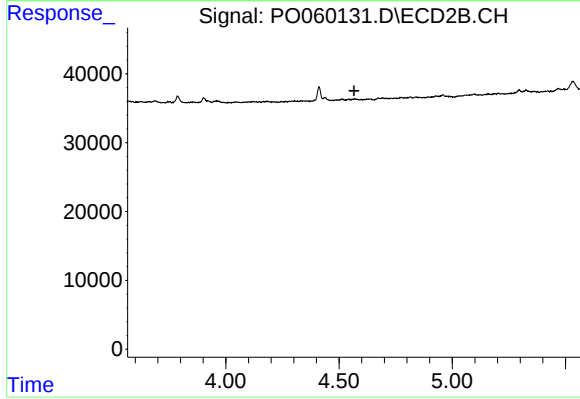

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

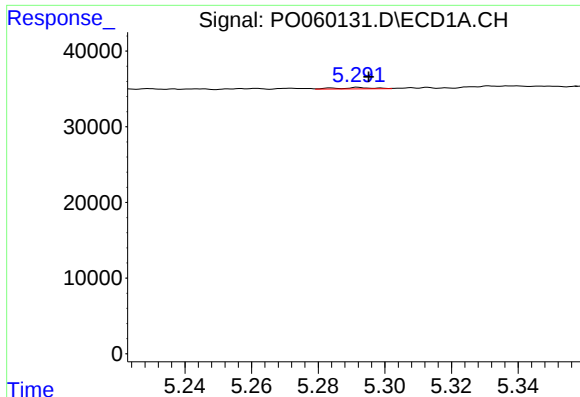

#13 AR-1232-3


R.T.: 5.292 min
Delta R.T.: -0.003 min
Response: 1278
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

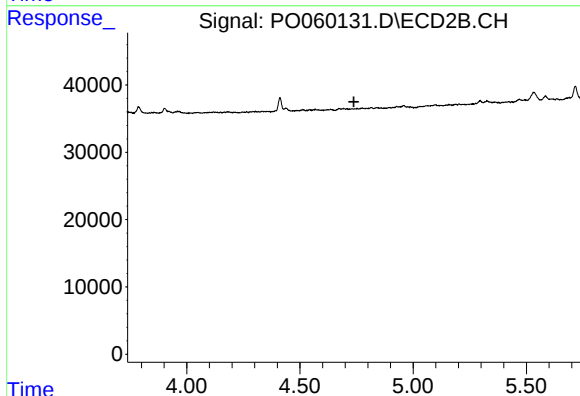


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

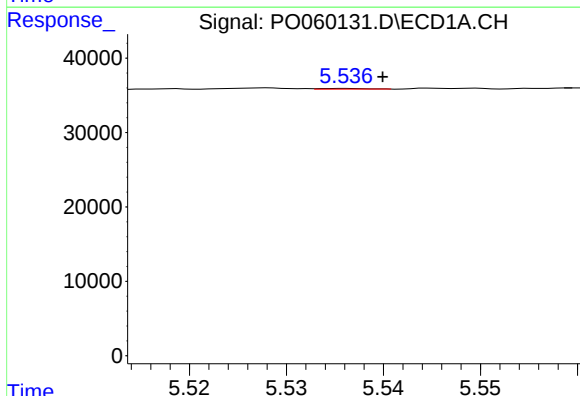


#14 AR-1232-4

R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 324
Conc: 0.41 ng/ml

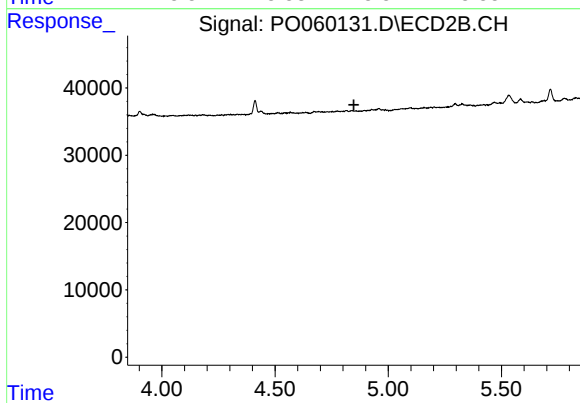

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

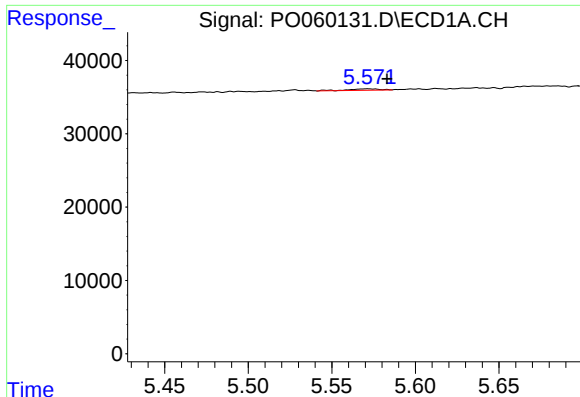

#15 AR-1232-5


R.T.: 5.571 min
Delta R.T.: -0.012 min
Response: 2678
Conc: 4.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

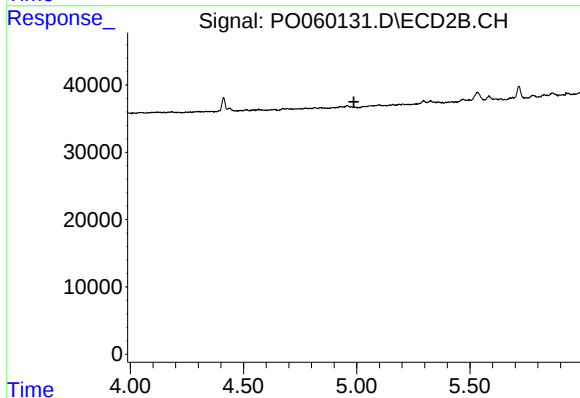


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

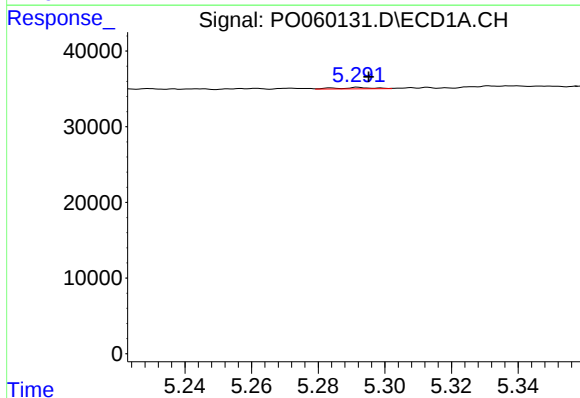


#16 AR-1242-1

R.T.: 5.292 min
Delta R.T.: -0.003 min
Response: 1278
Conc: 1.01 ng/ml

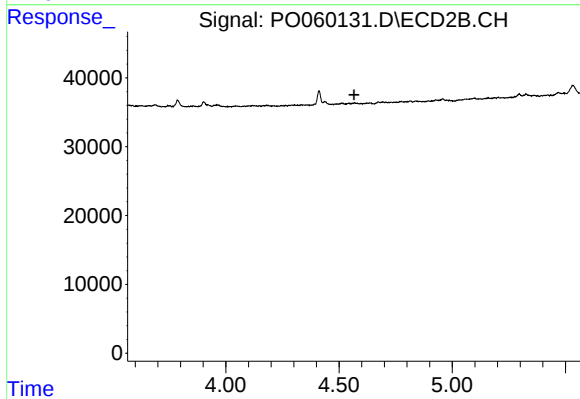

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

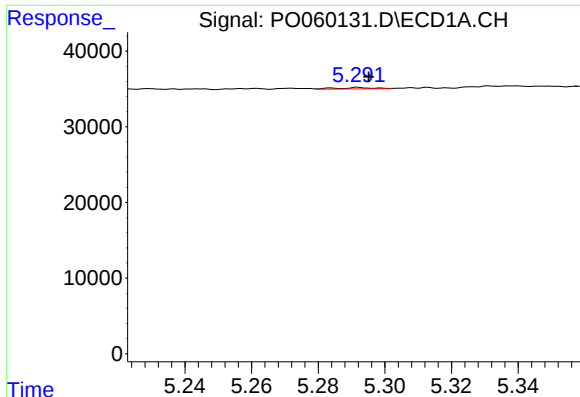

#17 AR-1242-2


R.T.: 5.292 min
Delta R.T.: -0.003 min
Response: 1278
Conc: 0.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

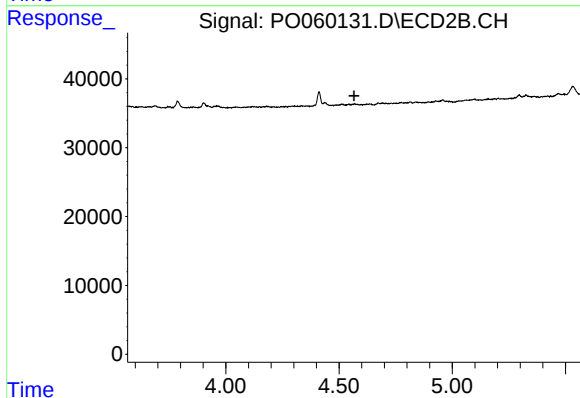


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

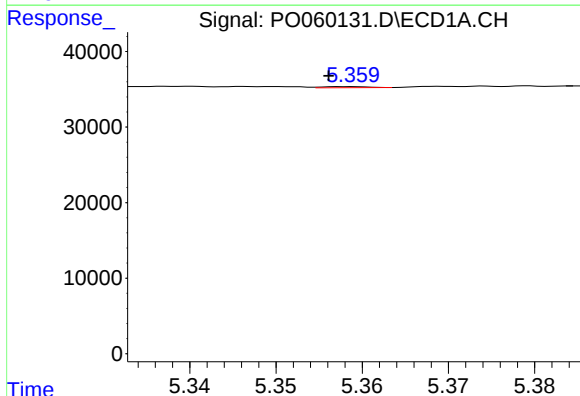


#18 AR-1242-3

R.T.: 5.358 min
Delta R.T.: 0.002 min
Response: 540
Conc: 0.46 ng/ml

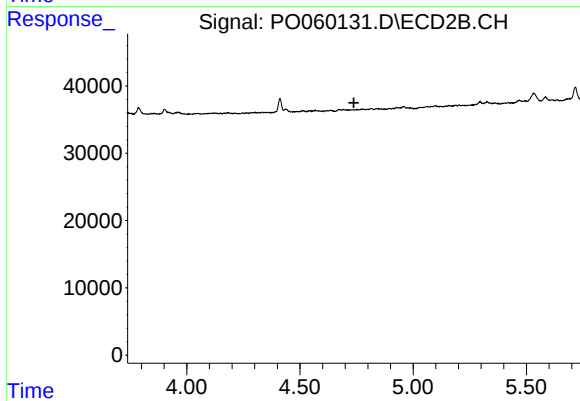

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

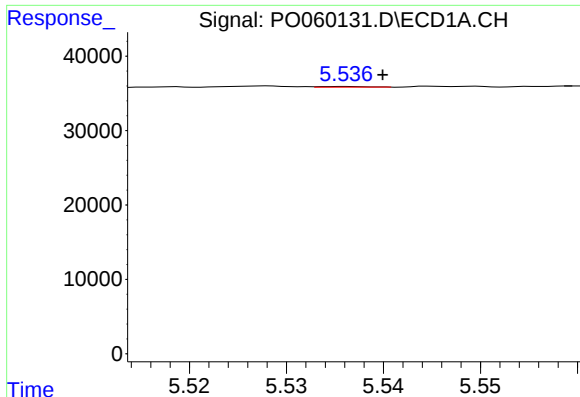

#19 AR-1242-4


R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 324
Conc: 0.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

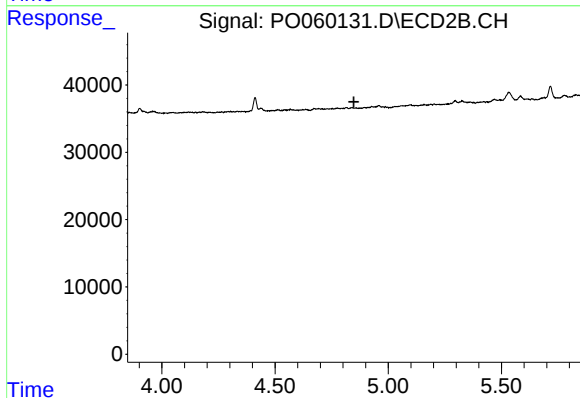


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

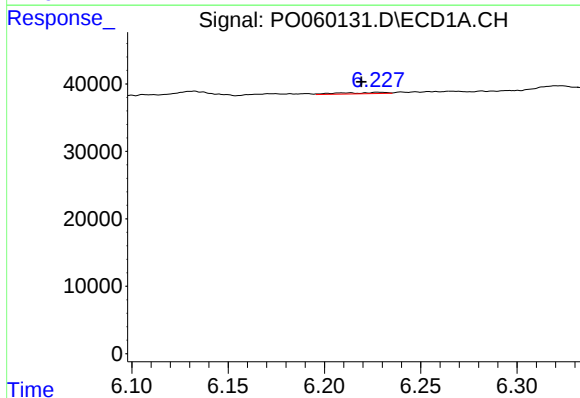


#20 AR-1242-5

R.T.: 6.228 min
Delta R.T.: 0.009 min
Response: 2977
Conc: 2.37 ng/ml

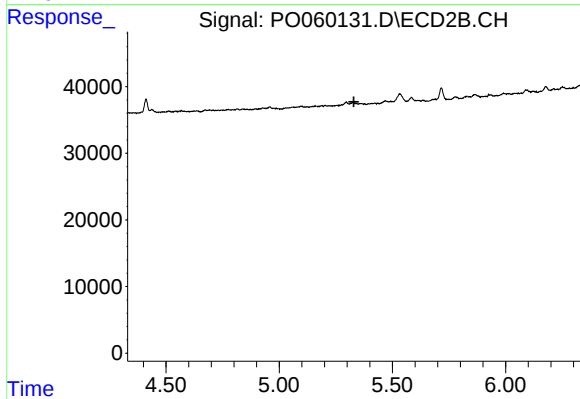

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

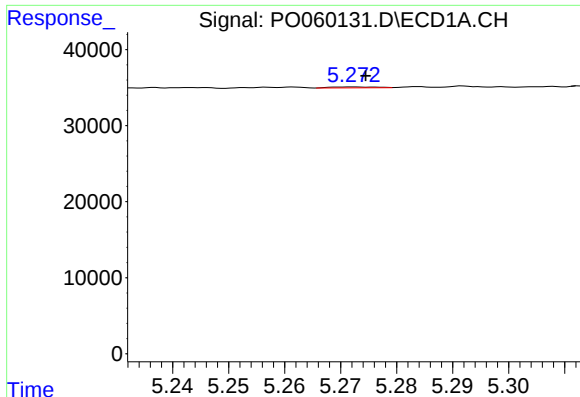

#21 AR-1248-1


R.T.: 5.272 min
Delta R.T.: -0.002 min
Response: 764
Conc: 0.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

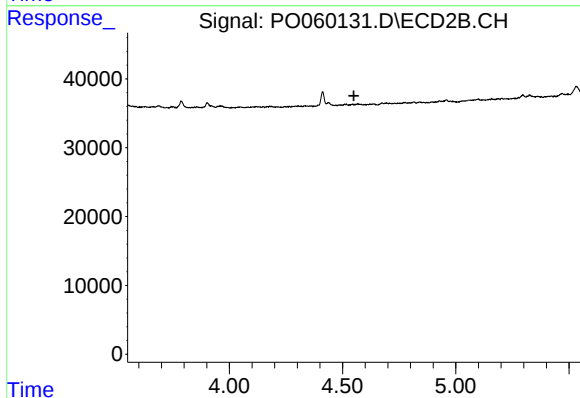


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

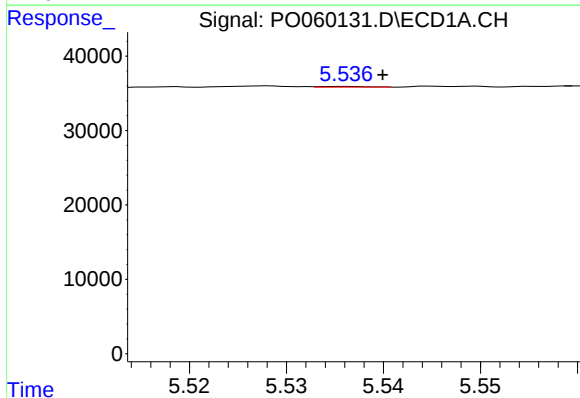


#22 AR-1248-2

R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 324
Conc: 0.22 ng/ml

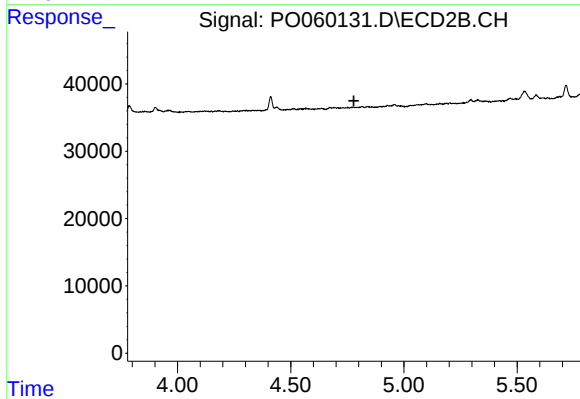

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

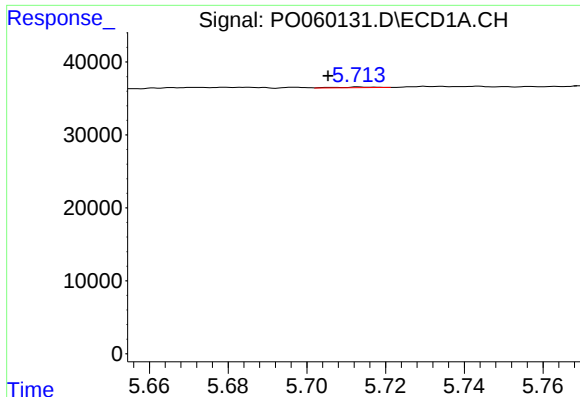

#23 AR-1248-3


R.T.: 5.713 min
Delta R.T.: 0.008 min
Response: 649
Conc: 0.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

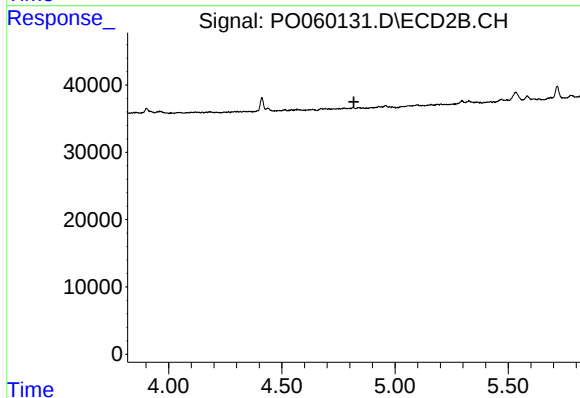


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

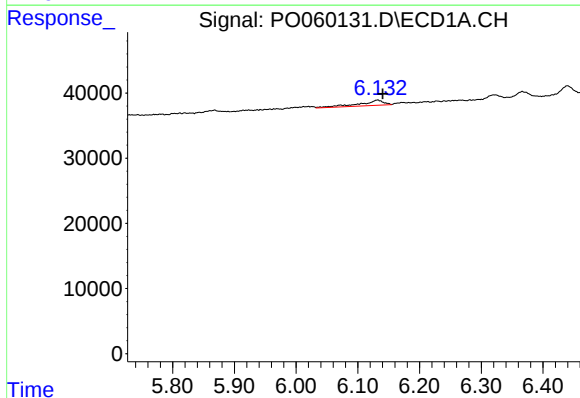


#24 AR-1248-4

R.T.: 6.132 min
Delta R.T.: -0.009 min
Response: 21445
Conc: 10.49 ng/ml

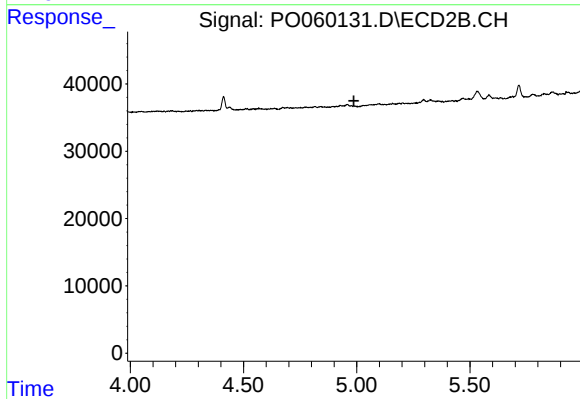

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

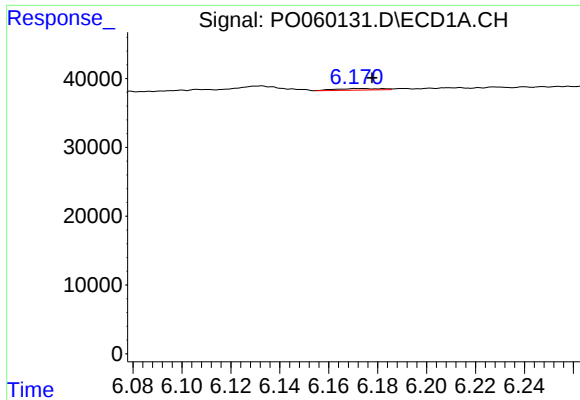

#25 AR-1248-5


R.T.: 6.173 min
Delta R.T.: -0.005 min
Response: 3016
Conc: 1.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

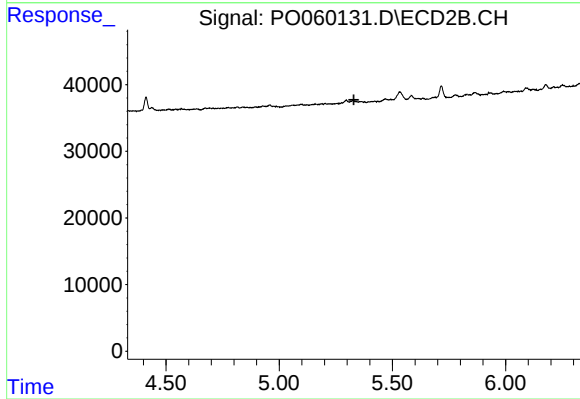


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

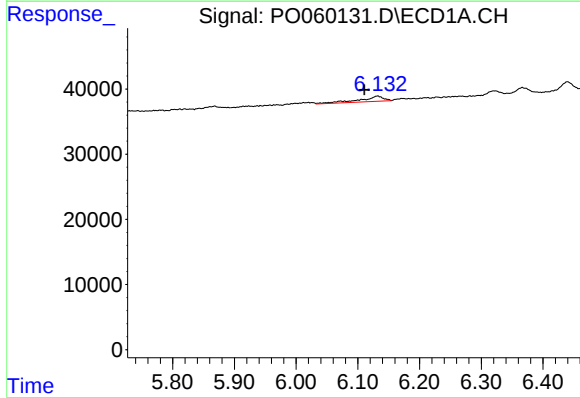


#26 AR-1254-1

R.T.: 6.132 min
Delta R.T.: 0.021 min
Response: 21445
Conc: 10.28 ng/ml

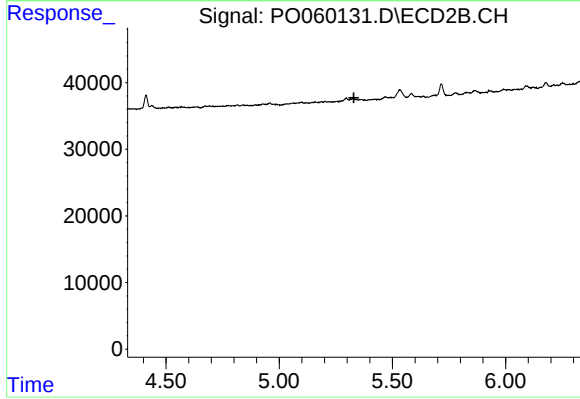

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

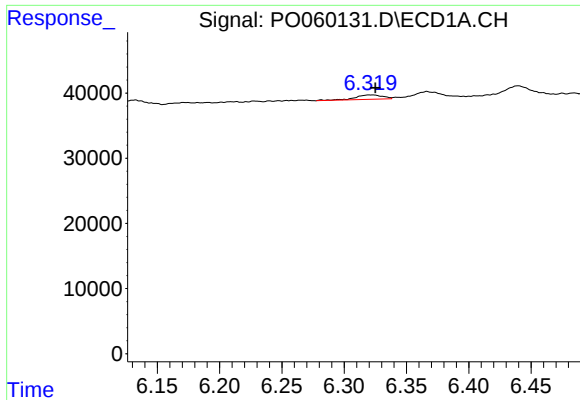

#27 AR-1254-2


R.T.: 6.322 min
Delta R.T.: -0.004 min
Response: 10356
Conc: 3.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

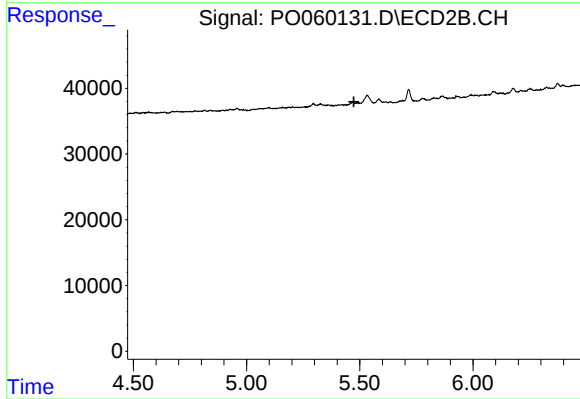


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.474 min
Response: 0
Conc: N.D.

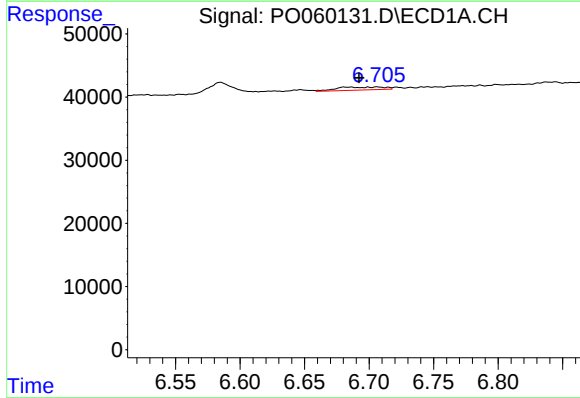


#28 AR-1254-3

R.T.: 6.681 min
Delta R.T.: -0.011 min
Response: 11782
Conc: 3.32 ng/ml

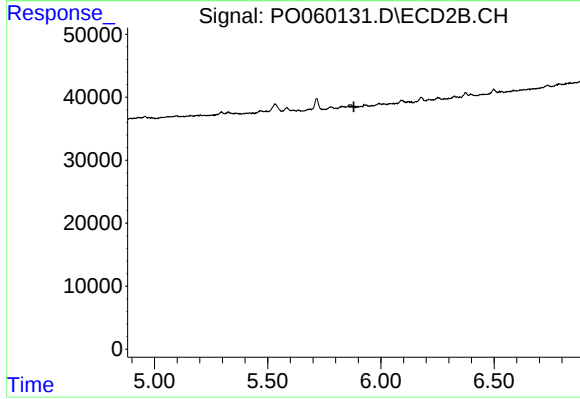

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.881 min
Response: 0
Conc: N.D.

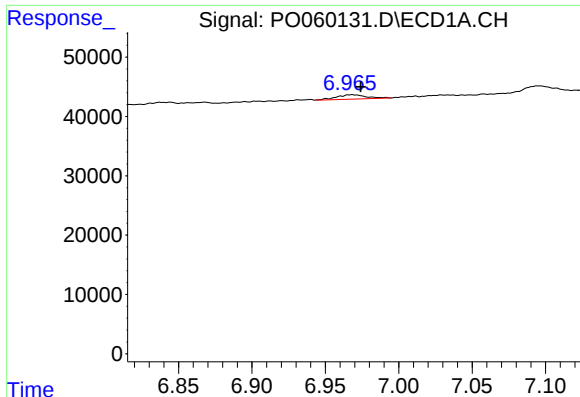

#29 AR-1254-4


R.T.: 6.968 min
Delta R.T.: -0.006 min
Response: 10654
Conc: 3.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

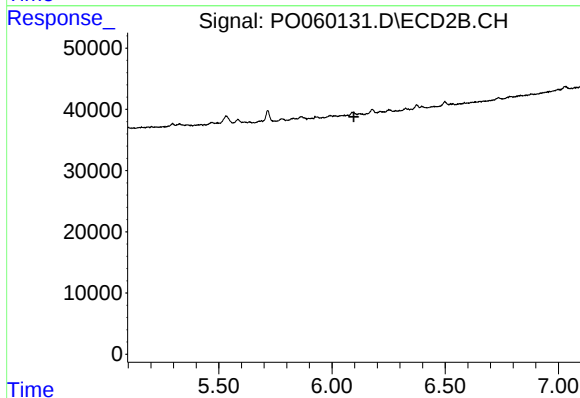


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

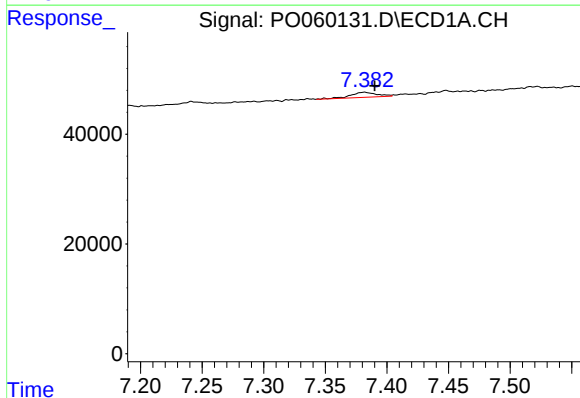


#30 AR-1254-5

R.T.: 7.382 min
Delta R.T.: -0.008 min
Response: 14215
Conc: 4.60 ng/ml

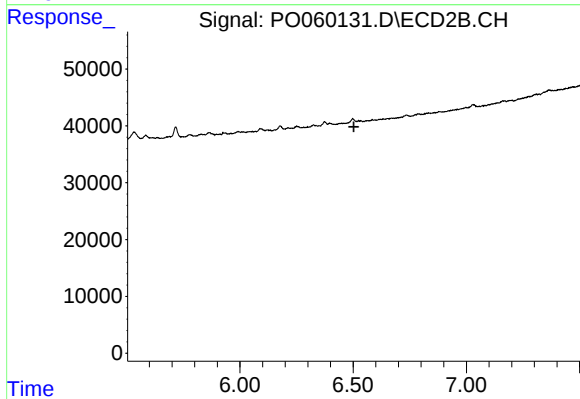

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.503 min
Response: 0
Conc: N.D.

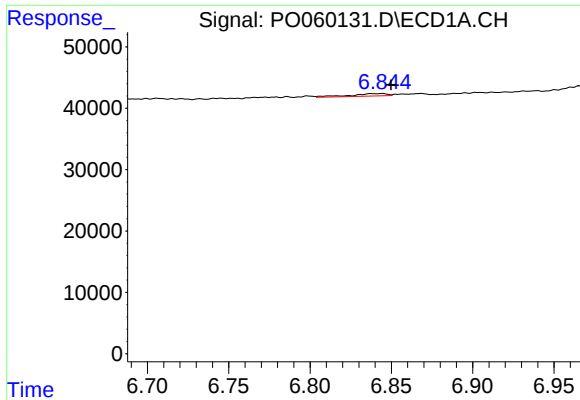

#31 AR-1260-1


R.T.: 6.844 min
Delta R.T.: -0.006 min
Response: 6350
Conc: 2.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

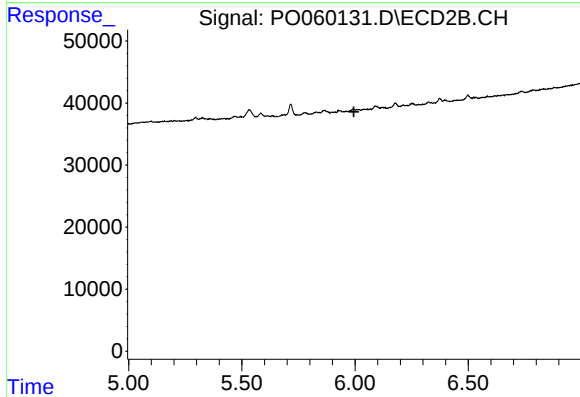


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.

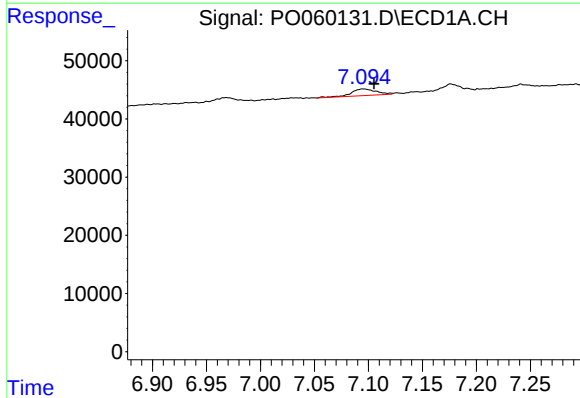


#32 AR-1260-2

R.T.: 7.096 min
Delta R.T.: -0.010 min
Response: 18474
Conc: 4.98 ng/ml

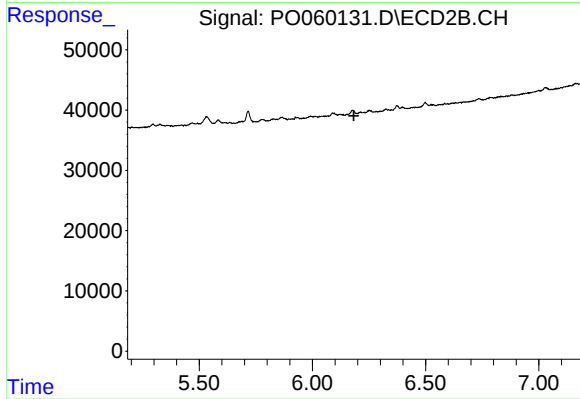

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.183 min
Response: 0
Conc: N.D.

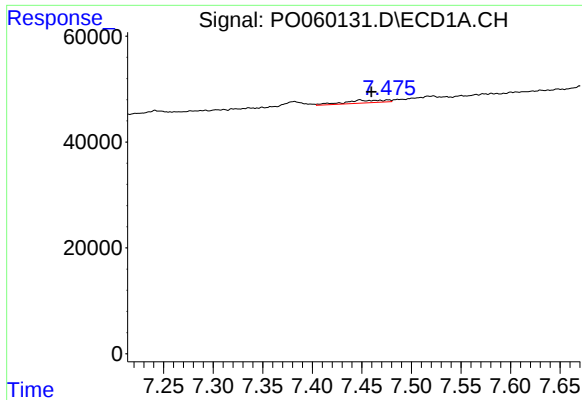

#33 AR-1260-3


R.T.: 7.448 min
Delta R.T.: -0.012 min
Response: 14837
Conc: 4.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

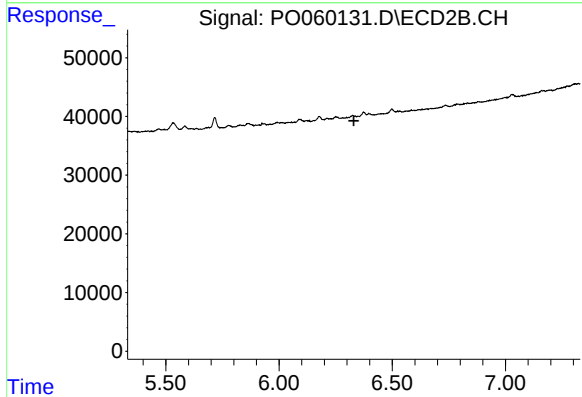


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

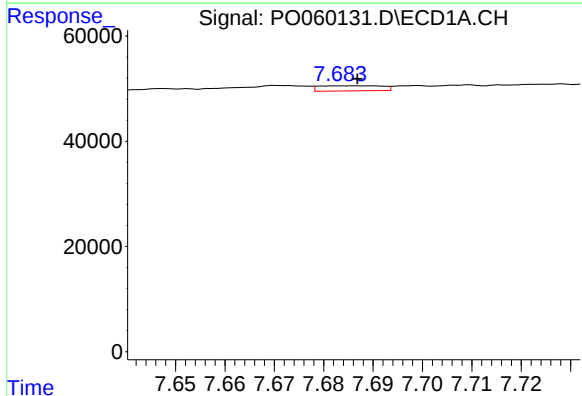


#34 AR-1260-4

R.T.: 7.688 min
Delta R.T.: 0.002 min
Response: 8603
Conc: 2.80 ng/ml

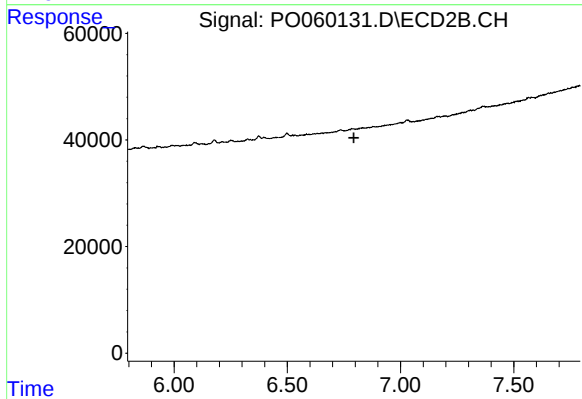

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

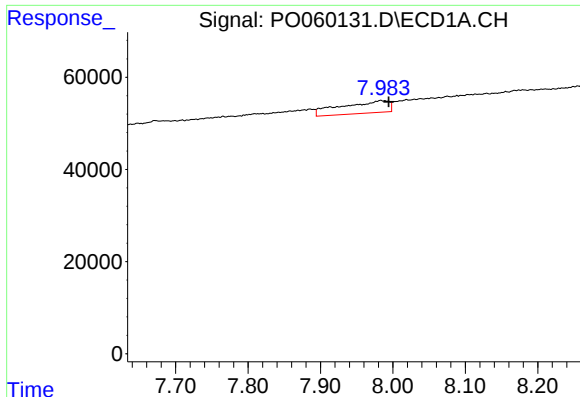

#35 AR-1260-5


R.T.: 7.983 min
Delta R.T.: -0.011 min
Response: 122103
Conc: 17.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

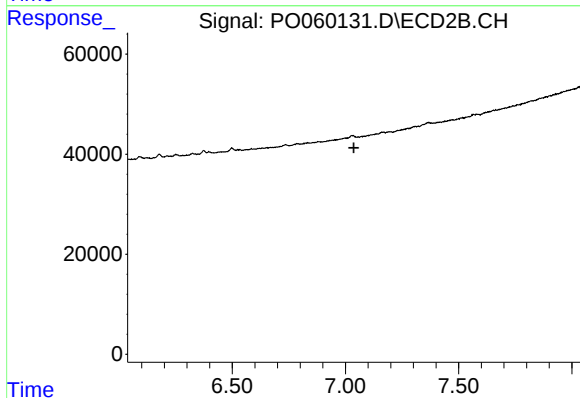


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

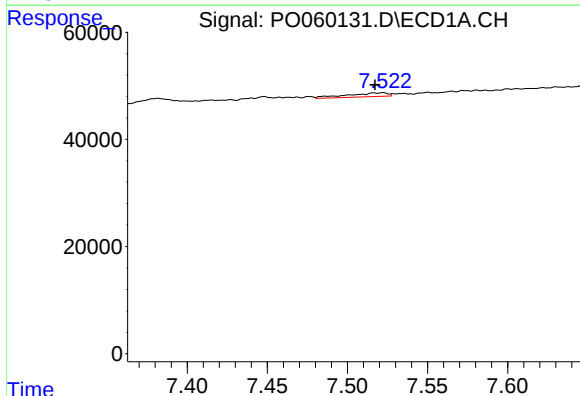


#36 AR-1262-1

R.T.: 7.522 min
Delta R.T.: 0.005 min
Response: 12615
Conc: 2.60 ng/ml

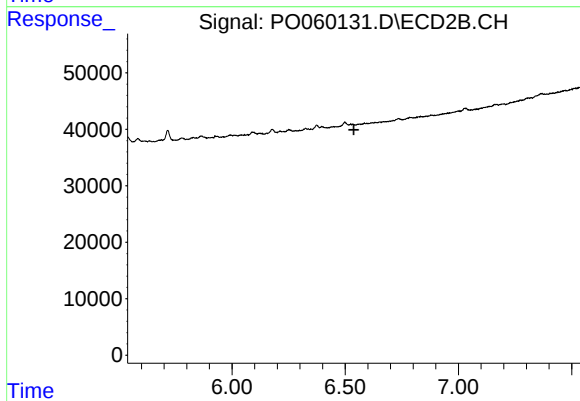

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.538 min
Response: 0
Conc: N.D.

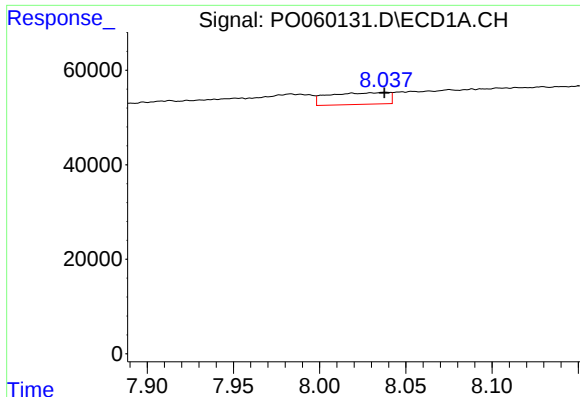

#37 AR-1262-2


R.T.: 8.038 min
Delta R.T.: 0.000 min
Response: 59919
Conc: 7.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

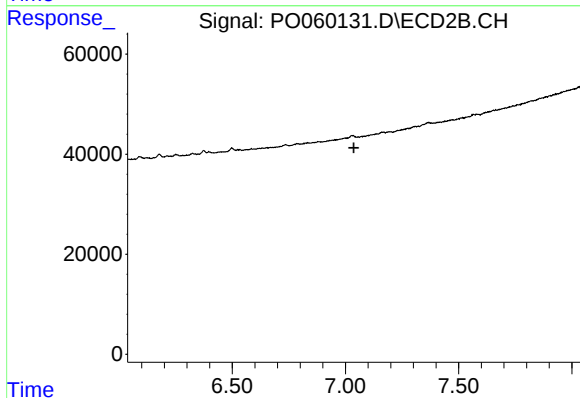


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

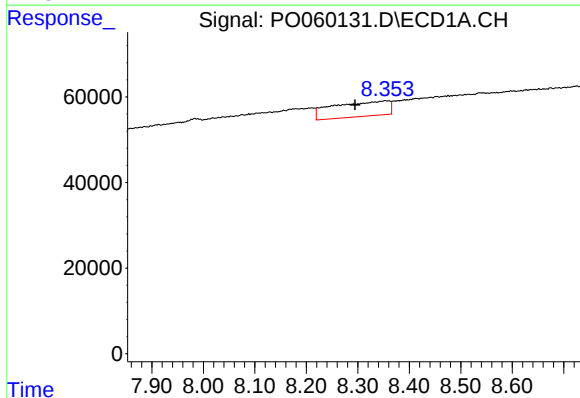


#38 AR-1262-3

R.T.: 8.353 min
Delta R.T.: 0.058 min
Response: 265419
Conc: 52.02 ng/ml

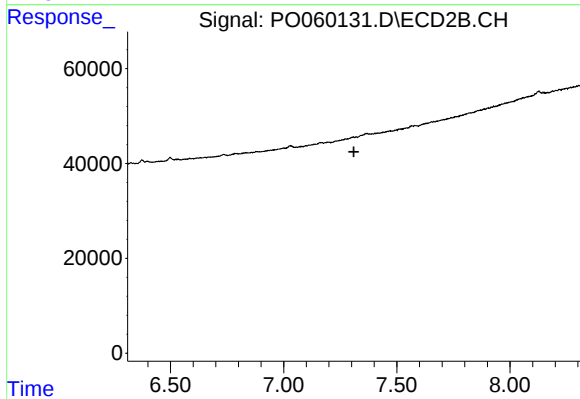

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

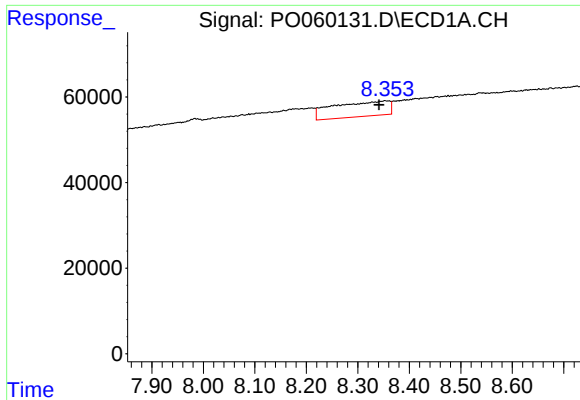

#39 AR-1262-4


R.T.: 8.353 min
Delta R.T.: 0.011 min
Response: 265419
Conc: 68.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

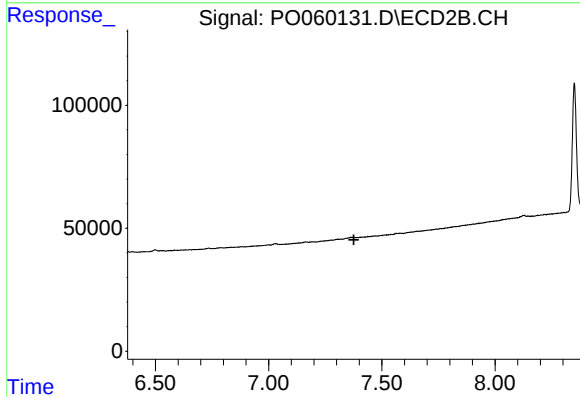


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.376 min
Response: 0
Conc: N.D.

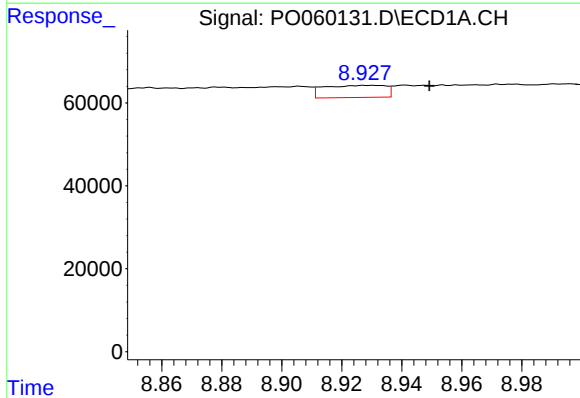


#40 AR-1262-5

R.T.: 8.930 min
Delta R.T.: -0.019 min
Response: 41443
Conc: 16.15 ng/ml

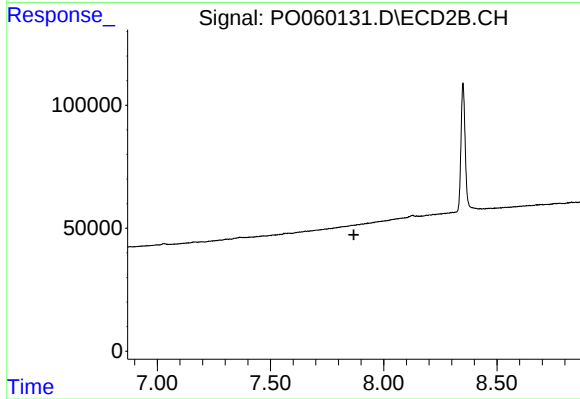

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 7.868 min
Response: 0
Conc: N.D.

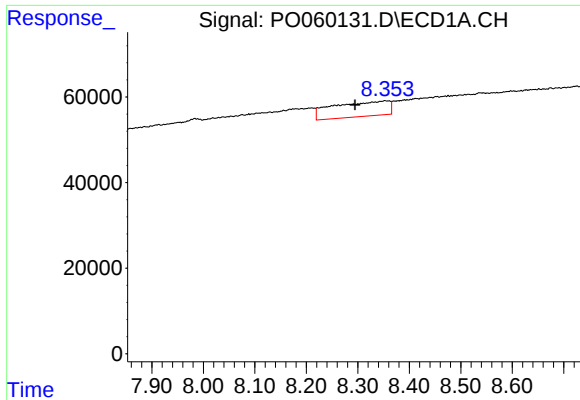

#41 AR-1268-1


R.T.: 8.353 min
Delta R.T.: 0.058 min
Response: 265419
Conc: 28.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

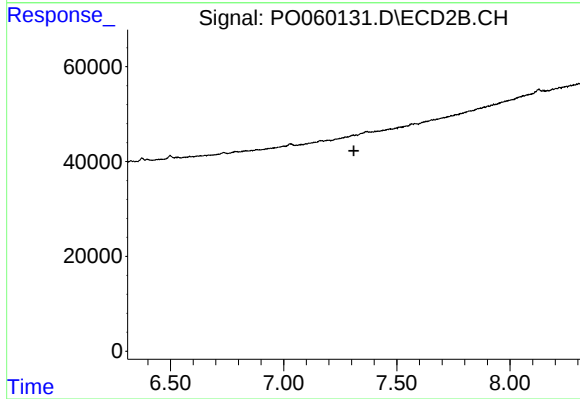


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

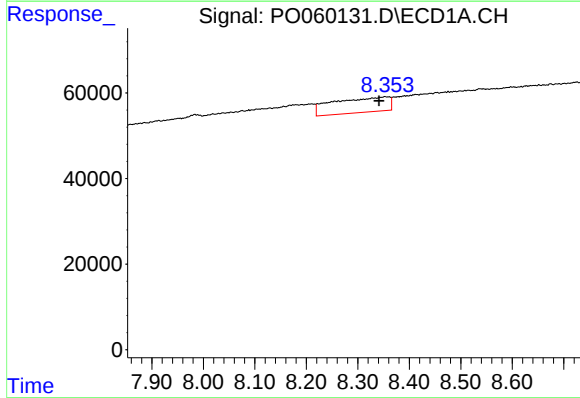


#42 AR-1268-2

R.T.: 8.353 min
Delta R.T.: 0.011 min
Response: 265419
Conc: 33.67 ng/ml

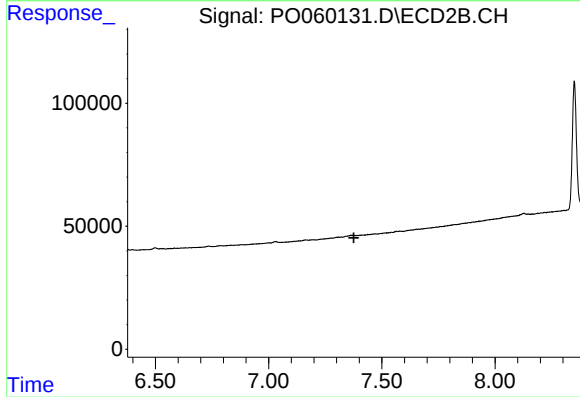

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.376 min
Response: 0
Conc: N.D.

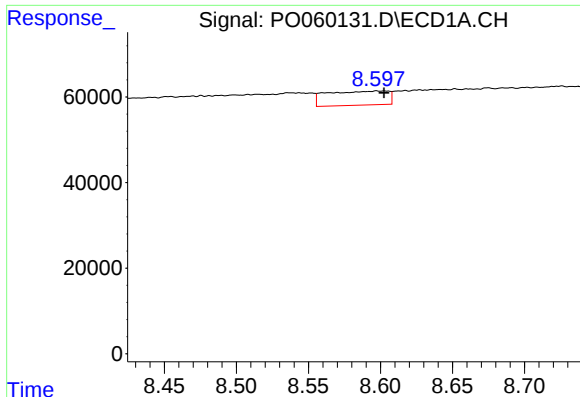

#43 AR-1268-3


R.T.: 8.597 min
Delta R.T.: -0.005 min
Response: 97165
Conc: 13.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

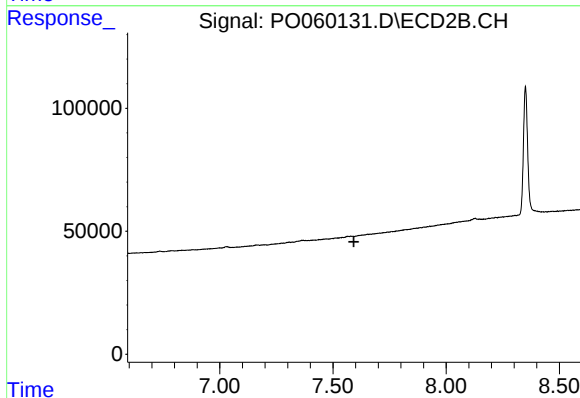


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

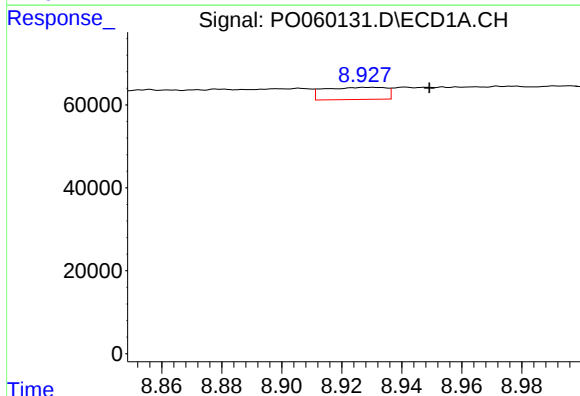


#44 AR-1268-4

R.T.: 8.930 min
Delta R.T.: -0.019 min
Response: 41443
Conc: 14.91 ng/ml

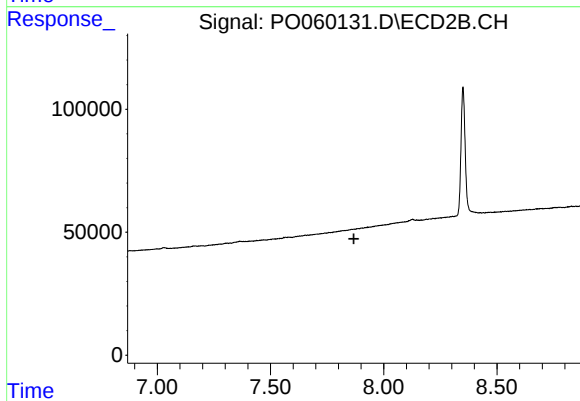

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.868 min
Response: 0
Conc: N.D.

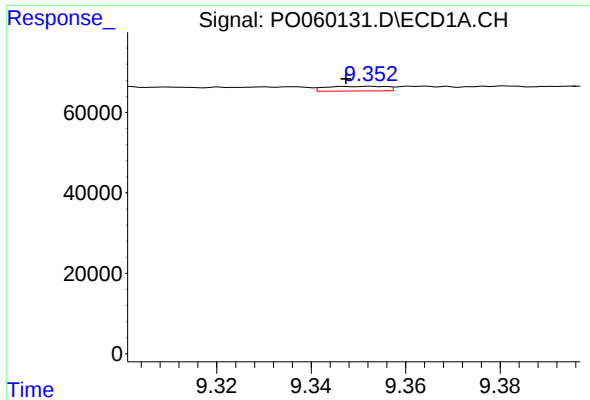

#45 AR-1268-5

R.T.: 9.353 min
Delta R.T.: 0.005 min
Response: 10258
Conc: 0.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP8-COMP

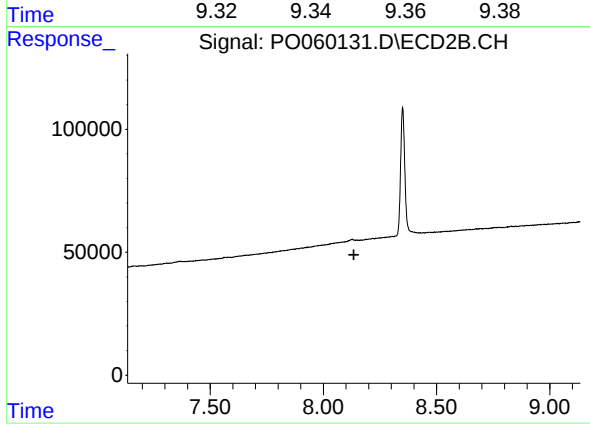

#45 AR-1268-5

R.T.: 8.128 min
Delta R.T.: -0.006 min
Response: -434969
Conc: N.D.