

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060076.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 9:26
 Operator : SM/AJ
 Sample : K4547-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 T7-S-G1-G4

Manual Integrations
 APPROVED

Ankita
 8/31/2019 3:12:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 13:37:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.124	3.497	1230615	1036085	35.148	28.784
2) SA Decachlor...	9.586	8.352	1197172	912515	22.503	22.631m
Target Compounds						
31) L7 AR-1260-1	6.846	5.991	913454	707332	338.841m	310.382
32) L7 AR-1260-2	7.102	6.179	744538	441111	200.658	150.556
33) L7 AR-1260-3	7.455	6.325	687415	582055	209.812	219.715
34) L7 AR-1260-4	7.680	6.789	939336	432973	305.841m	191.362 #
35) L7 AR-1260-5	7.988	7.032	1492657	1088801	210.800m	197.844

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083019\
Data File : PO060076.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 9:26
Operator : SM/AJ
Sample : K4547-15
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
T7-S-G1-G4


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 13:37:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

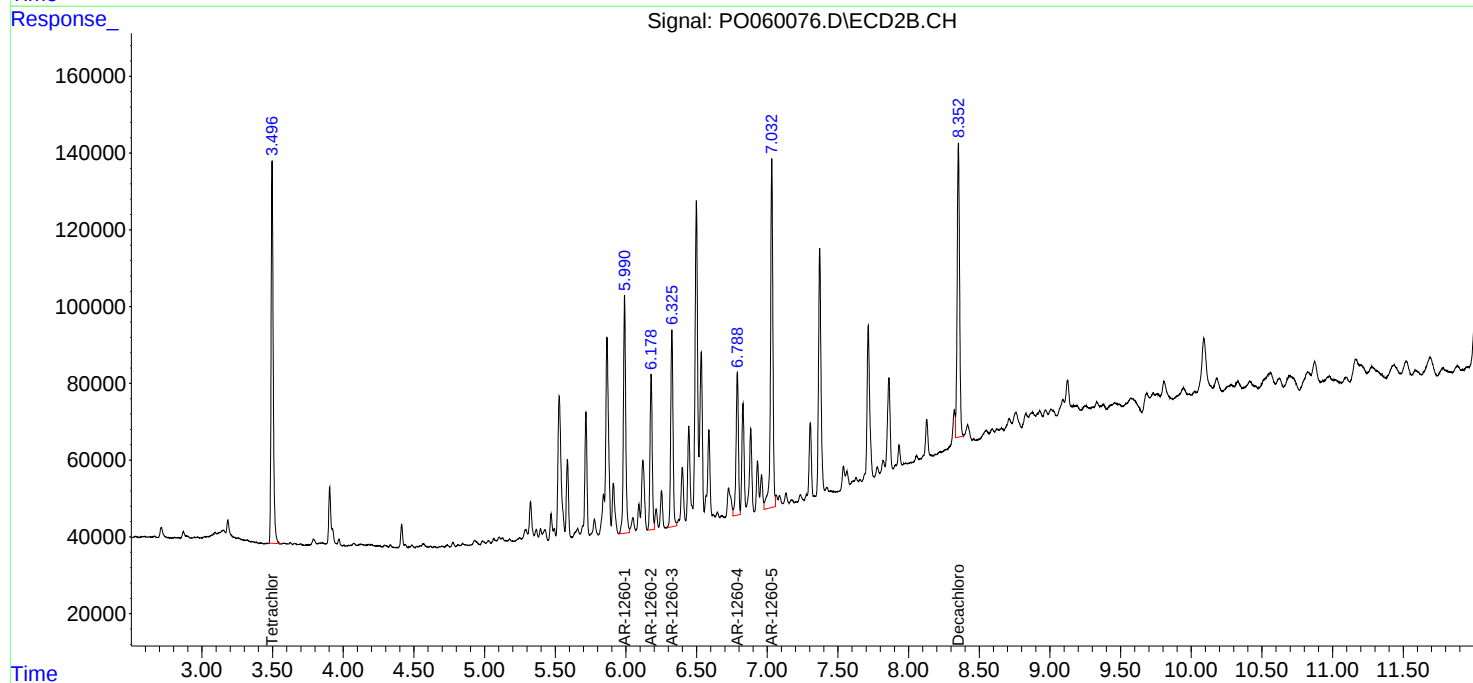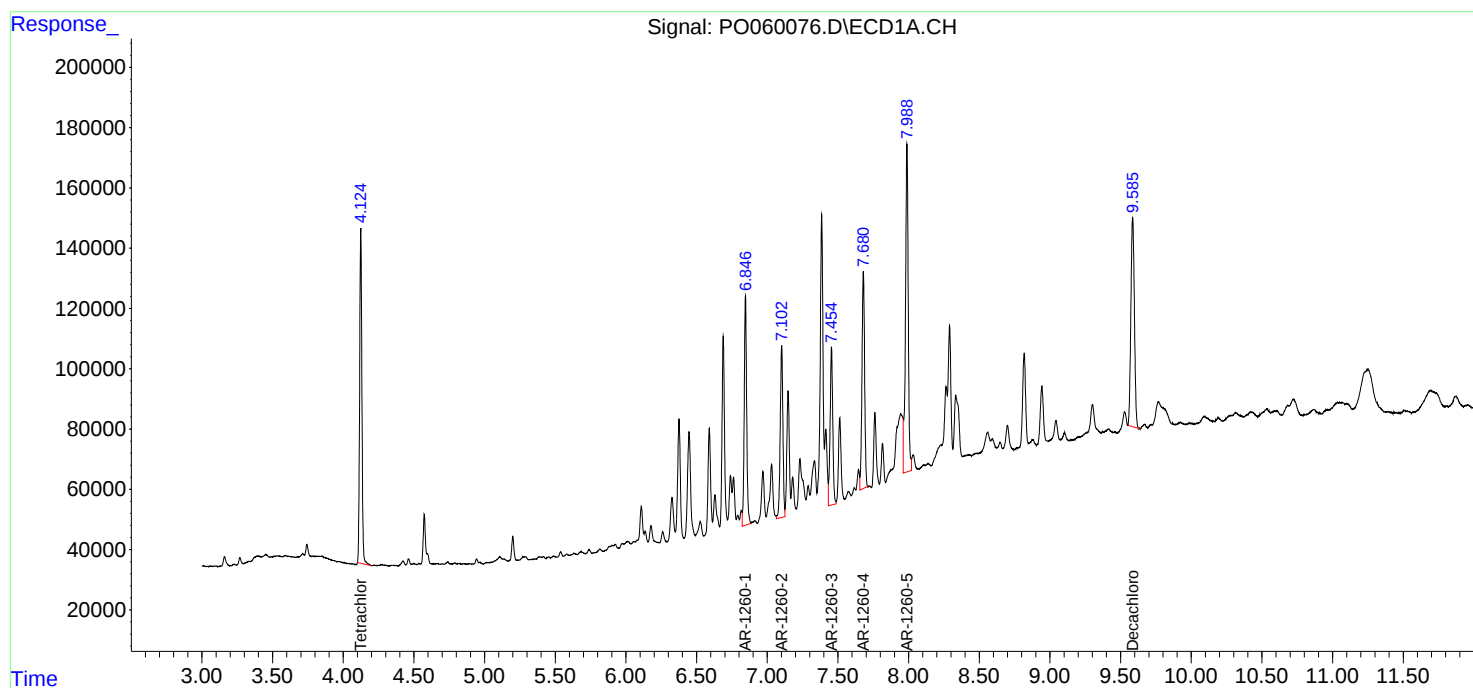

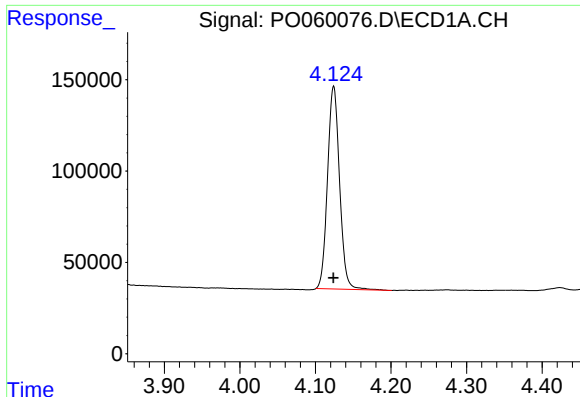


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 1230615
Conc: 35.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
T7-S-G1-G4


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:15 PM

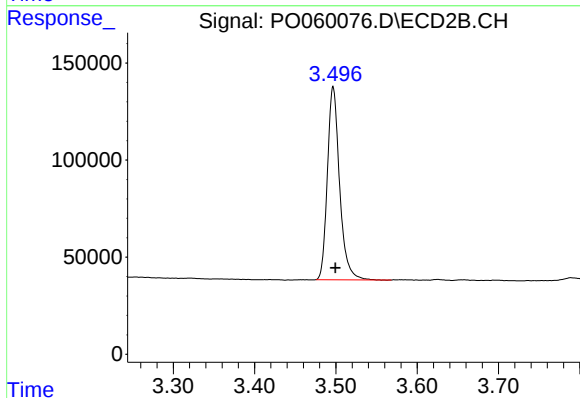


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.003 min
Response: 1036085
Conc: 28.78 ng/ml

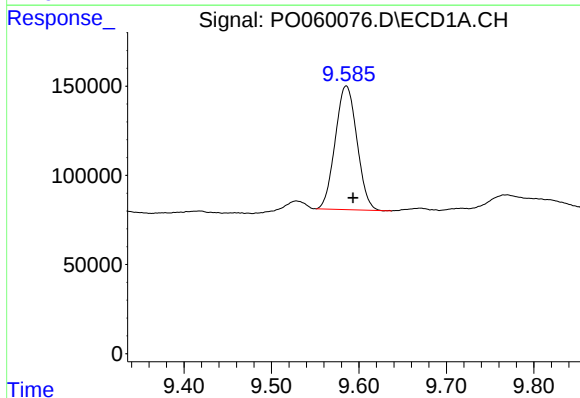


#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.008 min
Response: 1197172
Conc: 22.50 ng/ml

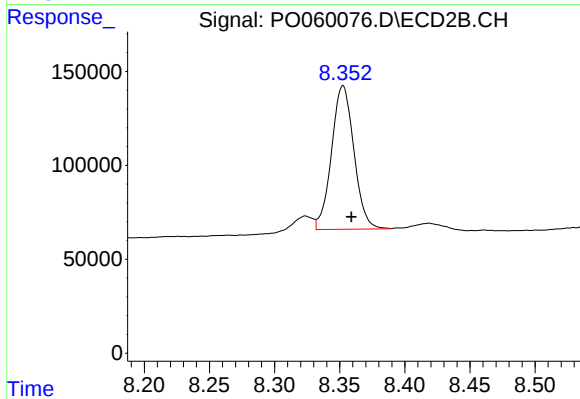

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: -0.007 min
Response: 912515
Conc: 22.63 ng/ml m

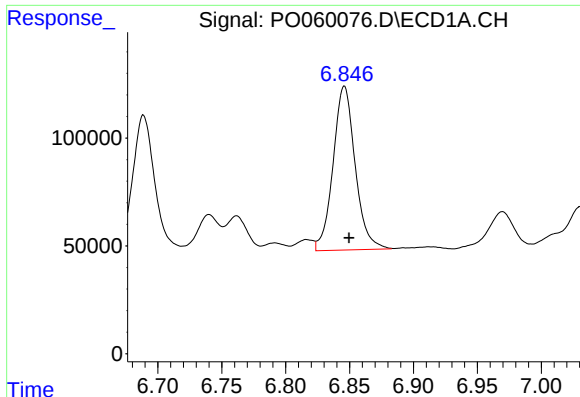


#31 AR-1260-1

R.T.: 6.846 min
Delta R.T.: -0.004 min
Response: 913454
Conc: 338.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
T7-S-G1-G4


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:15 PM

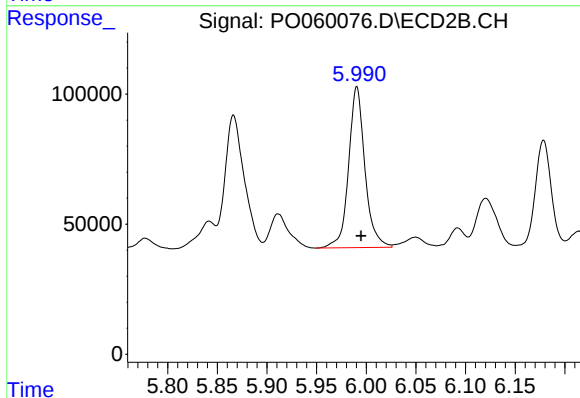


#31 AR-1260-1

R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 707332
Conc: 310.38 ng/ml

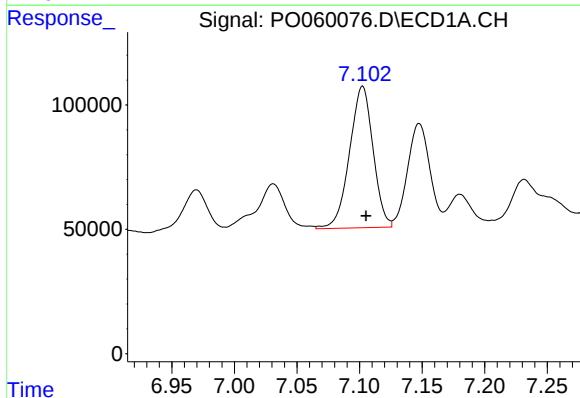


#32 AR-1260-2

R.T.: 7.102 min
Delta R.T.: -0.003 min
Response: 744538
Conc: 200.66 ng/ml

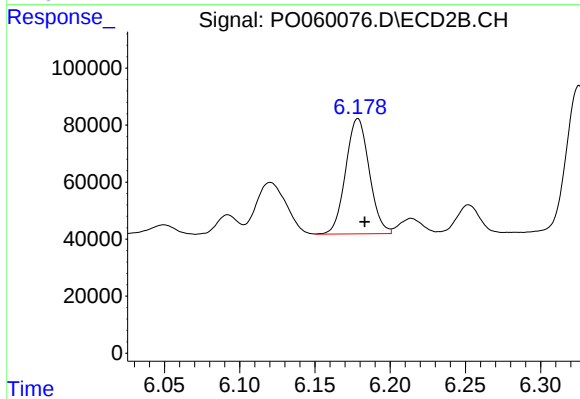

#32 AR-1260-2

R.T.: 6.179 min
Delta R.T.: -0.005 min
Response: 441111
Conc: 150.56 ng/ml

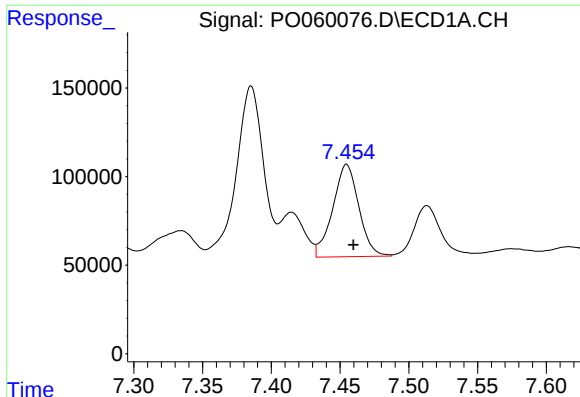


#33 AR-1260-3

R.T.: 7.455 min
Delta R.T.: -0.005 min
Response: 687415
Conc: 209.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
T7-S-G1-G4


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:15 PM

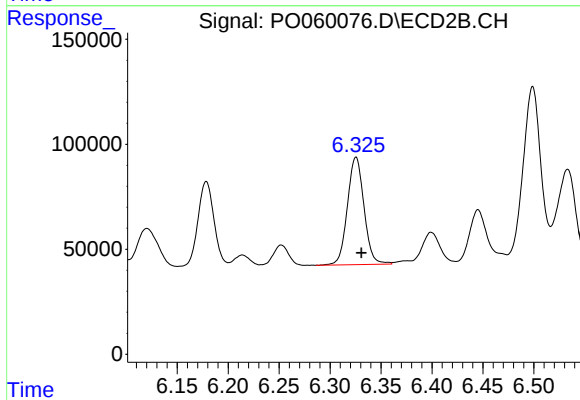


#33 AR-1260-3

R.T.: 6.325 min
Delta R.T.: -0.005 min
Response: 582055
Conc: 219.71 ng/ml

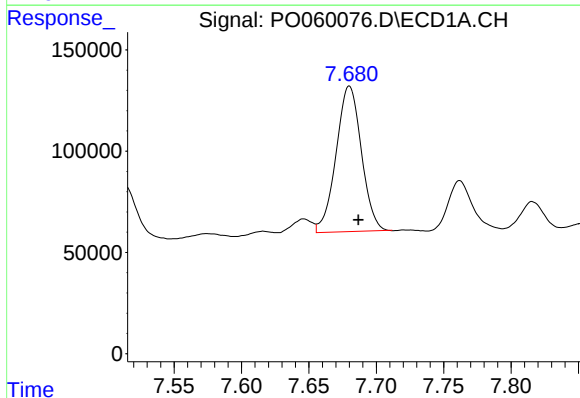


#34 AR-1260-4

R.T.: 7.680 min
Delta R.T.: -0.007 min
Response: 939336
Conc: 305.84 ng/ml m

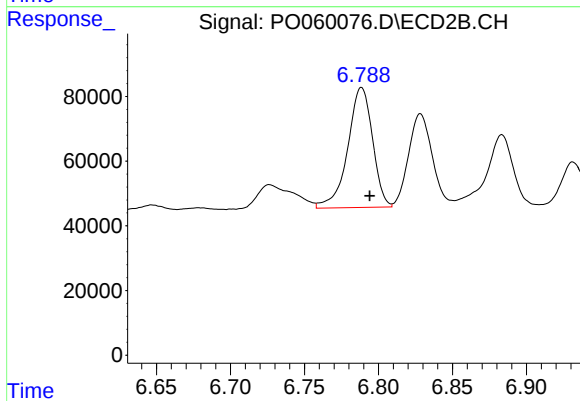

#34 AR-1260-4

R.T.: 6.789 min
Delta R.T.: -0.006 min
Response: 432973
Conc: 191.36 ng/ml

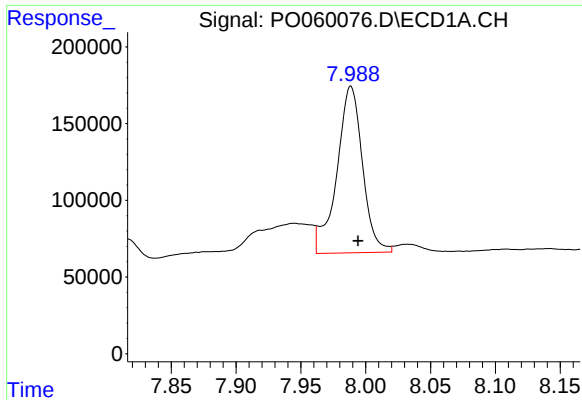


#35 AR-1260-5

R.T.: 7.988 min
Delta R.T.: -0.006 min
Response: 1492657
Conc: 210.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
T7-S-G1-G4

Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:15 PM

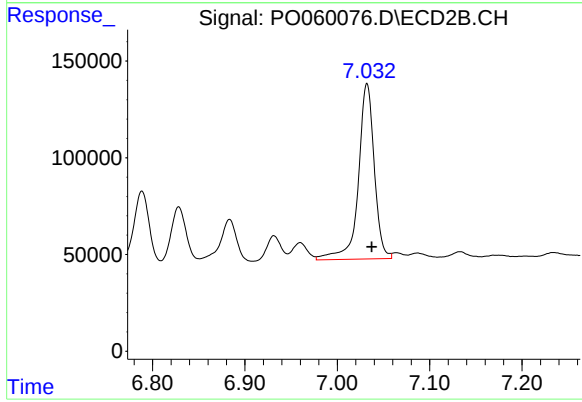

#35 AR-1260-5

R.T.: 7.032 min
Delta R.T.: -0.005 min
Response: 1088801
Conc: 197.84 ng/ml