

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060077.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 9:44
 Operator : SM/AJ
 Sample : K4596-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S403-K1-1.0-1.5-082819

Manual Integrations
 APPROVED

Ankita
 8/31/2019 3:12:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 13:38:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.124	3.496	1098073	964775	31.362	26.803
2) SA Decachlor...	9.584	8.352	1185153	888646	22.277	22.039
Target Compounds						
31) L7 AR-1260-1	6.846	5.991	605346	440080	224.550	193.110
32) L7 AR-1260-2	7.104	6.178	1889018	931813	509.104	318.038 #
33) L7 AR-1260-3	7.455	6.326	875381	502695	267.183	189.758 #
34) L7 AR-1260-4	7.680	6.788	761110	534612	247.812m	236.284
35) L7 AR-1260-5	7.988	7.032	1742614	1355365	246.100m	246.281

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060077.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 9:44
Operator : SM/AJ
Sample : K4596-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S403-K1-1.0-1.5-082819


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 13:38:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

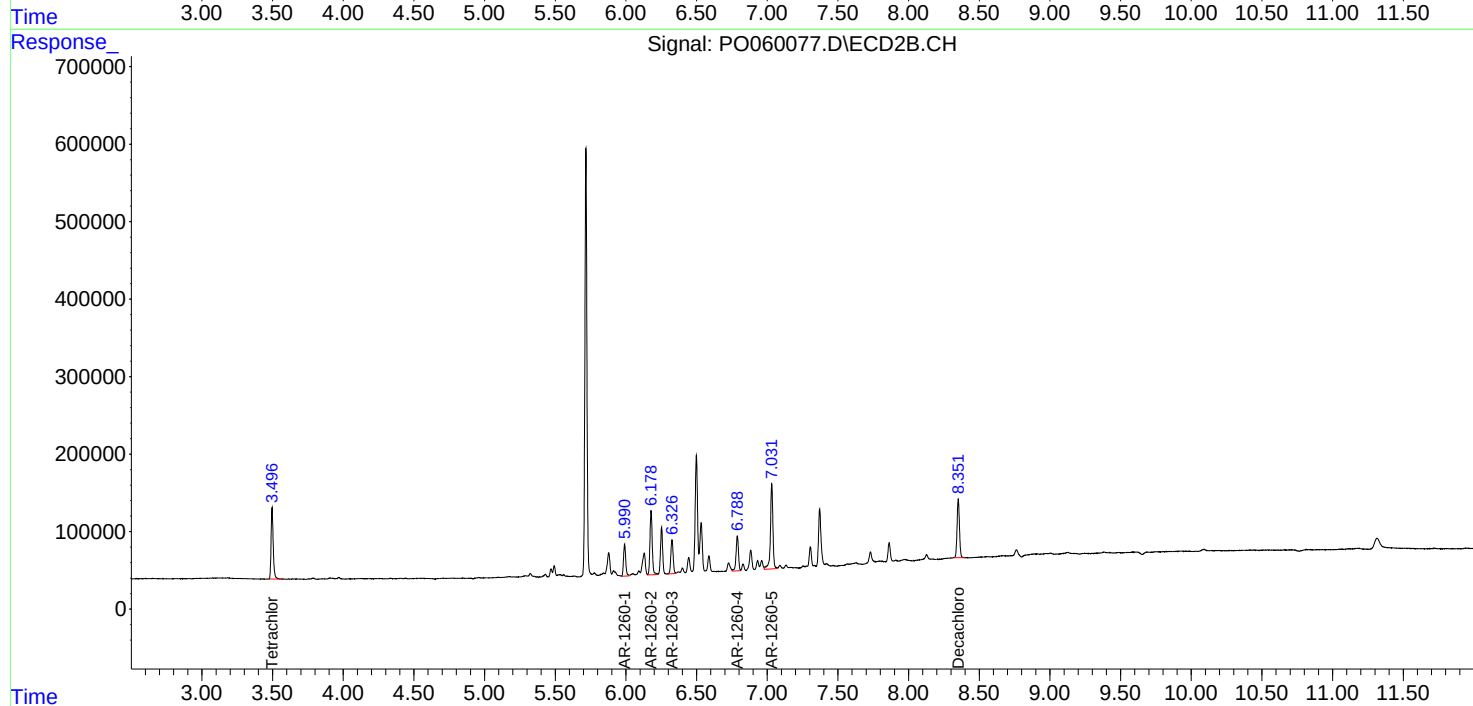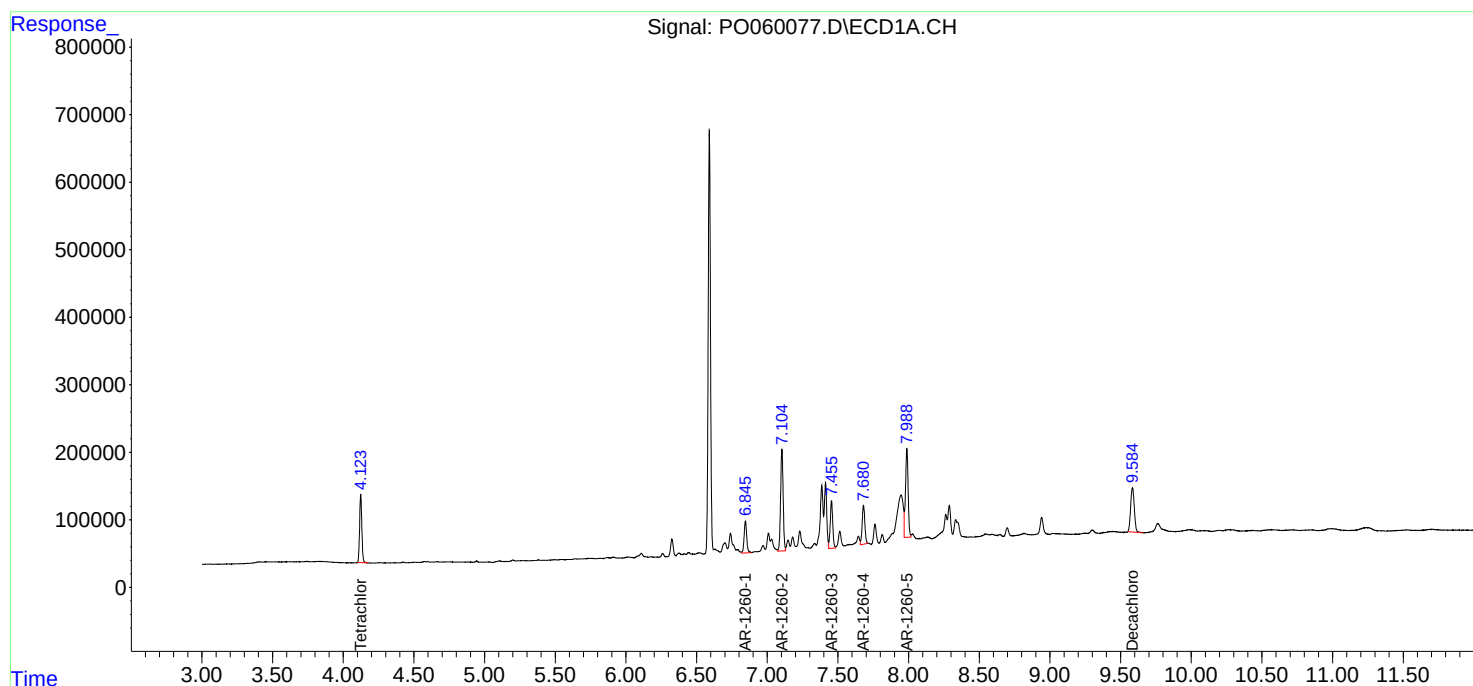

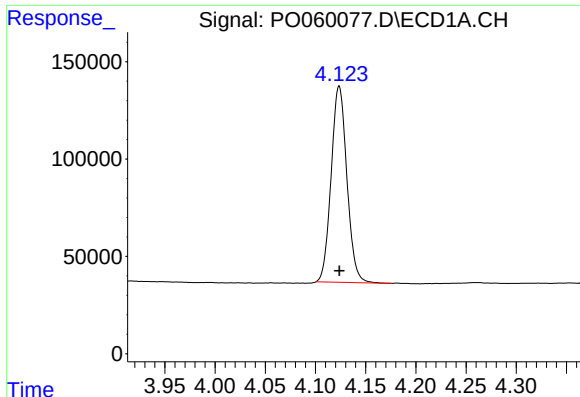


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 1098073
Conc: 31.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
S403-K1-1.0-1.5-082819


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:17 PM

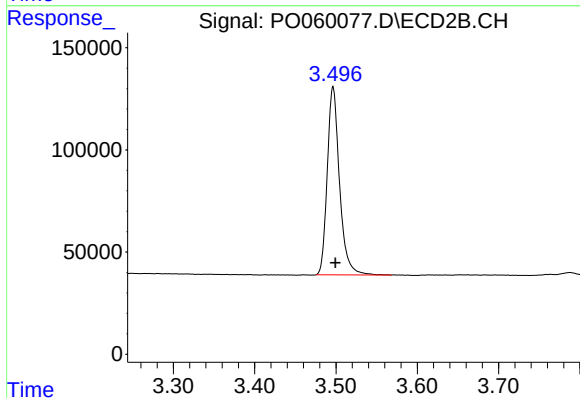


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.003 min
Response: 964775
Conc: 26.80 ng/ml

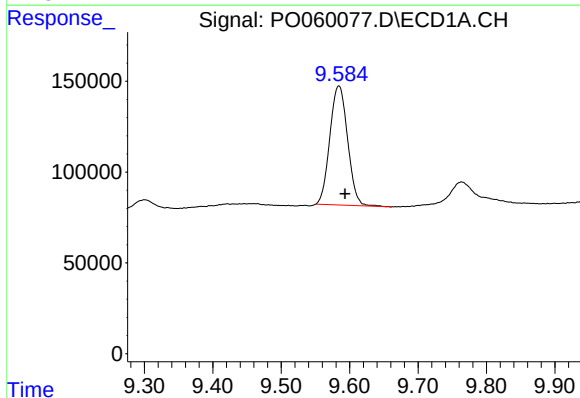


#2 Decachlorobiphenyl

R.T.: 9.584 min
Delta R.T.: -0.009 min
Response: 1185153
Conc: 22.28 ng/ml

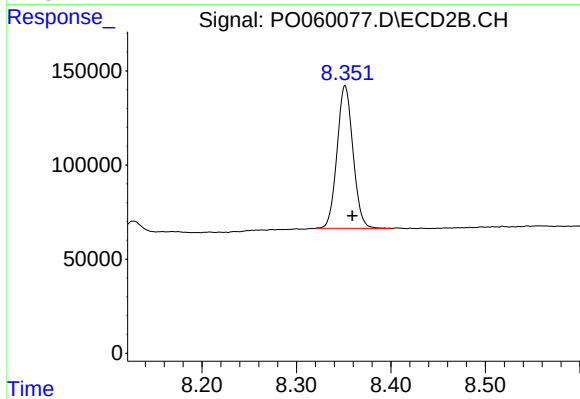

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: -0.008 min
Response: 888646
Conc: 22.04 ng/ml

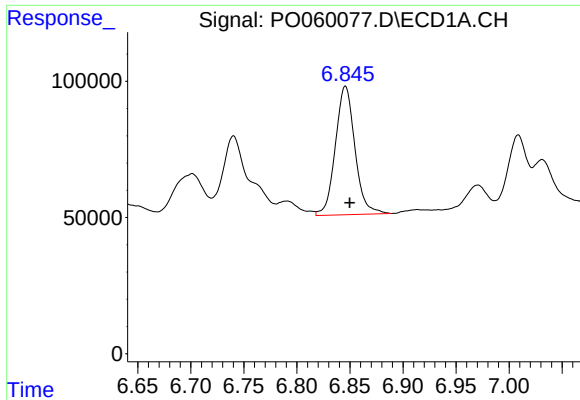


#31 AR-1260-1

R.T.: 6.846 min
Delta R.T.: -0.004 min
Response: 605346
Conc: 224.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
S403-K1-1.0-1.5-082819


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:17 PM

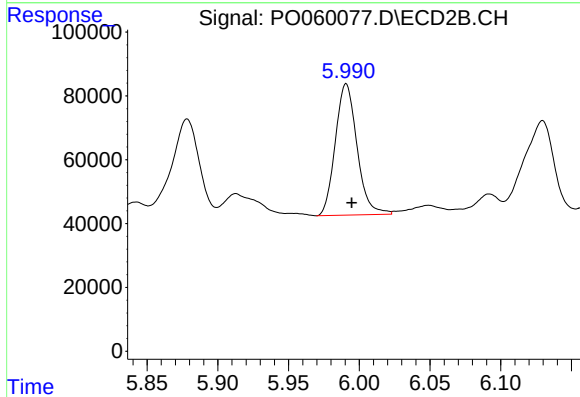


#31 AR-1260-1

R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 440080
Conc: 193.11 ng/ml

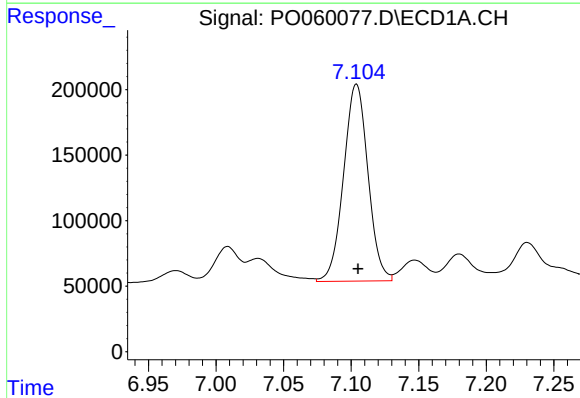


#32 AR-1260-2

R.T.: 7.104 min
Delta R.T.: -0.001 min
Response: 1889018
Conc: 509.10 ng/ml

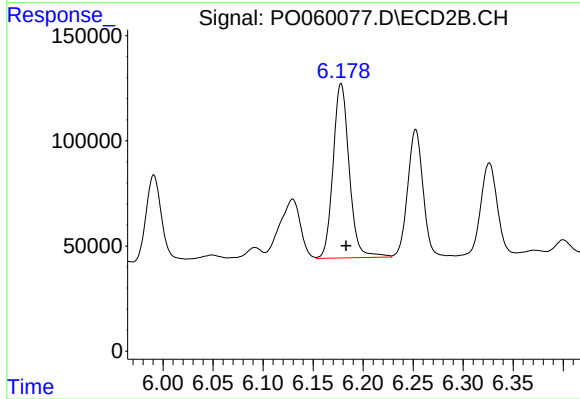

#32 AR-1260-2

R.T.: 6.178 min
Delta R.T.: -0.005 min
Response: 931813
Conc: 318.04 ng/ml

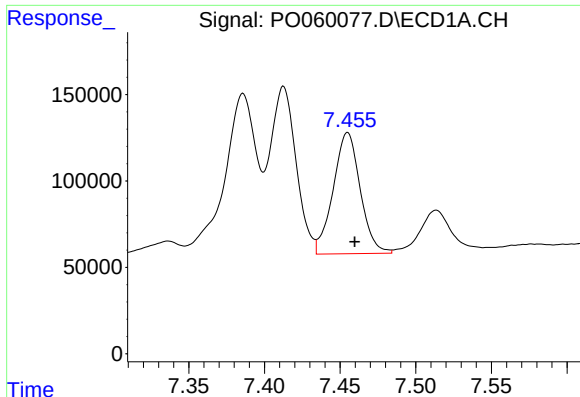


#33 AR-1260-3

R.T.: 7.455 min
Delta R.T.: -0.005 min
Response: 875381
Conc: 267.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
S403-K1-1.0-1.5-082819


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:17 PM

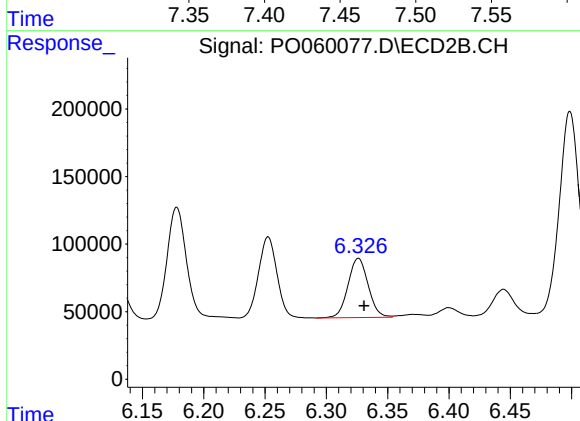


#33 AR-1260-3

R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 502695
Conc: 189.76 ng/ml

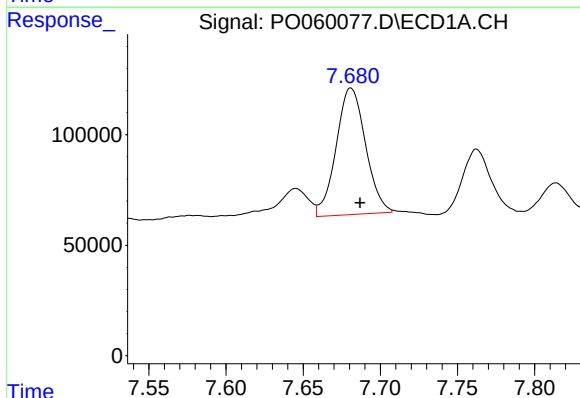


#34 AR-1260-4

R.T.: 7.680 min
Delta R.T.: -0.006 min
Response: 761110
Conc: 247.81 ng/ml m

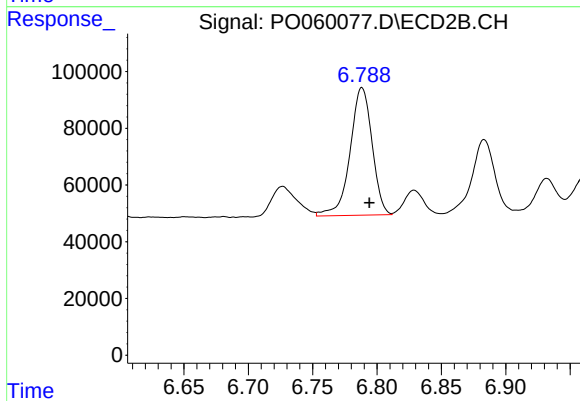

#34 AR-1260-4

R.T.: 6.788 min
Delta R.T.: -0.006 min
Response: 534612
Conc: 236.28 ng/ml

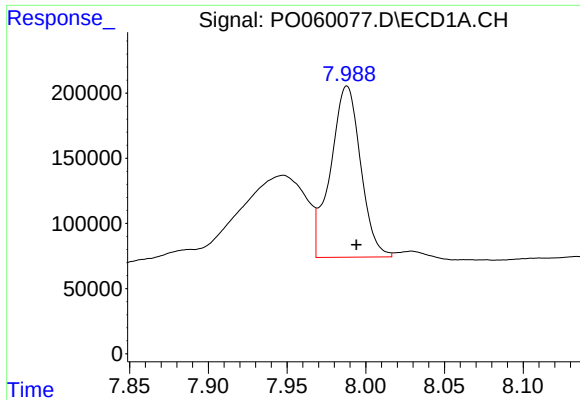


#35 AR-1260-5

R.T.: 7.988 min
Delta R.T.: -0.006 min
Response: 1742614
Conc: 246.10 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S403-K1-1.0-1.5-082819

Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:17 PM

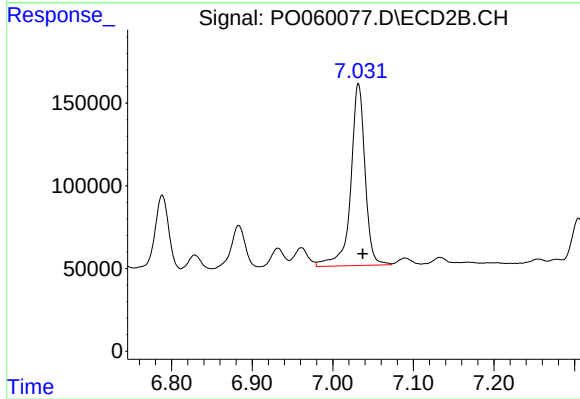

#35 AR-1260-5

R.T.: 7.032 min
Delta R.T.: -0.005 min
Response: 1355365
Conc: 246.28 ng/ml