

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060090.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 13:49
 Operator : SM/AJ
 Sample : PB122685BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB122685BL

Manual Integrations
 APPROVED

Ankita
 8/31/2019 3:12:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 16:52:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 28 13:30:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.123	3.497	658543	590072	18.809m	16.393
2) SA Decachlor...	9.584	8.353	842668	646861	15.840m	16.043

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060090.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 13:49
Operator : SM/AJ
Sample : PB122685BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB122685BL


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 16:52:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 28 13:30:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

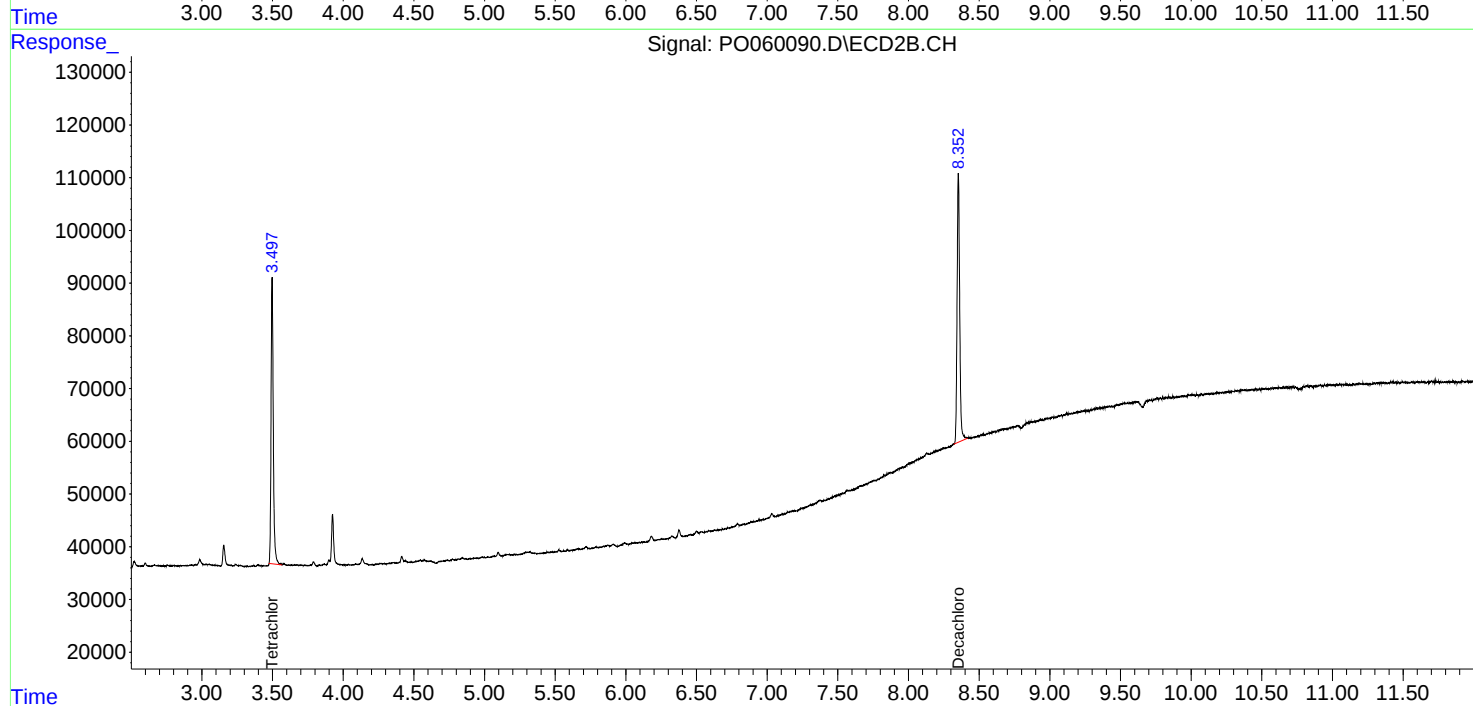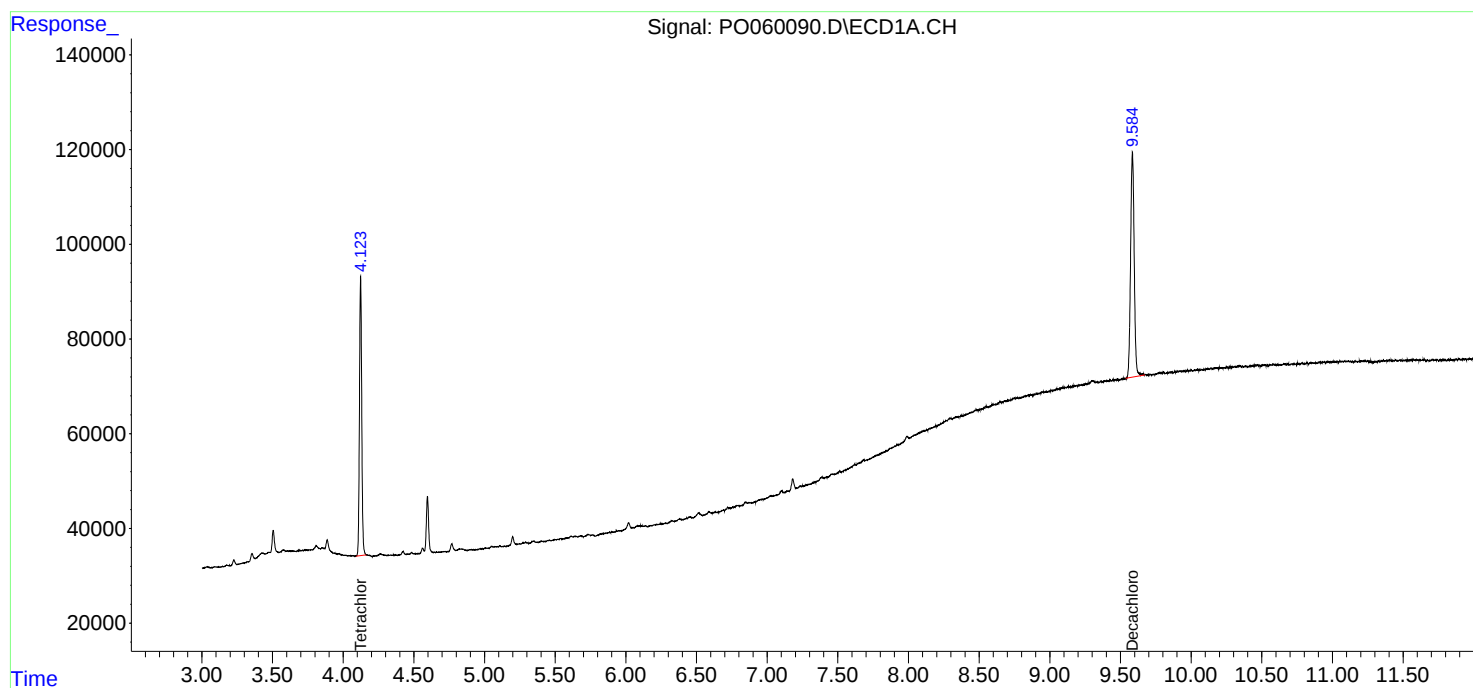

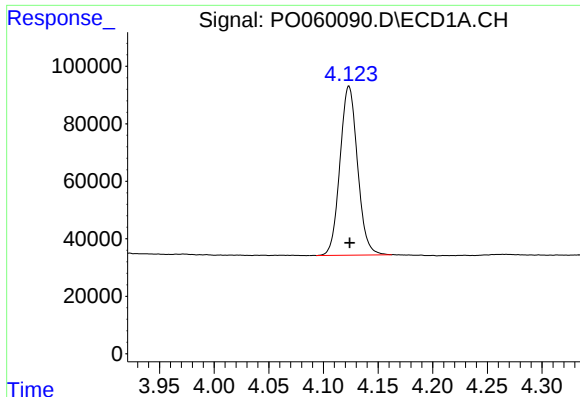


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: -0.001 min
Response: 658543
Conc: 18.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB122685BL


Manual Integrations
APPROVED

Ankita
8/31/2019 3:12:33 PM

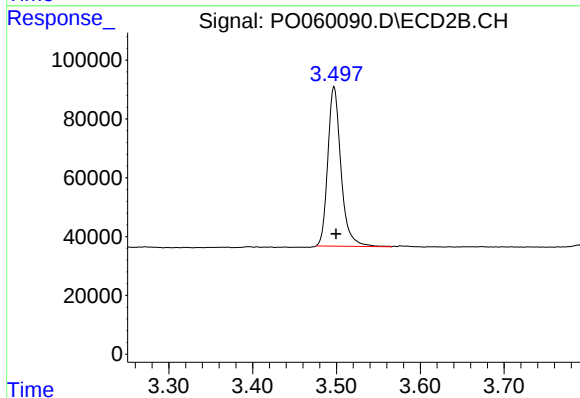


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.002 min
Response: 590072
Conc: 16.39 ng/ml

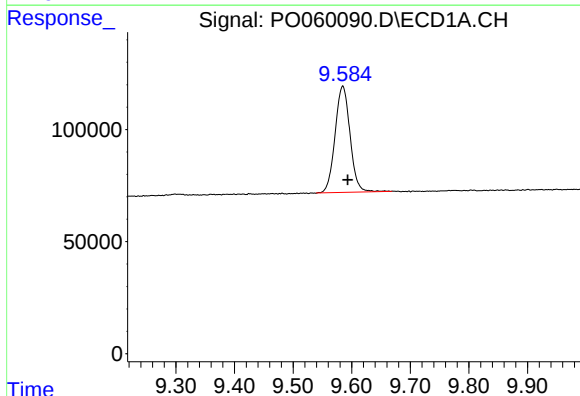

#2 Decachlorobiphenyl

R.T.: 9.584 min
Delta R.T.: -0.009 min
Response: 842668
Conc: 15.84 ng/ml m

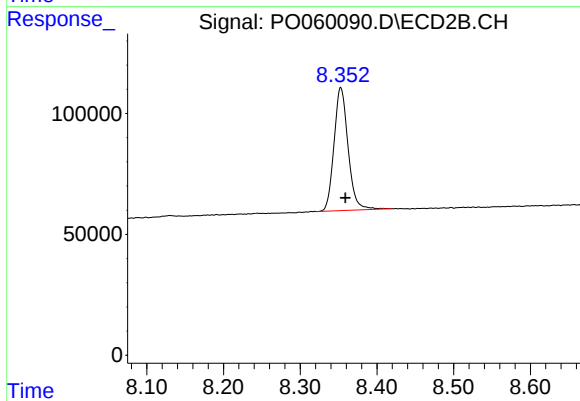

#2 Decachlorobiphenyl

R.T.: 8.353 min
Delta R.T.: -0.006 min
Response: 646861
Conc: 16.04 ng/ml