

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060101.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 17:02
Operator : SM/AJ
Sample : K4582-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RT-3422

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 23:20:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.123	3.497	856942	773192	24.475	21.480
2) SA Decachlor...	9.581	8.352	979373	768462	18.409	19.059

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060101.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 17:02
Operator : SM/AJ
Sample : K4582-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RT-3422

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 23:20:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

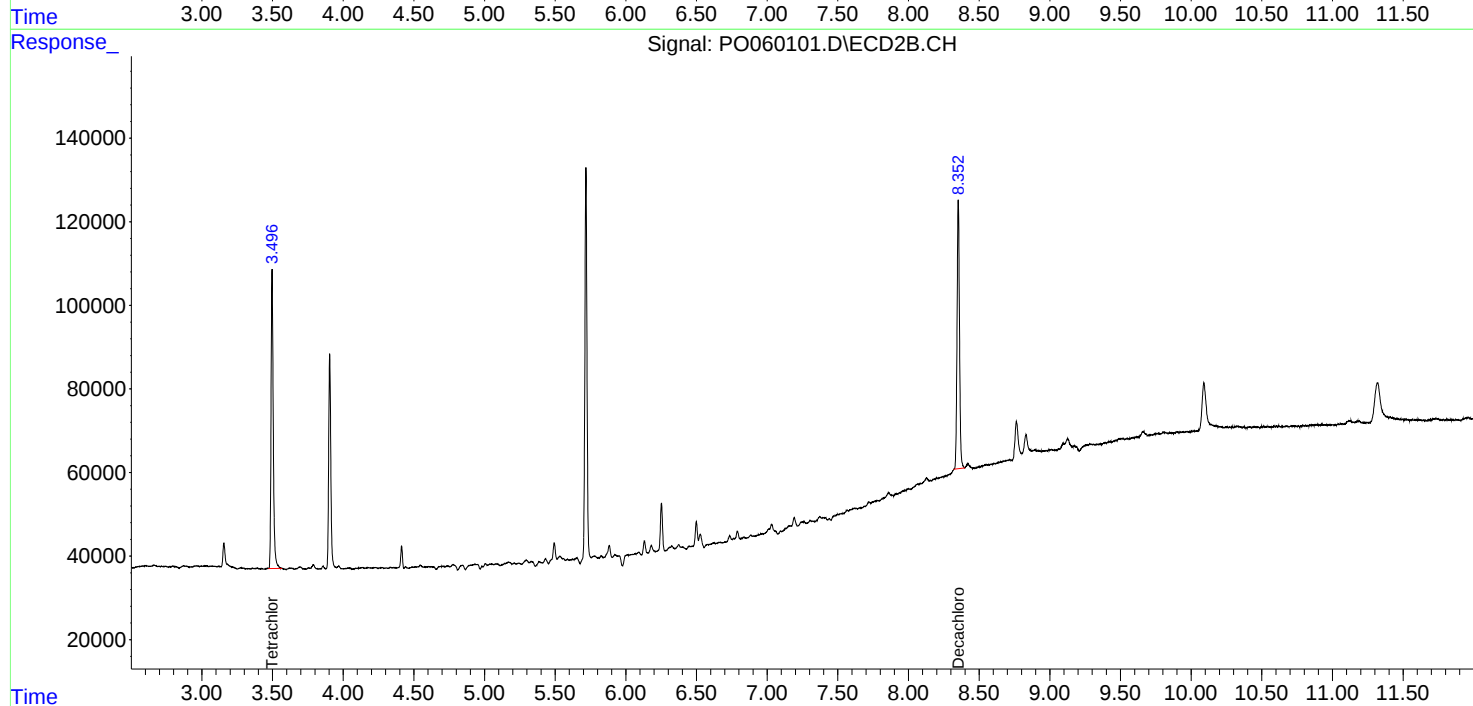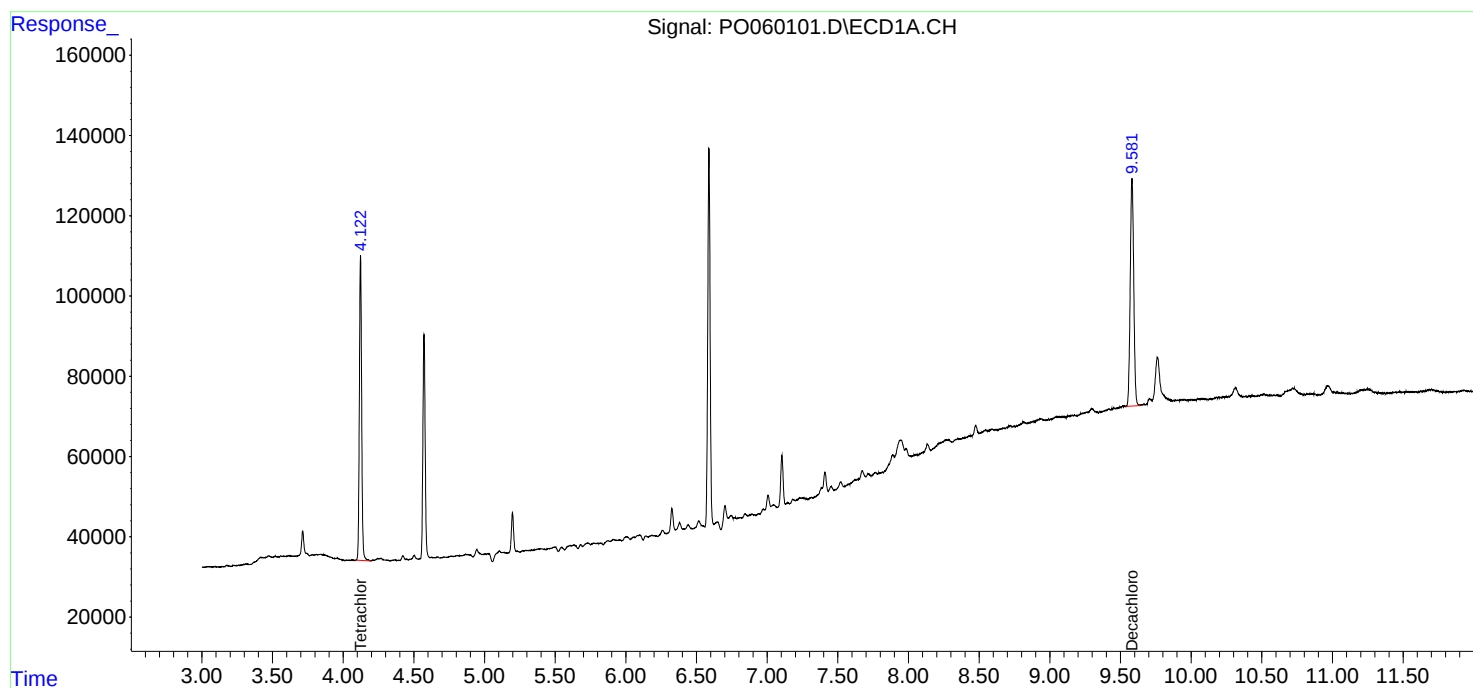


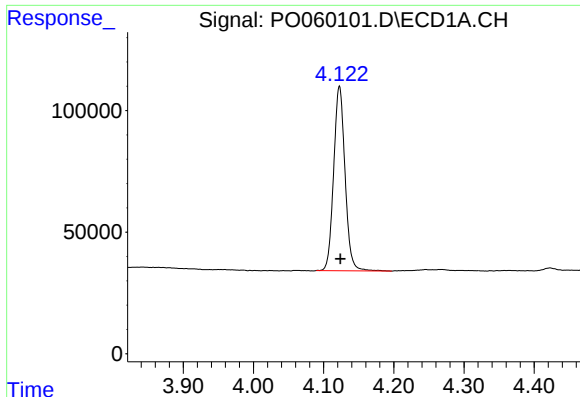

#1 Tetrachloro-m-xylene


R.T.: 4.123 min
Delta R.T.: -0.001 min
Response: 856942
Conc: 24.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-3422

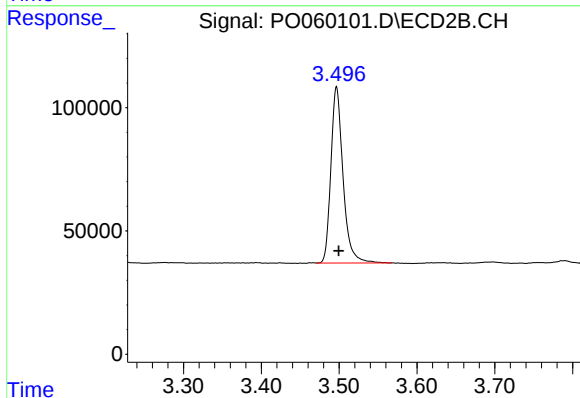


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.003 min
Response: 773192
Conc: 21.48 ng/ml

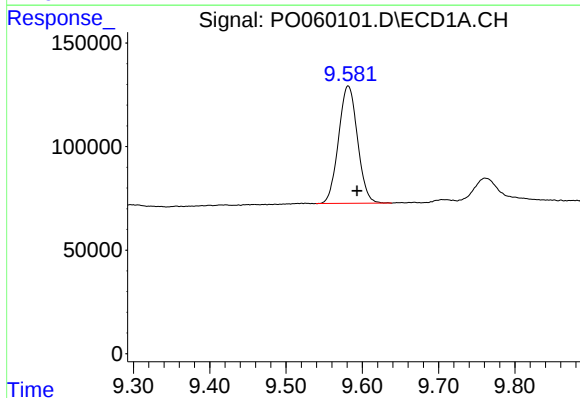

#2 Decachlorobiphenyl

R.T.: 9.581 min
Delta R.T.: -0.012 min
Response: 979373
Conc: 18.41 ng/ml

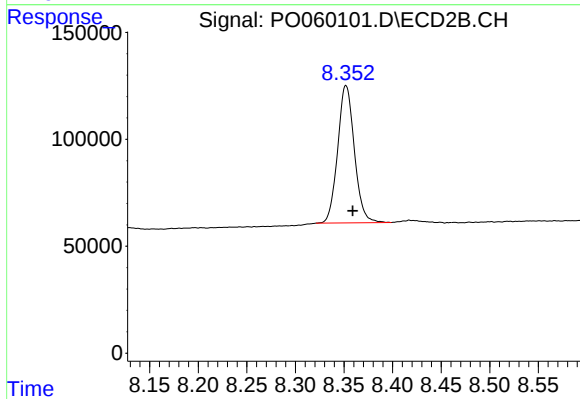

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: -0.007 min
Response: 768462
Conc: 19.06 ng/ml