

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2019 17:37
 Operator : SM/AJ
 Sample : K4587-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-057

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 23:21:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.123	3.496	870261	772351	24.856	21.457
2) SA Decachlor...	9.584	8.353	632994	494330	11.898	12.260

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2019 17:37
Operator : SM/AJ
Sample : K4587-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 23:21:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

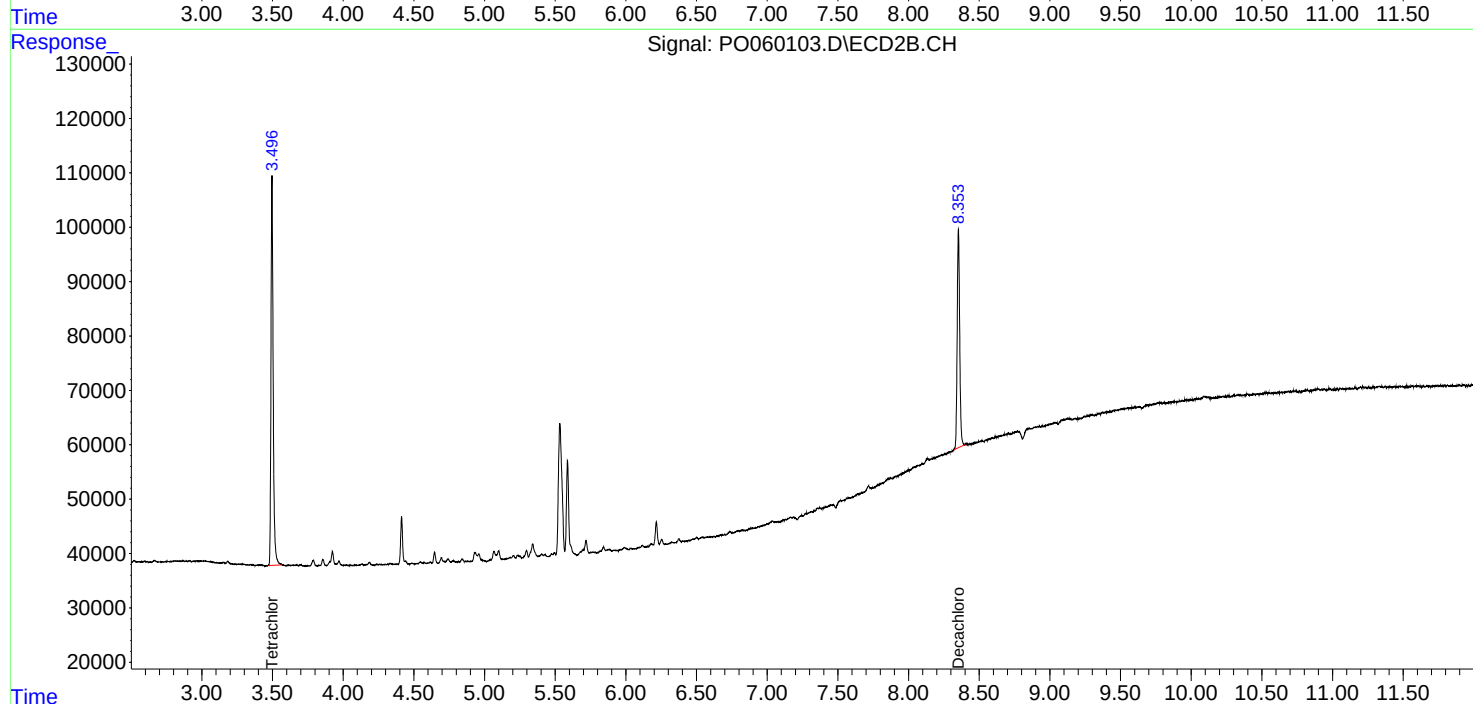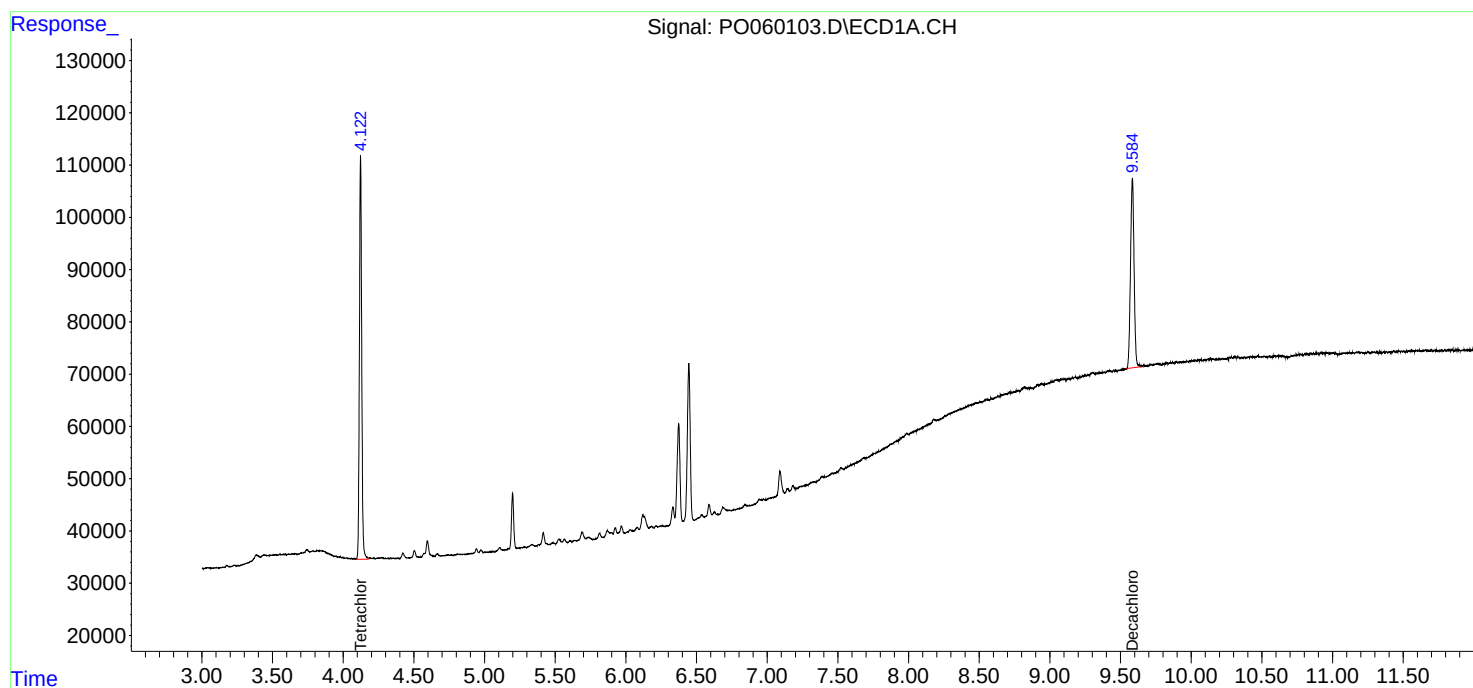


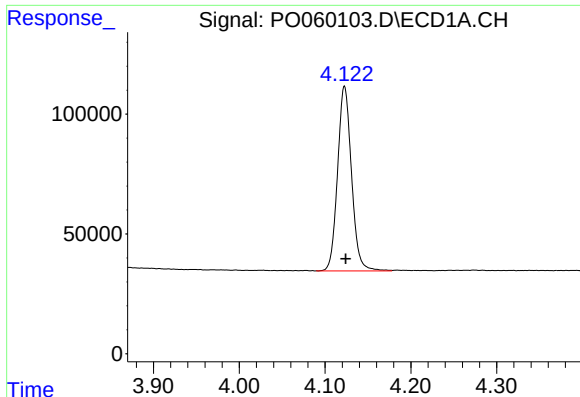

#1 Tetrachloro-m-xylene


R.T.: 4.123 min
Delta R.T.: -0.001 min
Response: 870261
Conc: 24.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-057

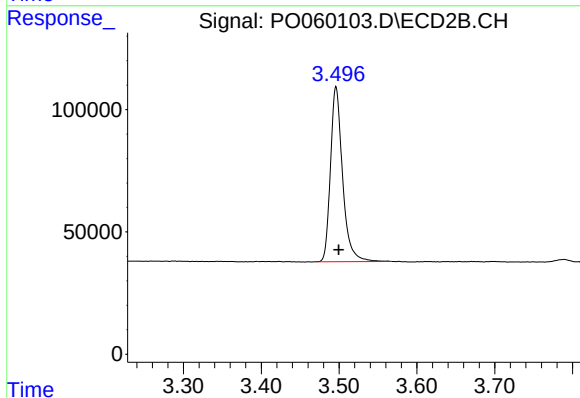


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.003 min
Response: 772351
Conc: 21.46 ng/ml

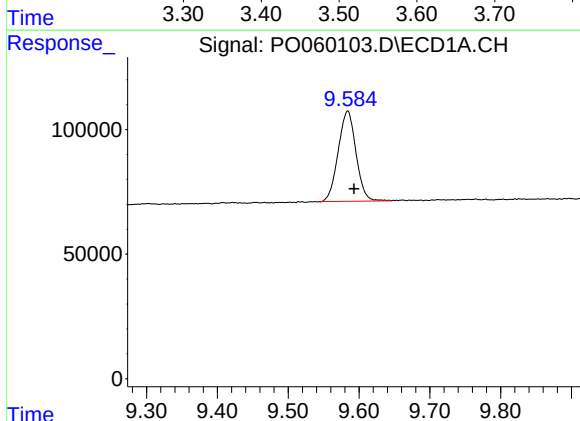

#2 Decachlorobiphenyl

R.T.: 9.584 min
Delta R.T.: -0.009 min
Response: 632994
Conc: 11.90 ng/ml

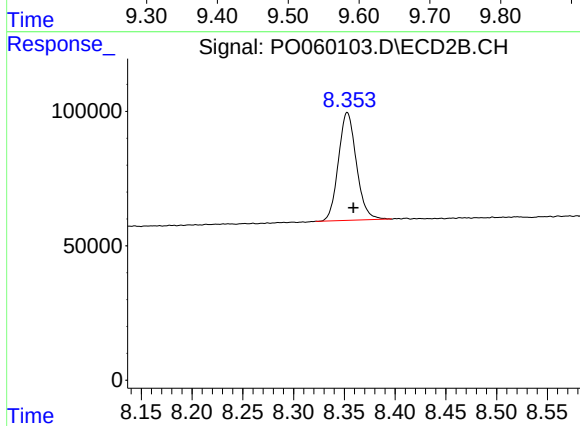

#2 Decachlorobiphenyl

R.T.: 8.353 min
Delta R.T.: -0.006 min
Response: 494330
Conc: 12.26 ng/ml