

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060145.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 6:08
 Operator : SM/AJ
 Sample : K4090-17
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-082919

Manual Integrations
 APPROVED

Ankita
 8/31/2019 3:13:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 06:24:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.121	3.496	1131263	1028358	32.310m	28.569
2) SA Decachlor...	9.576	8.350	1025279	781950	19.272	19.393

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060145.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 6:08
Operator : SM/AJ
Sample : K4090-17
Misc :
ALS Vial : 66 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-082919


Manual Integrations
APPROVED

Ankita
8/31/2019 3:13:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 06:24:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

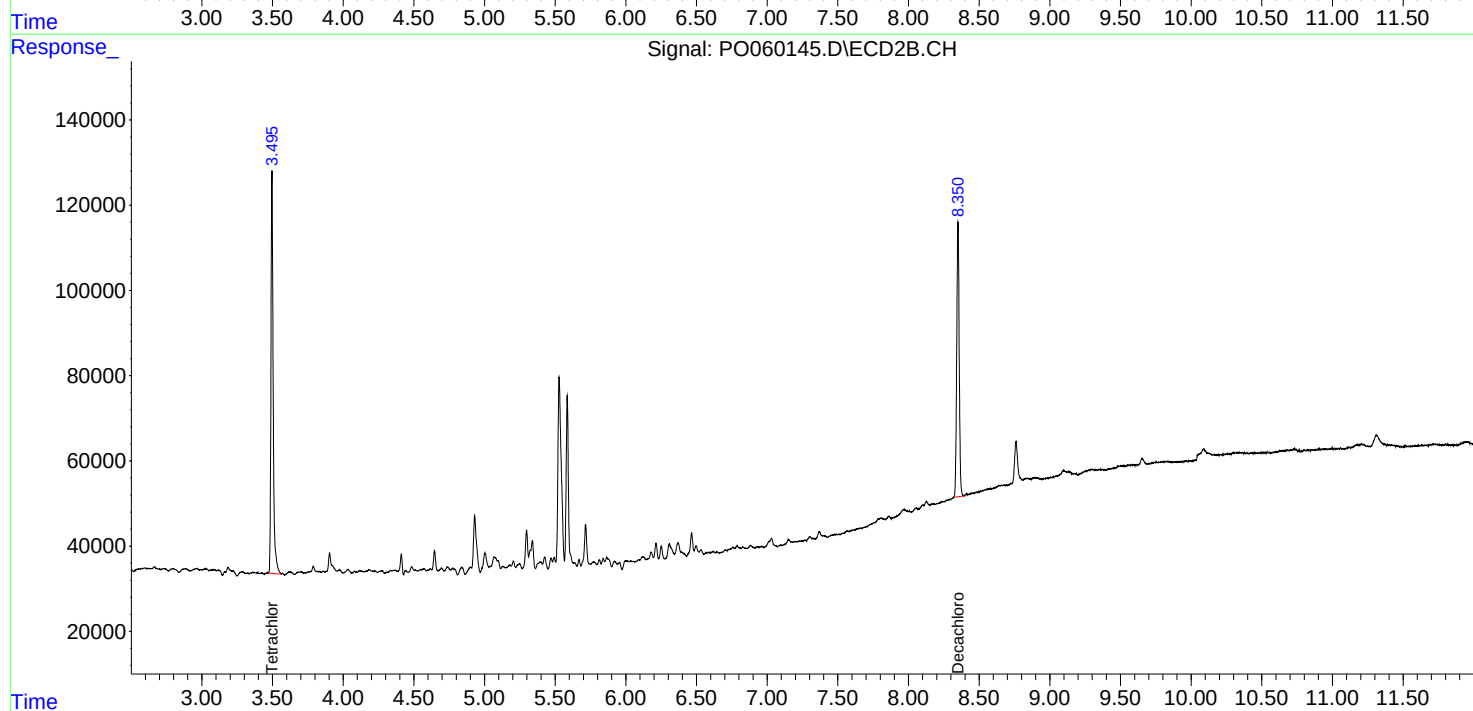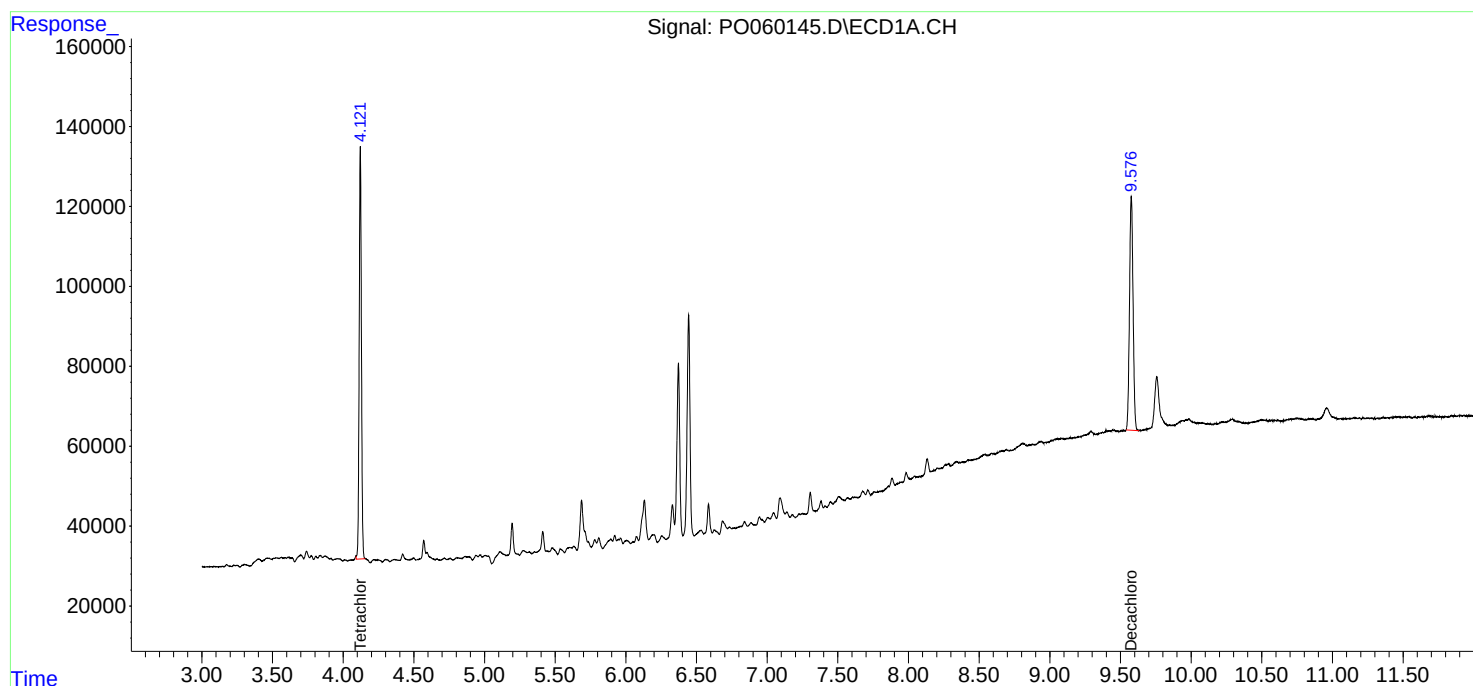

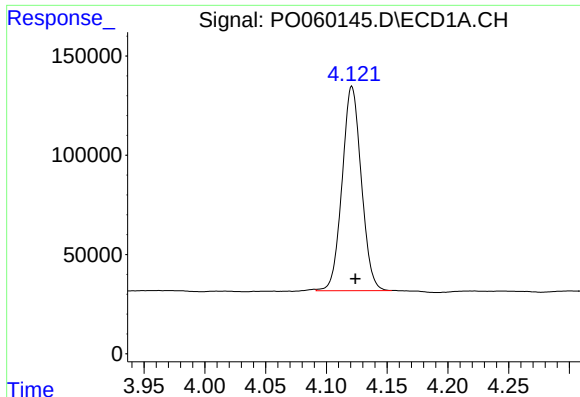


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: -0.003 min
Response: 1131263
Conc: 32.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-02-082919


Manual Integrations
APPROVED

Ankita
8/31/2019 3:13:59 PM

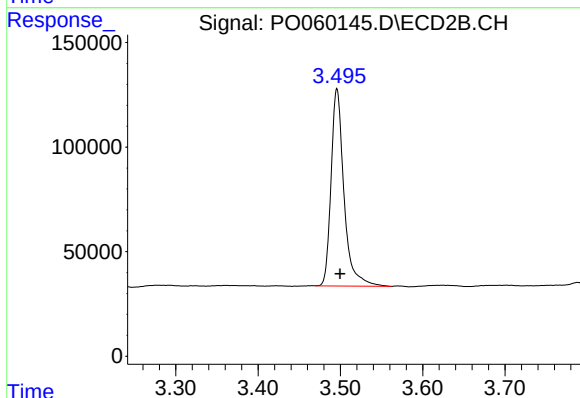


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.004 min
Response: 1028358
Conc: 28.57 ng/ml

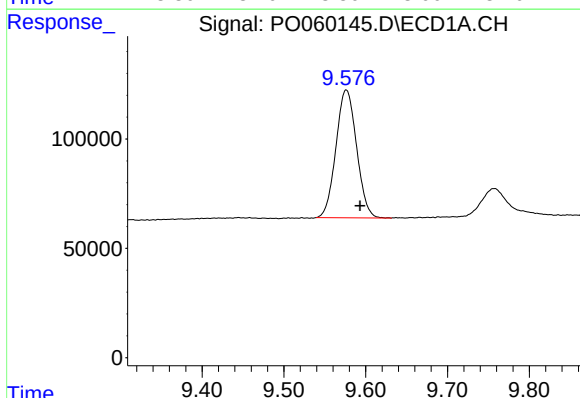

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.017 min
Response: 1025279
Conc: 19.27 ng/ml

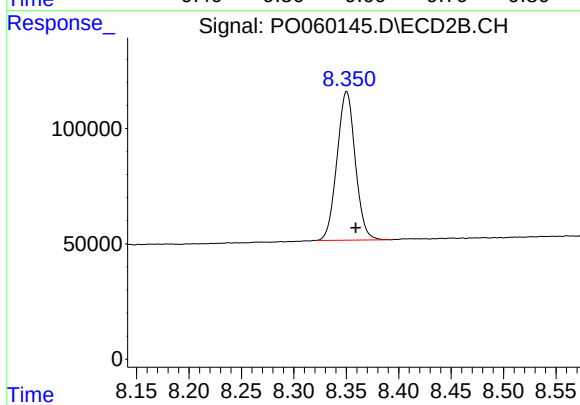

#2 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.009 min
Response: 781950
Conc: 19.39 ng/ml