

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060151.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 7:50
 Operator : SM/AJ
 Sample : K4570-03
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOUTH-AVENUE-3-ABCD

Manual Integrations
 APPROVED

Ankita
 9/3/2019 8:36:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 13:10:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.120	3.496	1071148	928535	30.593m	25.796
2) SA Decachlor...	9.575	8.348	903690	702212	16.987	17.416

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060151.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 7:50
Operator : SM/AJ
Sample : K4570-03
Misc :
ALS Vial : 72 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOUTH-AVENUE-3-ABCD


Manual Integrations
APPROVED

Ankita
9/3/2019 8:36:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 13:10:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

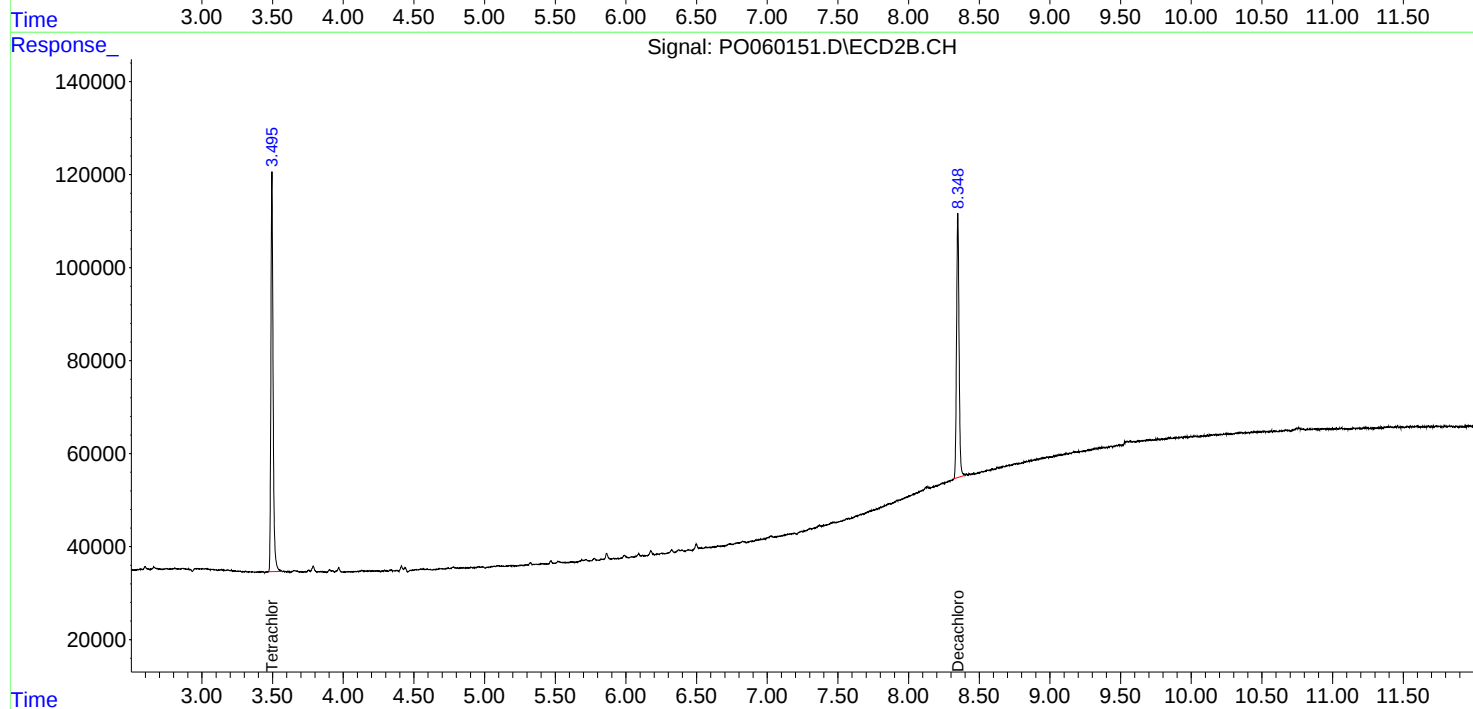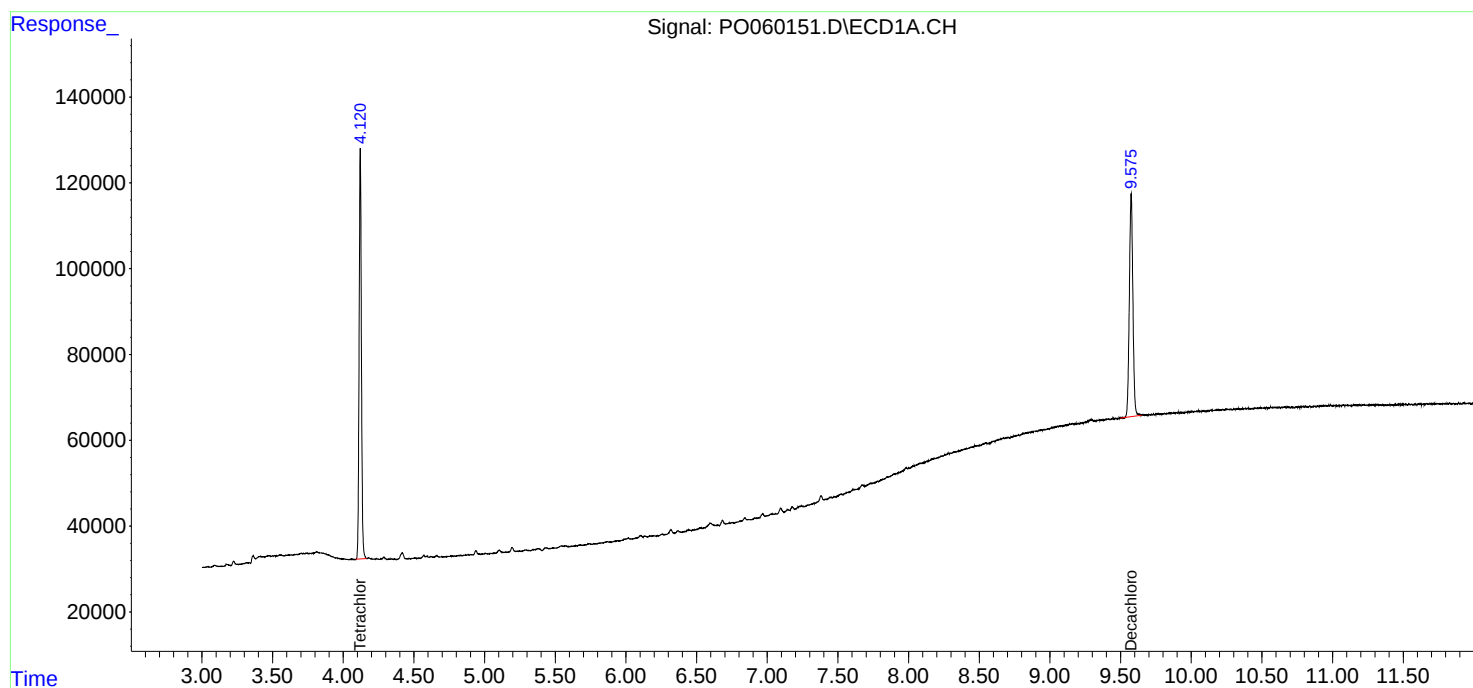

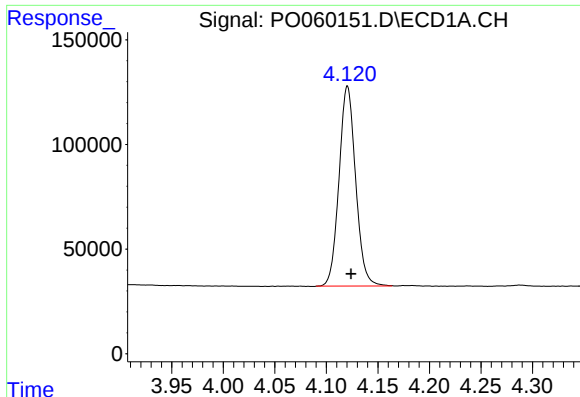


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: -0.004 min
Response: 1071148
Conc: 30.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SOUTH-AVENUE-3-ABCD


Manual Integrations
APPROVED

Ankita
9/3/2019 8:36:21 AM

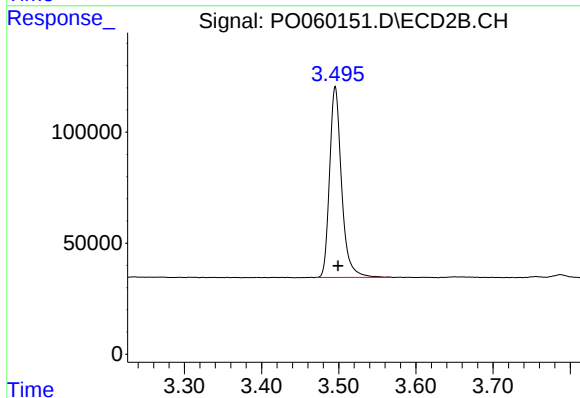


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.004 min
Response: 928535
Conc: 25.80 ng/ml

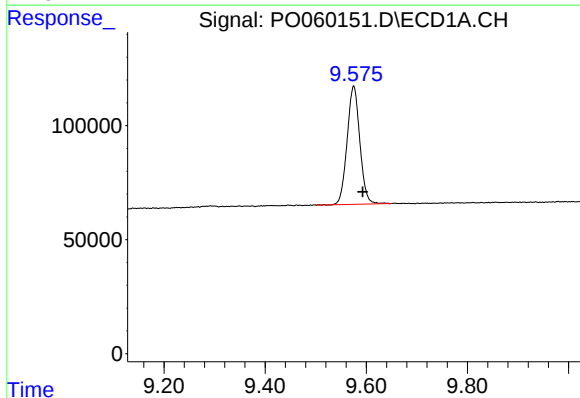

#2 Decachlorobiphenyl

R.T.: 9.575 min
Delta R.T.: -0.018 min
Response: 903690
Conc: 16.99 ng/ml

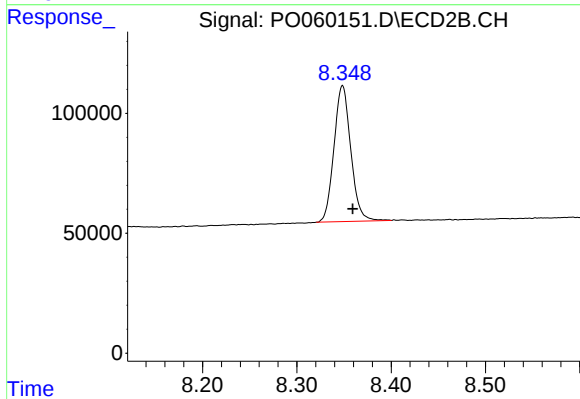

#2 Decachlorobiphenyl

R.T.: 8.348 min
Delta R.T.: -0.011 min
Response: 702212
Conc: 17.42 ng/ml