

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
 Data File : P0060154.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 8:40
 Operator : SM/AJ
 Sample : K4591-03
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3-30-32

Manual Integrations
 APPROVED

Ankita
 9/3/2019 8:36:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 13:11:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.116	3.496	932769	824232	26.641m	22.898
2) SA Decachlor...	9.572	8.348	855343	668334	16.078	16.575

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083019\
Data File : P0060154.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 8:40
Operator : SM/AJ
Sample : K4591-03
Misc :
ALS Vial : 75 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-3-30-32


Manual Integrations
APPROVED

Ankita
9/3/2019 8:36:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 13:11:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

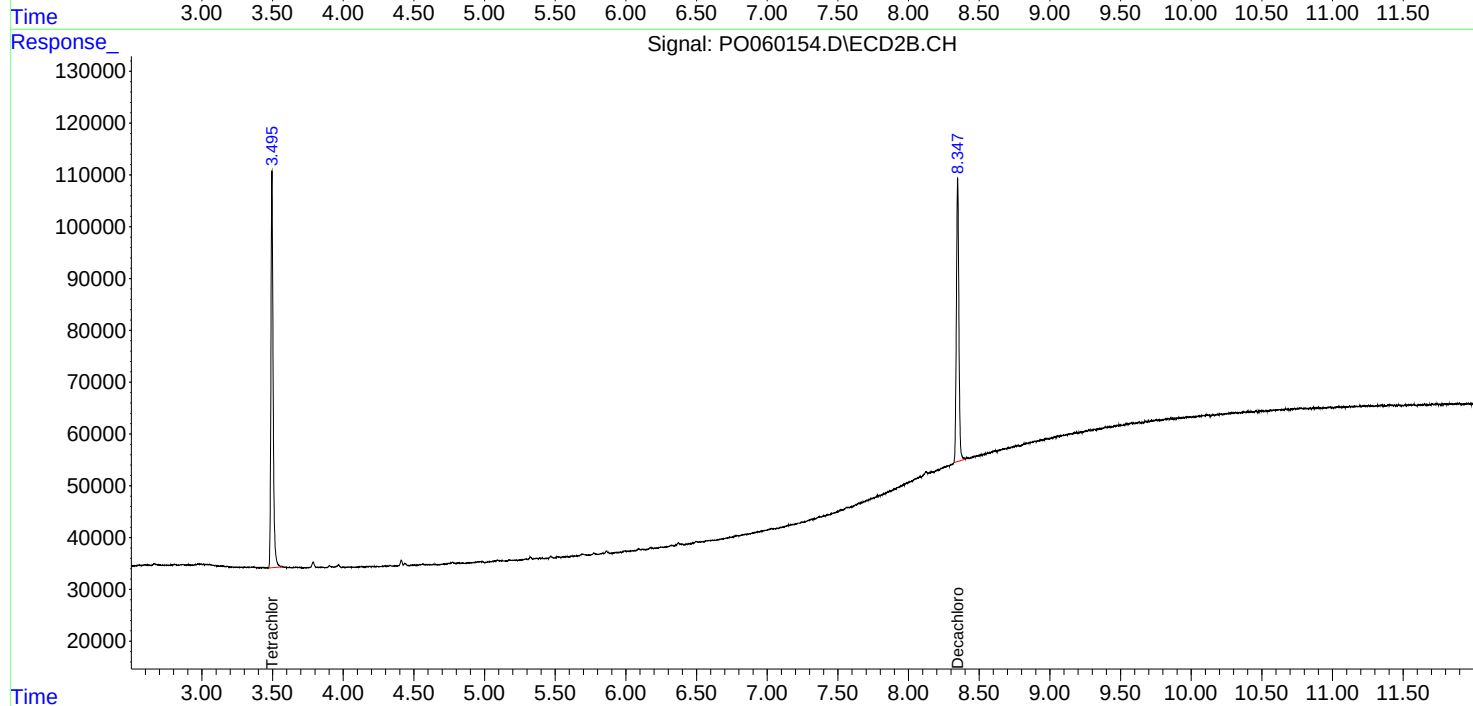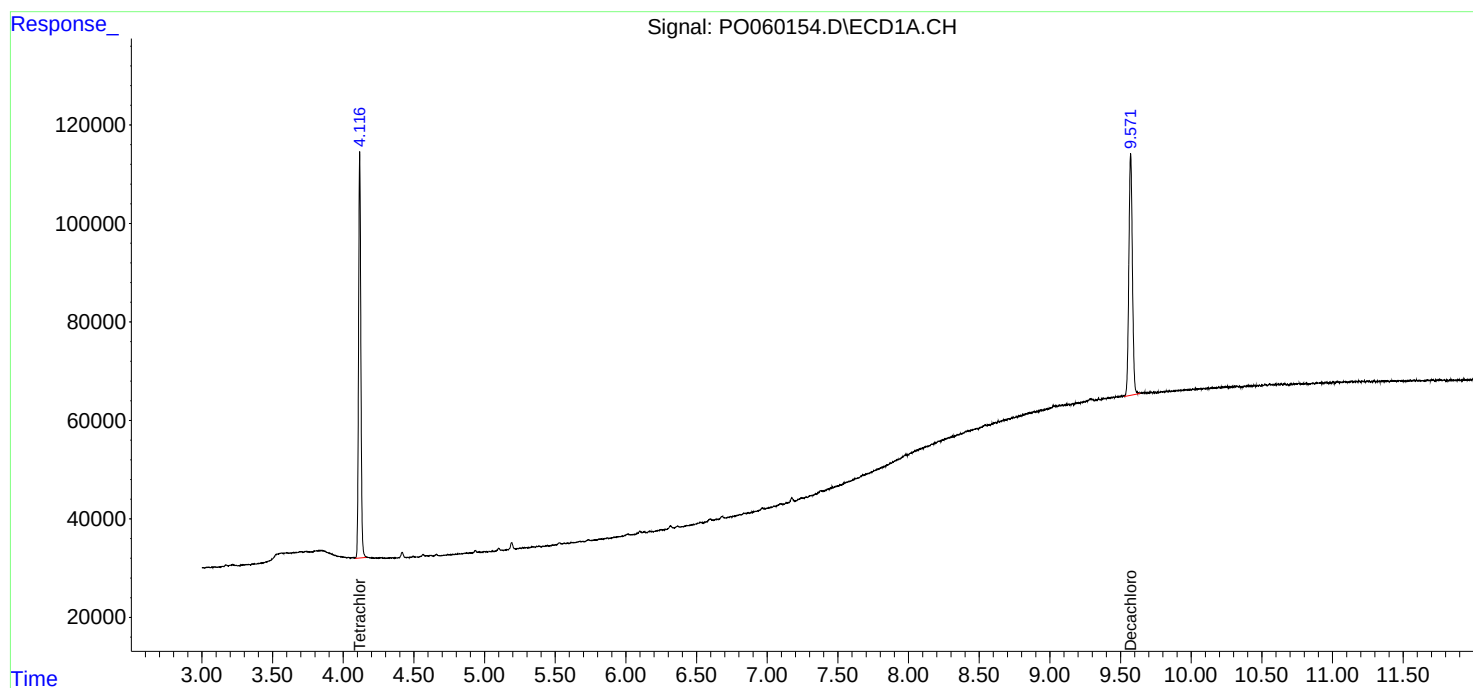

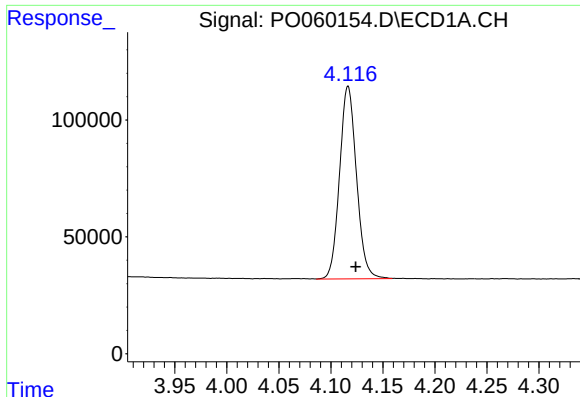


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.008 min
Response: 932769
Conc: 26.64 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-3-30-32


Manual Integrations
APPROVED

Ankita
9/3/2019 8:36:27 AM

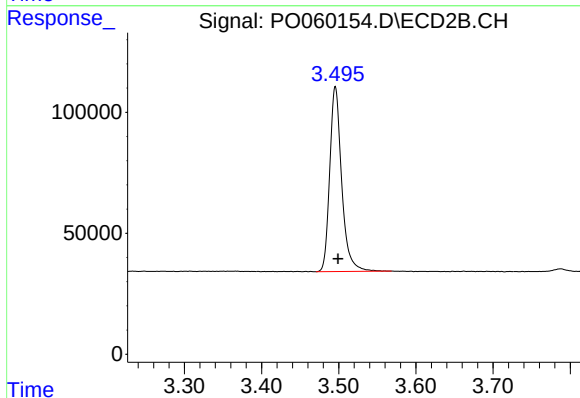


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.004 min
Response: 824232
Conc: 22.90 ng/ml

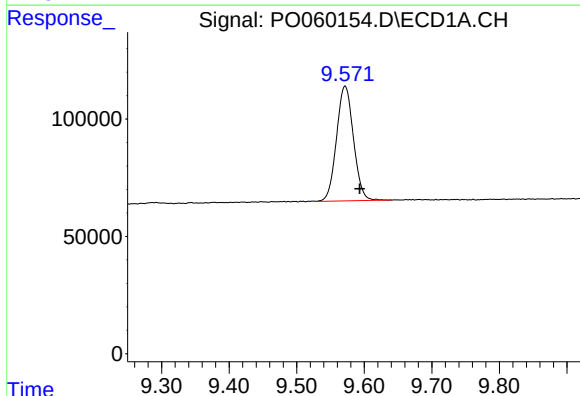

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.022 min
Response: 855343
Conc: 16.08 ng/ml

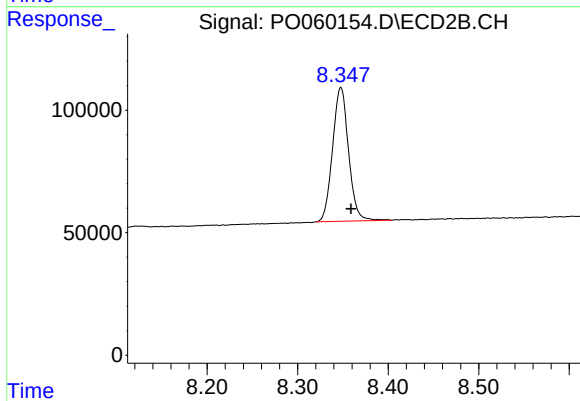

#2 Decachlorobiphenyl

R.T.: 8.348 min
Delta R.T.: -0.011 min
Response: 668334
Conc: 16.58 ng/ml