

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083021\
 Data File : P0080834.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 8:56
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 06:03:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 27 12:15:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	0.000	16482	0	0.201	N.D. #
2)	SA Decachlor...	11.019f	0.000	18711	0	0.298	N.D. #
Target Compounds							
28)	L6 AR-1254-3	7.821f	0.000	47734	0	8.821	N.D. #
38)	L8 AR-1262-3	9.488f	0.000	10330	0	3.080	N.D. #
39)	L8 AR-1262-4	9.542f	0.000	18880	0	9.318	N.D. #
40)	L8 AR-1262-5	10.232	0.000	6268	0	2.258	N.D. #
41)	L9 AR-1268-1	9.488f	0.000	10330	0	1.163	N.D. #
42)	L9 AR-1268-2	9.542f	0.000	18880	0	2.292	N.D. #
44)	L9 AR-1268-4	10.232	0.000	6268	0	2.065	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083021\
Data File : PO080834.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 8:56
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 06:03:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 27 12:15:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

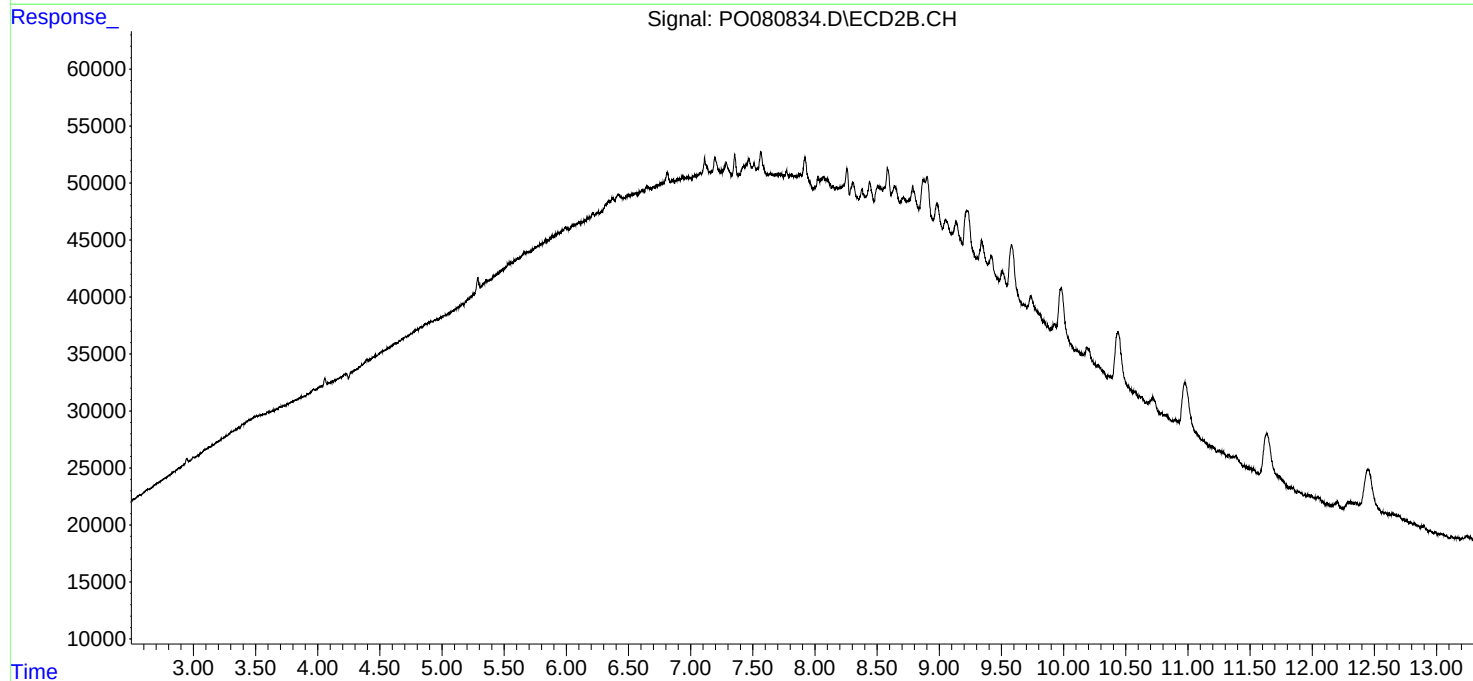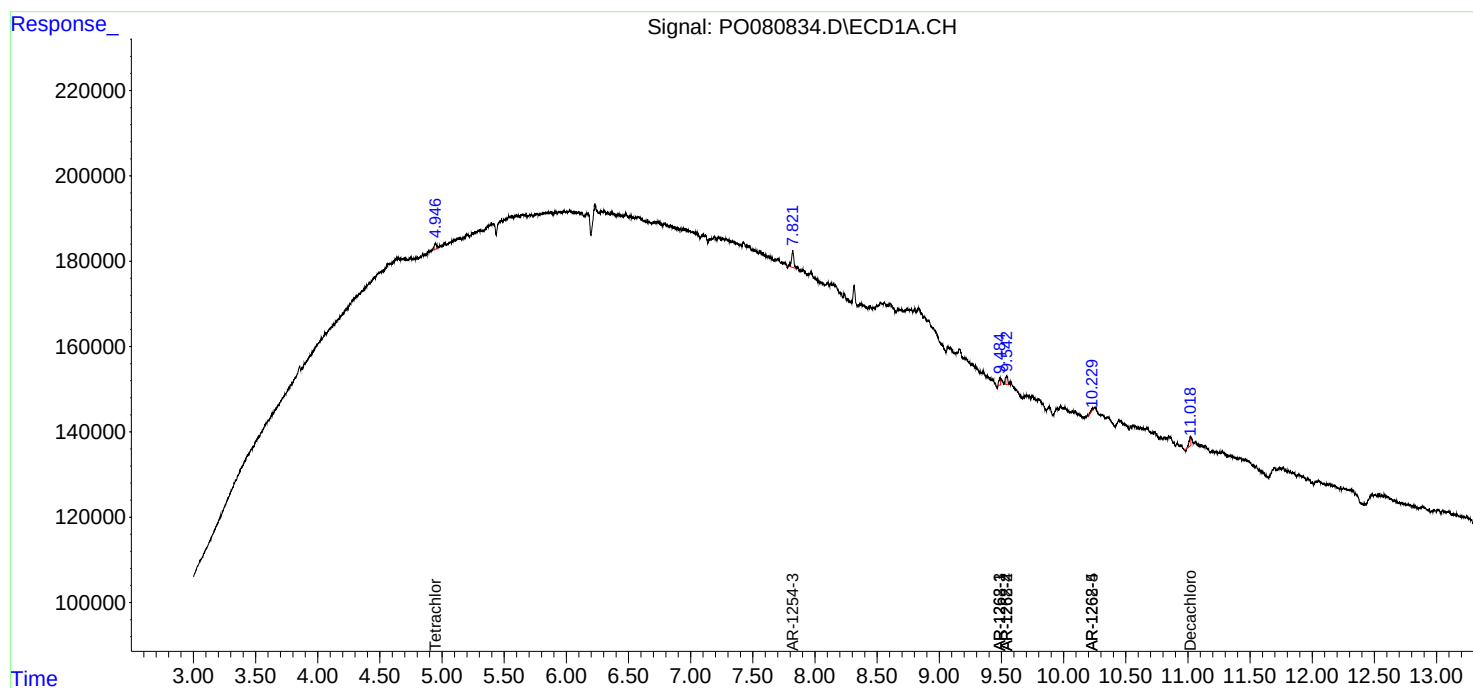


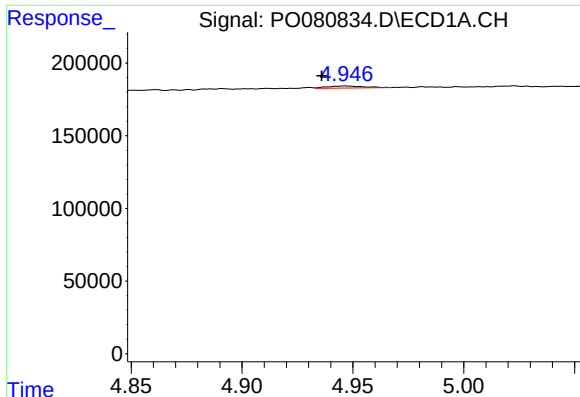

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: 0.011 min
Response: 16482
Conc: 0.20 ng/ml

Instrument :
ECD_O
ClientSampleId :

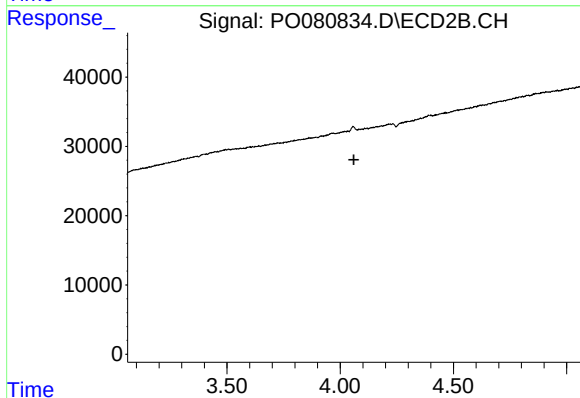


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.061 min
Response: 0
Conc: N.D.

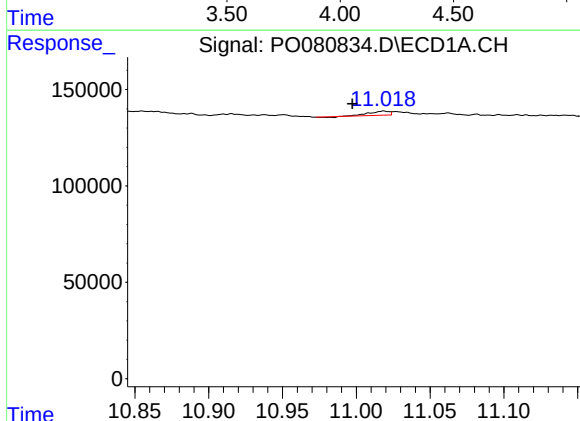


#2 Decachlorobiphenyl

R.T.: 11.019 min
Delta R.T.: 0.021 min
Response: 18711
Conc: 0.30 ng/ml

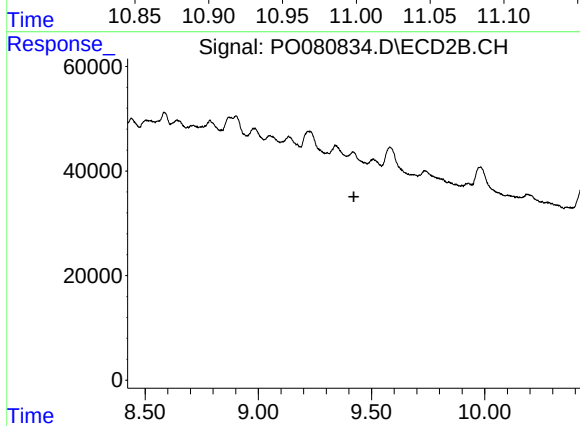

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.422 min
Response: 0
Conc: N.D.

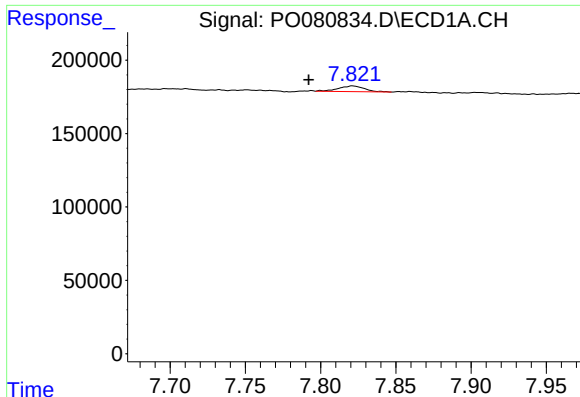

#28 AR-1254-3


R.T.: 7.821 min
Delta R.T.: 0.029 min
Response: 47734
Conc: 8.82 ng/ml

Instrument :
ECD_O
ClientSampleId :

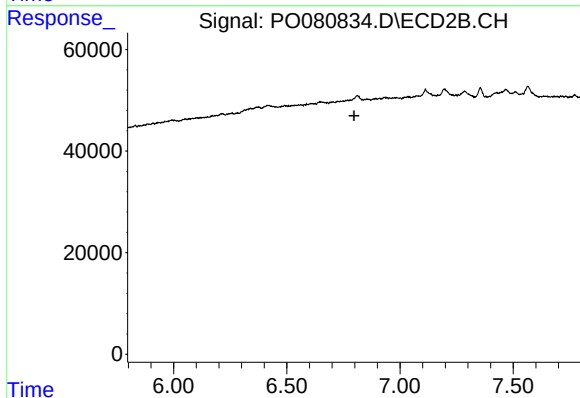


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.797 min
Response: 0
Conc: N.D.

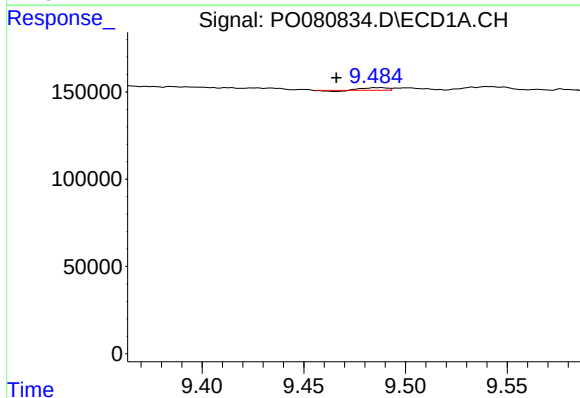


#38 AR-1262-3

R.T.: 9.488 min
Delta R.T.: 0.022 min
Response: 10330
Conc: 3.08 ng/ml

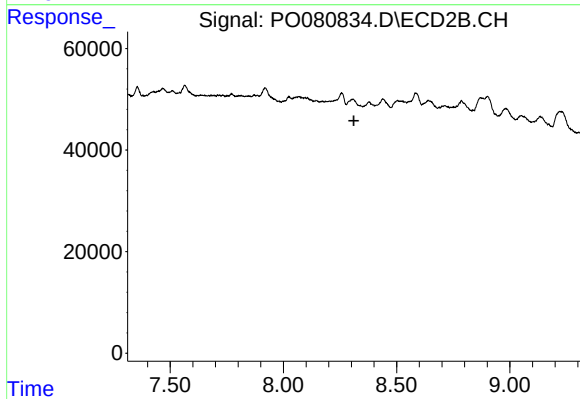

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

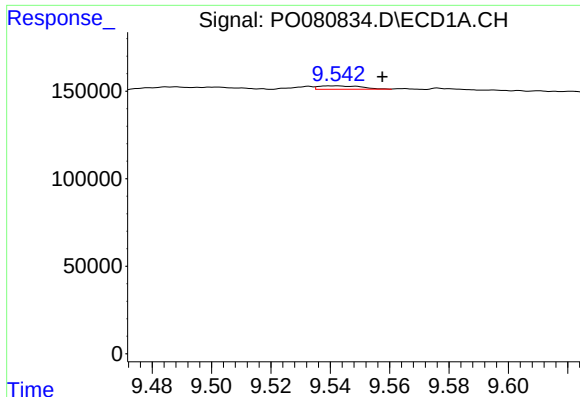

#39 AR-1262-4


R.T.: 9.542 min
Delta R.T.: -0.016 min
Response: 18880
Conc: 9.32 ng/ml

Instrument :
ECD_O
ClientSampleId :

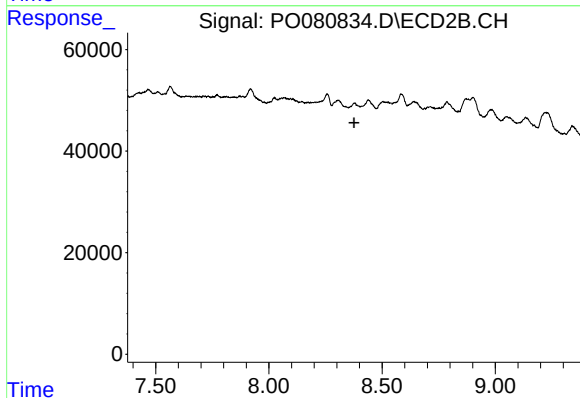


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.376 min
Response: 0
Conc: N.D.

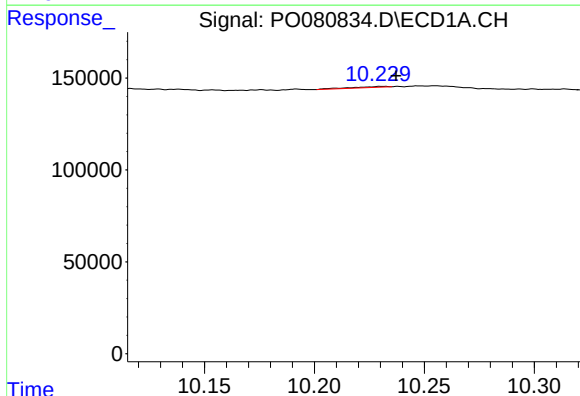


#40 AR-1262-5

R.T.: 10.232 min
Delta R.T.: -0.005 min
Response: 6268
Conc: 2.26 ng/ml

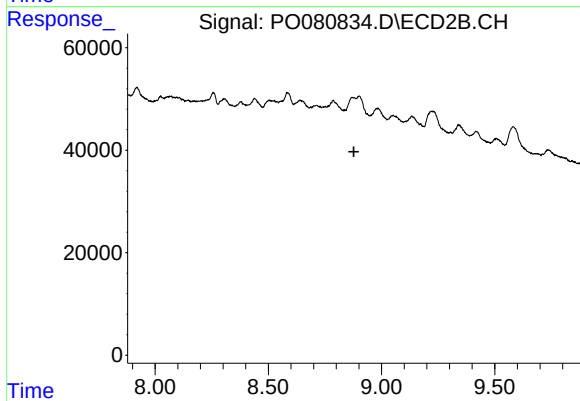

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.878 min
Response: 0
Conc: N.D.

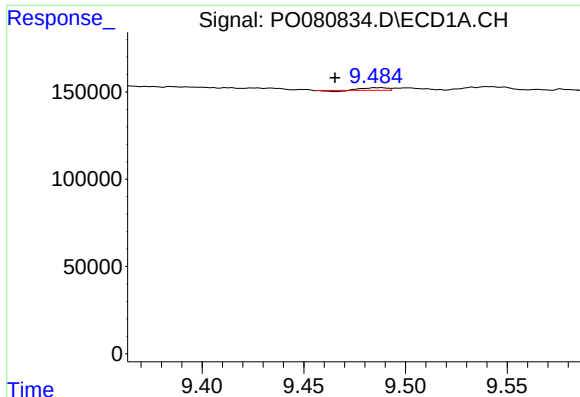

#41 AR-1268-1


R.T.: 9.488 min
Delta R.T.: 0.023 min
Response: 10330
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

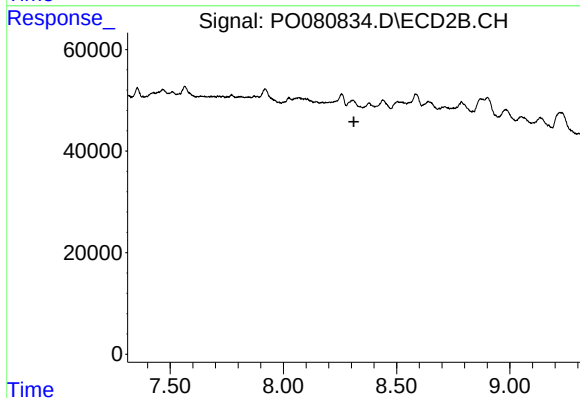


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

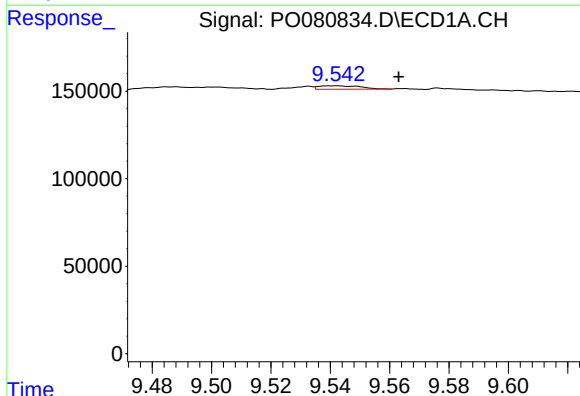


#42 AR-1268-2

R.T.: 9.542 min
Delta R.T.: -0.021 min
Response: 18880
Conc: 2.29 ng/ml

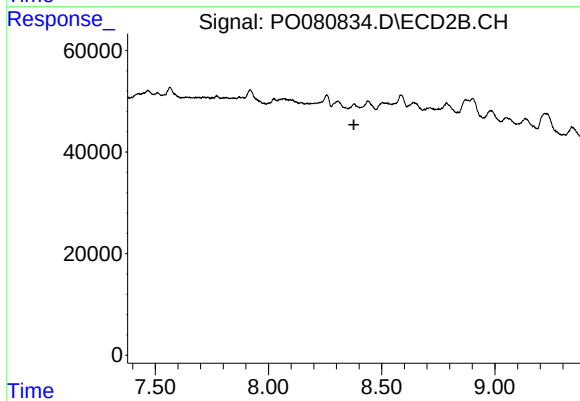

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.377 min
Response: 0
Conc: N.D.

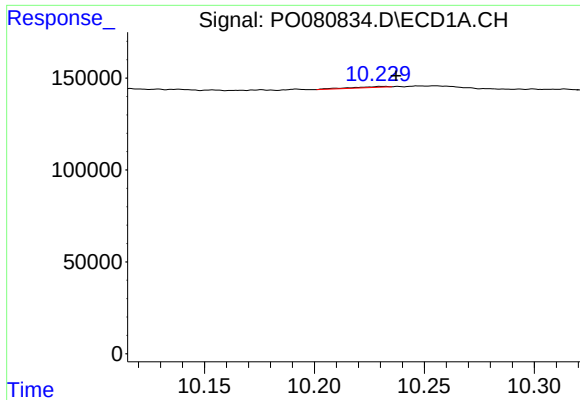

#44 AR-1268-4

R.T.: 10.232 min
Delta R.T.: -0.005 min
Response: 6268
Conc: 2.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

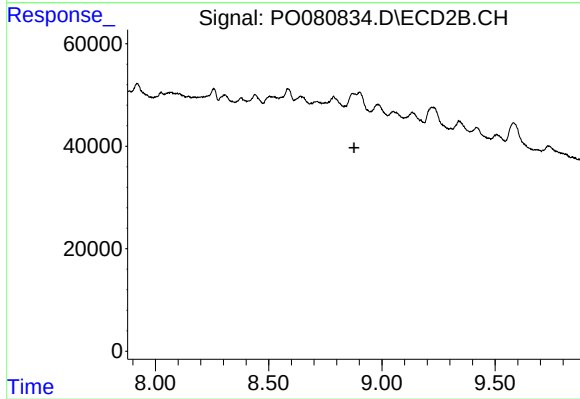

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.877 min
Response: 0
Conc: N.D.