

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083021\
 Data File : P0080840.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 14:40
 Operator : DD\AJ
 Sample : PB138783BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 06:07:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 27 12:15:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.937	4.060	1781056	570504	21.702	21.169
2)	SA Decachlor...	11.004	9.424	1395484	598682	22.256	21.939
Target Compounds							
8)	L2 AR-1221-1	5.190	0.000	42942	0	46.263	N.D. #
9)	L2 AR-1221-2	5.292	0.000	22617	0	31.967	N.D. #
28)	L6 AR-1254-3	7.814f	0.000	98698	0	18.238	N.D. #
32)	L7 AR-1260-2	8.205f	0.000	74367	0	15.640	N.D. #
33)	L7 AR-1260-3	8.572f	0.000	57351	0	19.792	N.D. #
35)	L7 AR-1260-5	9.144	0.000	194394	0	28.522	N.D. #
36)	L8 AR-1262-1	8.572f	0.000	57351	0	12.530	N.D. #
37)	L8 AR-1262-2	9.144	0.000	194394	0	24.630	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083021\
Data File : PO080840.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 14:40
Operator : DD\AJ
Sample : PB138783BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 06:07:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 27 12:15:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

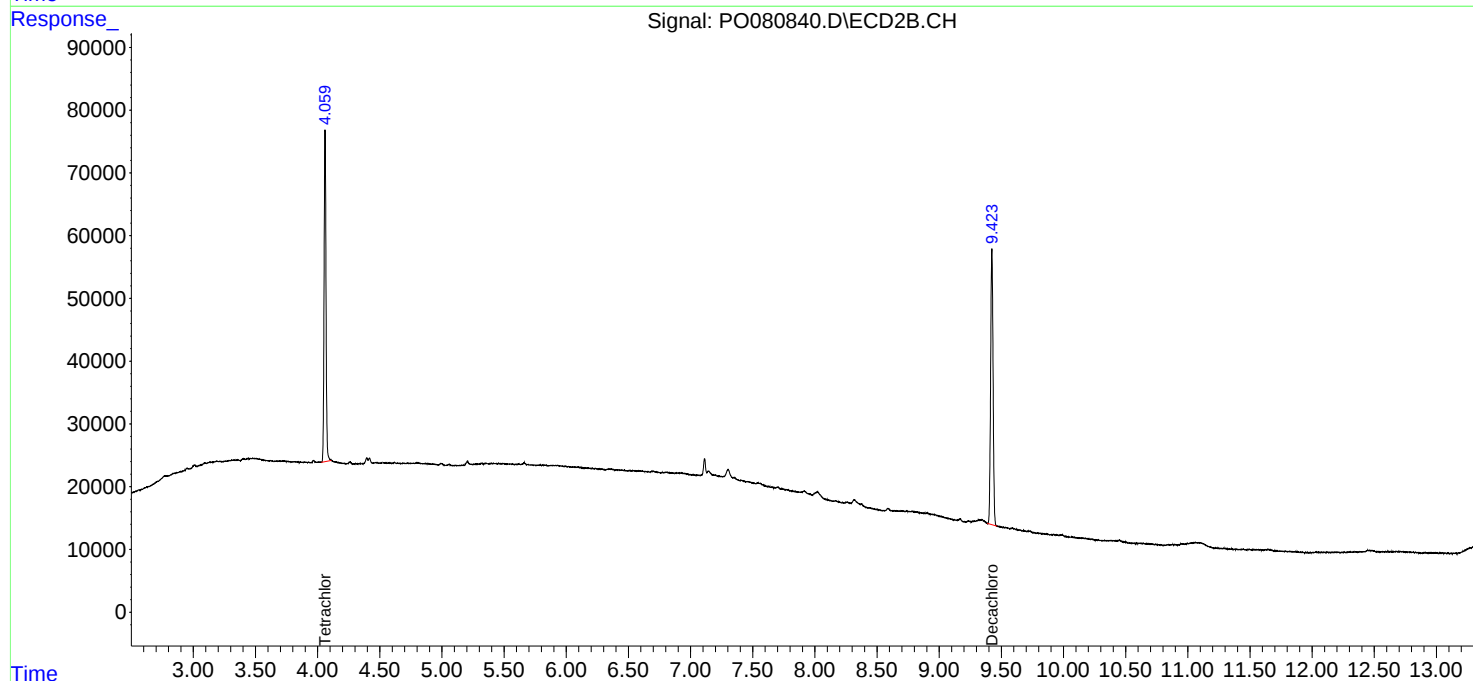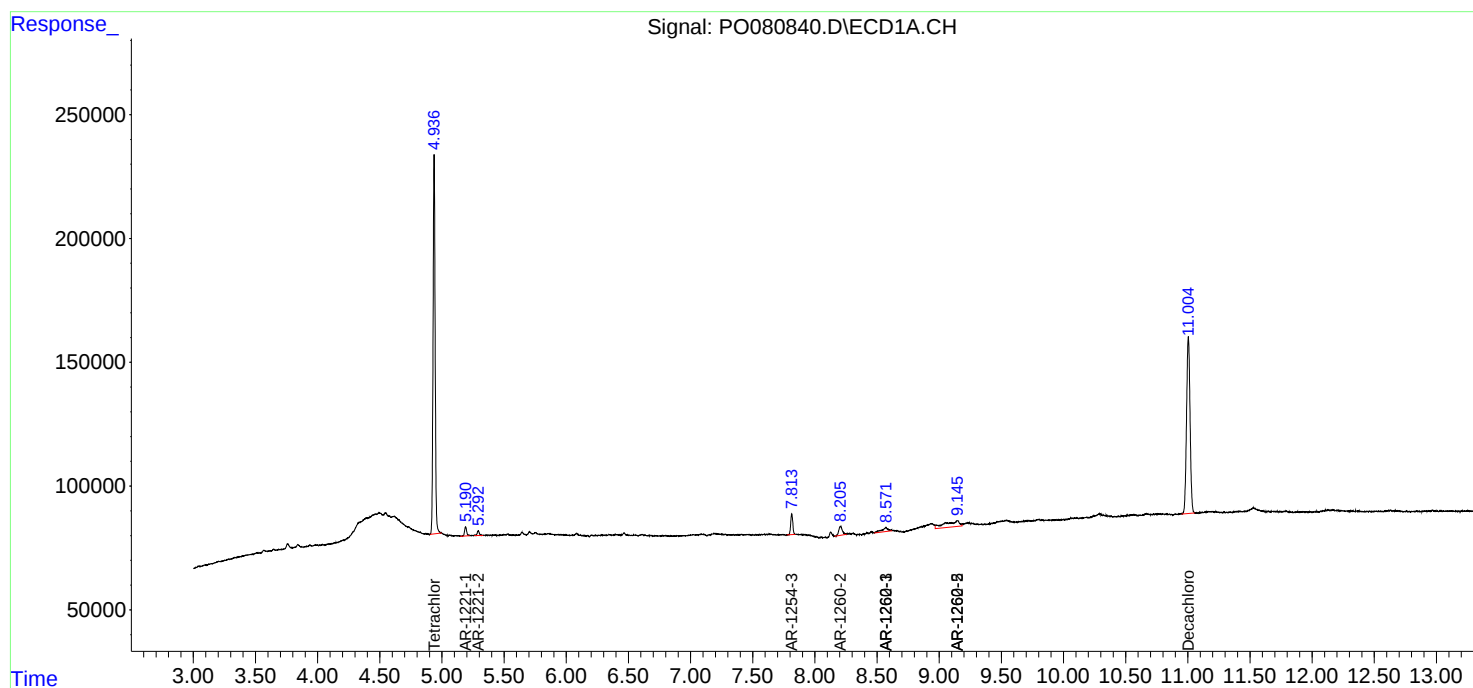


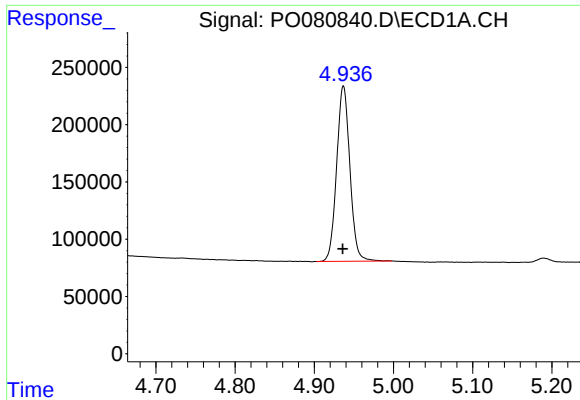

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 1781056
Conc: 21.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

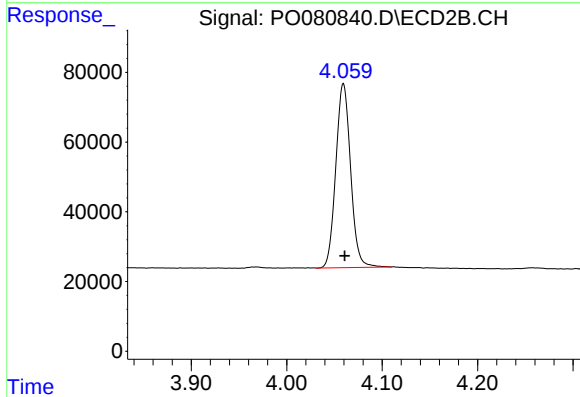


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.001 min
Response: 570504
Conc: 21.17 ng/ml

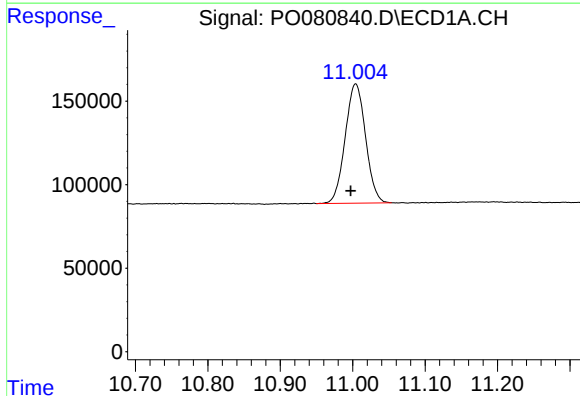


#2 Decachlorobiphenyl

R.T.: 11.004 min
Delta R.T.: 0.007 min
Response: 1395484
Conc: 22.26 ng/ml

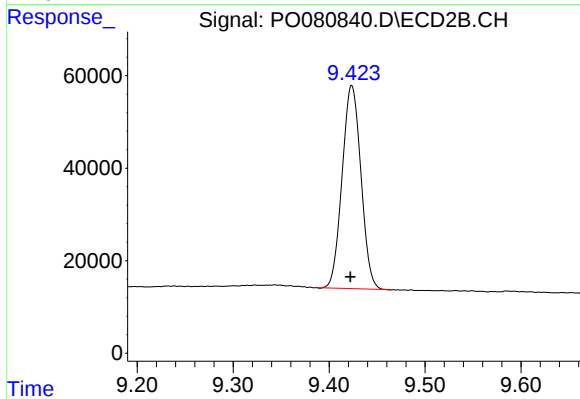

#2 Decachlorobiphenyl


R.T.: 9.424 min
Delta R.T.: 0.001 min
Response: 598682
Conc: 21.94 ng/ml

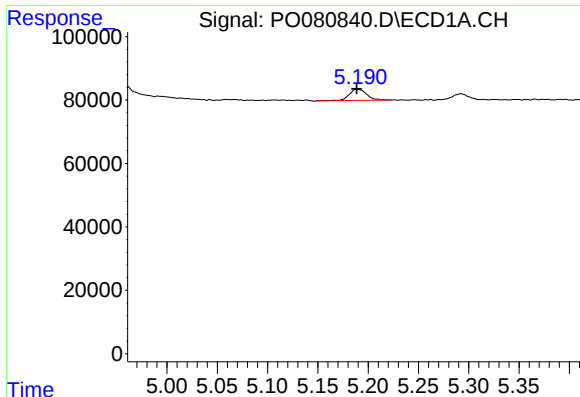

#8 AR-1221-1


R.T.: 5.190 min
Delta R.T.: 0.001 min
Response: 42942
Conc: 46.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

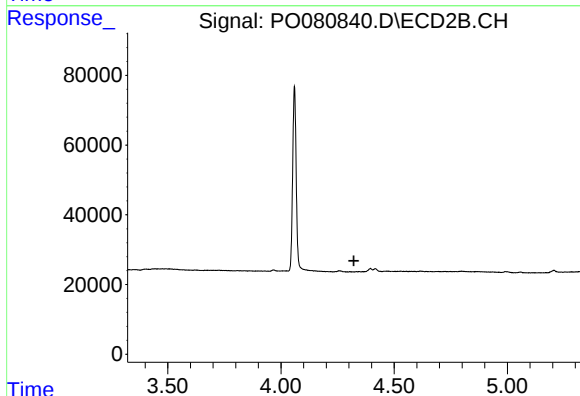


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.322 min
Response: 0
Conc: N.D.

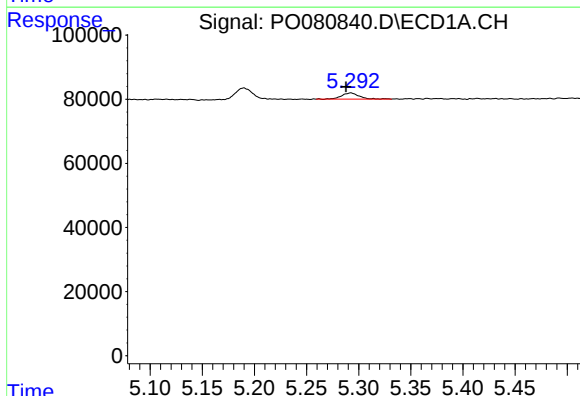


#9 AR-1221-2

R.T.: 5.292 min
Delta R.T.: 0.004 min
Response: 22617
Conc: 31.97 ng/ml

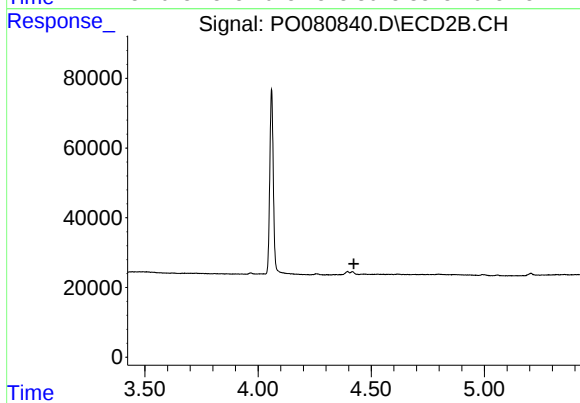

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.423 min
Response: 0
Conc: N.D.

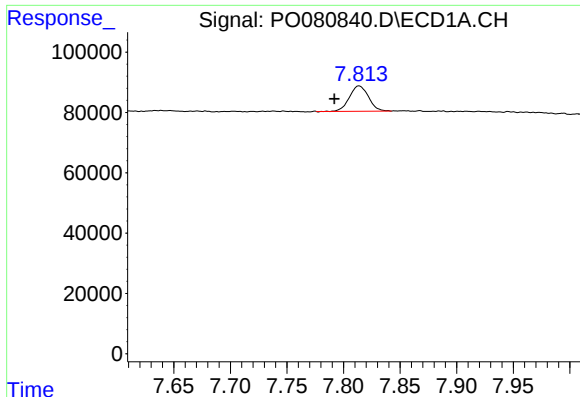

#28 AR-1254-3


R.T.: 7.814 min
Delta R.T.: 0.022 min
Response: 98698
Conc: 18.24 ng/ml

Instrument :
ECD_O
ClientSampleId :

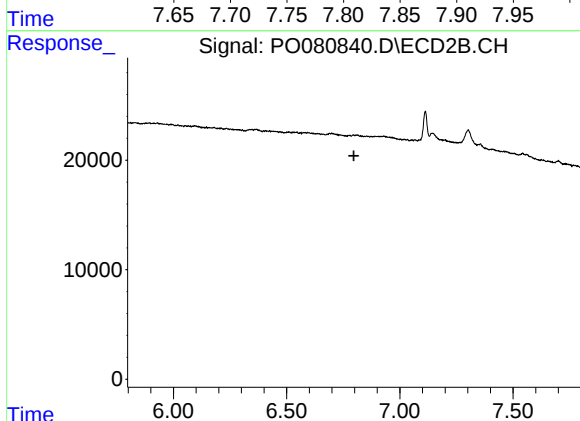


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.797 min
Response: 0
Conc: N.D.

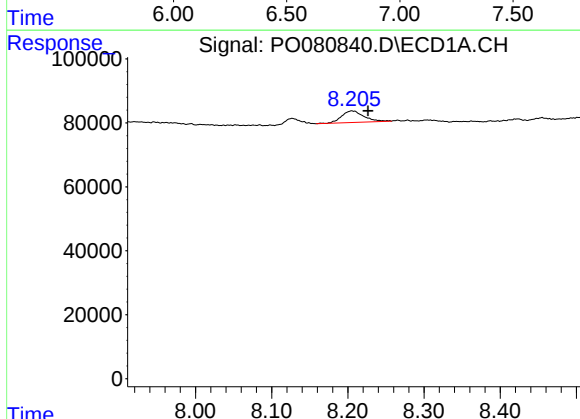


#32 AR-1260-2

R.T.: 8.205 min
Delta R.T.: -0.021 min
Response: 74367
Conc: 15.64 ng/ml

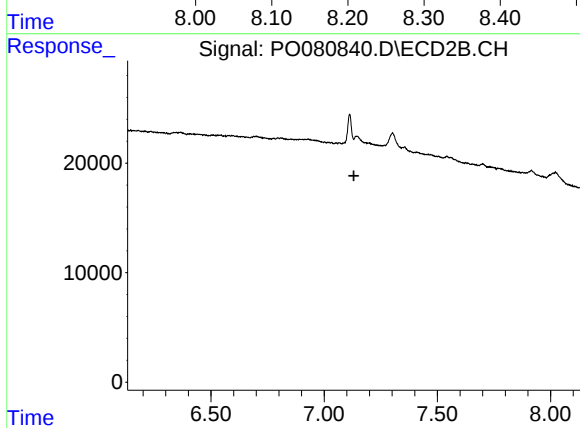

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.131 min
Response: 0
Conc: N.D.

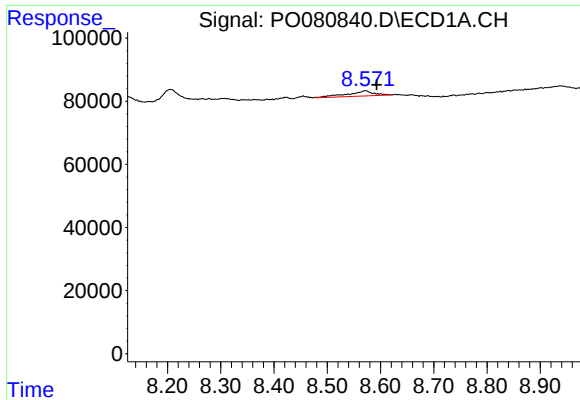

#33 AR-1260-3


R.T.: 8.572 min
Delta R.T.: -0.021 min
Response: 57351
Conc: 19.79 ng/ml

Instrument :
ECD_O
ClientSampleId :

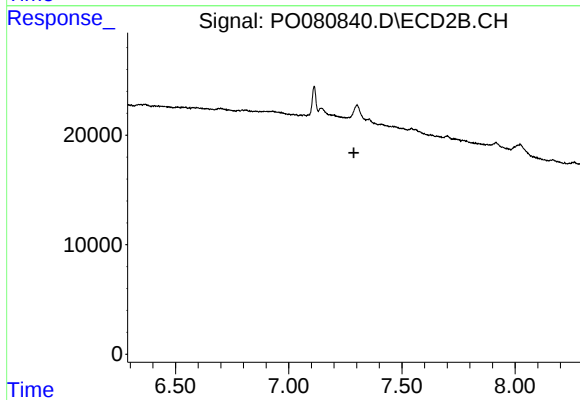


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.288 min
Response: 0
Conc: N.D.

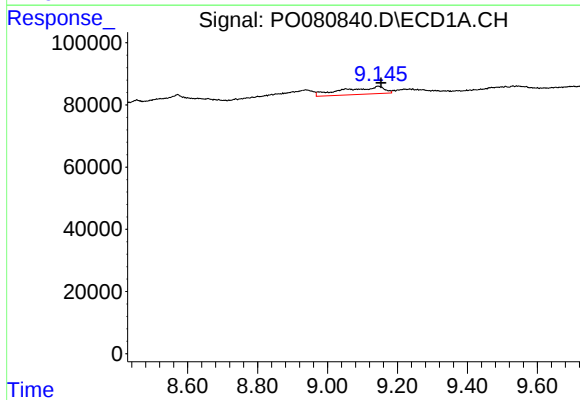


#35 AR-1260-5

R.T.: 9.144 min
Delta R.T.: -0.009 min
Response: 194394
Conc: 28.52 ng/ml

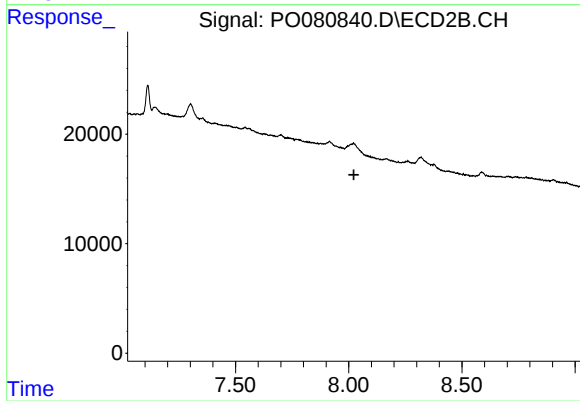

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.023 min
Response: 0
Conc: N.D.

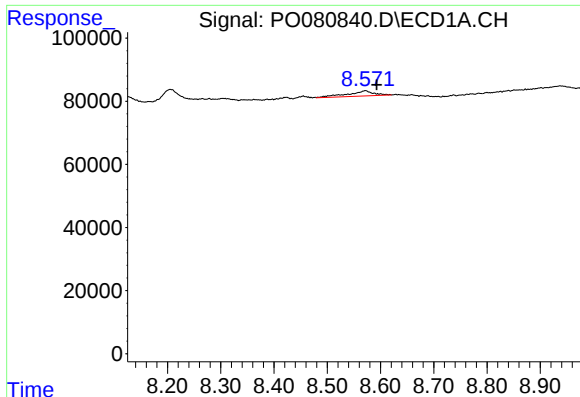

#36 AR-1262-1


R.T.: 8.572 min
Delta R.T.: -0.021 min
Response: 57351
Conc: 12.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

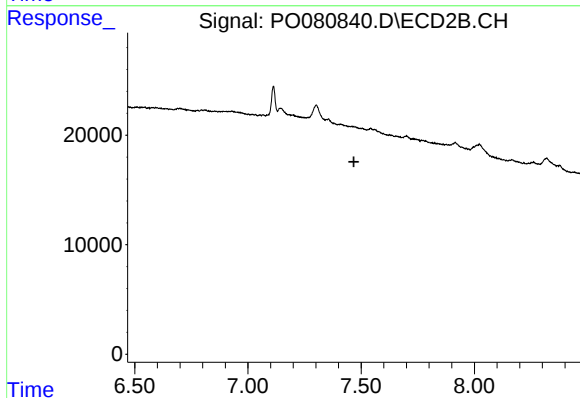


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.468 min
Response: 0
Conc: N.D.

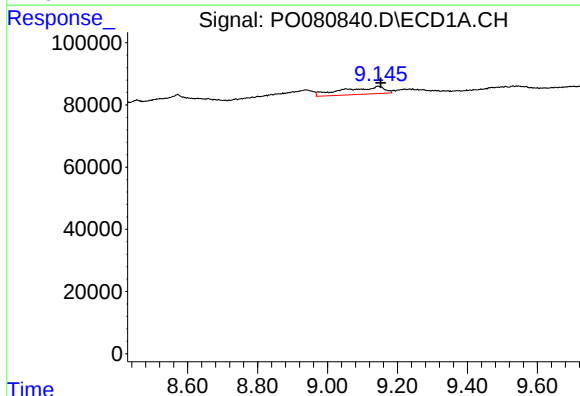

#37 AR-1262-2

R.T.: 9.144 min
Delta R.T.: -0.008 min
Response: 194394
Conc: 24.63 ng/ml

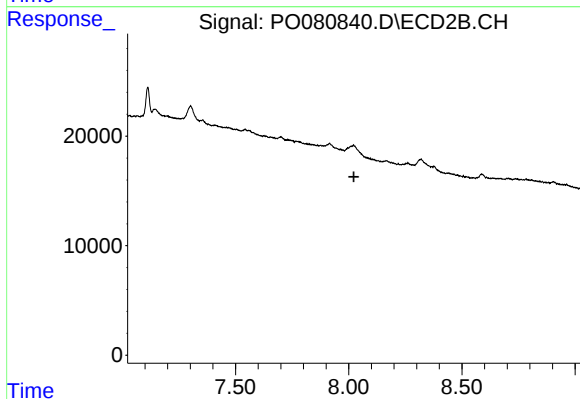

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.023 min
Response: 0
Conc: N.D.