

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0083118\
 Data File : P0048690.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2018 10:35
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 11:46:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.385	3.622	5255323	6180291	27.743	22.829
2)	SA Decachlor...	10.064	8.595	3388231	3171865	19.676	18.939
Target Compounds							
9)	L2 AR-1221-2	4.695	3.919	47539	87140	31.355	45.295 #
10)	L2 AR-1221-3	4.746	0.000	625766	0	126.137	N.D. #
14)	L3 AR-1232-4	6.405	0.000	48006	0	29.639	N.D. #
15)	L3 AR-1232-5	6.405	0.000	48006	0	20.403	N.D. #
22)	L5 AR-1248-2	6.405	0.000	48006	0	8.260	N.D. #
23)	L5 AR-1248-3	6.405	0.000	48006	0	6.221	N.D. #
24)	L5 AR-1248-4	6.405	0.000	48006	0	6.554	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083118\
Data File : P0048690.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2018 10:35
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 11:46:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

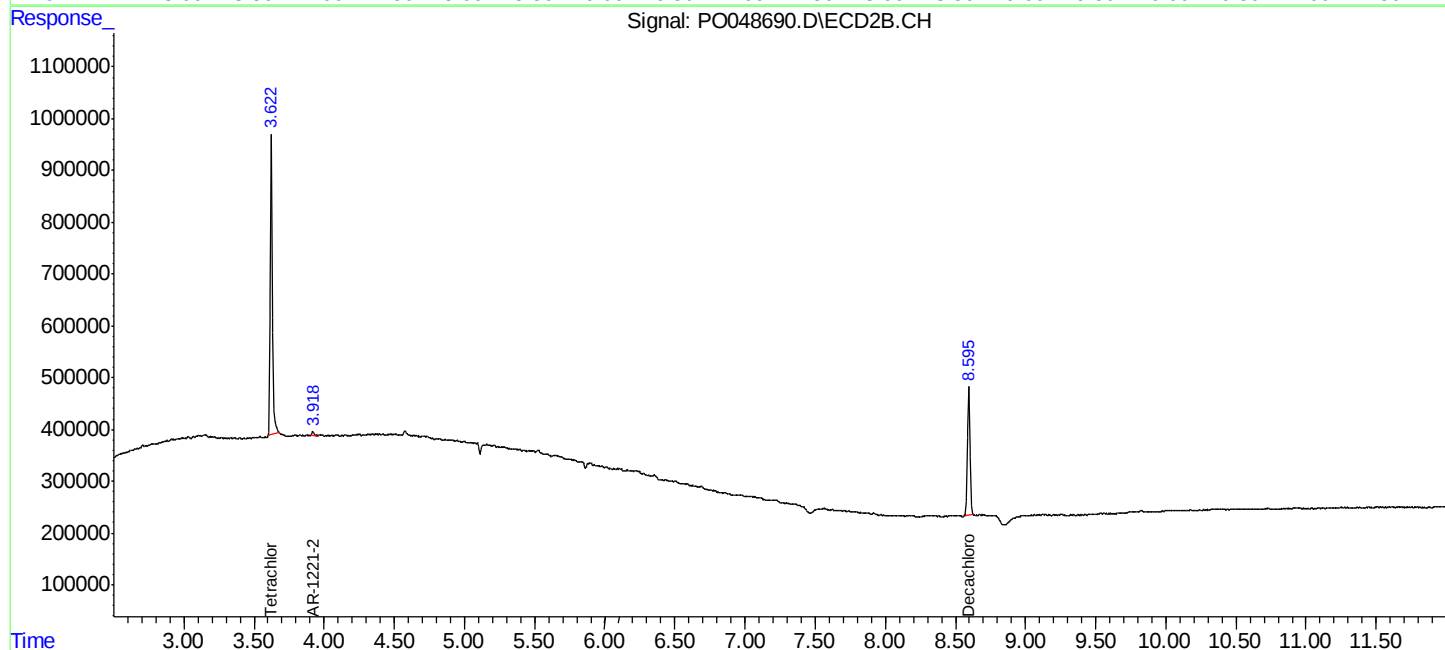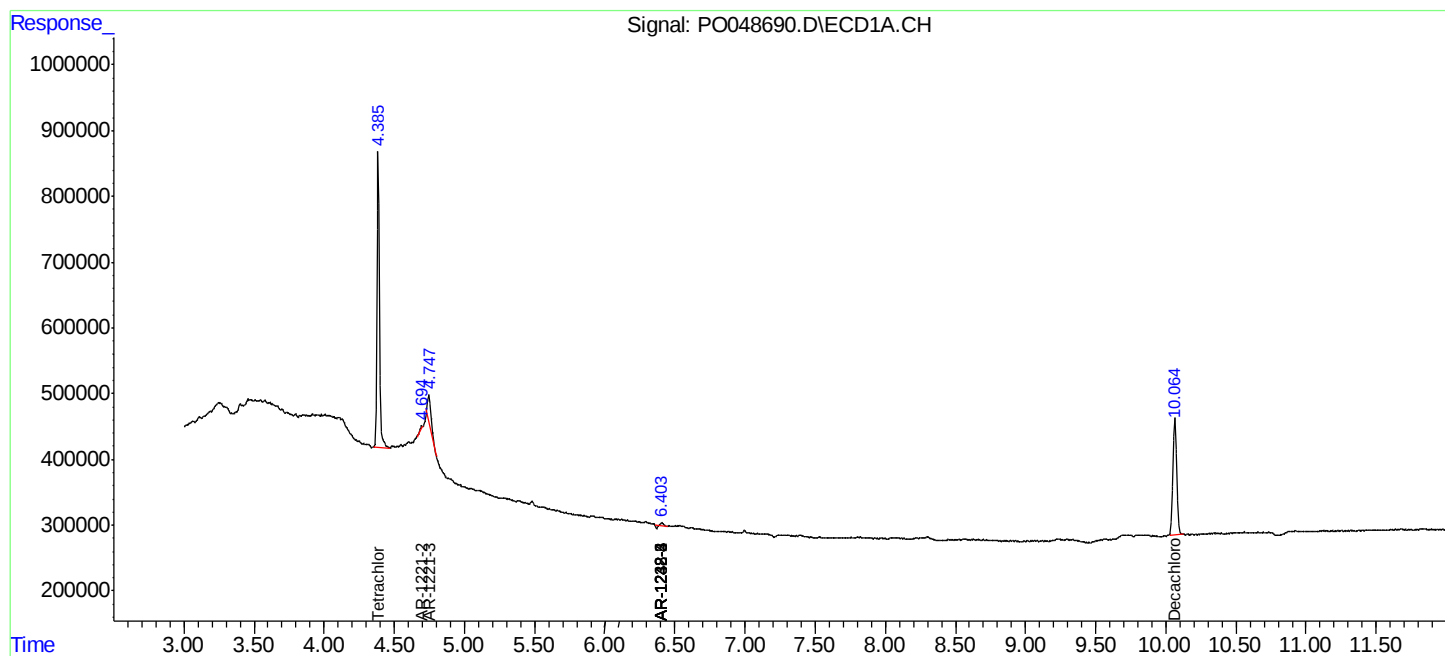


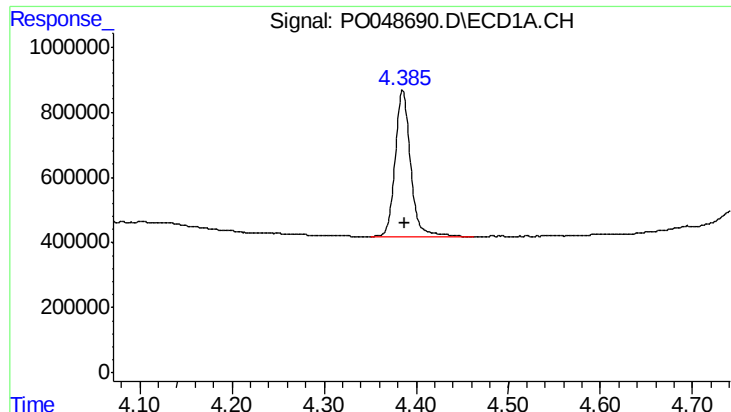

#1 Tetrachloro-m-xylene


R.T.: 4.385 min
Delta R.T.: -0.002 min
Response: 5255323
Conc: 27.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

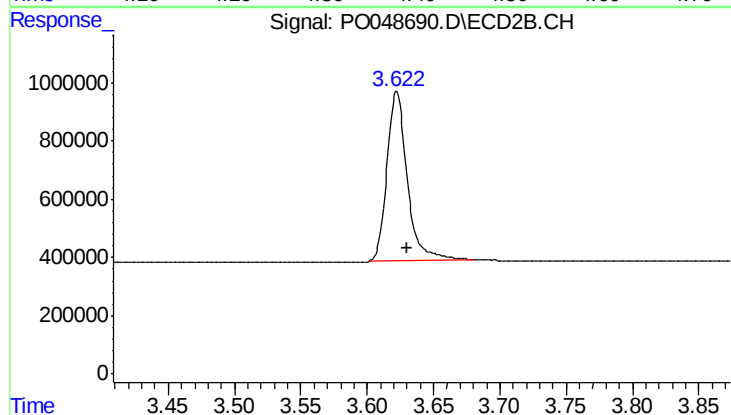


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.008 min
Response: 6180291
Conc: 22.83 ng/ml

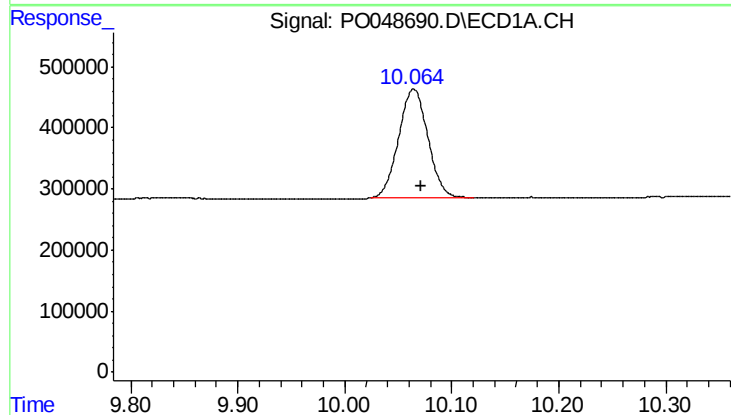


#2 Decachlorobiphenyl

R.T.: 10.064 min
Delta R.T.: -0.008 min
Response: 3388231
Conc: 19.68 ng/ml

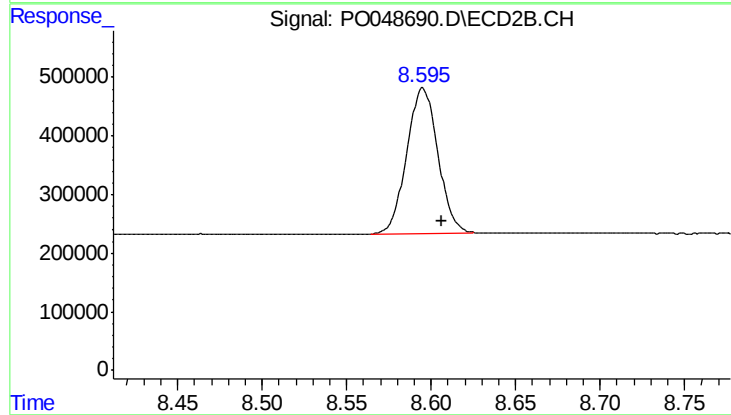

#2 Decachlorobiphenyl


R.T.: 8.595 min
Delta R.T.: -0.011 min
Response: 3171865
Conc: 18.94 ng/ml

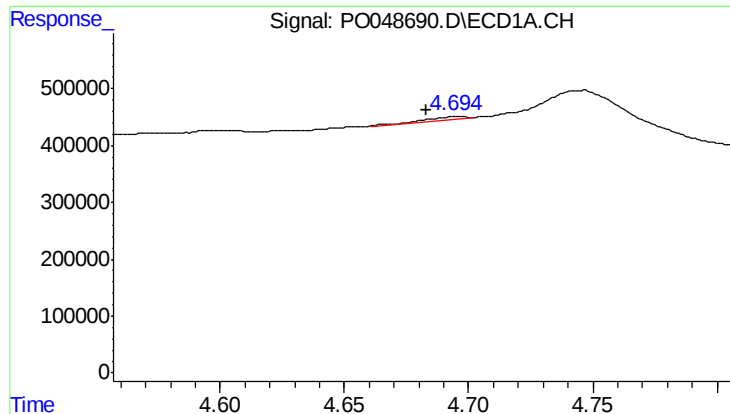

#9 AR-1221-2


R.T.: 4.695 min
Delta R.T.: 0.012 min
Response: 47539
Conc: 31.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

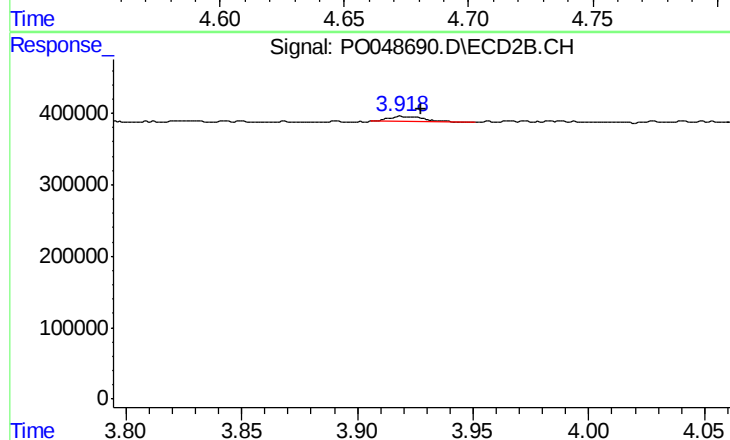


#9 AR-1221-2

R.T.: 3.919 min
Delta R.T.: -0.008 min
Response: 87140
Conc: 45.30 ng/ml

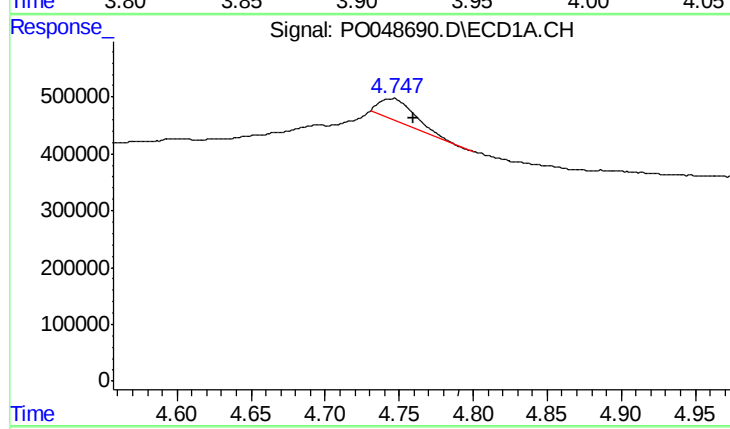


#10 AR-1221-3

R.T.: 4.746 min
Delta R.T.: -0.013 min
Response: 625766
Conc: 126.14 ng/ml

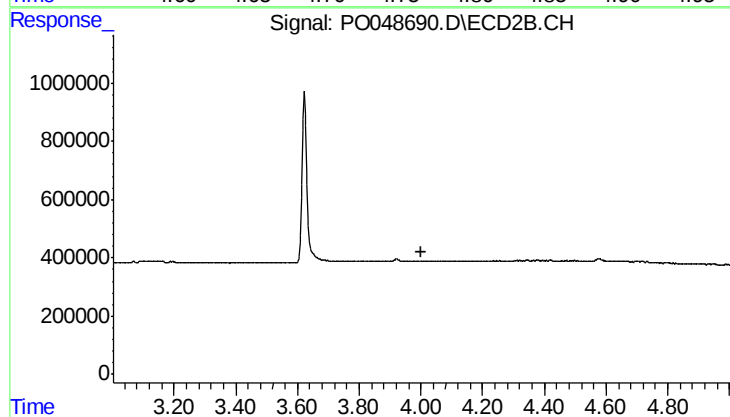

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.003 min
Response: 0
Conc: N.D.

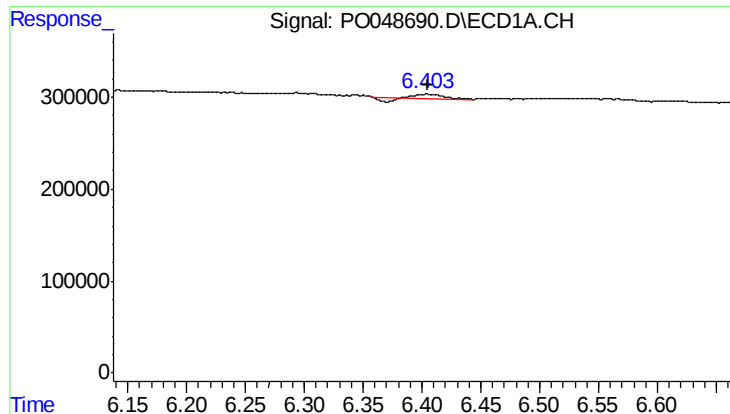

#14 AR-1232-4


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 48006
Conc: 29.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

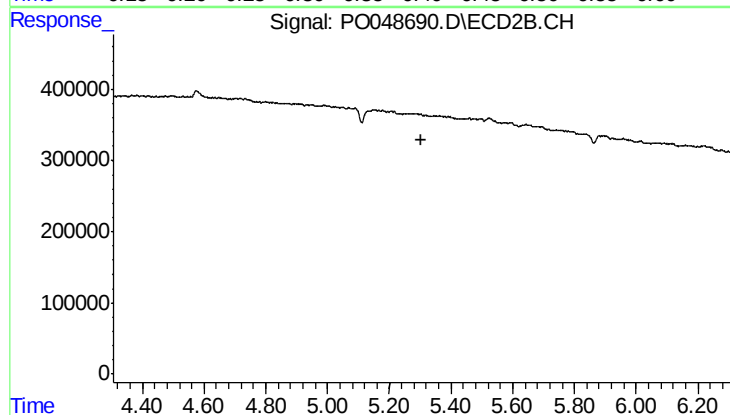


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.306 min
Response: 0
Conc: N.D.

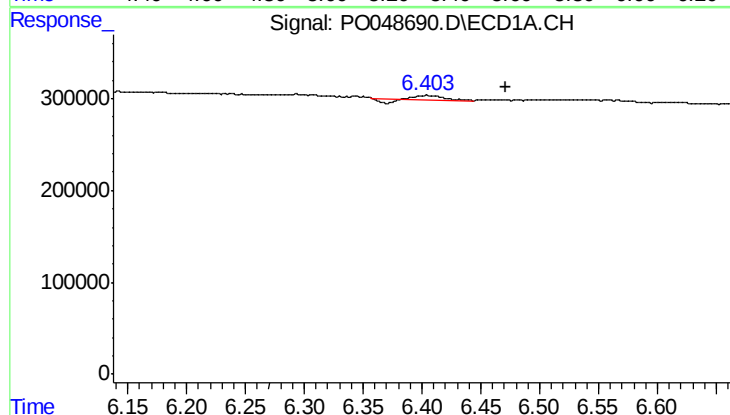


#15 AR-1232-5

R.T.: 6.405 min
Delta R.T.: -0.067 min
Response: 48006
Conc: 20.40 ng/ml

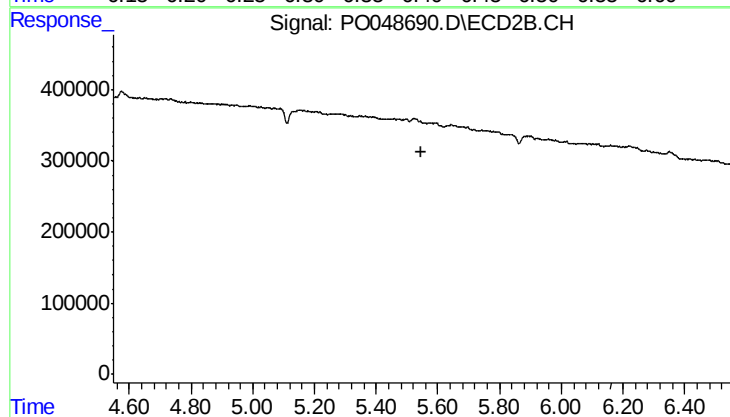

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

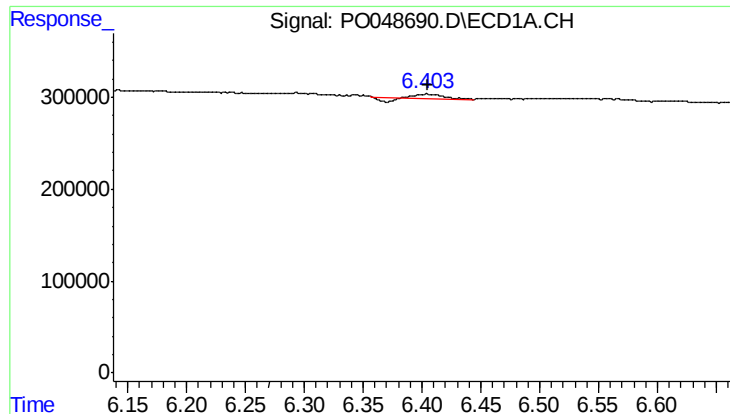

#22 AR-1248-2


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 48006
Conc: 8.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

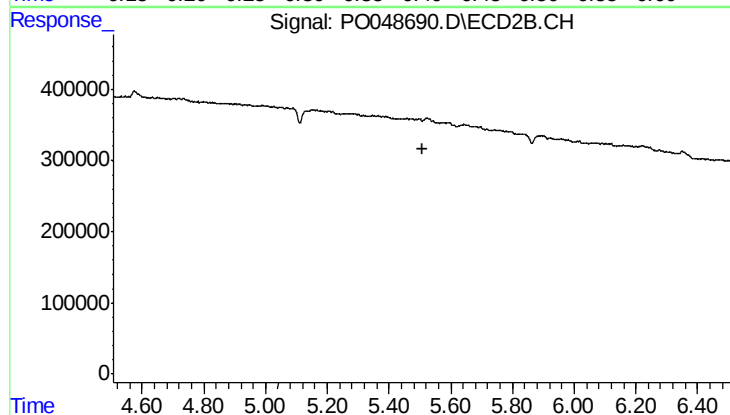


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.507 min
Response: 0
Conc: N.D.

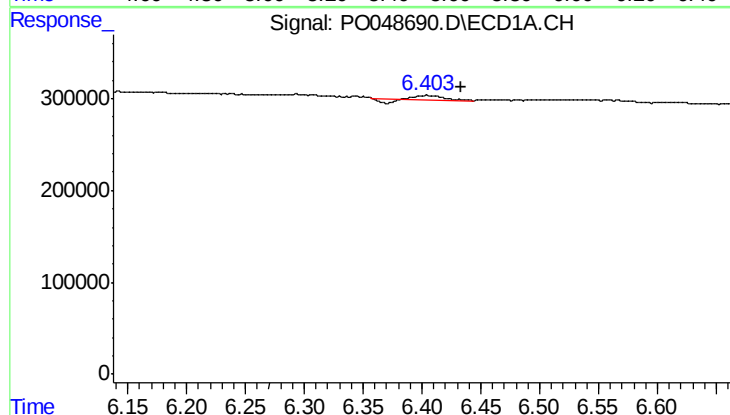


#23 AR-1248-3

R.T.: 6.405 min
Delta R.T.: -0.028 min
Response: 48006
Conc: 6.22 ng/ml

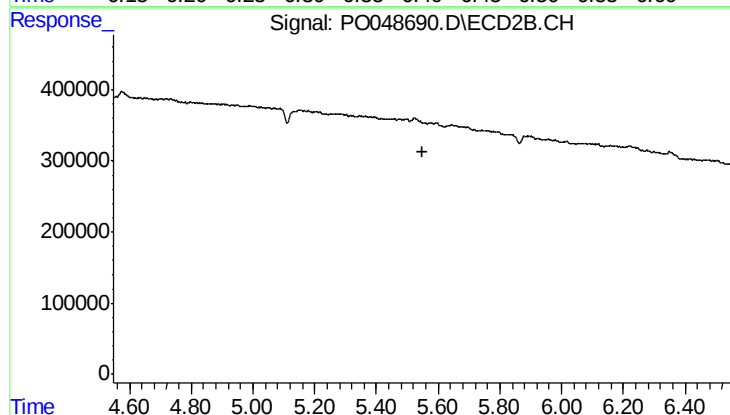

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

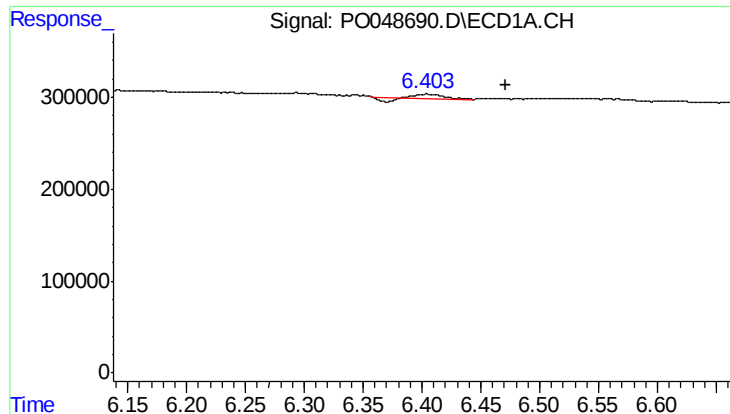

#24 AR-1248-4

R.T.: 6.405 min
Delta R.T.: -0.067 min
Response: 48006
Conc: 6.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

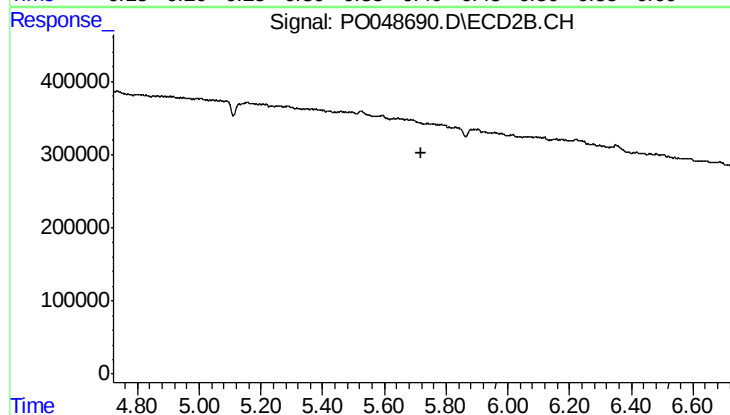

#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.721 min
Response: 0
Conc: N.D.