

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083119\
 Data File : P0060193.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2019 20:30
 Operator : SM/AJ
 Sample : K4624-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 T-11-A1-A4-(0-4)

Manual Integrations
 APPROVED

Ankita
 9/3/2019 4:34:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 23:16:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.116	3.497	922829	695501	26.357	19.322 #
2)	SA Decachlor...	9.569	8.346	847465	725761	15.930	18.000m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083119\
Data File : PO060193.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2019 20:30
Operator : SM/AJ
Sample : K4624-06
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
T-11-A1-A4-(0-4)


Manual Integrations
APPROVED

Ankita
9/3/2019 4:34:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 23:16:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

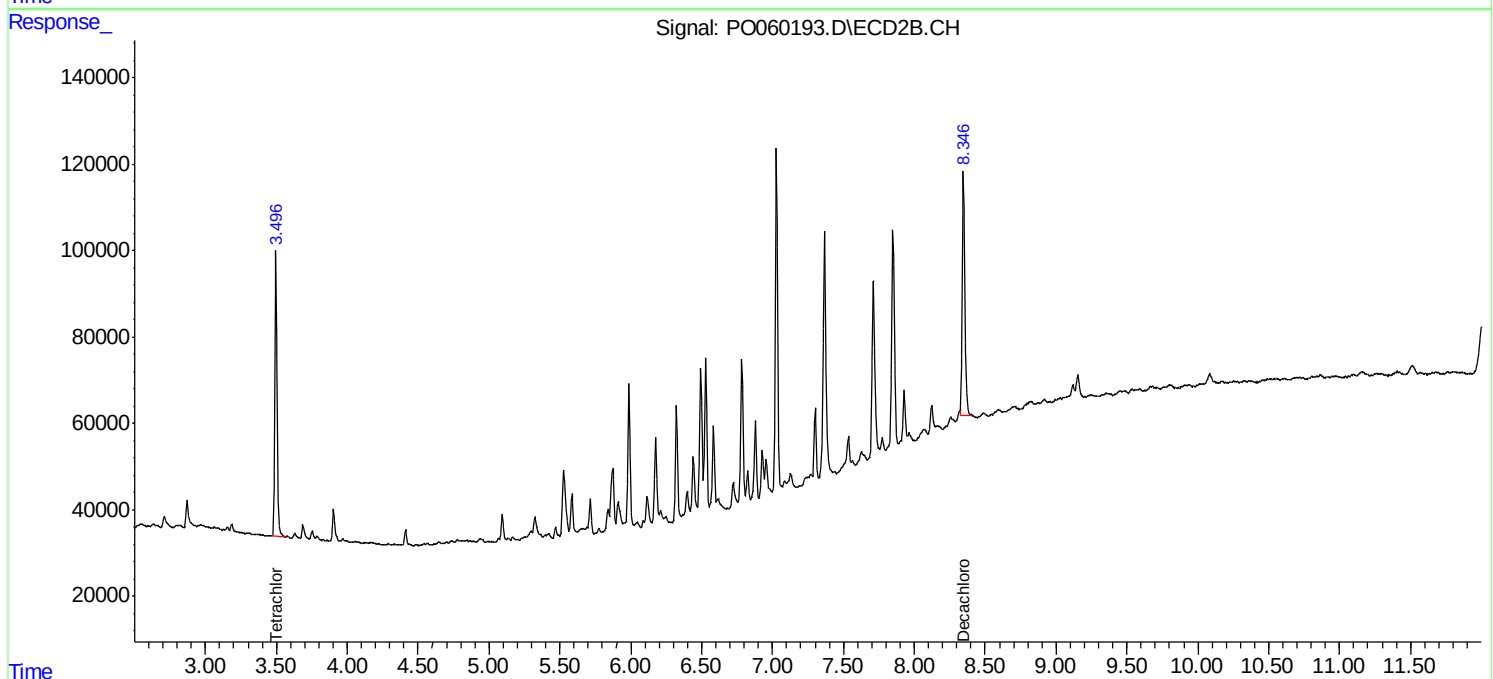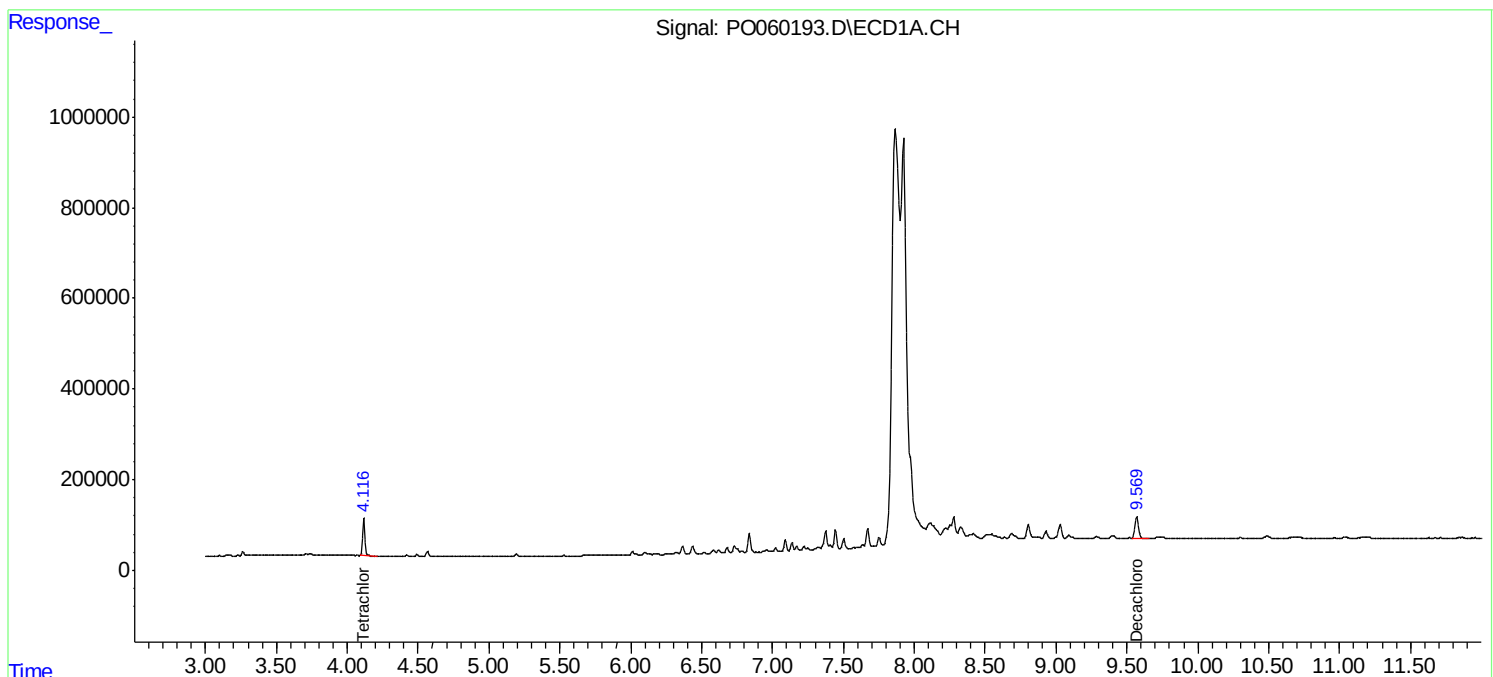

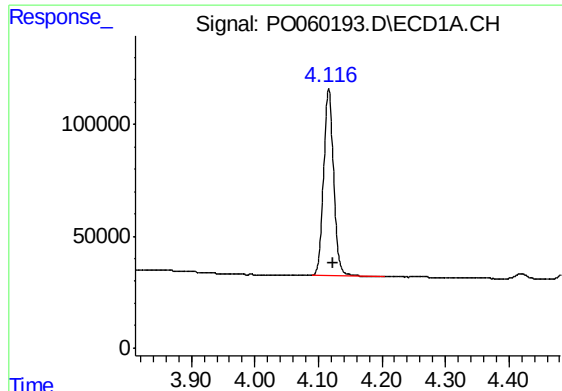


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.008 min
Response: 922829
Conc: 26.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
T-11-A1-A4-(0-4)


Manual Integrations
APPROVED

Ankita
9/3/2019 4:34:41 PM

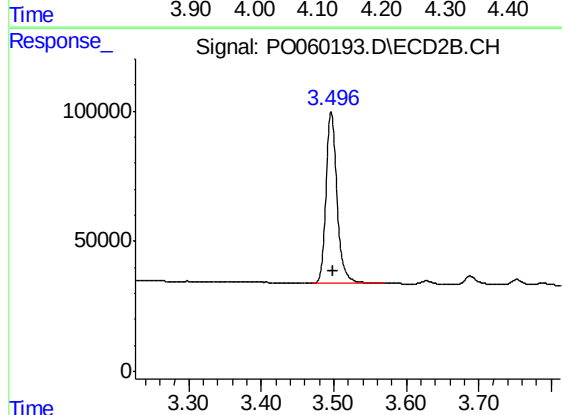


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.003 min
Response: 695501
Conc: 19.32 ng/ml

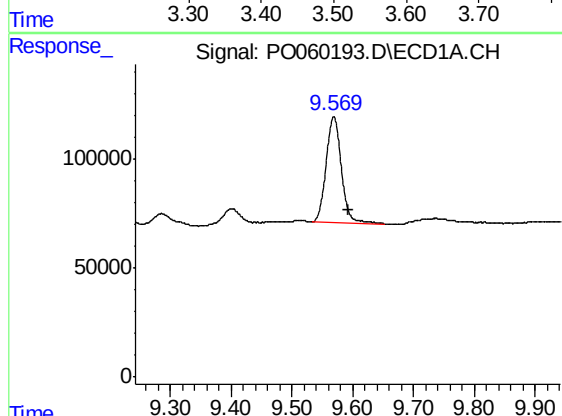

#2 Decachlorobiphenyl

R.T.: 9.569 min
Delta R.T.: -0.024 min
Response: 847465
Conc: 15.93 ng/ml

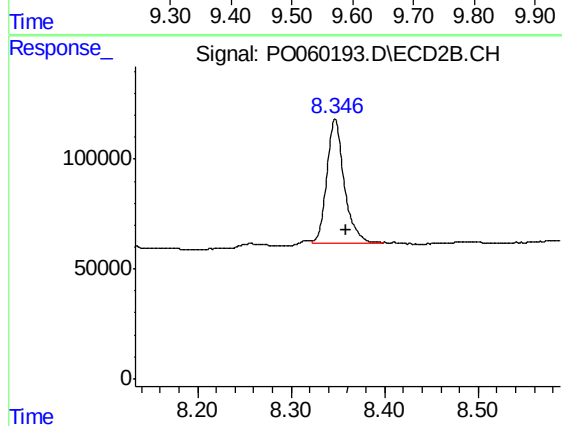

#2 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: -0.013 min
Response: 725761
Conc: 18.00 ng/ml m