

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
 Data File : P0071025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2020 10:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 10:58:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.537	1789967	1032211	23.178	23.284
2) SA Decachlor...	9.970	8.720	2048307	1272994	22.385	22.163
Target Compounds						
30) L6 AR-1254-5	7.864	0.000	127094	0	24.157	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
Data File : P0071025.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2020 10:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 10:58:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

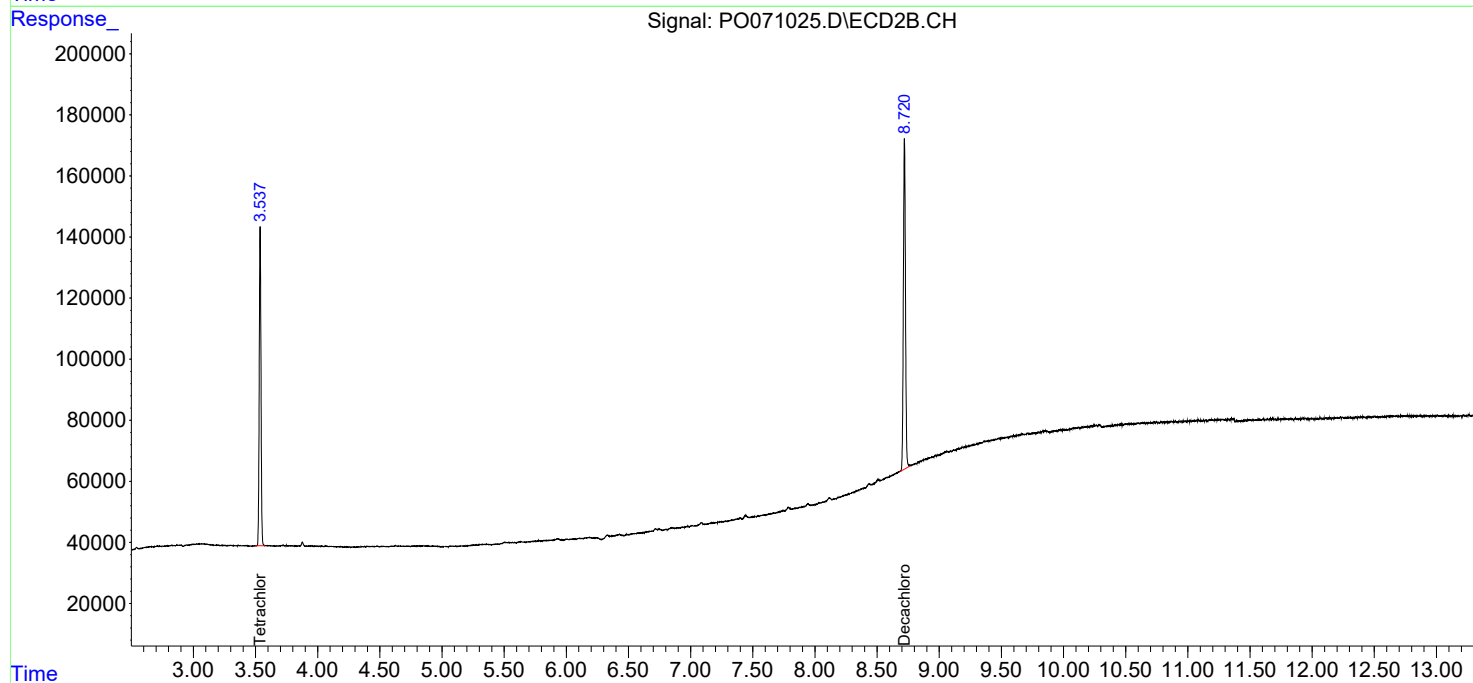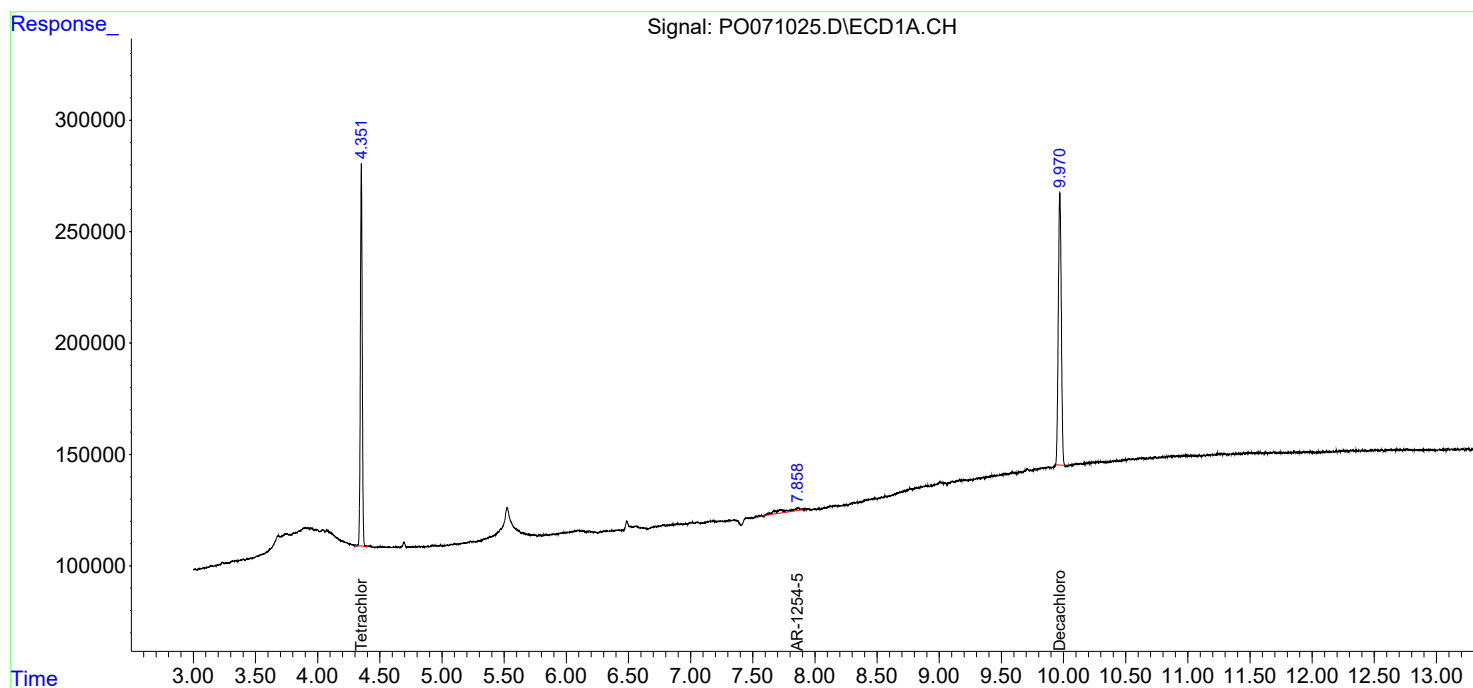


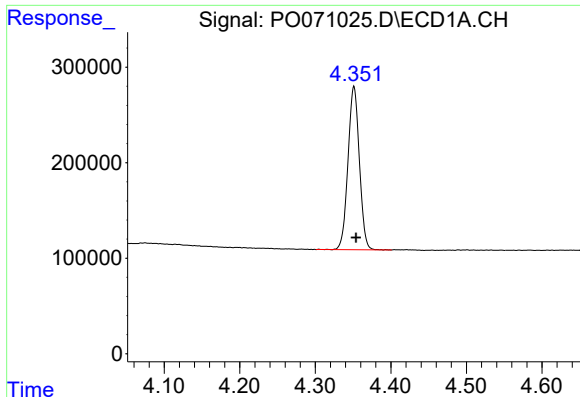

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 1789967
Conc: 23.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

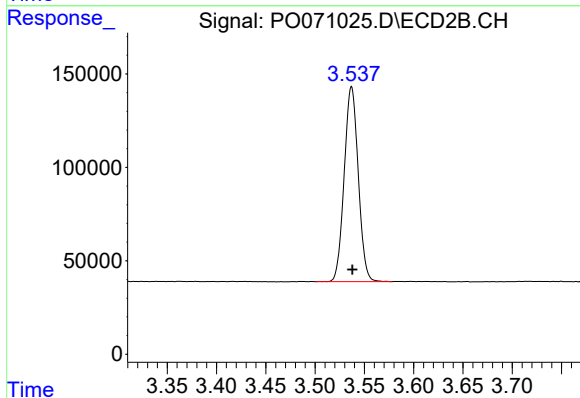


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 1032211
Conc: 23.28 ng/ml

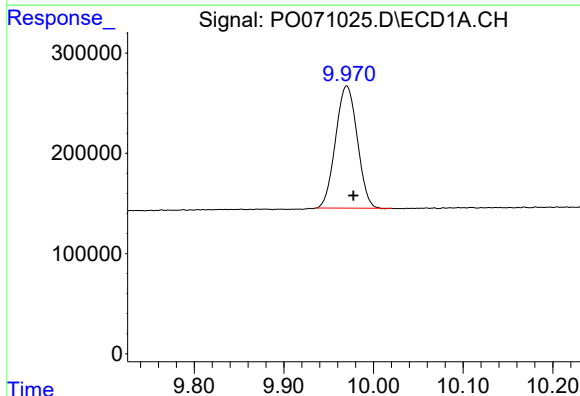


#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.007 min
Response: 2048307
Conc: 22.39 ng/ml

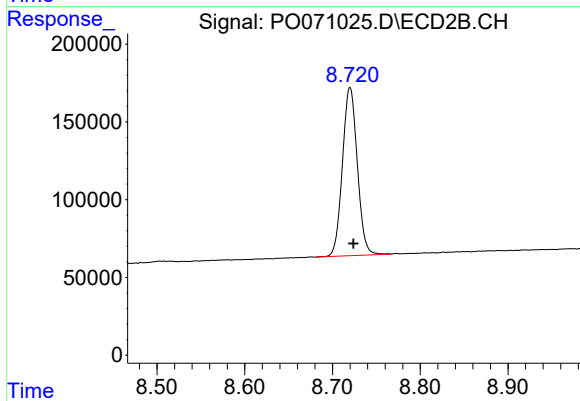

#2 Decachlorobiphenyl


R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 1272994
Conc: 22.16 ng/ml

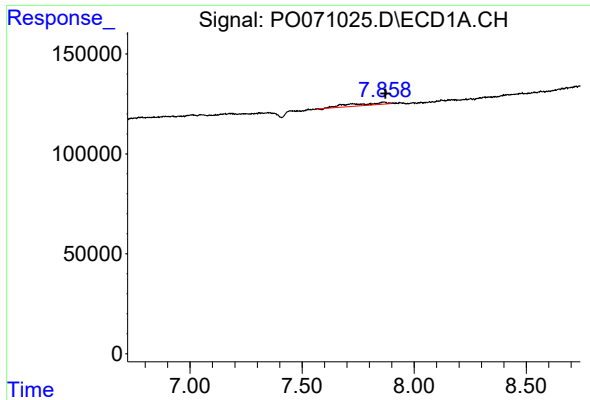

#30 AR-1254-5

R.T.: 7.864 min
Delta R.T.: -0.006 min
Response: 127094
Conc: 24.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

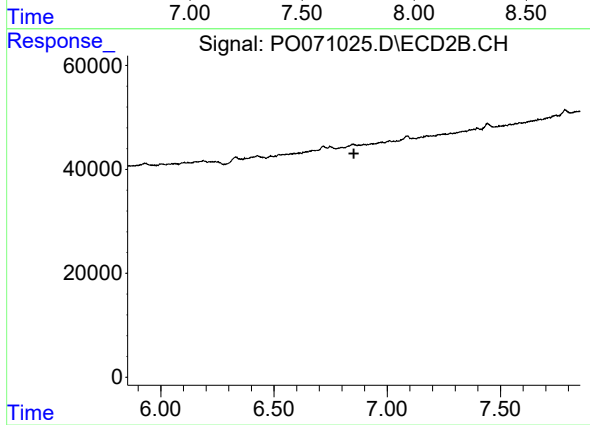

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.