

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
 Data File : P0071058.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2020 21:45
 Operator : DD\AJ
 Sample : L3847-29
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LINDEN-JOP-BH-12-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 05:23:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.351	3.537	1703734	975253	22.061	21.999
2)	SA Decachlor...	9.970	8.720	1331106	725371	14.547	12.629
Target Compounds							
20)	L4 AR-1242-5	6.633	0.000	74275	0	35.877	N.D. #
25)	L5 AR-1248-5	6.633	0.000	74275	0	22.266	N.D. #
28)	L6 AR-1254-3	7.171f	0.000	140839	0	24.456	N.D. #
34)	L7 AR-1260-4	8.146f	0.000	37869	0	7.147	N.D. #
35)	L7 AR-1260-5	8.471	0.000	34630	0	2.833	N.D. #
37)	L8 AR-1262-2	8.471	0.000	34630	0	2.622	N.D. #
39)	L8 AR-1262-4	8.814f	0.000	11331	0	3.454	N.D. #
42)	L9 AR-1268-2	8.814f	0.000	11331	0	0.841	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083120\
Data File : PO071058.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2020 21:45
Operator : DD\AJ
Sample : L3847-29
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-12-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 05:23:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

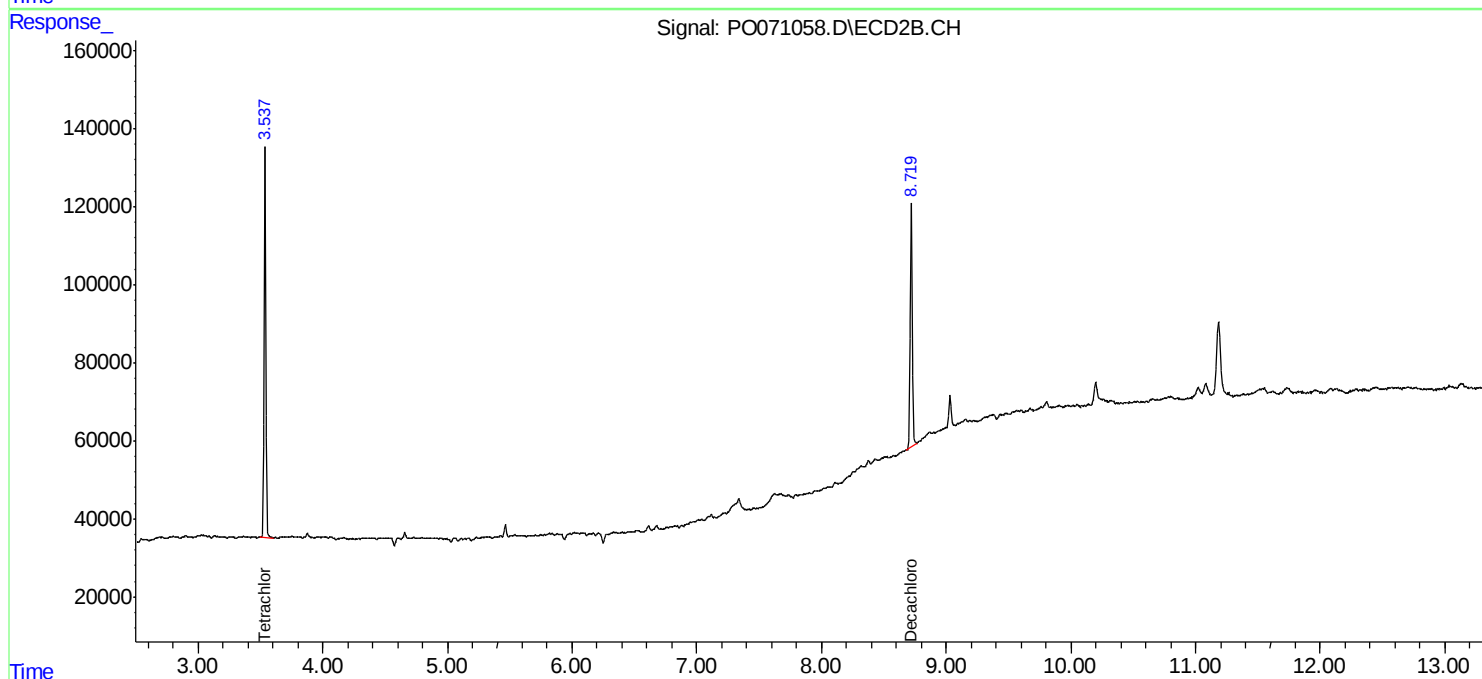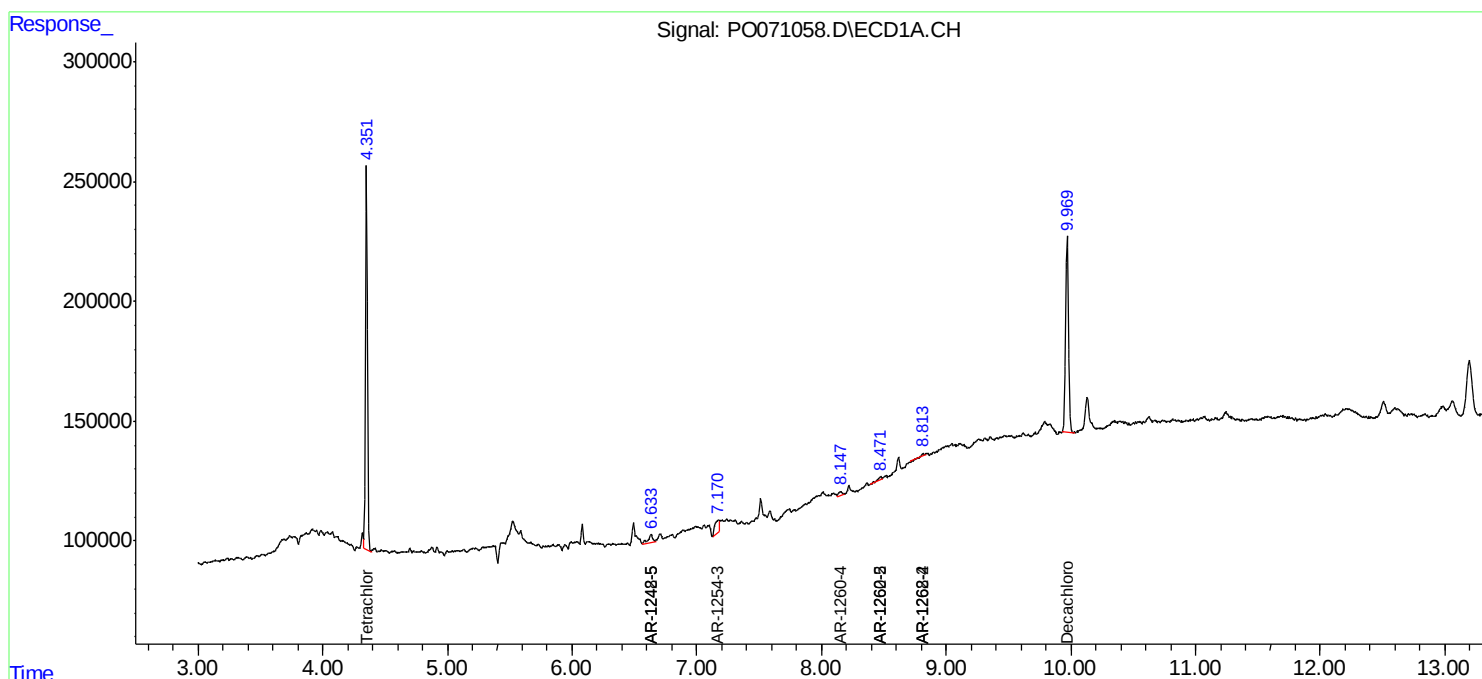


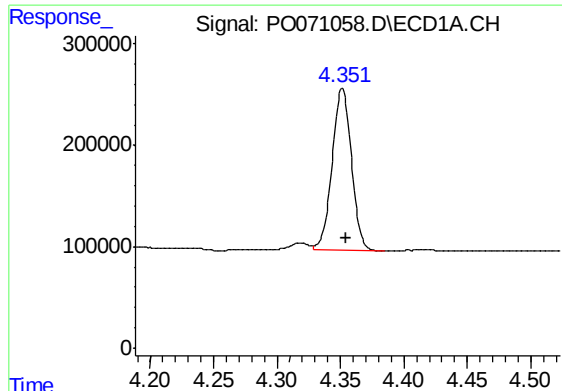

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 1703734
Conc: 22.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-12-C

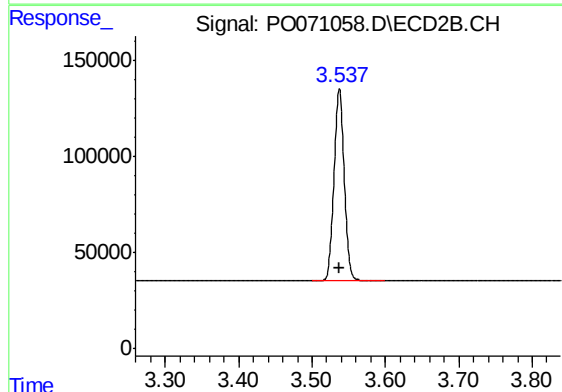


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 975253
Conc: 22.00 ng/ml

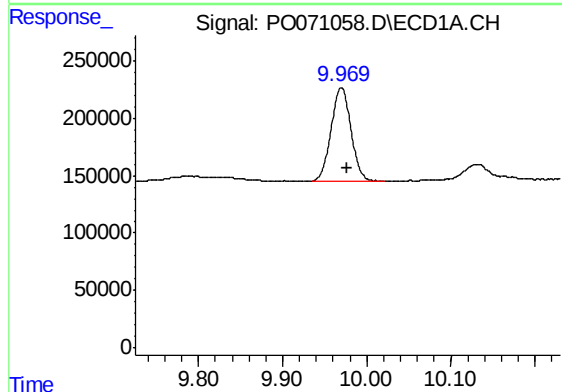


#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.008 min
Response: 1331106
Conc: 14.55 ng/ml

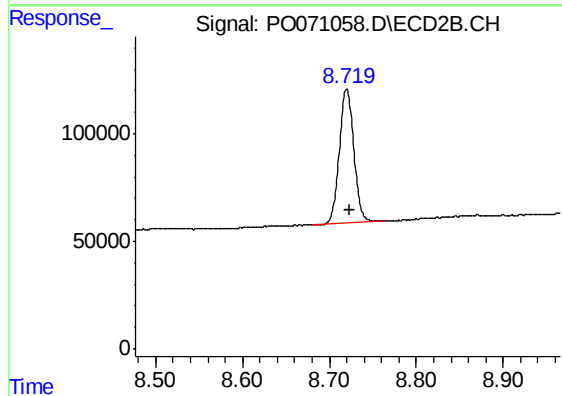

#2 Decachlorobiphenyl


R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 725371
Conc: 12.63 ng/ml

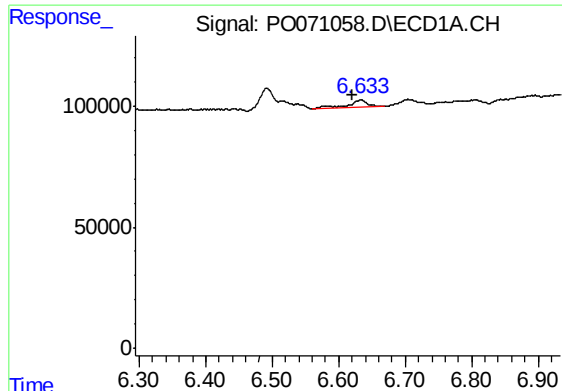

#20 AR-1242-5


R.T.: 6.633 min
Delta R.T.: 0.013 min
Response: 74275
Conc: 35.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-12-C

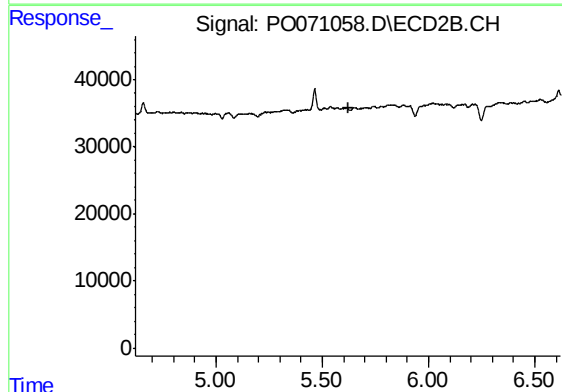


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.621 min
Response: 0
Conc: N.D.

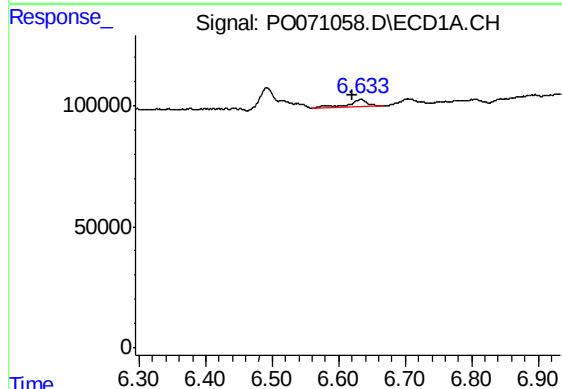


#25 AR-1248-5

R.T.: 6.633 min
Delta R.T.: 0.013 min
Response: 74275
Conc: 22.27 ng/ml

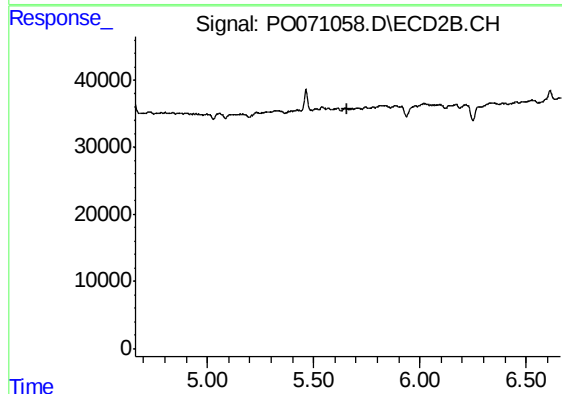

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.661 min
Response: 0
Conc: N.D.

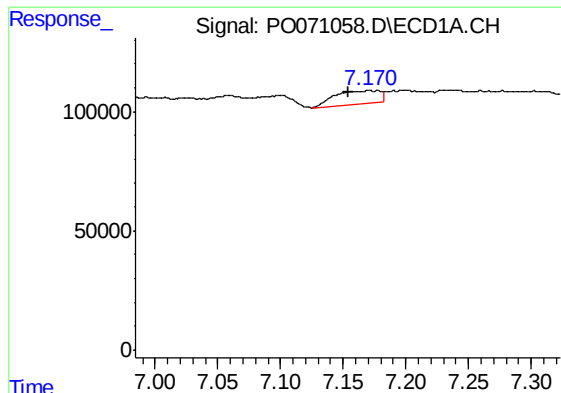

#28 AR-1254-3


R.T.: 7.171 min
Delta R.T.: 0.017 min
Response: 140839
Conc: 24.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-12-C

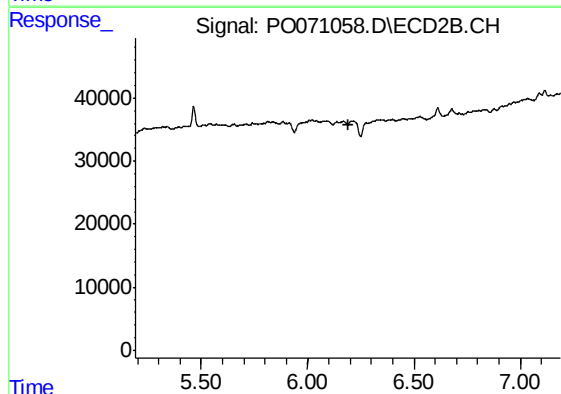


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.190 min
Response: 0
Conc: N.D.

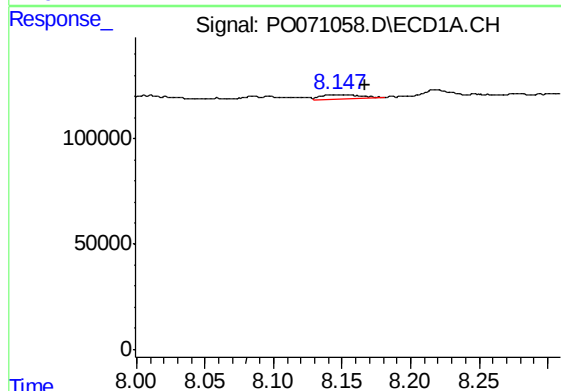


#34 AR-1260-4

R.T.: 8.146 min
Delta R.T.: -0.021 min
Response: 37869
Conc: 7.15 ng/ml

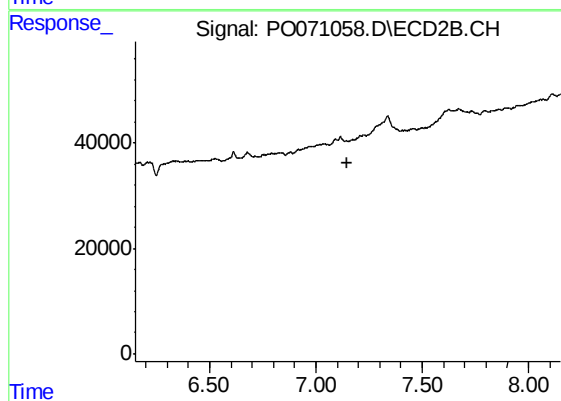

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.150 min
Response: 0
Conc: N.D.

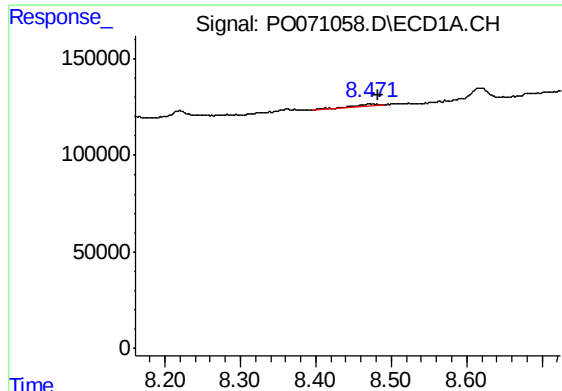

#35 AR-1260-5


R.T.: 8.471 min
Delta R.T.: -0.012 min
Response: 34630
Conc: 2.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-12-C

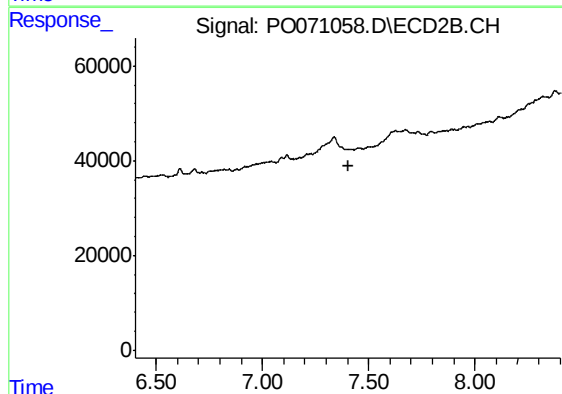


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.402 min
Response: 0
Conc: N.D.

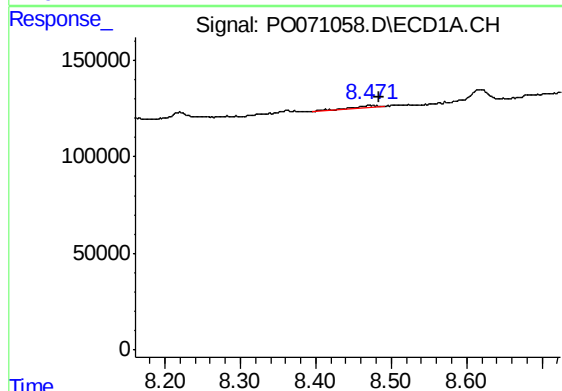


#37 AR-1262-2

R.T.: 8.471 min
Delta R.T.: -0.013 min
Response: 34630
Conc: 2.62 ng/ml

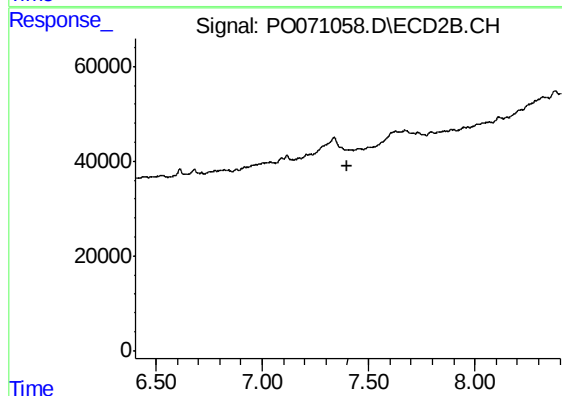

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.403 min
Response: 0
Conc: N.D.

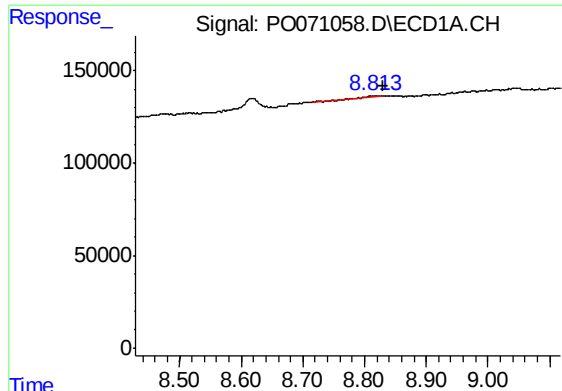

#39 AR-1262-4


R.T.: 8.814 min
Delta R.T.: -0.016 min
Response: 11331
Conc: 3.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-12-C

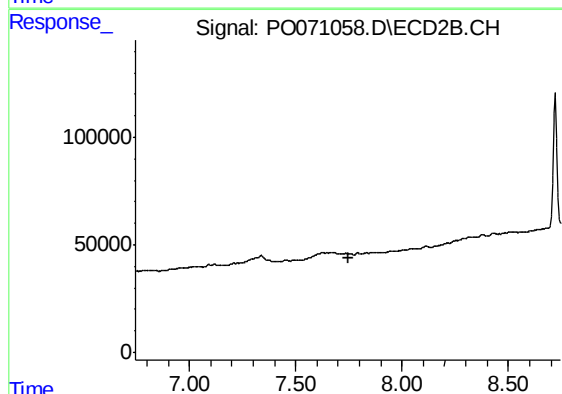


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.746 min
Response: 0
Conc: N.D.

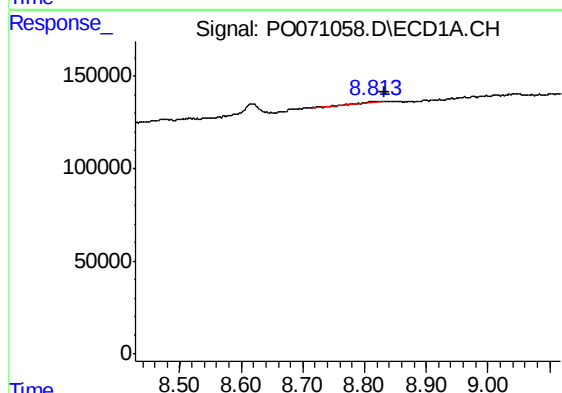

#42 AR-1268-2

R.T.: 8.814 min
Delta R.T.: -0.018 min
Response: 11331
Conc: 0.84 ng/ml

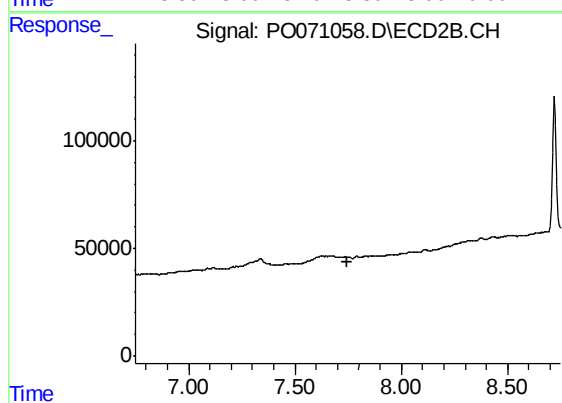

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.749 min
Response: 0
Conc: N.D.