

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
 Data File : P0071034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2020 14:28
 Operator : DD\AJ
 Sample : L3837-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 789UMR-TP11-0612-01

Manual Integrations
 APPROVED

Ankita
 9/1/2020 1:30:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 16:21:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.545	71025	8988	0.920	0.203m#
2) SA Decachlor...	9.972	8.720	25910	33337	0.283m	0.580m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
Data File : P0071034.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2020 14:28
Operator : DD\AJ
Sample : L3837-17
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
789UMR-TP11-0612-01


Manual Integrations
APPROVED

Ankita
9/1/2020 1:30:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 16:21:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

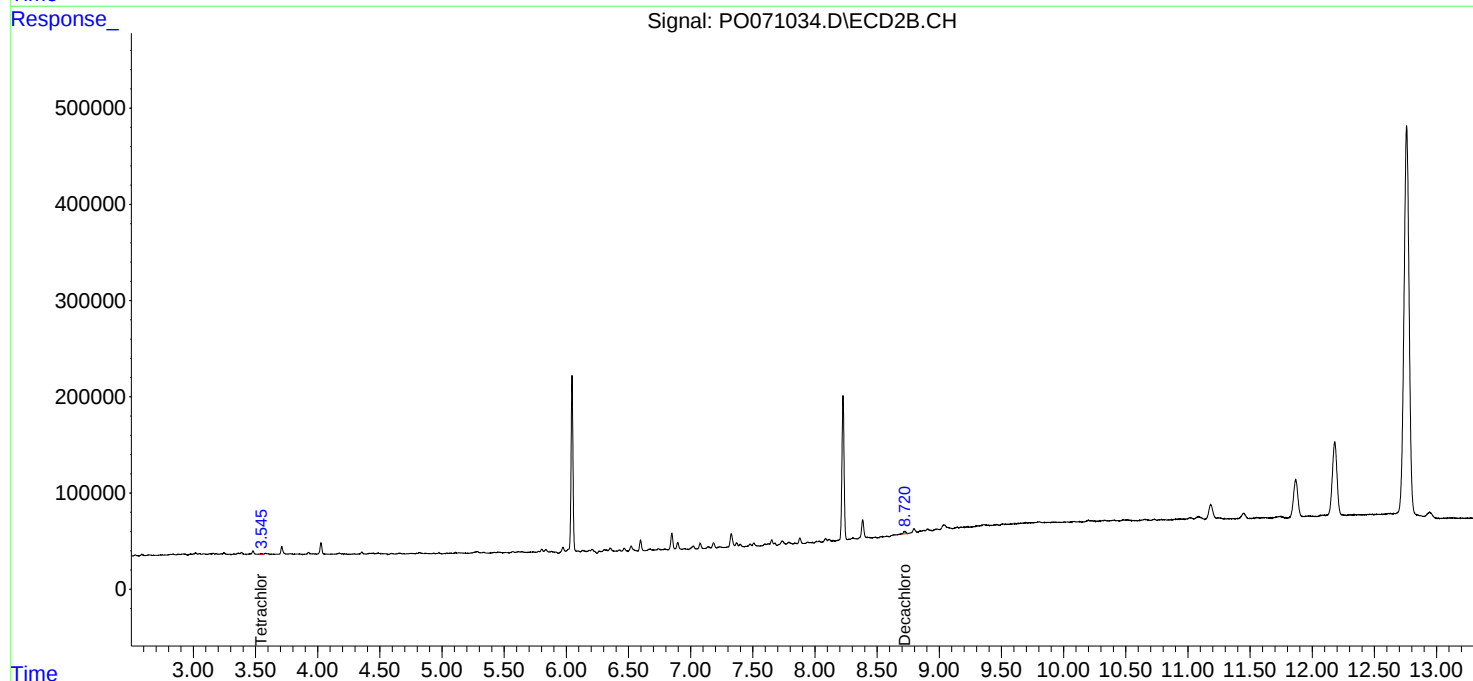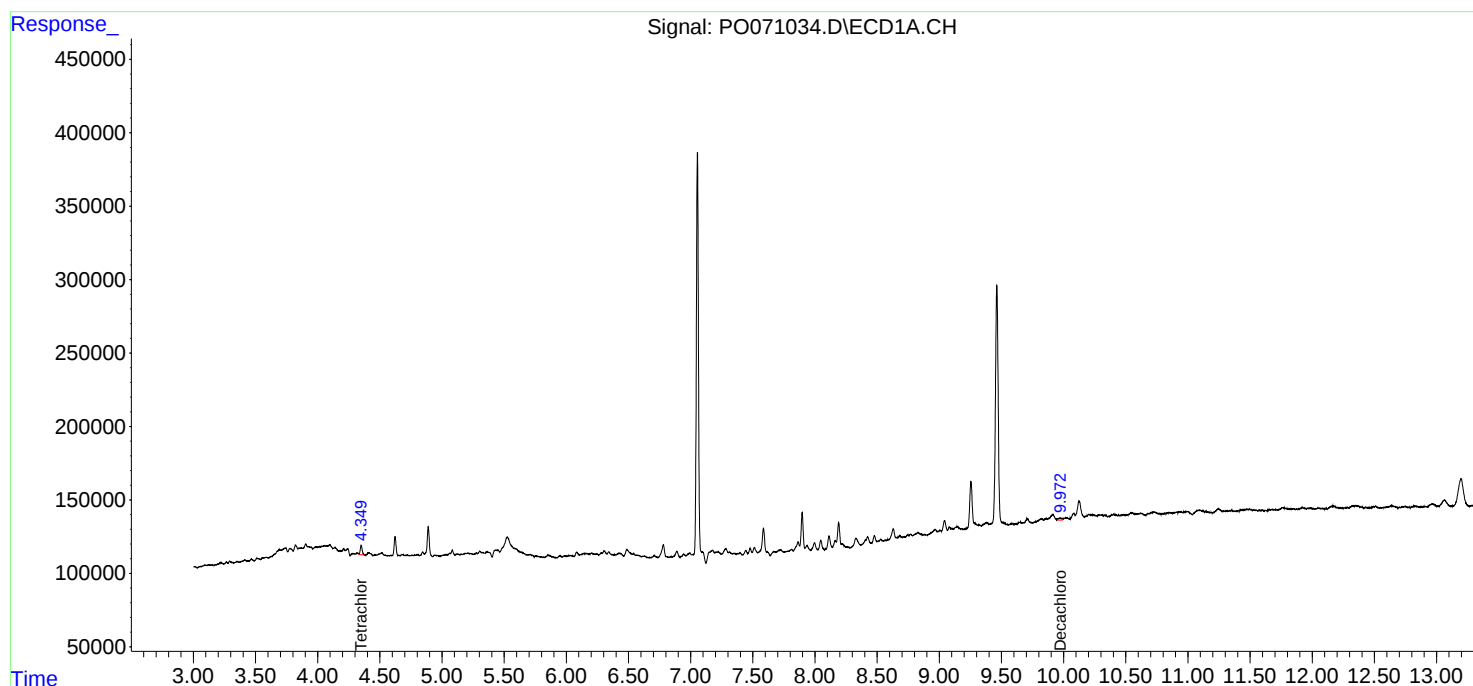

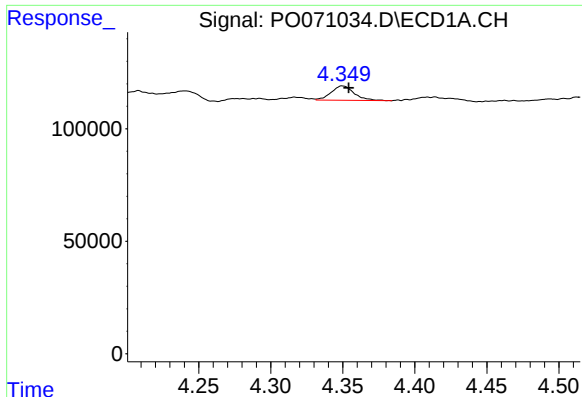


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.004 min
Response: 71025
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
789UMR-TP11-0612-01


Manual Integrations
APPROVED

Ankita
9/1/2020 1:30:32 PM

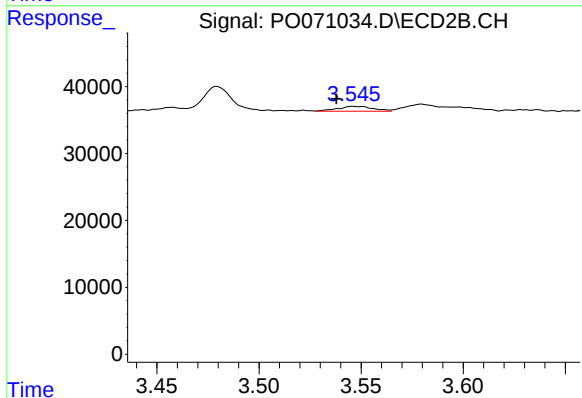


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.007 min
Response: 8988
Conc: 0.20 ng/ml m

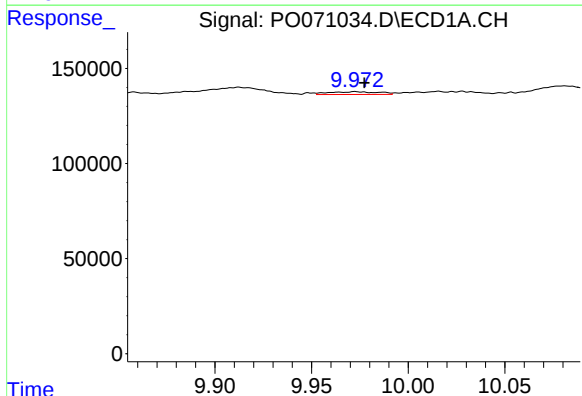

#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.005 min
Response: 25910
Conc: 0.28 ng/ml m

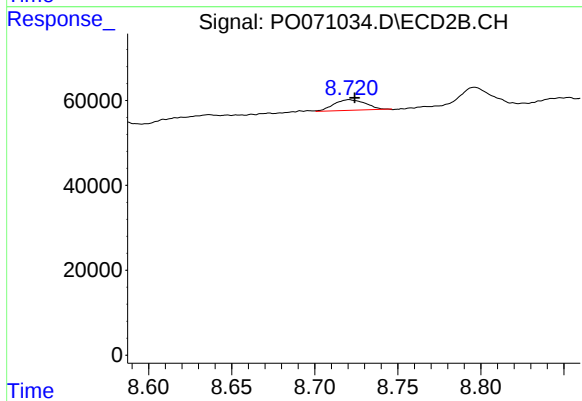

#2 Decachlorobiphenyl

R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 33337
Conc: 0.58 ng/ml m