

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
Data File : P0071045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2020 18:03
Operator : DD\AJ
Sample : L3847-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-09-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 04:19:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.537	1710566	1081964	22.150	24.406
2) SA Decachlor...	9.970	8.720	1970722	1005124	21.537	17.499

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083120\
Data File : P0071045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2020 18:03
Operator : DD\AJ
Sample : L3847-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-09-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 04:19:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

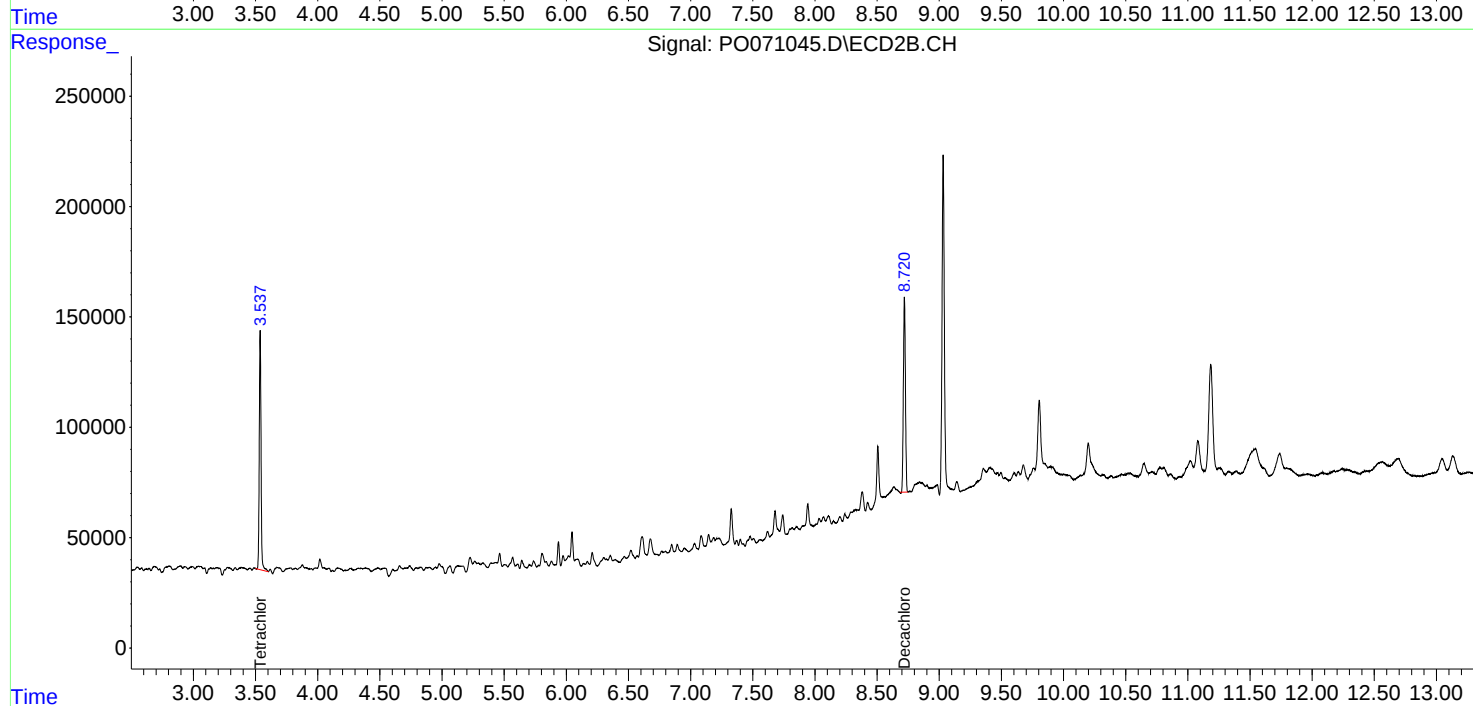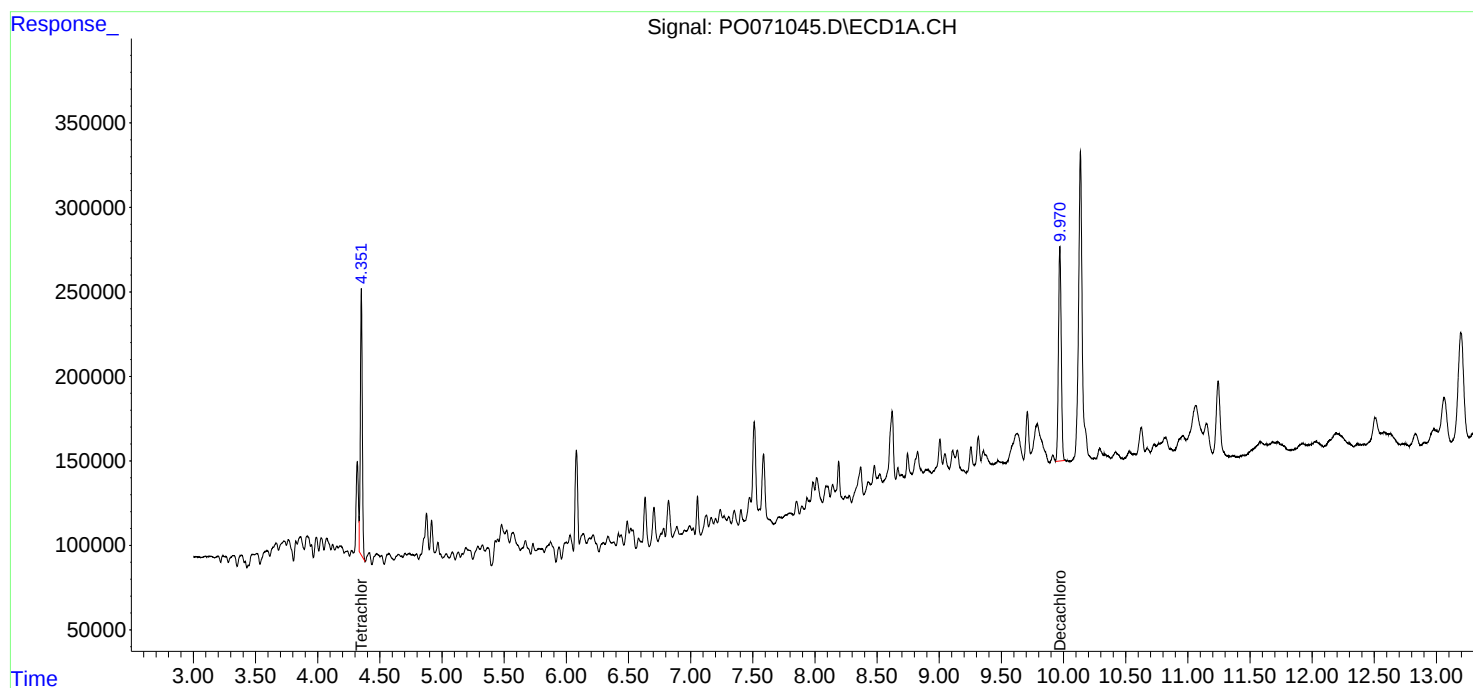


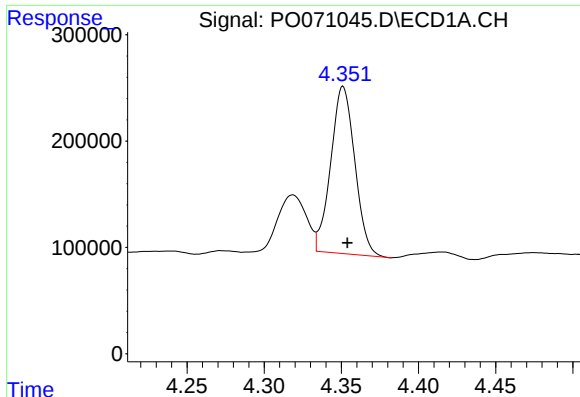

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 1710566
Conc: 22.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-JOP-BH-09-A

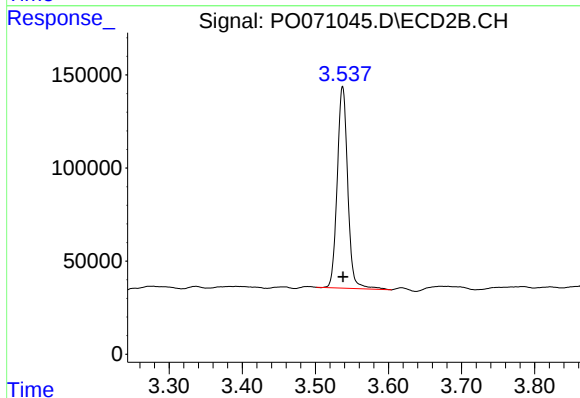


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 1081964
Conc: 24.41 ng/ml

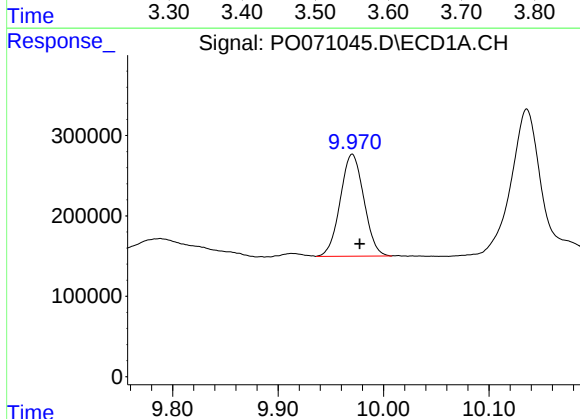

#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.007 min
Response: 1970722
Conc: 21.54 ng/ml

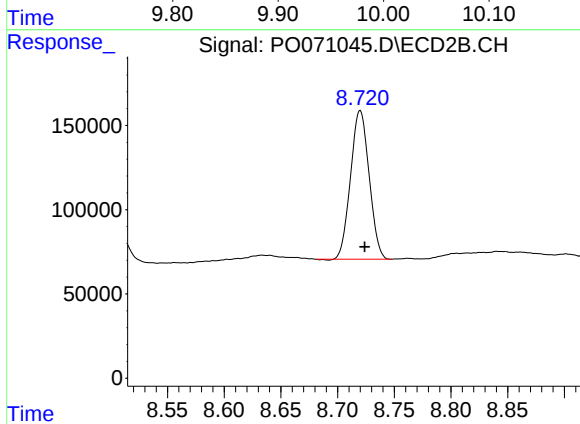

#2 Decachlorobiphenyl

R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 1005124
Conc: 17.50 ng/ml